

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031423\
Data File : VX034482.D
Acq On : 15 Mar 2023 04:40
Operator : JC/MD
Sample : 01903-03 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE103D2-20230310DL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M

Title : SW846 8260

Signal : TIC: VX034482.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.563	69	78	81	rBV3	9133	18441	1.25%	0.215%
2	4.556	560	569	579	rBV	5372	16759	1.13%	0.195%
3	5.379	692	704	721	rBV2	161396	477067	32.29%	5.557%
4	5.550	721	732	747	rVB	273813	780758	52.85%	9.094%
5	5.952	786	798	812	rBV2	188662	504750	34.17%	5.879%
6	6.757	919	930	944	rBV	449778	1065516	72.13%	12.411%
7	7.123	979	990	1009	rBV	346837	763265	51.67%	8.890%
8	8.647	1233	1240	1258	rBV	947103	1477309	100.00%	17.207%
9	10.049	1465	1470	1485	rBV	900651	1269285	85.92%	14.784%
10	11.079	1634	1639	1651	rBV	850605	1056250	71.50%	12.303%
11	12.018	1788	1793	1804	rBV	876722	1156123	78.26%	13.466%




Sum of corrected areas: 8585523

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031423\
Data File : VX034482.D
Acq On : 15 Mar 2023 04:40
Operator : JC/MD
Sample : 01903-03 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE103D2-20230310DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

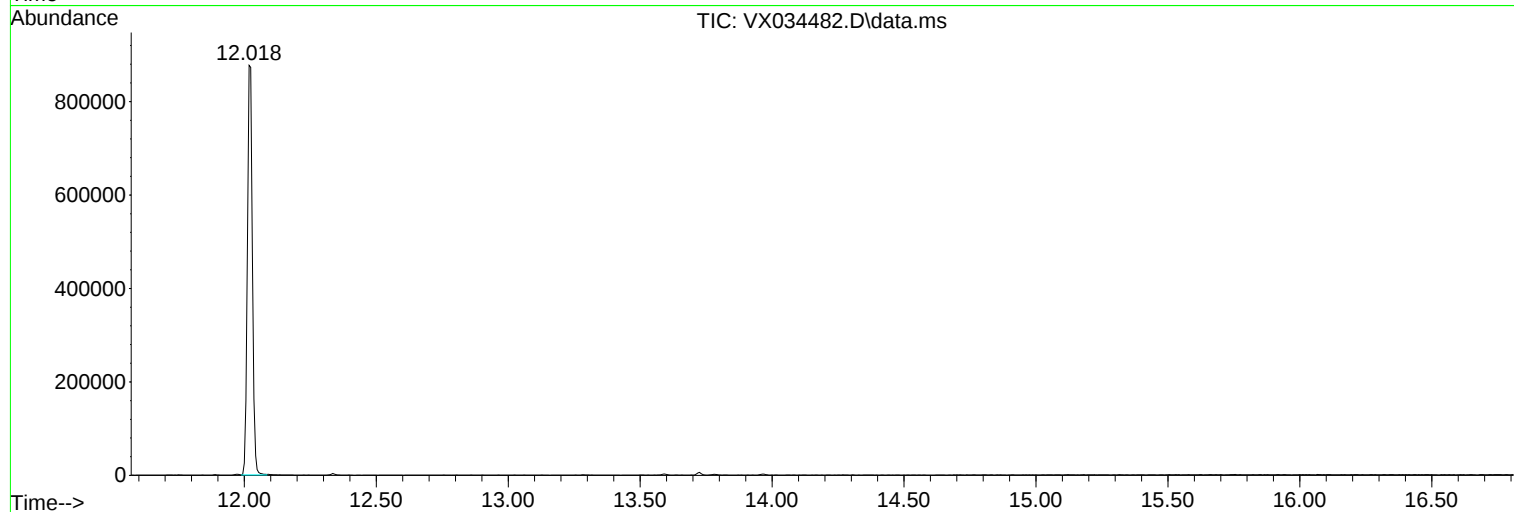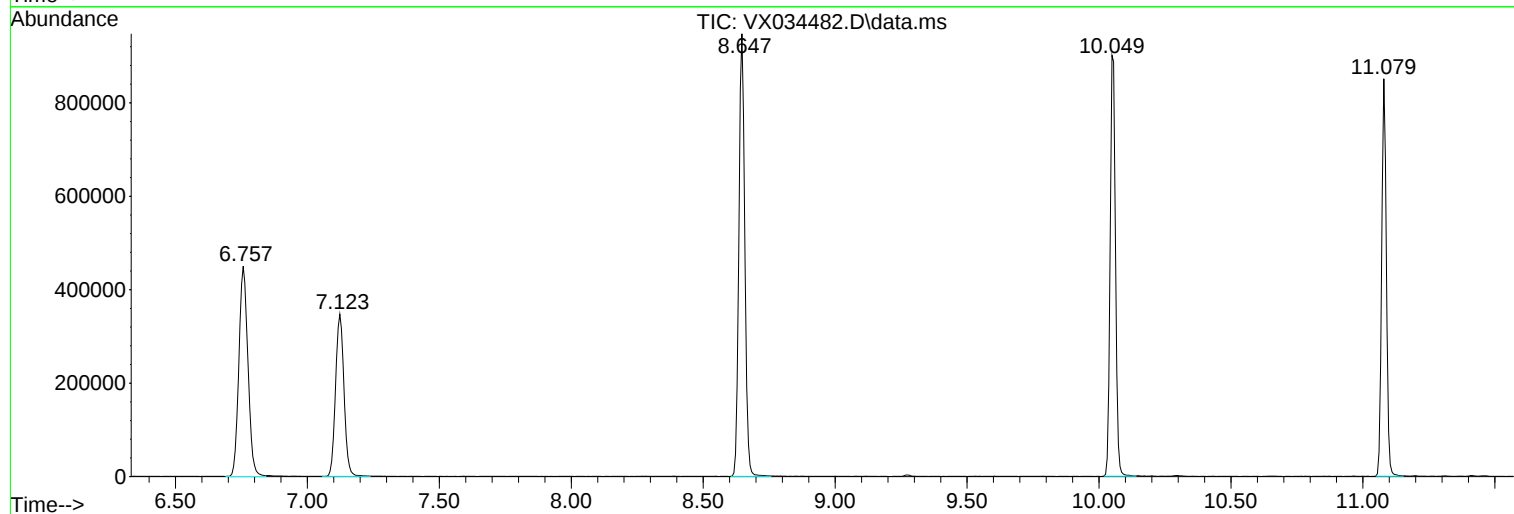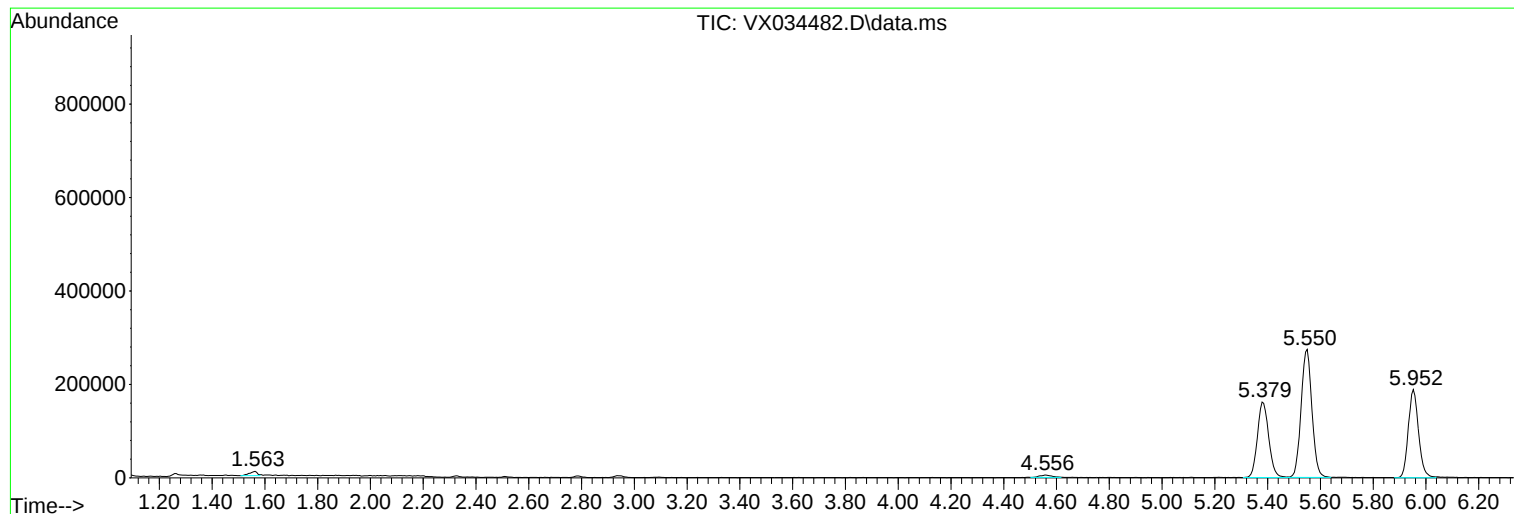

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031423\
Data File : VX034482.D
Acq On : 15 Mar 2023 04:40
Operator : JC/MD
Sample : 01903-03 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE103D2-20230310DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031423\
Data File : VX034482.D
Acq On : 15 Mar 2023 04:40
Operator : JC/MD
Sample : 01903-03 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE103D2-20230310DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------