

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031423\
Data File : VX034490.D
Acq On : 15 Mar 2023 07:48
Operator : JC/MD
Sample : 01903-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TT150S1-20230310

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M

Title : SW846 8260

Signal : TIC: VX034490.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	40	rBV	15421	40313	2.96%	0.544%
2	1.563	69	78	81	rBV4	8113	17625	1.30%	0.238%
3	5.385	694	705	721	rBV2	147207	434764	31.97%	5.864%
4	5.550	721	732	746	rVV	252788	711020	52.29%	9.591%
5	5.952	788	798	816	rBV	172785	468825	34.48%	6.324%
6	6.757	921	930	948	rBV	402186	976033	71.77%	13.165%
7	7.123	982	990	1005	rBV2	110318	248055	18.24%	3.346%
8	8.647	1233	1240	1257	rBV	867936	1359863	100.00%	18.343%
9	9.275	1337	1343	1348	rBV	17224	26831	1.97%	0.362%
10	10.055	1465	1471	1484	rBV	830943	1155605	84.98%	15.587%
11	11.079	1634	1639	1651	rBV	778575	950506	69.90%	12.821%
12	12.024	1788	1794	1804	rBV	787867	1024261	75.32%	13.816%




Sum of corrected areas: 7413701

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031423\
Data File : VX034490.D
Acq On : 15 Mar 2023 07:48
Operator : JC/MD
Sample : 01903-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TT150S1-20230310

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

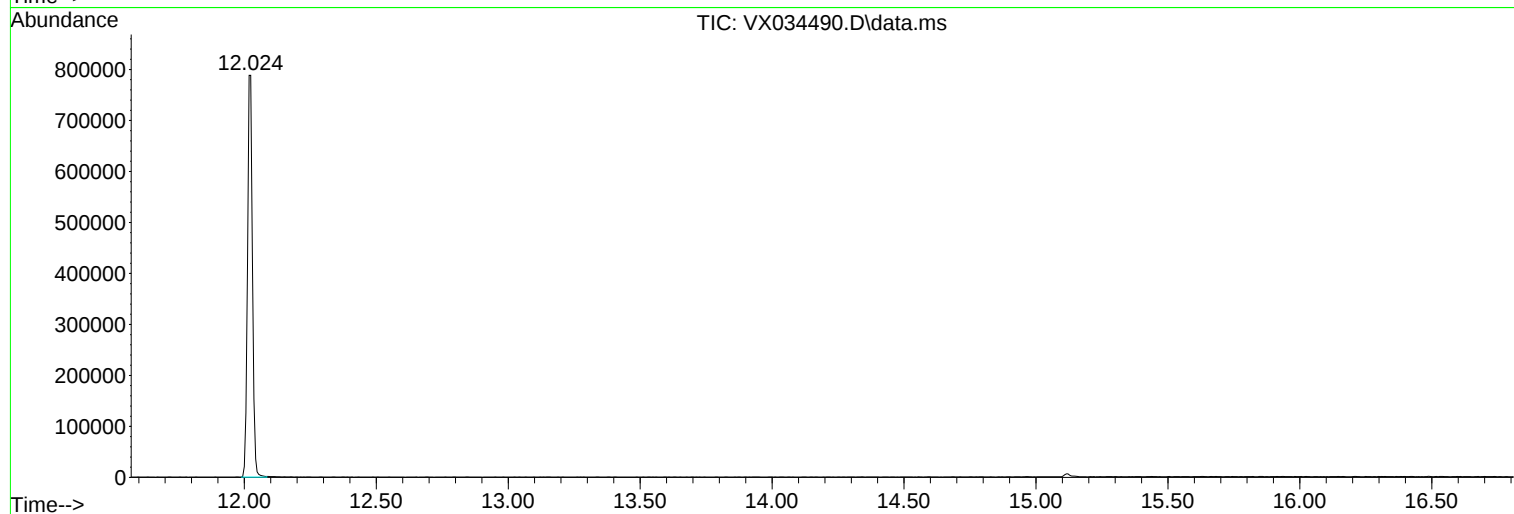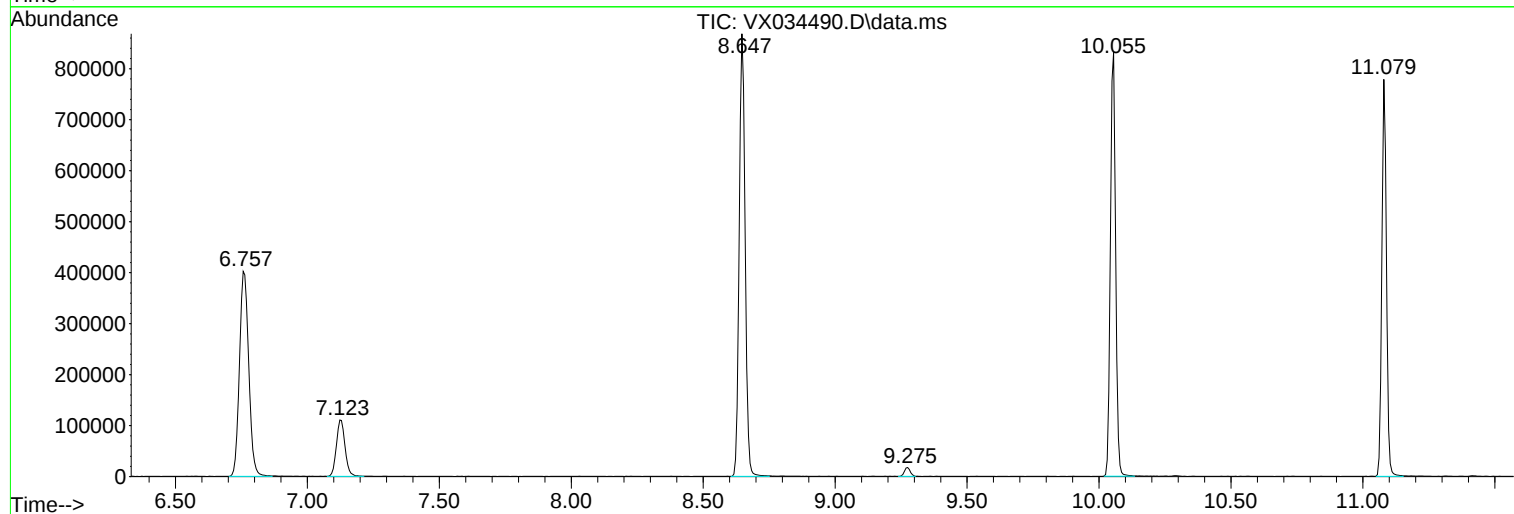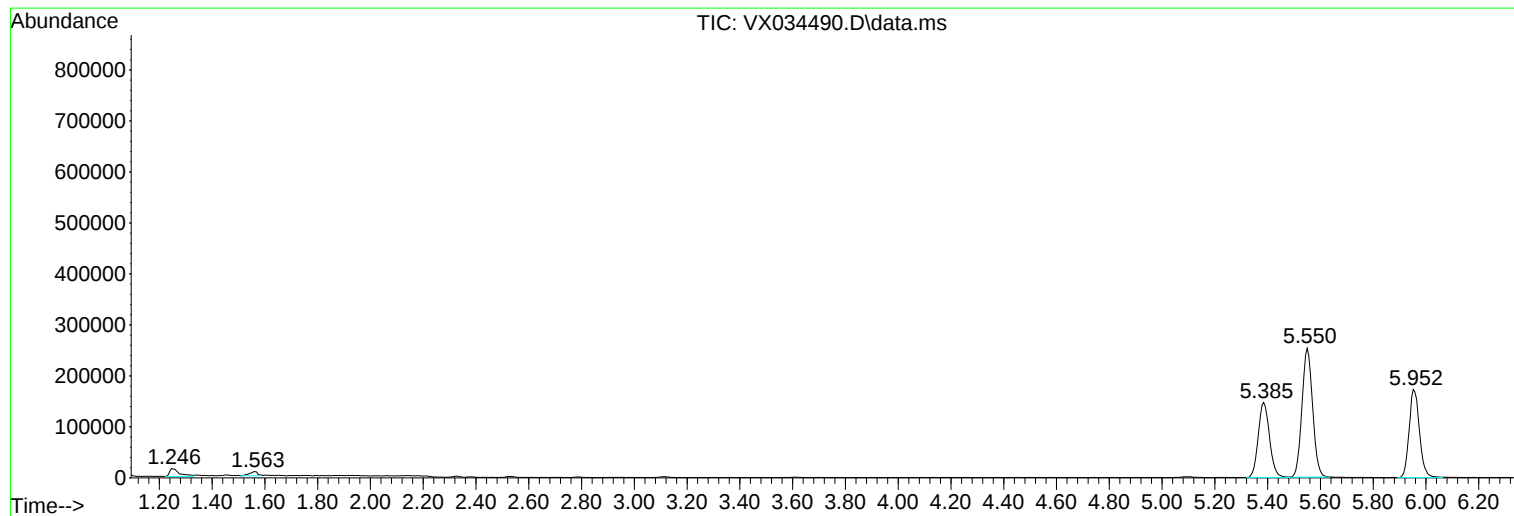

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031423\
Data File : VX034490.D
Acq On : 15 Mar 2023 07:48
Operator : JC/MD
Sample : 01903-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TT150S1-20230310

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031423\
Data File : VX034490.D
Acq On : 15 Mar 2023 07:48
Operator : JC/MD
Sample : 01903-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TT150S1-20230310

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------