
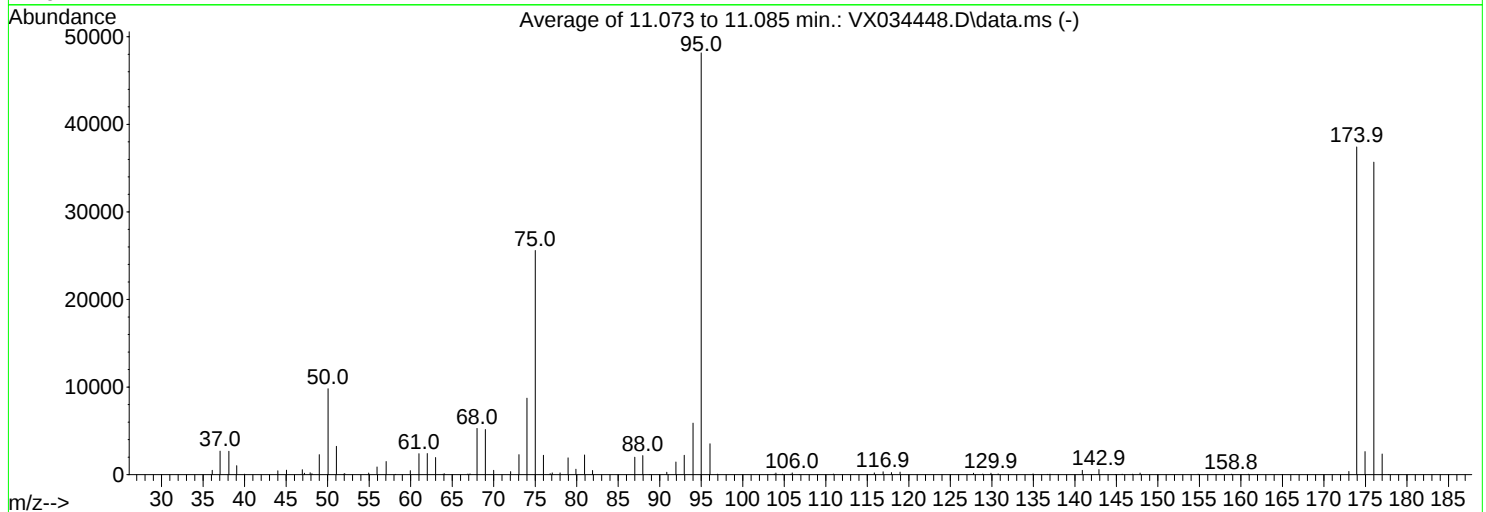


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031423\
Data File : VX034448.D
Acq On : 14 Mar 2023 08:24
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Title : SW846 8260
Last Update : Mon Mar 13 10:29:32 2023

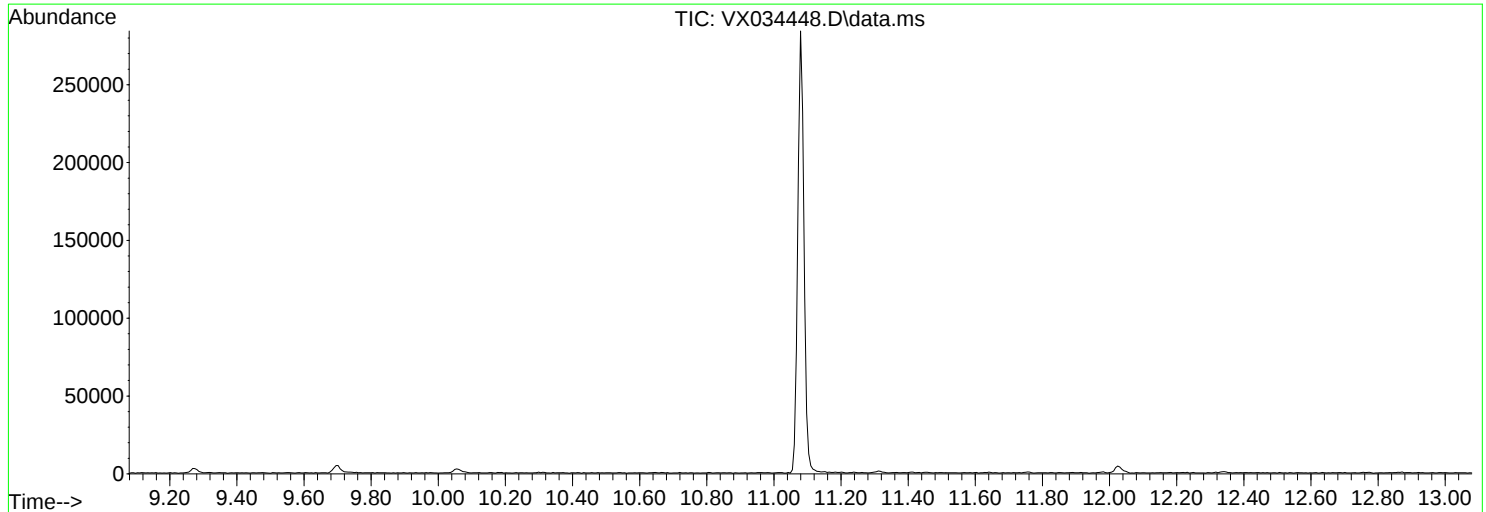

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	9807	PASS
75	95	30	60	53.2	25605	PASS
95	95	100	100	100.0	48163	PASS
96	95	5	9	7.3	3523	PASS
173	174	0.00	2	1.0	372	PASS
174	95	50	100	77.7	37411	PASS
175	174	5	9	7.0	2637	PASS
176	174	95	101	95.4	35685	PASS
177	176	5	9	6.6	2350	PASS