
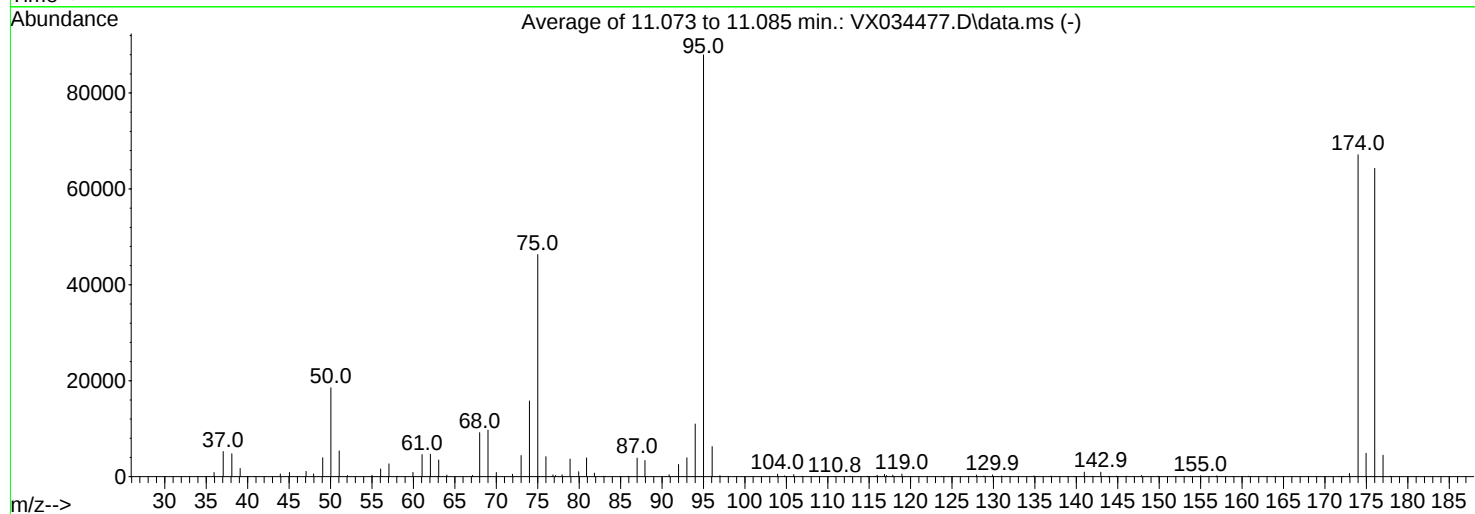


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031423\
Data File : VX034477.D
Acq On : 15 Mar 2023 02:02
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Title : SW846 8260
Last Update : Mon Mar 13 10:29:32 2023

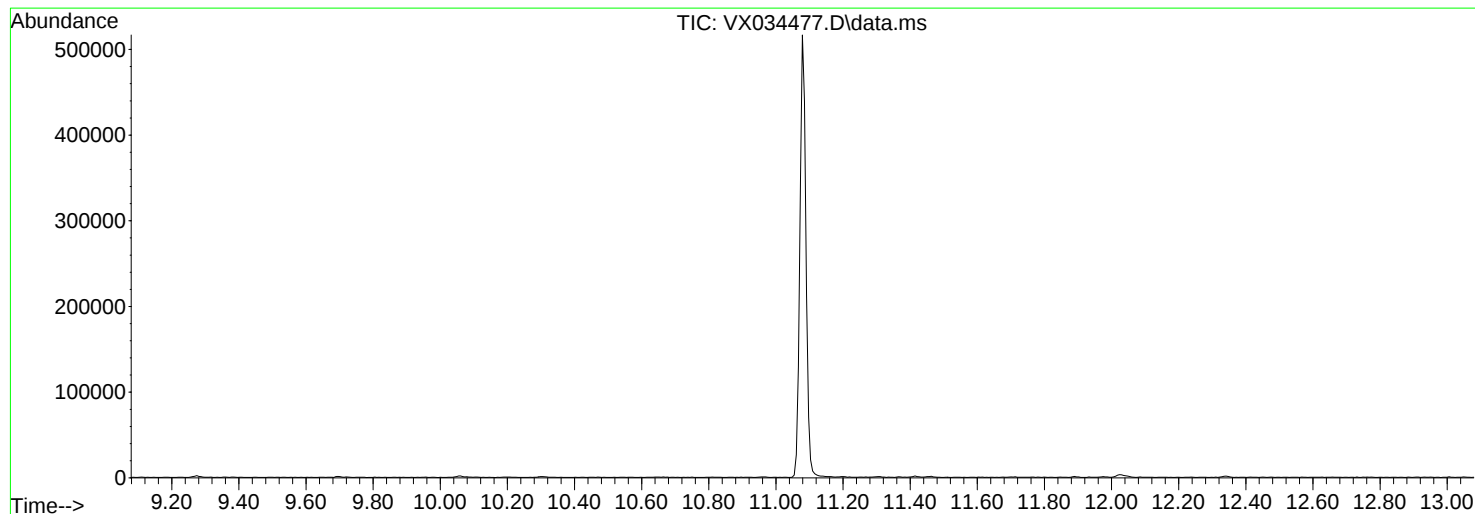

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.0	18513	PASS
75	95	30	60	52.7	46323	PASS
95	95	100	100	100.0	87965	PASS
96	95	5	9	7.1	6286	PASS
173	174	0.00	2	1.0	673	PASS
174	95	50	100	76.3	67152	PASS
175	174	5	9	7.2	4858	PASS
176	174	95	101	95.8	64312	PASS
177	176	5	9	6.9	4465	PASS