

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031425\
 Data File : VX045289.D
 Acq On : 14 Mar 2025 12:09
 Operator : JC/MD
 Sample : Q1502-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PT-VOA-WP

Quant Time: Mar 15 03:57:12 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X022125W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Sat Feb 22 01:06:36 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Bromochloromethane	4.891	128	15579	30.000	ug/l	0.00
28) 1,4-Difluorobenzene	6.757	114	85357	30.000	ug/l	0.00
57) Chlorobenzene-d5	10.049	117	77634	30.000	ug/l	0.00
System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	5.952	65	50115	33.120	ug/l	0.00
Spiked Amount 30.000	Range 91 - 110		Recovery = 110.400%#			
60) 4-Bromofluorobenzene	11.079	95	42282	29.138	ug/l	0.00
Spiked Amount 30.000	Range 63 - 112		Recovery = 97.133%			
63) Toluene-d8	8.647	98	132949	30.955	ug/l	0.00
Spiked Amount 30.000	Range 91 - 112		Recovery = 103.200%			
Target Compounds						Qvalue
5) Bromomethane	1.593	94	35096	66.427	ug/l	97
7) Trichlorofluoromethane	1.874	101	180810	88.633	ug/l	99
10) 1,1-Dichloroethene	2.307	96	103720	87.642	ug/l	90
15) Acetone	2.380	58	29571	160.623	ug/l	91
18) Methylene Chloride	2.782	84	66680	50.093	ug/l	97
19) trans-1,2-Dichloroethene	3.081	96	92070	76.896	ug/l	94
22) cis-1,2-Dichloroethene	4.483	96	153863	107.237	ug/l	93
24) Methyl tert-Butyl Ether	3.111	73	200165	51.821	ug/l	97
25) Chloroform	5.087	83	159427	69.773	ug/l	96
30) 2-Butanone	4.562	43	38742	42.718	ug/l	95
33) Carbon Tetrachloride	5.666	117	46492	28.957	ug/l	98
34) Benzene	6.031	78	539322	109.531	ug/l	99
36) 1,2-Dichloroethane	6.080	62	62324	36.970	ug/l	95
37) Trichloroethene	7.123	130	58559	50.835	ug/l	97
39) 1,2-Dichloropropane	7.421	63	94256	76.996	ug/l	99
40) Dibromomethane	7.574	93	88604	100.863	ug/l	98
41) Bromodichloromethane	7.818	83	27549	15.779	ug/l	99
48) t-1,3-Dichloropropene	8.976	75	115891	68.864	ug/l	99
49) cis-1,3-Dichloropropene	8.360	75	100250	52.623	ug/l	94
58) 4-Methyl-2-Pentanone	8.574	43	229183	129.774	ug/l	99
59) 2-Hexanone	9.427	43	188355	147.557	ug/l	98
61) Tetrachloroethene	9.269	164	115257	120.564	ug/l	95
62) Toluene	8.714	91	520098	101.132	ug/l	100
64) Chlorobenzene	10.073	112	354147	111.129	ug/l	97
65) 1,1,1,2-Tetrachloroethane	10.159	131	111641	106.168	ug/l	99
66) Ethyl Benzene	10.189	91	196906	34.972	ug/l	95
67) m/p-Xylenes	10.299	106	146407	69.792	ug/l	96
68) o-Xylene	10.640	106	286905	139.393	ug/l	97
69) Styrene	10.653	104	296336	86.204	ug/l	90
76) 1,3,5-Trimethylbenzene	11.451	105	390858	89.198	ug/l	99
83) 1,3-Dichlorobenzene	11.969	146	107129	47.089	ug/l	99
87) 1,2-Dichlorobenzene	12.335	146	259016	116.034	ug/l	99
91) Naphthalene	13.774	128	409326	85.803	ug/l	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031425\
Data File : VX045289.D
Acq On : 14 Mar 2025 12:09
Operator : JC/MD
Sample : Q1502-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PT-VOA-WP

Quant Time: Mar 15 03:57:12 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X022125W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Sat Feb 22 01:06:36 2025
Response via : Initial Calibration




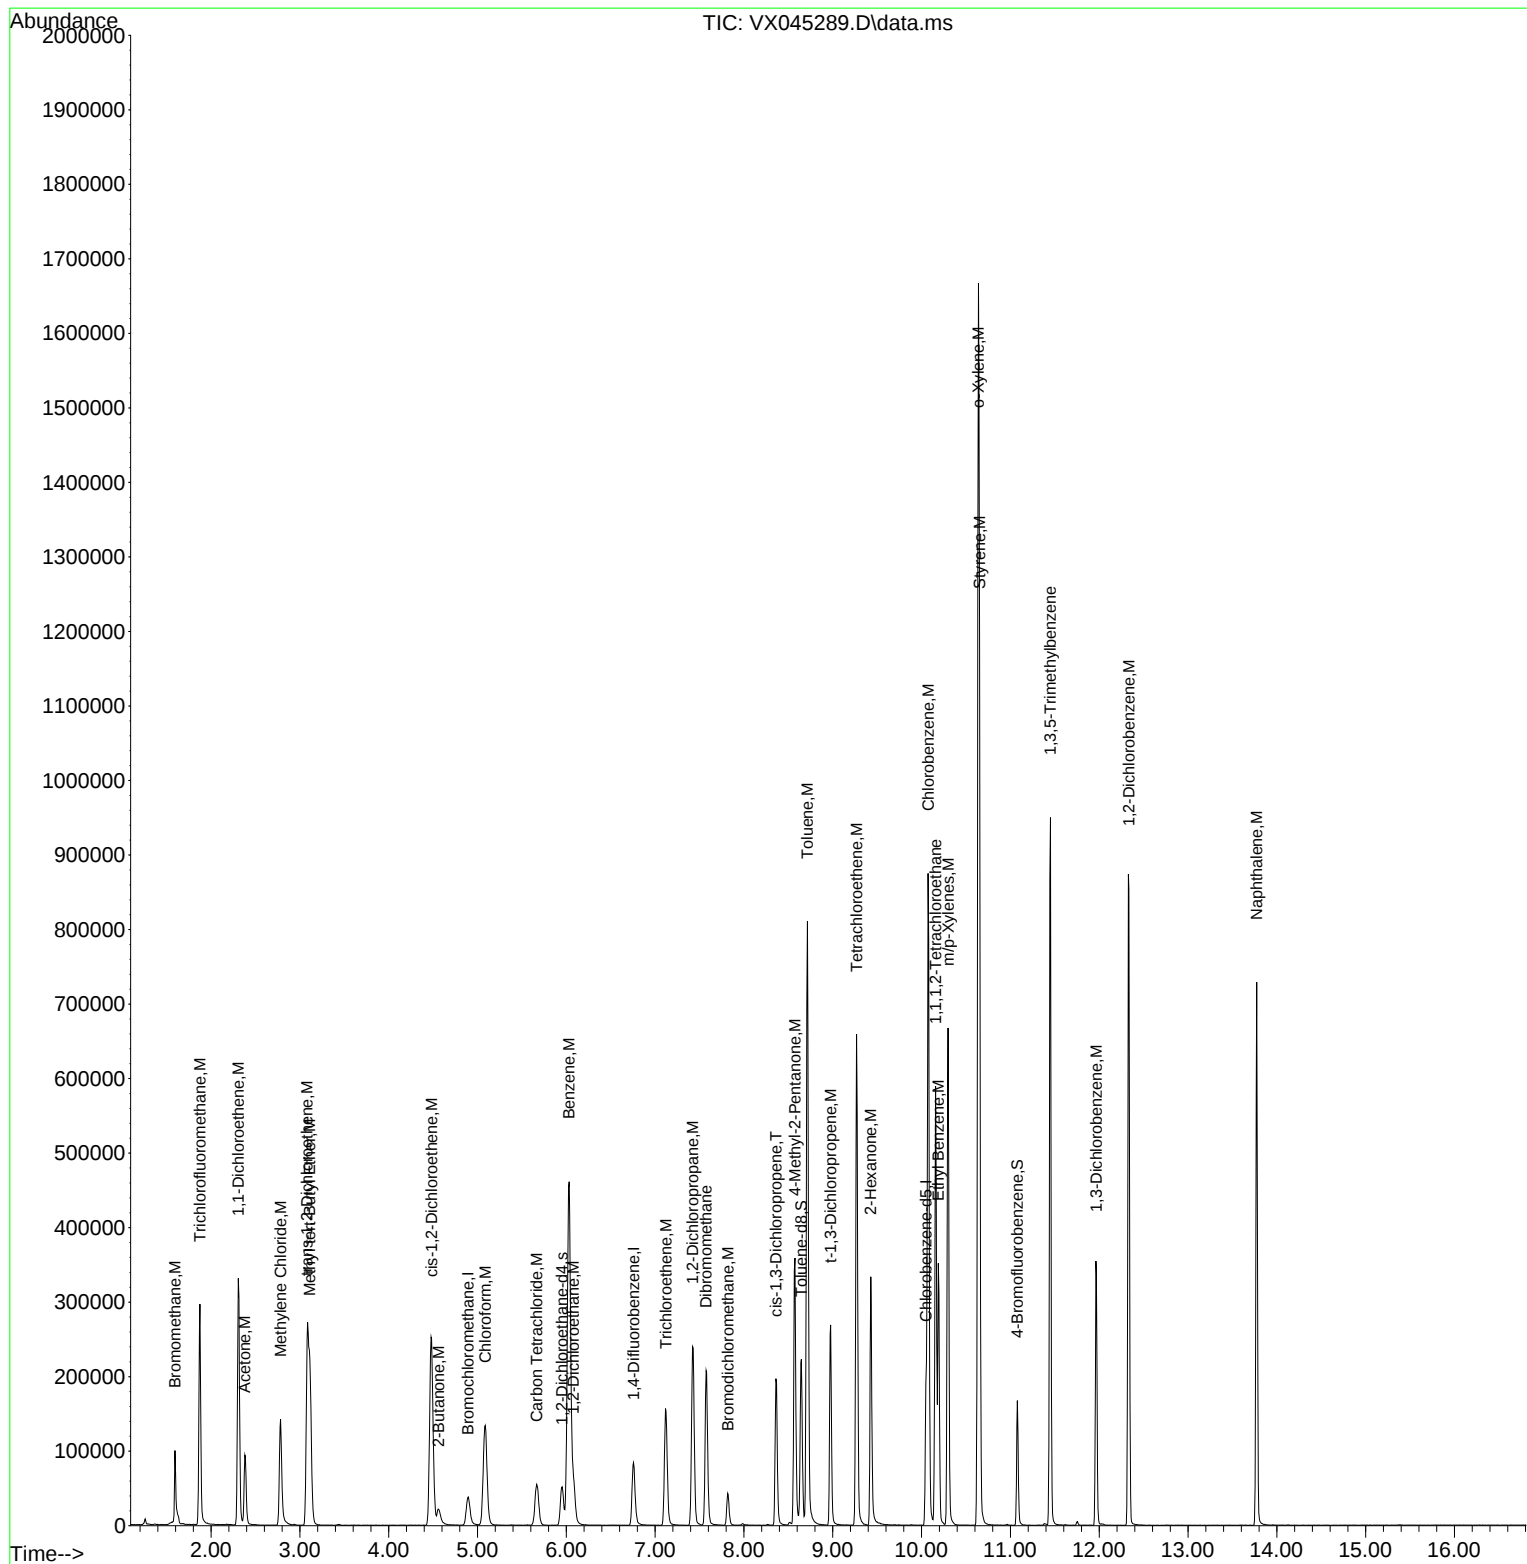




#1
Bromochloromethane
Concen: 30.000 ug/l
RT: 4.891 min Scan# 61
Delta R.T. 0.006 min
Lab File: VX045289.D
Acq: 14 Mar 2025 12:09




Instrument :
MSVOA_X
ClientSampleId :
PT-VOA-WP


Tgt Ion:128 Resp: 15579
Ion Ratio Lower Upper
128 100
49 187.3 0.0 449.7
130 128.3 0.0 312.7

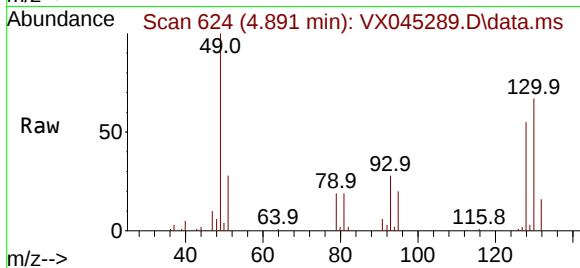

#5
Bromomethane
Concen: 66.427 ug/l
RT: 1.593 min Scan# 83
Delta R.T. -0.000 min
Lab File: VX045289.D
Acq: 14 Mar 2025 12:09

Tgt Ion: 94 Resp: 35096
Ion Ratio Lower Upper
94 100
96 93.1 72.2 108.4


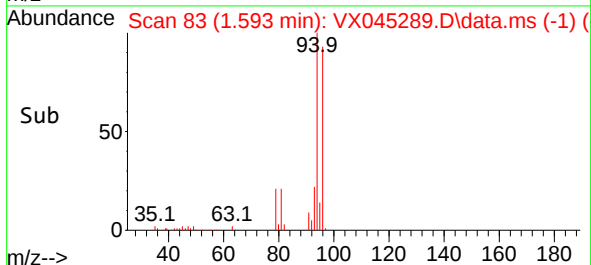

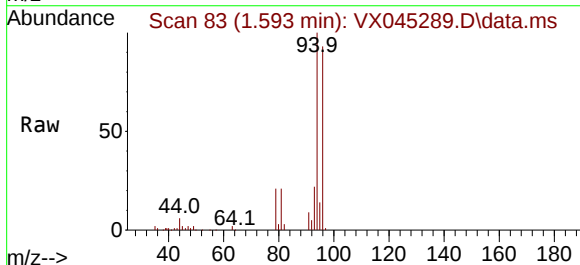




#7
Trichlorofluoromethane
Concen: 88.633 ug/l
RT: 1.874 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX045289.D
Acq: 14 Mar 2025 12:09




Instrument :
MSVOA_X
ClientSampleId :
PT-VOA-WP


Tgt Ion:101 Resp: 180810
Ion Ratio Lower Upper
101 100
103 62.1 48.8 73.2

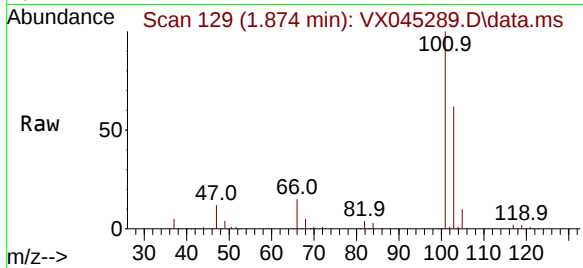

#10
1,1-Dichloroethene
Concen: 87.642 ug/l
RT: 2.307 min Scan# 200
Delta R.T. -0.006 min
Lab File: VX045289.D
Acq: 14 Mar 2025 12:09

Tgt Ion: 96 Resp: 103720
Ion Ratio Lower Upper
96 100
61 172.6 124.2 186.2
98 61.9 51.1 76.7


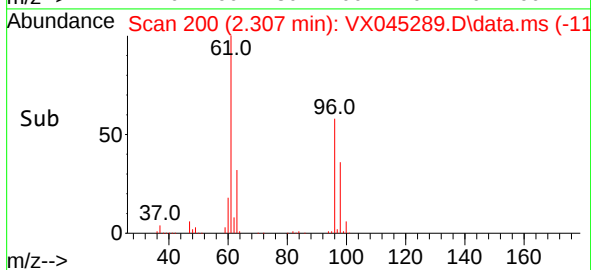

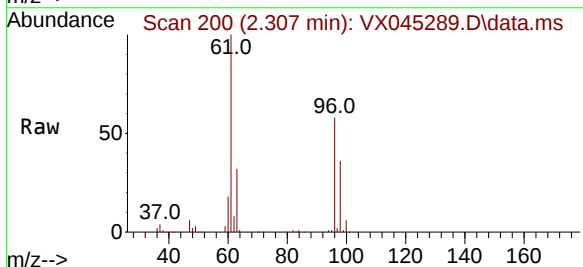




#15
Acetone
Concen: 160.623 ug/l
RT: 2.380 min Scan# 212
Delta R.T. -0.000 min
Lab File: VX045289.D
Acq: 14 Mar 2025 12:09




Instrument :
MSVOA_X
ClientSampleId :
PT-VOA-WP


Tgt Ion: 58 Resp: 29571
Ion Ratio Lower Upper
58 100
43 342.9 258.6 388.0

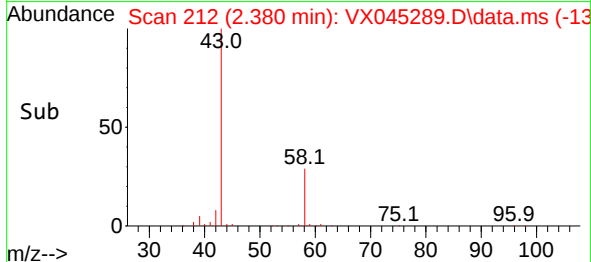

#18
Methylene Chloride
Concen: 50.093 ug/l
RT: 2.782 min Scan# 278
Delta R.T. -0.000 min
Lab File: VX045289.D
Acq: 14 Mar 2025 12:09

Tgt Ion: 84 Resp: 66680
Ion Ratio Lower Upper
84 100
49 133.1 102.8 154.2
51 39.5 30.1 45.1
86 64.5 50.2 75.4




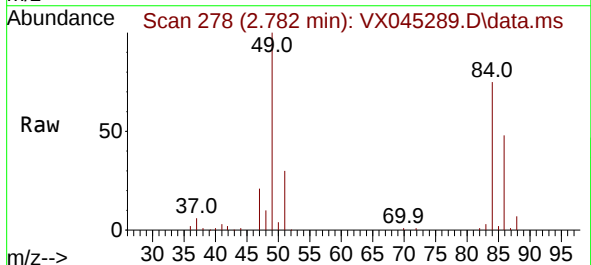




#19
trans-1,2-Dichloroethene
Concen: 76.896 ug/l
RT: 3.081 min Scan# 31
Delta R.T. -0.000 min
Lab File: VX045289.D
Acq: 14 Mar 2025 12:09




Instrument :
MSVOA_X
ClientSampleId :
PT-VOA-WP


Tgt Ion: 96 Resp: 92070
Ion Ratio Lower Upper
96 100
61 142.9 108.6 163.0
98 62.0 46.5 69.7

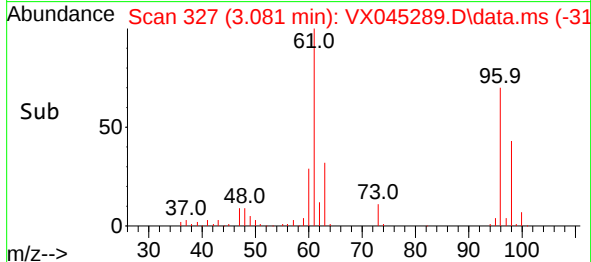

#22
cis-1,2-Dichloroethene
Concen: 107.237 ug/l
RT: 4.483 min Scan# 557
Delta R.T. -0.000 min
Lab File: VX045289.D
Acq: 14 Mar 2025 12:09

Tgt Ion: 96 Resp: 153863
Ion Ratio Lower Upper
96 100
61 135.7 118.9 178.3
98 64.1 50.7 76.1


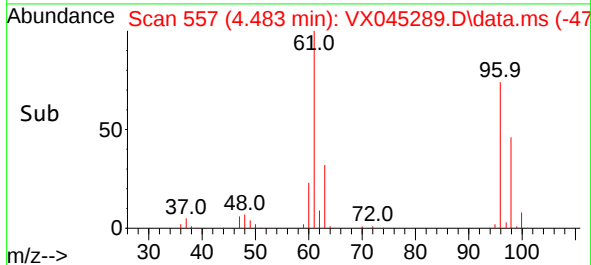






#24
Methyl tert-Butyl Ether
Concen: 51.821 ug/l
RT: 3.111 min Scan# 311
Delta R.T. 0.006 min
Lab File: VX045289.D
Acq: 14 Mar 2025 12:09




Instrument :
MSVOA_X
ClientSampleId :
PT-VOA-WP


Tgt Ion: 73 Resp: 200165
Ion Ratio Lower Upper
73 100
43 23.2 17.4 26.0

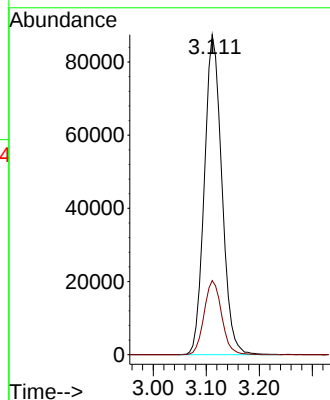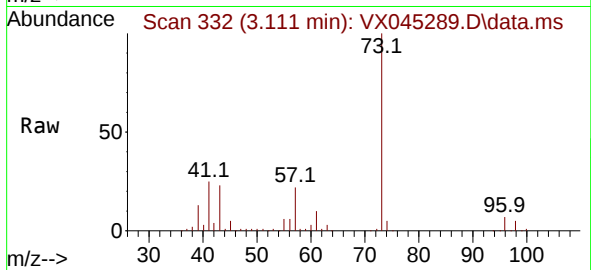

#25
Chloroform
Concen: 69.773 ug/l
RT: 5.087 min Scan# 656
Delta R.T. -0.000 min
Lab File: VX045289.D
Acq: 14 Mar 2025 12:09

Tgt Ion: 83 Resp: 159427
Ion Ratio Lower Upper
83 100
85 61.8 51.7 77.5

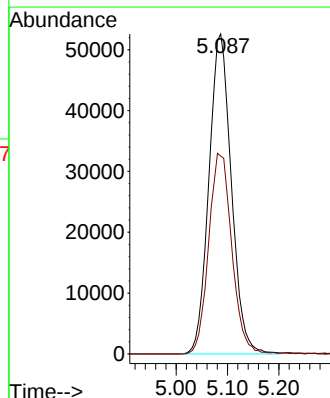



#27

1,2-Dichloroethane-d4

Concen: 33.120 ug/l

RT: 5.952 min Scan# 797

Delta R.T. 0.006 min

Lab File: VX045289.D

Acq: 14 Mar 2025 12:09

Instrument :

MSVOA_X

ClientSampleId :





PT-VOA-WP

Tgt Ion: 65 Resp: 50115

Ion Ratio Lower Upper

65 100

67 51.9 42.6 64.0

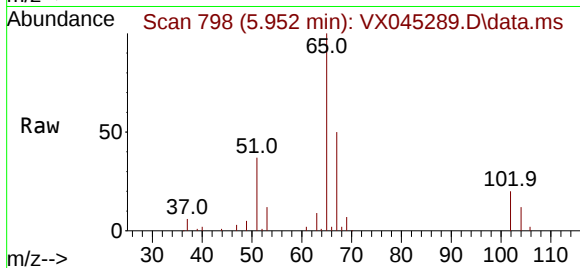

#28

1,4-Difluorobenzene

Concen: 30.000 ug/l

RT: 6.757 min Scan# 930

Delta R.T. -0.000 min

Lab File: VX045289.D

Acq: 14 Mar 2025 12:09




Tgt Ion: 114 Resp: 85357


Ion Ratio Lower Upper

114 100

63 21.9 16.8 25.2

88 16.4 12.7 19.1




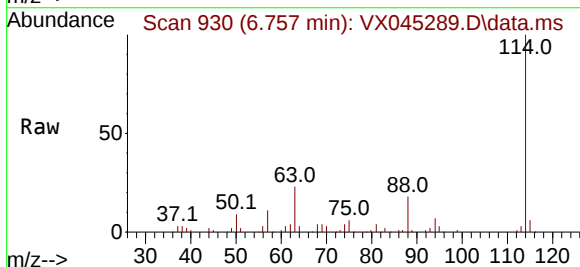


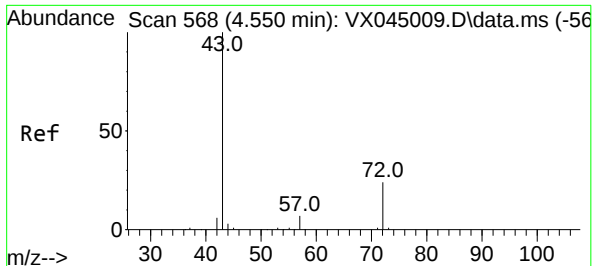

#30
2-Butanone
Concen: 42.718 ug/l
RT: 4.562 min Scan# 51
Delta R.T. 0.012 min
Lab File: VX045289.D
Acq: 14 Mar 2025 12:09




Instrument :
MSVOA_X
ClientSampleId :
PT-VOA-WP


Tgt Ion: 43 Resp: 38742
Ion Ratio Lower Upper
43 100
57 7.1 6.2 9.2
72 22.3 20.2 30.2

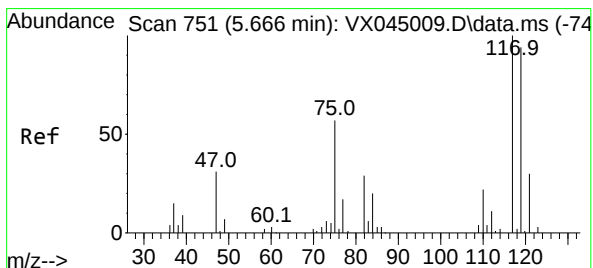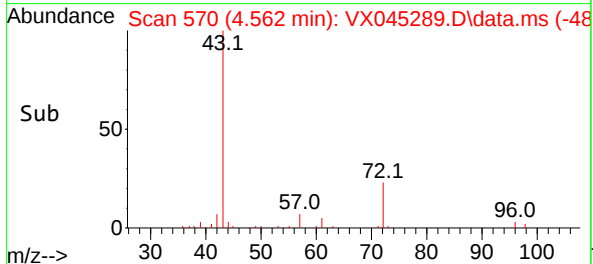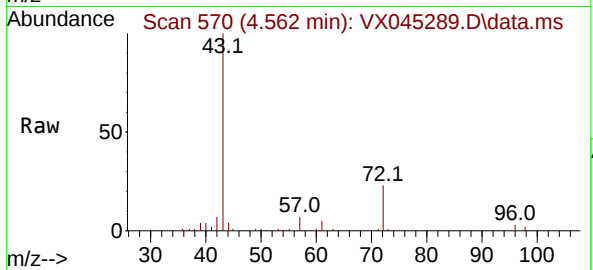

#33
Carbon Tetrachloride
Concen: 28.957 ug/l
RT: 5.666 min Scan# 751
Delta R.T. -0.000 min
Lab File: VX045289.D
Acq: 14 Mar 2025 12:09

Tgt Ion: 117 Resp: 46492
Ion Ratio Lower Upper
117 100
119 91.2 75.1 112.7
121 30.1 23.9 35.9


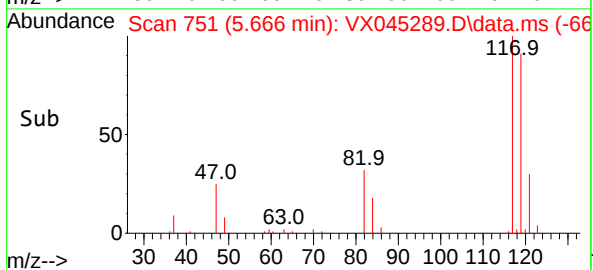

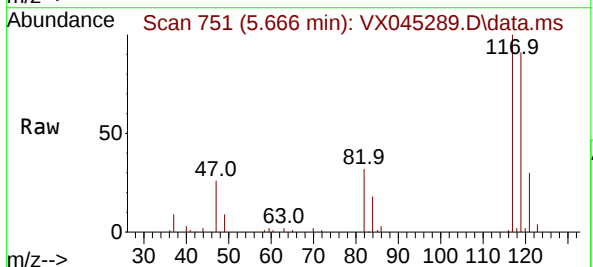




#34
Benzene
Concen: 109.531 ug/l
RT: 6.031 min Scan# 811
Delta R.T. -0.000 min
Lab File: VX045289.D
Acq: 14 Mar 2025 12:09




Instrument :
MSVOA_X
ClientSampleId :
PT-VOA-WP


Tgt Ion: 78 Resp: 539322
Ion Ratio Lower Upper
78 100
77 24.2 19.6 29.4
51 18.0 13.8 20.6

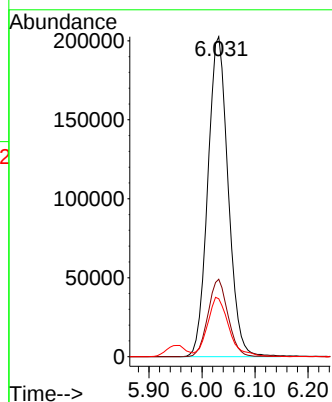

#36
1,2-Dichloroethane
Concen: 36.970 ug/l
RT: 6.080 min Scan# 819
Delta R.T. -0.000 min
Lab File: VX045289.D
Acq: 14 Mar 2025 12:09

Tgt Ion: 62 Resp: 62324
Ion Ratio Lower Upper
62 100
98 8.1 7.9 11.9





#37

Trichloroethene

Concen: 50.835 ug/l

RT: 7.123 min Scan# 990

Delta R.T. 0.006 min

Lab File: VX045289.D

Acq: 14 Mar 2025 12:09

Instrument :

MSVOA_X

ClientSampleId :





PT-VOA-WP

Tgt Ion:130 Resp: 58559

Ion Ratio Lower Upper

130 100

95 101.6 79.0 118.4

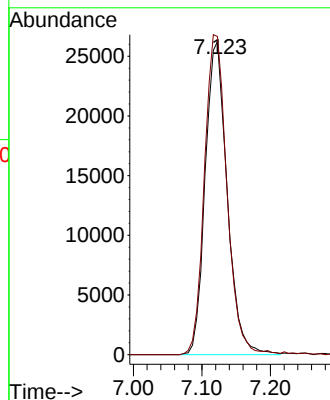

#39

1,2-Dichloropropane

Concen: 76.996 ug/l

RT: 7.421 min Scan# 1039

Delta R.T. -0.006 min

Lab File: VX045289.D




Acq: 14 Mar 2025 12:09


Tgt Ion: 63 Resp: 94256

Ion Ratio Lower Upper

63 100

65 30.1 24.3 36.5


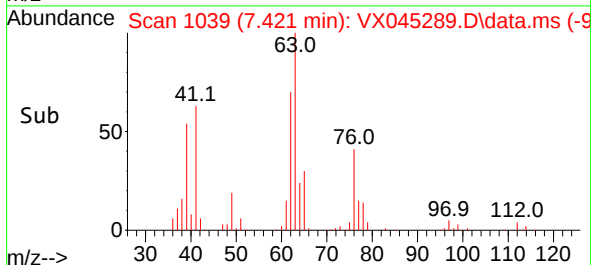
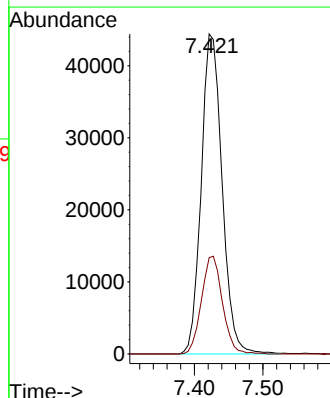
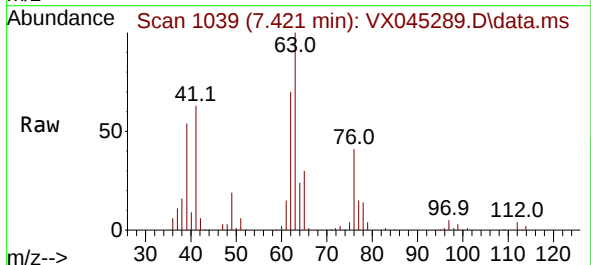


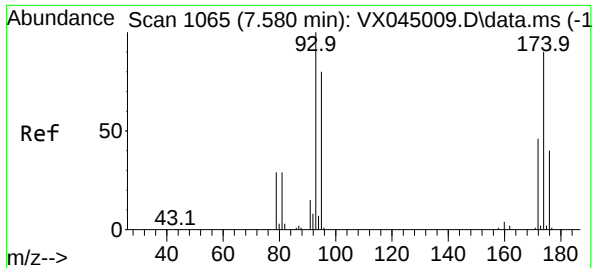

#40
Dibromomethane
Concen: 100.863 ug/l
RT: 7.574 min Scan# 1104
Delta R.T. -0.006 min
Lab File: VX045289.D
Acq: 14 Mar 2025 12:09




Instrument :
MSVOA_X
ClientSampleId :
PT-VOA-WP


Tgt Ion: 93 Resp: 88604
Ion Ratio Lower Upper
93 100
95 81.3 0.0 162.6
174 85.3 0.0 178.8

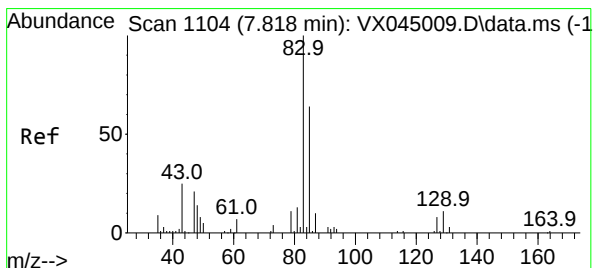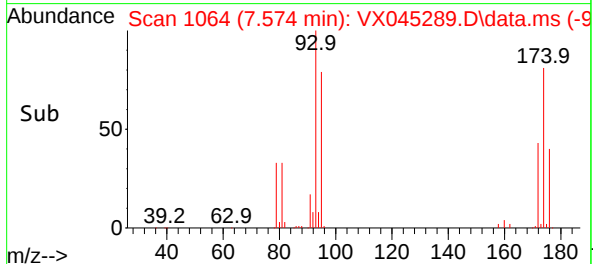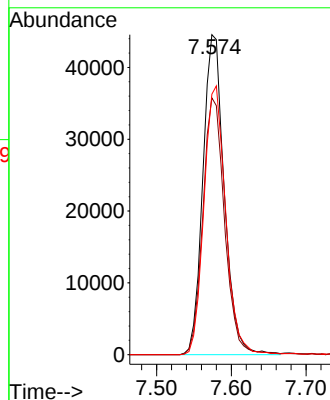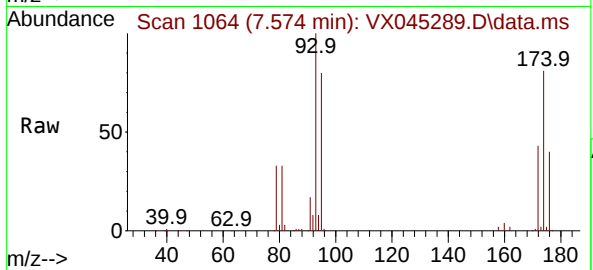

#41
Bromodichloromethane
Concen: 15.779 ug/l
RT: 7.818 min Scan# 1104
Delta R.T. -0.000 min
Lab File: VX045289.D
Acq: 14 Mar 2025 12:09

Tgt Ion: 83 Resp: 27549
Ion Ratio Lower Upper
83 100
85 62.9 51.0 76.6
127 8.3 6.1 9.1

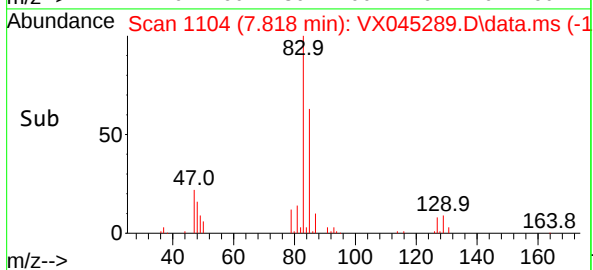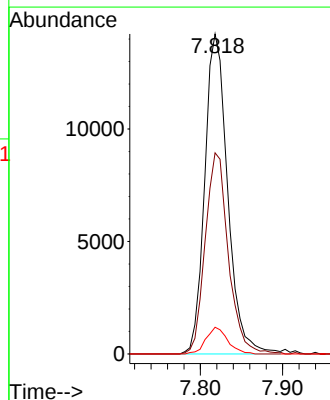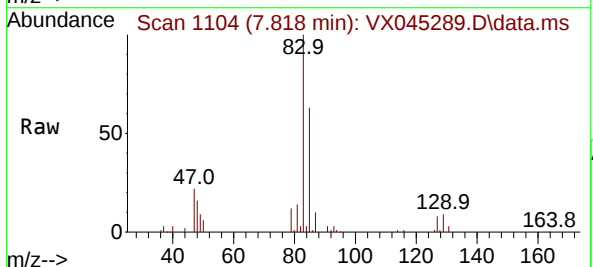



#48

t-1,3-Dichloropropene

Concen: 68.864 ug/l

RT: 8.976 min Scan# 11

Delta R.T. -0.000 min

Lab File: VX045289.D

Acq: 14 Mar 2025 12:09

Instrument :

MSVOA_X

ClientSampleId :





PT-VOA-WP

Tgt Ion: 75 Resp: 115891

Ion Ratio Lower Upper

75 100

77 31.6 25.7 38.5

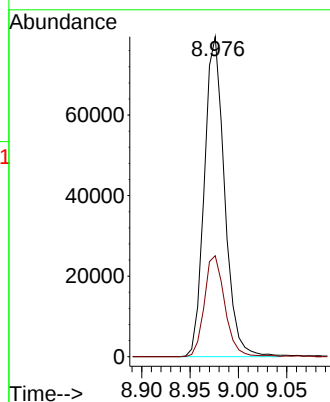

#49

cis-1,3-Dichloropropene

Concen: 52.623 ug/l

RT: 8.360 min Scan# 1193

Delta R.T. -0.000 min

Lab File: VX045289.D

Acq: 14 Mar 2025 12:09




Tgt Ion: 75 Resp: 100250


Ion Ratio Lower Upper

75 100

77 31.0 25.9 38.9

39 58.5 42.3 63.5

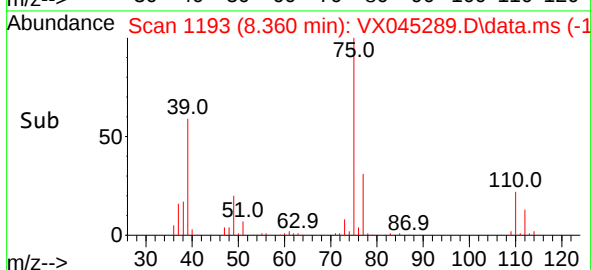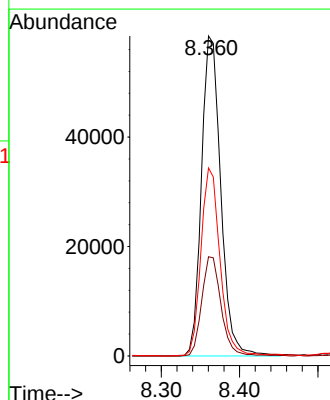



#57

Chlorobenzene-d5

Concen: 30.000 ug/l

RT: 10.049 min Scan# 1470

Delta R.T. -0.000 min

Lab File: VX045289.D

Acq: 14 Mar 2025 12:09

Instrument :

MSVOA_X

ClientSampleId :

PT-VOA-WP





Tgt Ion:117 Resp: 77634

Ion Ratio Lower Upper

117 100

82 59.0 45.8 68.8

119 32.0 25.5 38.3



#58

4-Methyl-2-Pentanone

Concen: 129.774 ug/l

RT: 8.574 min Scan# 1228

Delta R.T. 0.006 min

Lab File: VX045289.D

Acq: 14 Mar 2025 12:09




Tgt Ion: 43 Resp: 229183


Ion Ratio Lower Upper

43 100

58 36.4 29.5 44.3

85 15.7 12.9 19.3


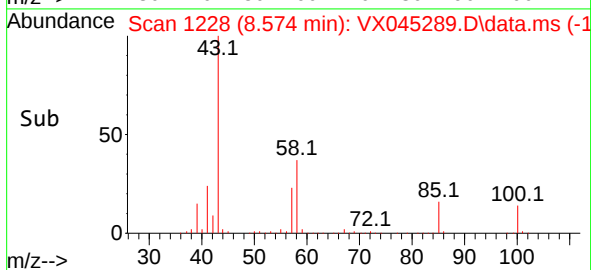






#59
2-Hexanone
Concen: 147.557 ug/l
RT: 9.427 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX045289.D
Acq: 14 Mar 2025 12:09




Instrument :
MSVOA_X
ClientSampleId :
PT-VOA-WP


Tgt Ion: 43 Resp: 188355
Ion Ratio Lower Upper
43 100
58 50.2 41.6 62.4
57 17.1 13.8 20.6



#60
4-Bromofluorobenzene
Concen: 29.138 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX045289.D
Acq: 14 Mar 2025 12:09


Tgt Ion: 95 Resp: 42282
Ion Ratio Lower Upper
95 100
174 73.1 59.5 89.3
176 68.9 55.5 83.3








#61
Tetrachloroethene
Concen: 120.564 ug/l
RT: 9.269 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX045289.D
Acq: 14 Mar 2025 12:09

Instrument :
MSVOA_X
ClientSampleId :
PT-VOA-WP







Tgt Ion:164 Resp: 115257
Ion Ratio Lower Upper
164 100
166 122.3 100.3 150.5
129 101.7 75.5 113.3
131 97.8 74.9 112.3

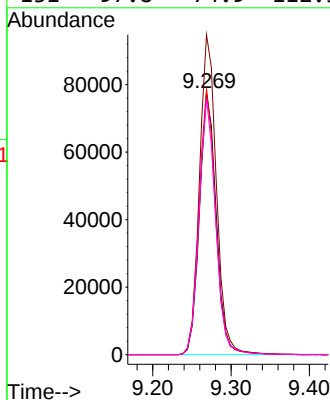

#62
Toluene
Concen: 101.132 ug/l
RT: 8.714 min Scan# 1251
Delta R.T. -0.000 min
Lab File: VX045289.D
Acq: 14 Mar 2025 12:09

Tgt Ion: 91 Resp: 520098
Ion Ratio Lower Upper
91 100
92 58.3 46.9 70.3



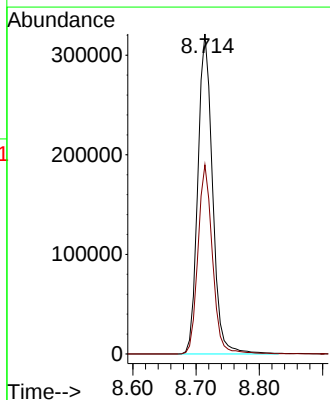
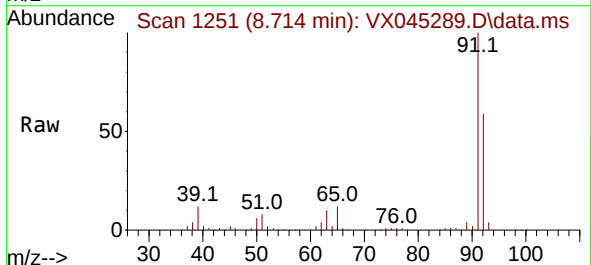




#63
Toluene-d8
Concen: 30.955 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX045289.D
Acq: 14 Mar 2025 12:09




Instrument :
MSVOA_X
ClientSampleId :
PT-VOA-WP


Tgt Ion: 98 Resp: 132949
Ion Ratio Lower Upper
98 100
100 64.4 51.7 77.5

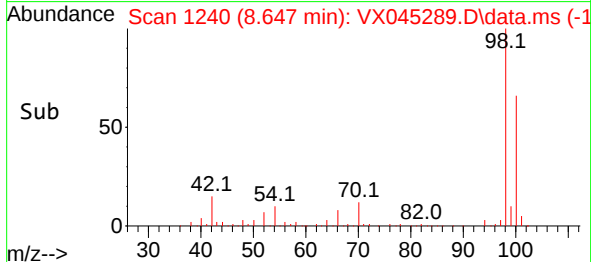

#64
Chlorobenzene
Concen: 111.129 ug/l
RT: 10.073 min Scan# 1474
Delta R.T. -0.000 min
Lab File: VX045289.D
Acq: 14 Mar 2025 12:09

Tgt Ion: 112 Resp: 354147
Ion Ratio Lower Upper
112 100
114 32.5 24.7 37.1


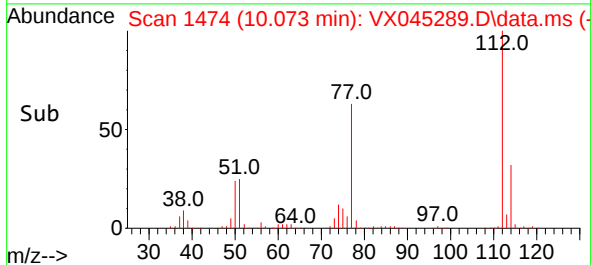






#65
 1,1,1,2-Tetrachloroethane
 Concen: 106.168 ug/l
 RT: 10.159 min Scan# 1488
 Delta R.T. -0.000 min
 Lab File: VX045289.D
 Acq: 14 Mar 2025 12:09




Instrument :
 MSVOA_X
 ClientSampleId :
 PT-VOA-WP


Tgt Ion:131 Resp: 111641
 Ion Ratio Lower Upper
 131 100
 133 95.7 0.0 187.8
 119 66.0 0.0 133.0

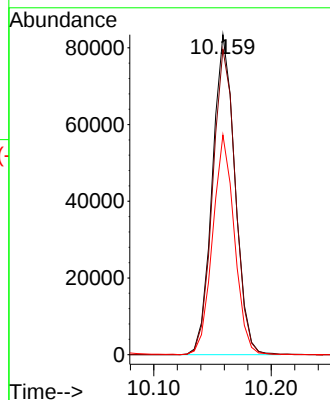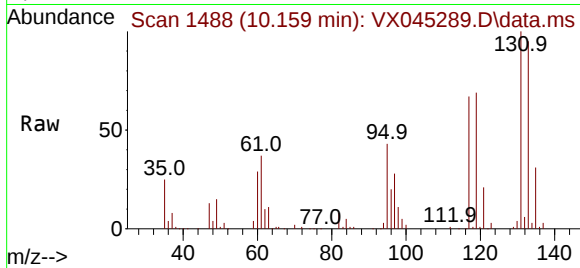

#66
 Ethyl Benzene
 Concen: 34.972 ug/l
 RT: 10.189 min Scan# 1493
 Delta R.T. -0.000 min
 Lab File: VX045289.D
 Acq: 14 Mar 2025 12:09

Tgt Ion: 91 Resp: 196906
 Ion Ratio Lower Upper
 91 100
 106 29.1 25.4 38.2



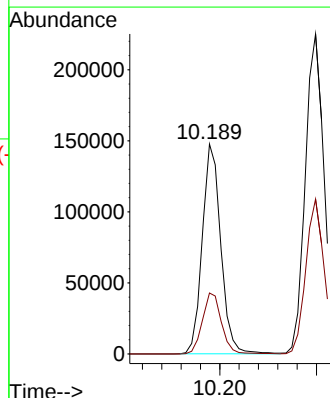
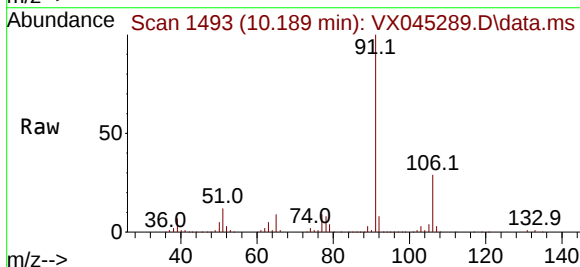




#67
m/p-Xylenes
Concen: 69.792 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. -0.000 min
Lab File: VX045289.D
Acq: 14 Mar 2025 12:09




Instrument :
MSVOA_X
ClientSampleId :
PT-VOA-WP


Tgt Ion:106 Resp: 146407
Ion Ratio Lower Upper
106 100
91 210.7 163.7 245.5

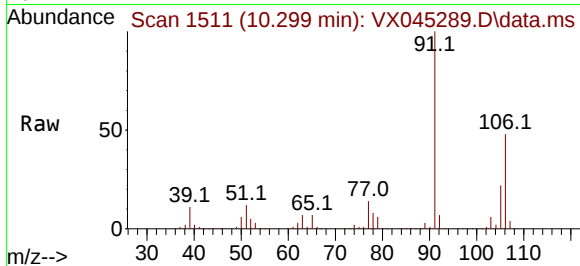

#68
o-Xylene
Concen: 139.393 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. -0.000 min
Lab File: VX045289.D
Acq: 14 Mar 2025 12:09

Tgt Ion:106 Resp: 286905
Ion Ratio Lower Upper
106 100
91 224.0 109.7 329.1

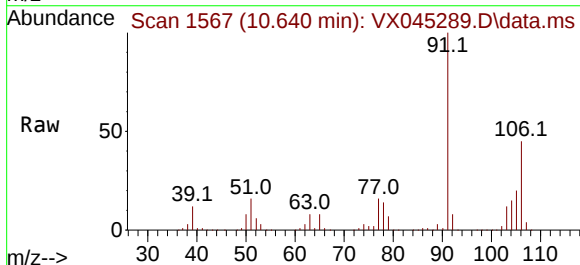



#69

Styrene

Concen: 86.204 ug/l

RT: 10.653 min Scan# 11

Delta R.T. -0.000 min

Lab File: VX045289.D

Acq: 14 Mar 2025 12:09

Instrument :

MSVOA_X

ClientSampleId :

PT-VOA-WP





Tgt Ion:104 Resp: 296336

Ion Ratio Lower Upper

104 100

78 59.8 41.4 62.0

103 59.2 43.0 64.4

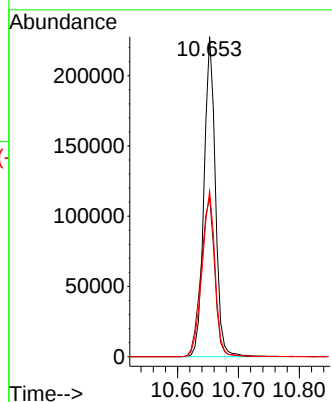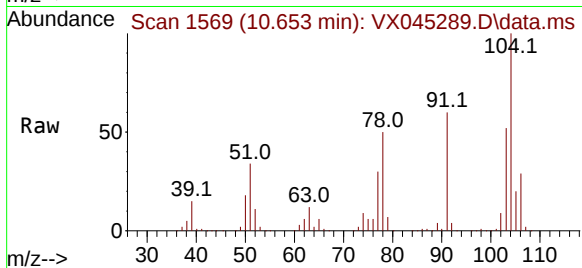

#76

1,3,5-Trimethylbenzene

Concen: 89.198 ug/l

RT: 11.451 min Scan# 1700

Delta R.T. -0.000 min

Lab File: VX045289.D




Acq: 14 Mar 2025 12:09


Tgt Ion:105 Resp: 390858

Ion Ratio Lower Upper

105 100

120 46.7 0.0 94.4


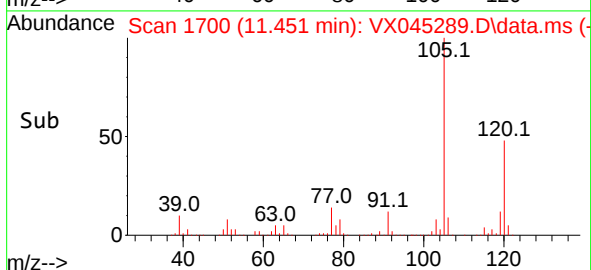

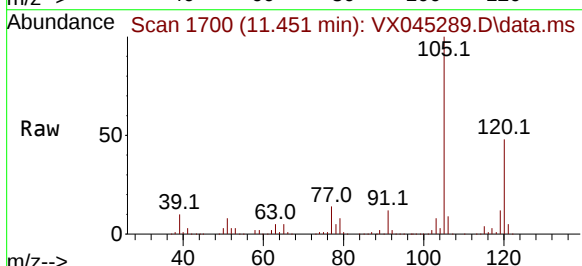




#83
1,3-Dichlorobenzene
Concen: 47.089 ug/l
RT: 11.969 min Scan# 1785
Delta R.T. -0.000 min
Lab File: VX045289.D
Acq: 14 Mar 2025 12:09




Instrument :
MSVOA_X
ClientSampleId :
PT-VOA-WP


Tgt Ion:146 Resp: 107129
Ion Ratio Lower Upper
146 100
111 42.0 20.2 60.5
148 62.6 31.2 93.6

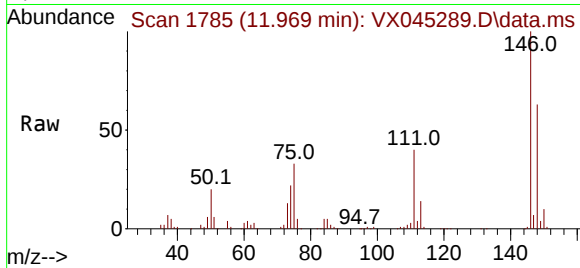

#87
1,2-Dichlorobenzene
Concen: 116.034 ug/l
RT: 12.335 min Scan# 1845
Delta R.T. -0.000 min
Lab File: VX045289.D
Acq: 14 Mar 2025 12:09

Tgt Ion:146 Resp: 259016
Ion Ratio Lower Upper
146 100
111 44.0 21.7 65.1
148 63.2 31.8 95.4

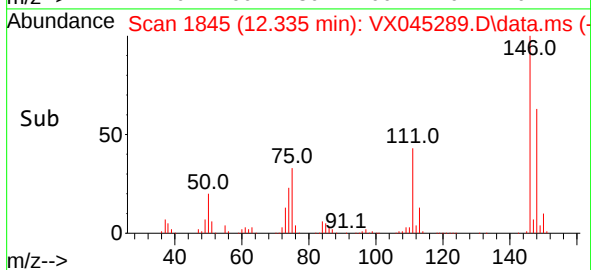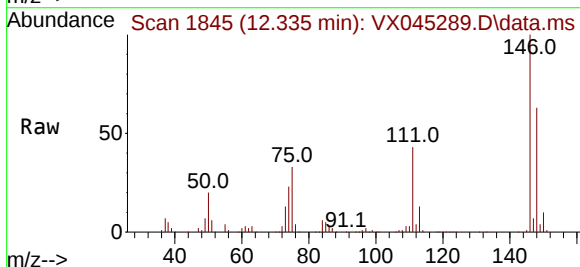



#91
Naphthalene
Concen: 85.803 ug/l
RT: 13.774 min Scan# 2081
Delta R.T. -0.000 min
Lab File: VX045289.D
Acq: 14 Mar 2025 12:09

Instrument :
MSVOA_X
ClientSampleId :
PT-VOA-WP

Tgt Ion:128 Resp: 409326
Ion Ratio Lower Upper
128 100
127 12.9 10.5 15.7
129 10.9 8.7 13.1

