
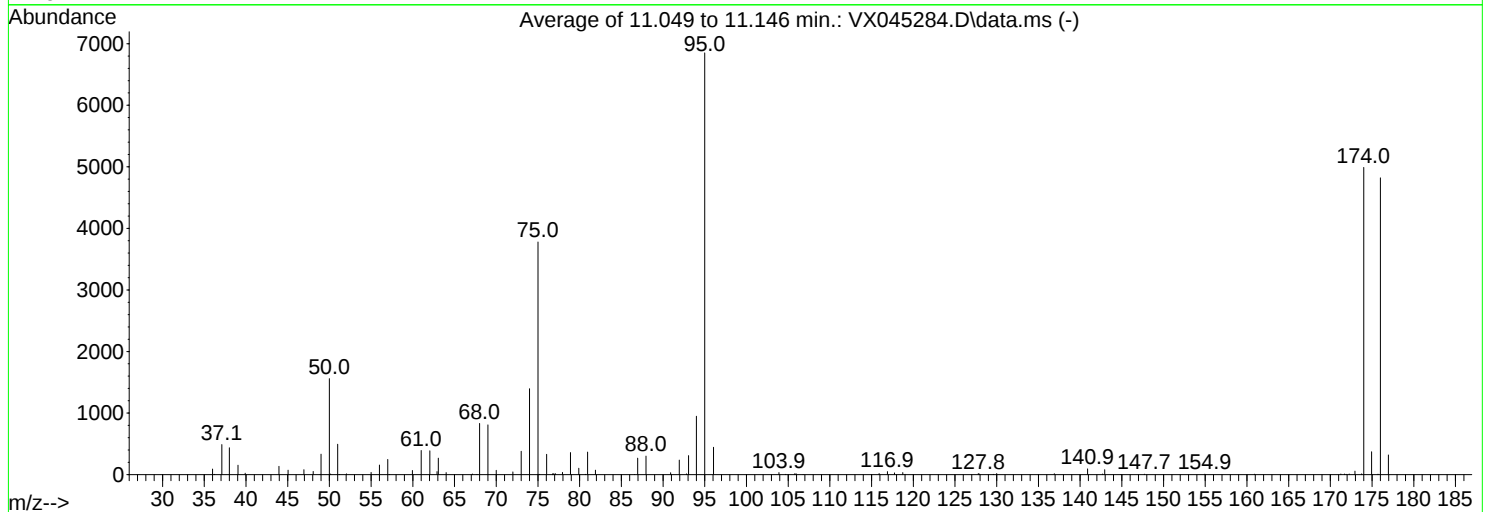


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031425\
Data File : VX045284.D
Acq On : 14 Mar 2025 09:28
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X022125W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Sat Feb 22 01:06:36 2025

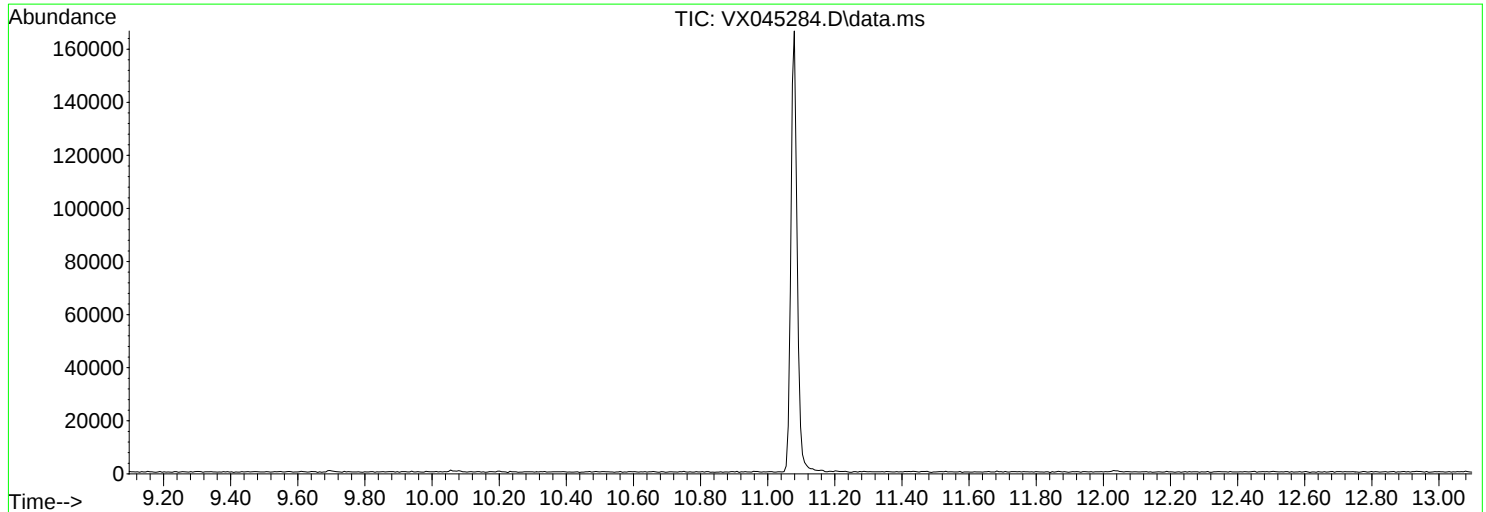

AutoFind: Averaged scan 1634 to 1650; Bkg corrected with scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.8	1559	PASS
75	95	30	60	55.2	3779	PASS
95	95	100	100	100.0	6851	PASS
96	95	5	9	6.5	445	PASS
173	174	0.00	2	1.2	58	PASS
174	95	50	100	72.8	4989	PASS
175	174	5	9	7.4	371	PASS
176	174	95	101	96.7	4822	PASS
177	176	5	9	6.6	320	PASS