

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX031519\
 Data File : VX008123.D
 Acq On : 15 Mar 2019 23:04
 Operator : JC/SP
 Sample : K1856-08
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-TT-AOC22-MW08-20190311

Quant Time: Mar 16 11:03:03 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X031419W.M
 Quant Title : SW846 8260
 QLast Update : Fri Mar 15 03:56:35 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	240884	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	364552	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	350387	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	175077	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.07	65	121787	50.12	ug/l	0.00
Spiked Amount 50.000			Recovery	=	100.24%	
35) Dibromofluoromethane	5.51	113	118678	51.34	ug/l	0.00
Spiked Amount 50.000			Recovery	=	102.68%	
50) Toluene-d8	8.71	98	439136	49.94	ug/l	0.00
Spiked Amount 50.000			Recovery	=	99.88%	
62) 4-Bromofluorobenzene	11.13	95	160136	50.84	ug/l	0.00
Spiked Amount 50.000			Recovery	=	101.68%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX031519\
Data File : VX008123.D
Acq On : 15 Mar 2019 23:04
Operator : JC/SP
Sample : K1856-08
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-TT-AOC22-MW08-20190311

Quant Time: Mar 16 11:03:03 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X031419W.M
Quant Title : SW846 8260
QLast Update : Fri Mar 15 03:56:35 2019
Response via : Initial Calibration

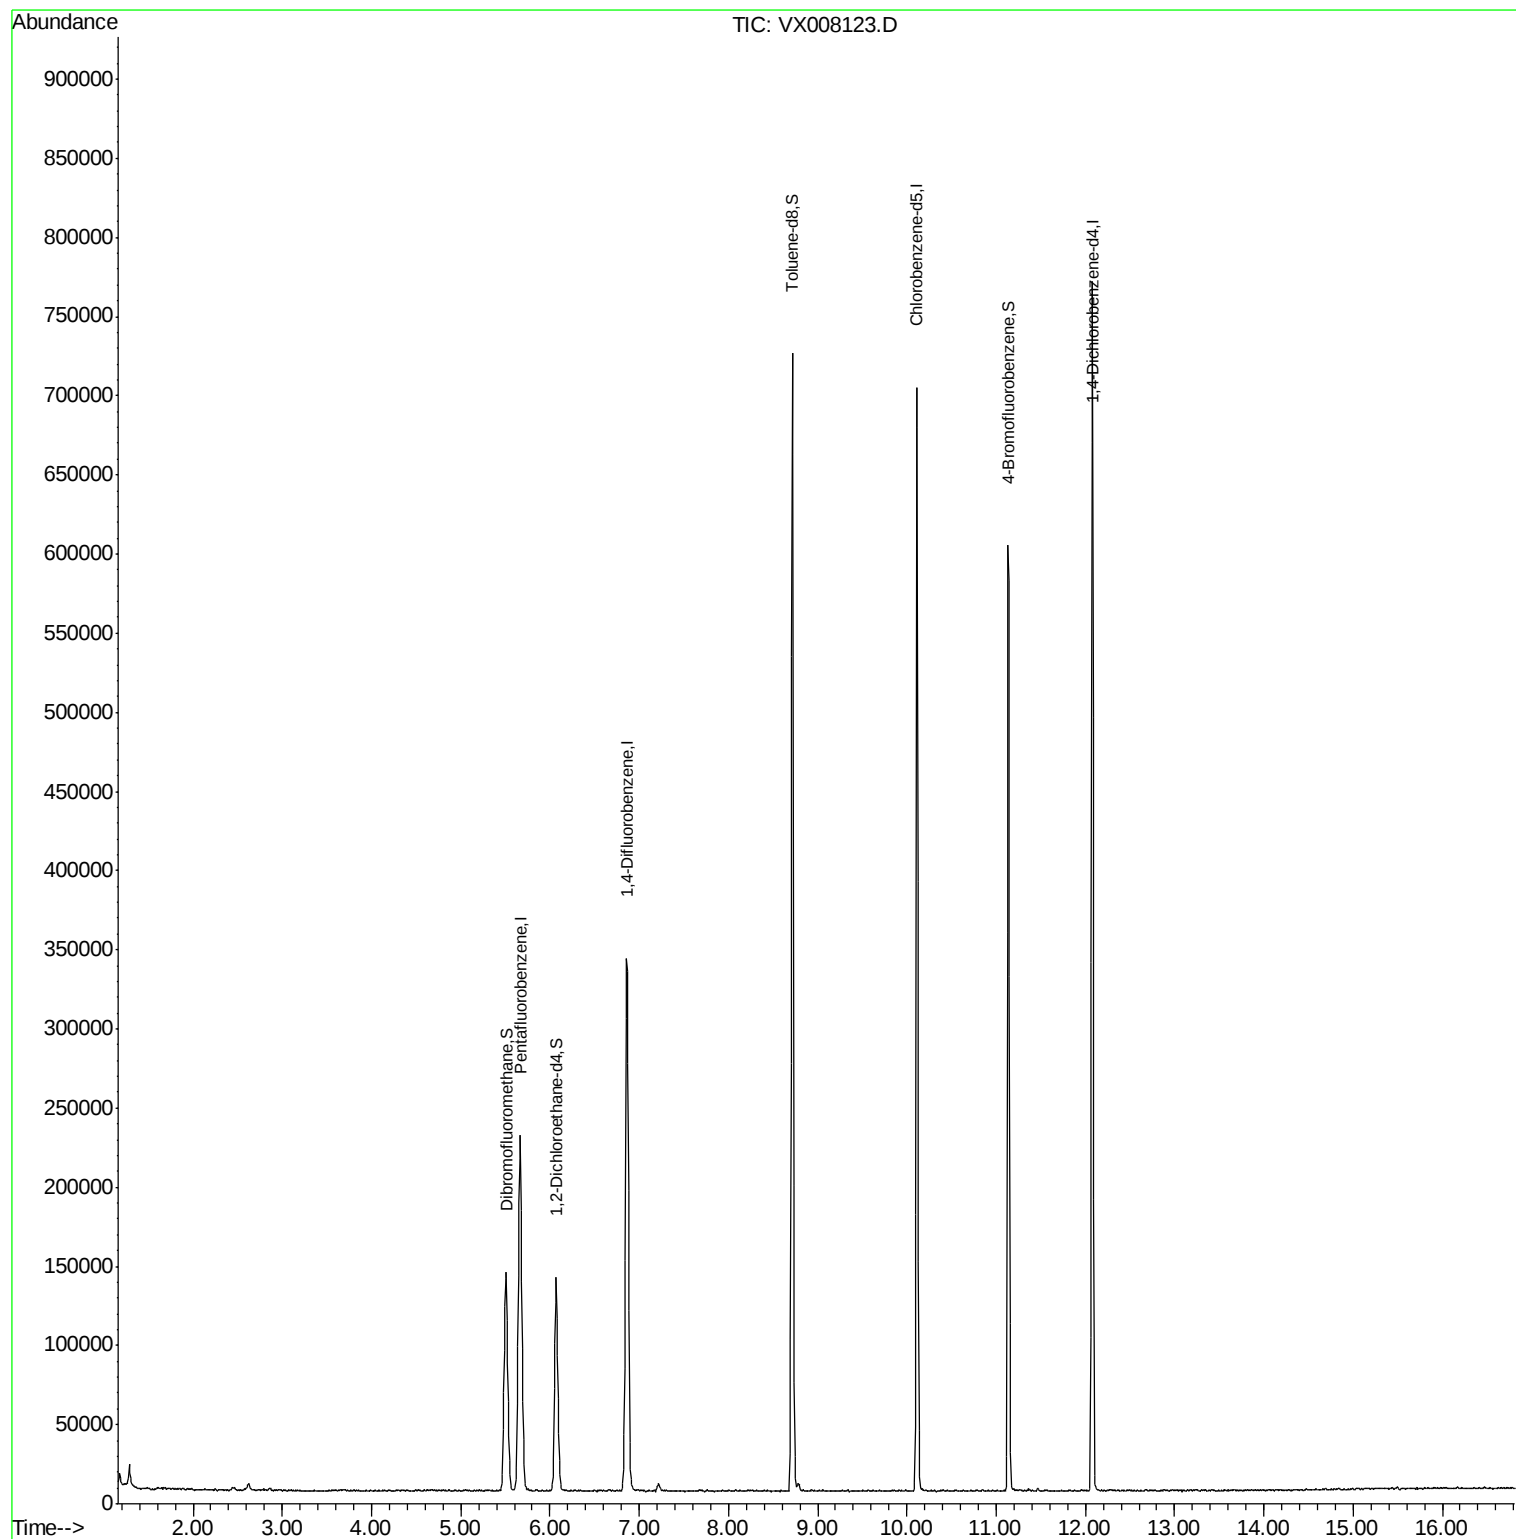

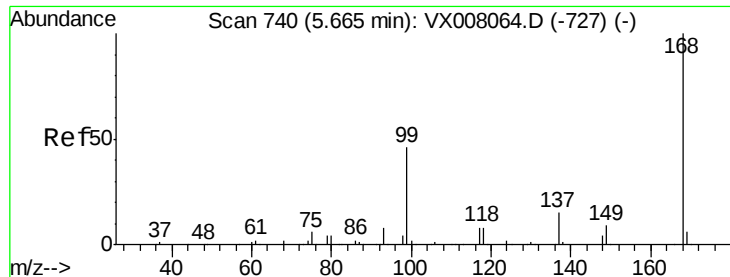

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 740

Delta R.T. 0.00 min

Lab File: VX008123.D

Acq: 15 Mar 2019 23:04

Instrument :

MSVOA_X

ClientSampleId :


BP-TT-AOC22-MW08-20190311

Tot Ion:168 Resp: 240884

Ion Ratio Lower Upper

168 100

99 46.8 37.6 56.4

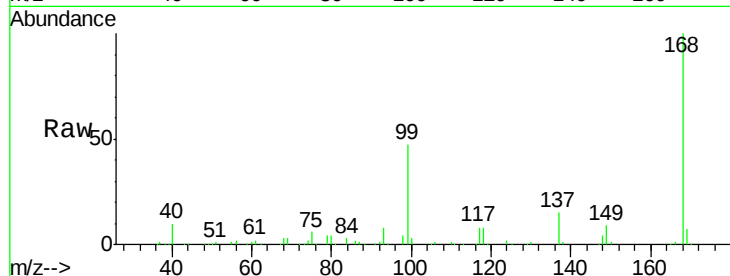

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.67

80000



60000

40000

20000

0

Time--> 5.50 5.60 5.70 5.80

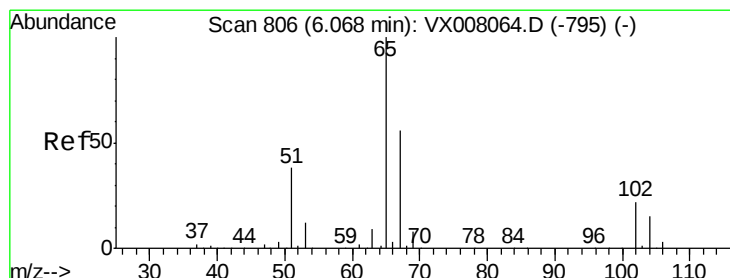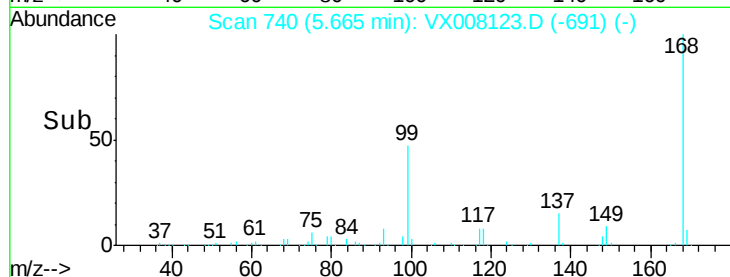

#33

1,2-Dichloroethane-d4

Concen: 50.120 ug/l

RT: 6.07 min Scan# 806

Delta R.T. 0.00 min

Lab File: VX008123.D


Acq: 15 Mar 2019 23:04

Tgt Ion: 65 Resp: 121787

Ion Ratio Lower Upper

65 100

67 53.8 0.0 110.0

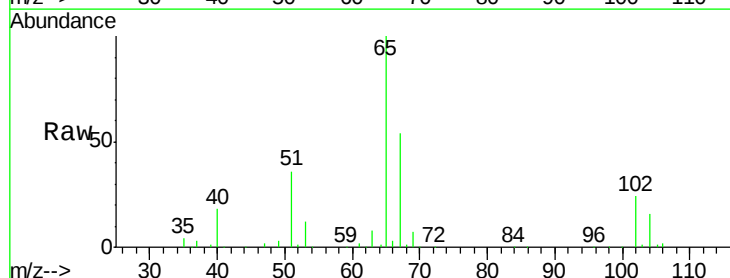

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.07

50000

40000


30000


20000

10000

0

Time--> 6.00 6.10 6.20

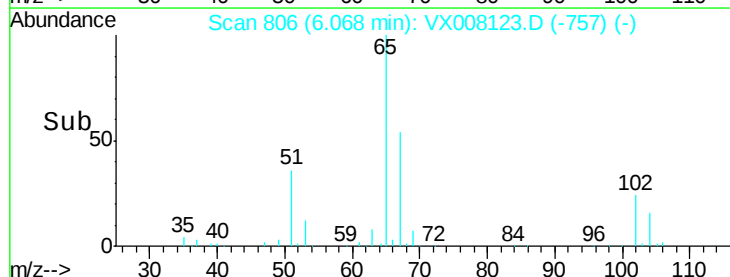


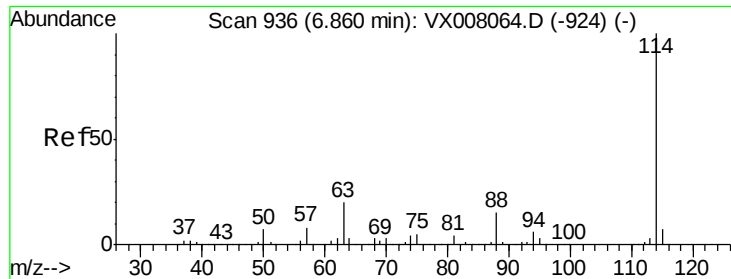




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.86 min Scan# 936
Delta R.T. 0.00 min
Lab File: VX008123.D
Acq: 15 Mar 2019 23:04

Instrument :
MSVOA_X
ClientSampleId :
BP-TT-AOC22-MW08-20190311

Tot Ion:114 Resp: 364552
Ion Ratio Lower Upper
114 100
63 18.3 0.0 39.8
88 15.0 0.0 31.4

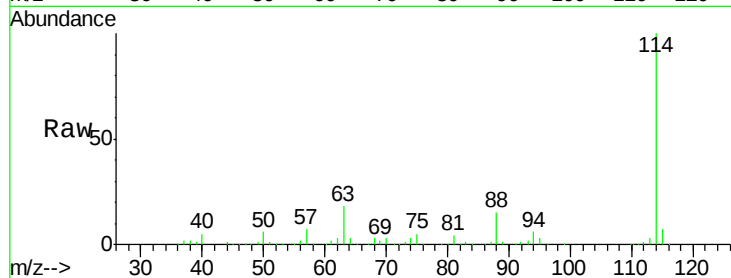


Abundance Ion 113.90 (113.60 to 114.60): V
Ion 63.00 (62.70 to 63.70): VX
Ion 87.90 (87.60 to 88.60): VX

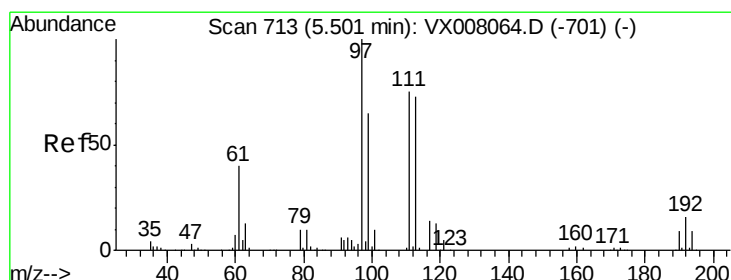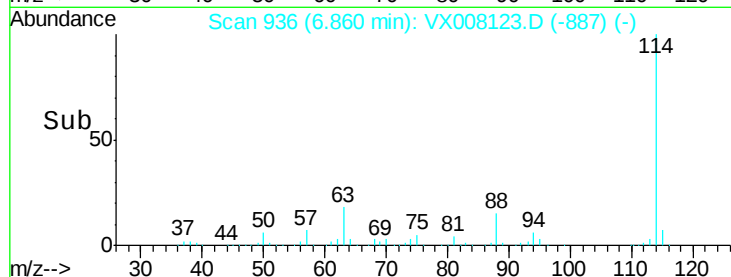
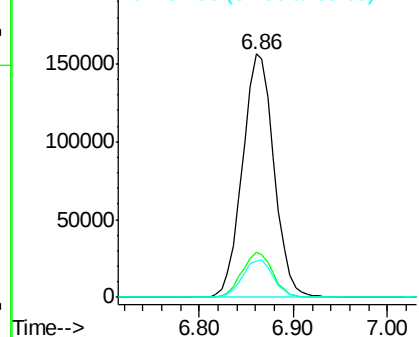



#35
Dibromofluoromethane
Concen: 51.336 ug/l
RT: 5.51 min Scan# 714
Delta R.T. 0.01 min
Lab File: VX008123.D
Acq: 15 Mar 2019 23:04

Tgt Ion:113 Resp: 118678
Ion Ratio Lower Upper
113 100
111 102.0 81.4 122.0
192 25.8 19.4 29.0

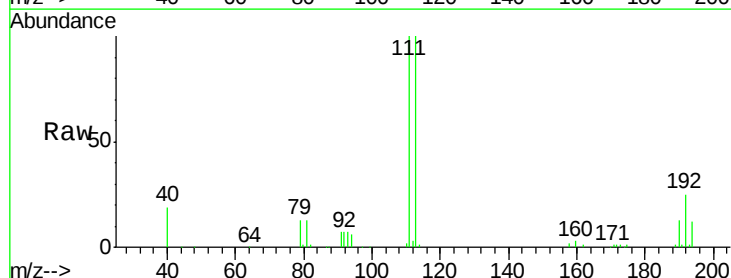

Abundance Ion 112.80 (112.50 to 113.50): V
Ion 110.80 (110.50 to 111.50): V
Ion 191.70 (191.40 to 192.40): V



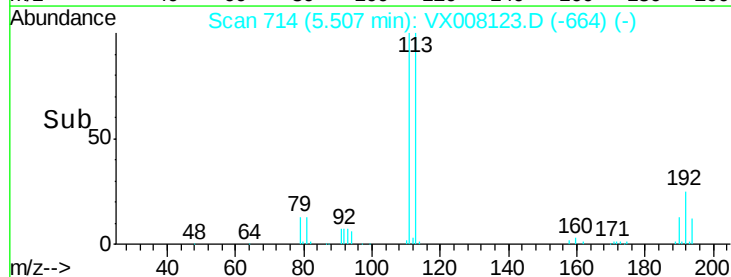
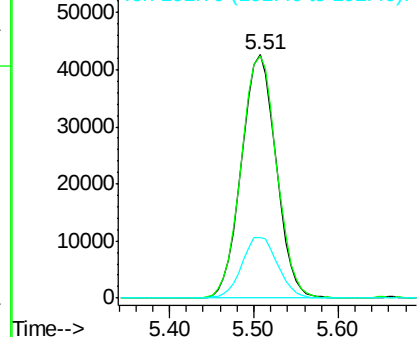


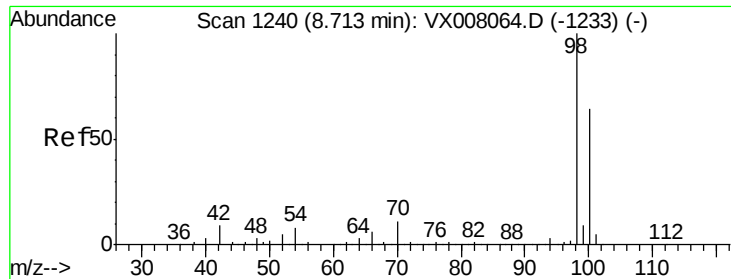

#50
Toluene-d8
Concen: 49.945 ug/l
RT: 8.71 min Scan# 1240
Delta R.T. 0.00 min
Lab File: VX008123.D
Acq: 15 Mar 2019 23:04




Instrument :
MSVOA_X
ClientSampleId :
BP-TT-AOC22-MW08-20190311


Tot Ion: 98 Resp: 439136
Ion Ratio Lower Upper
98 100
100 65.1 51.7 77.5

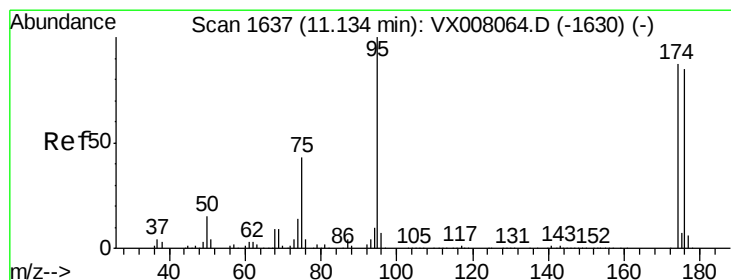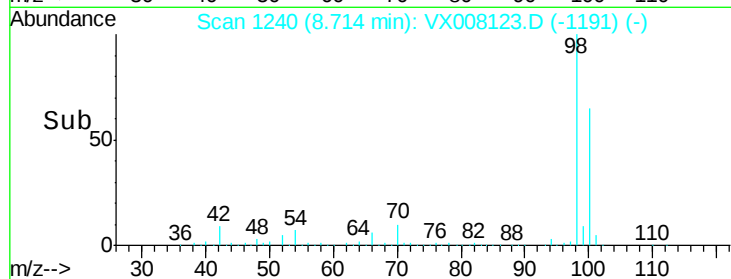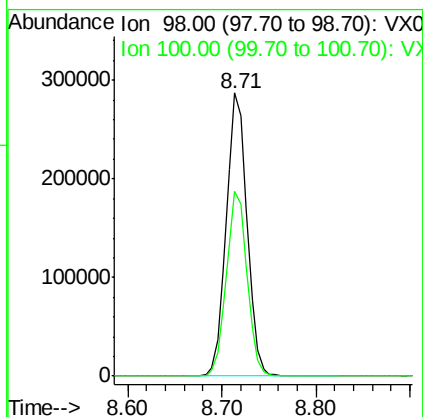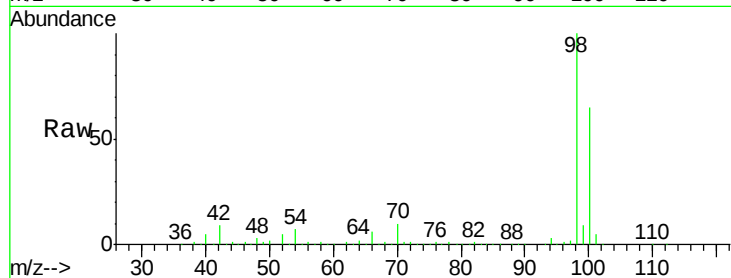

#62
4-Bromofluorobenzene
Concen: 50.841 ug/l
RT: 11.13 min Scan# 1637
Delta R.T. 0.00 min
Lab File: VX008123.D
Acq: 15 Mar 2019 23:04

Tgt Ion: 95 Resp: 160136
Ion Ratio Lower Upper
95 100
174 98.5 0.0 182.8
176 94.9 0.0 178.0

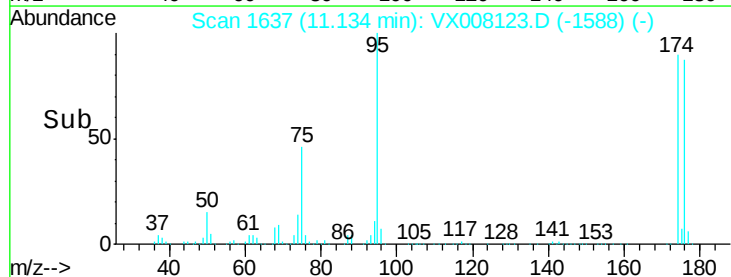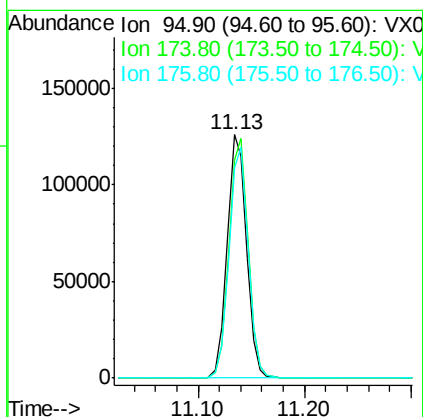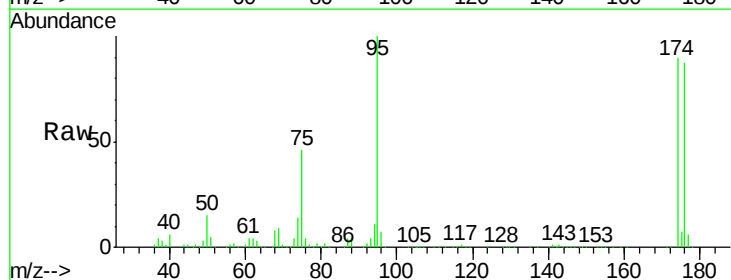


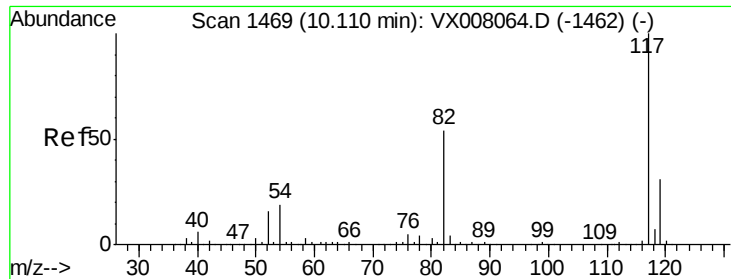




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.11 min Scan# 1469
Delta R.T. 0.00 min
Lab File: VX008123.D
Acq: 15 Mar 2019 23:04

Instrument :
MSVOA_X
ClientSampleId :
BP-TT-AOC22-MW08-20190311

Tot Ion:117 Resp: 350387
Ion Ratio Lower Upper
117 100
82 52.2 44.3 66.5
119 32.4 25.3 37.9

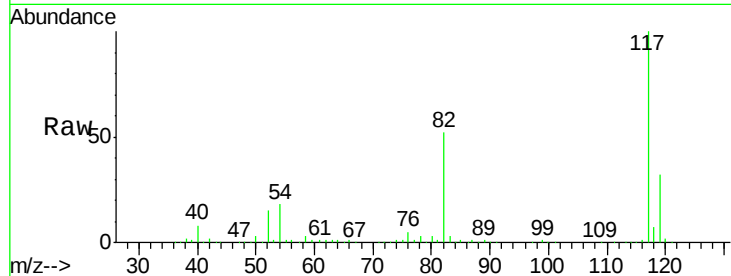


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VX0
Ion 118.90 (118.60 to 119.60): V

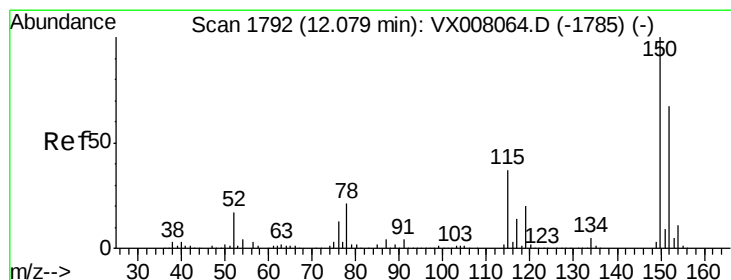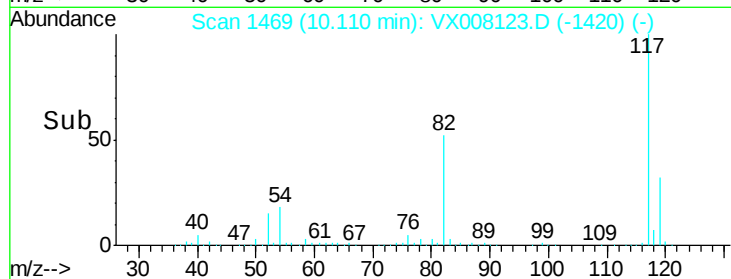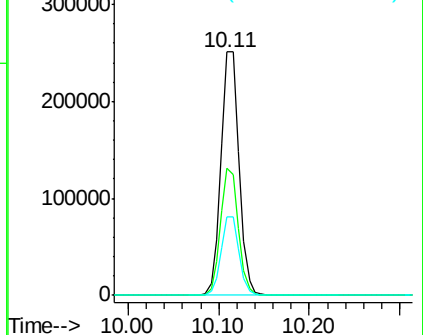

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.08 min Scan# 1792
Delta R.T. 0.00 min
Lab File: VX008123.D
Acq: 15 Mar 2019 23:04

Tgt Ion:152 Resp: 175077
Ion Ratio Lower Upper
152 100
115 53.2 38.6 115.7
150 155.8 0.0 348.4

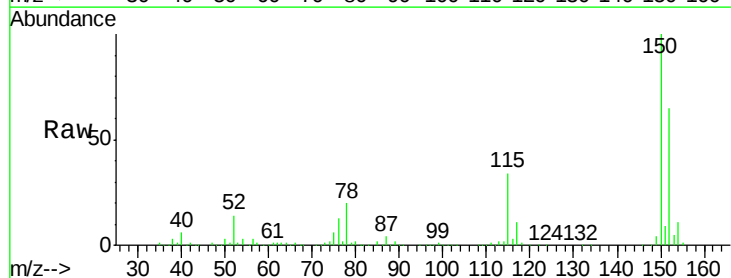

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

