


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX031519\
 Data File : VX008101.D
 Acq On : 15 Mar 2019 11:44
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\624X030819W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Fri Mar 08 12:01:36 2019

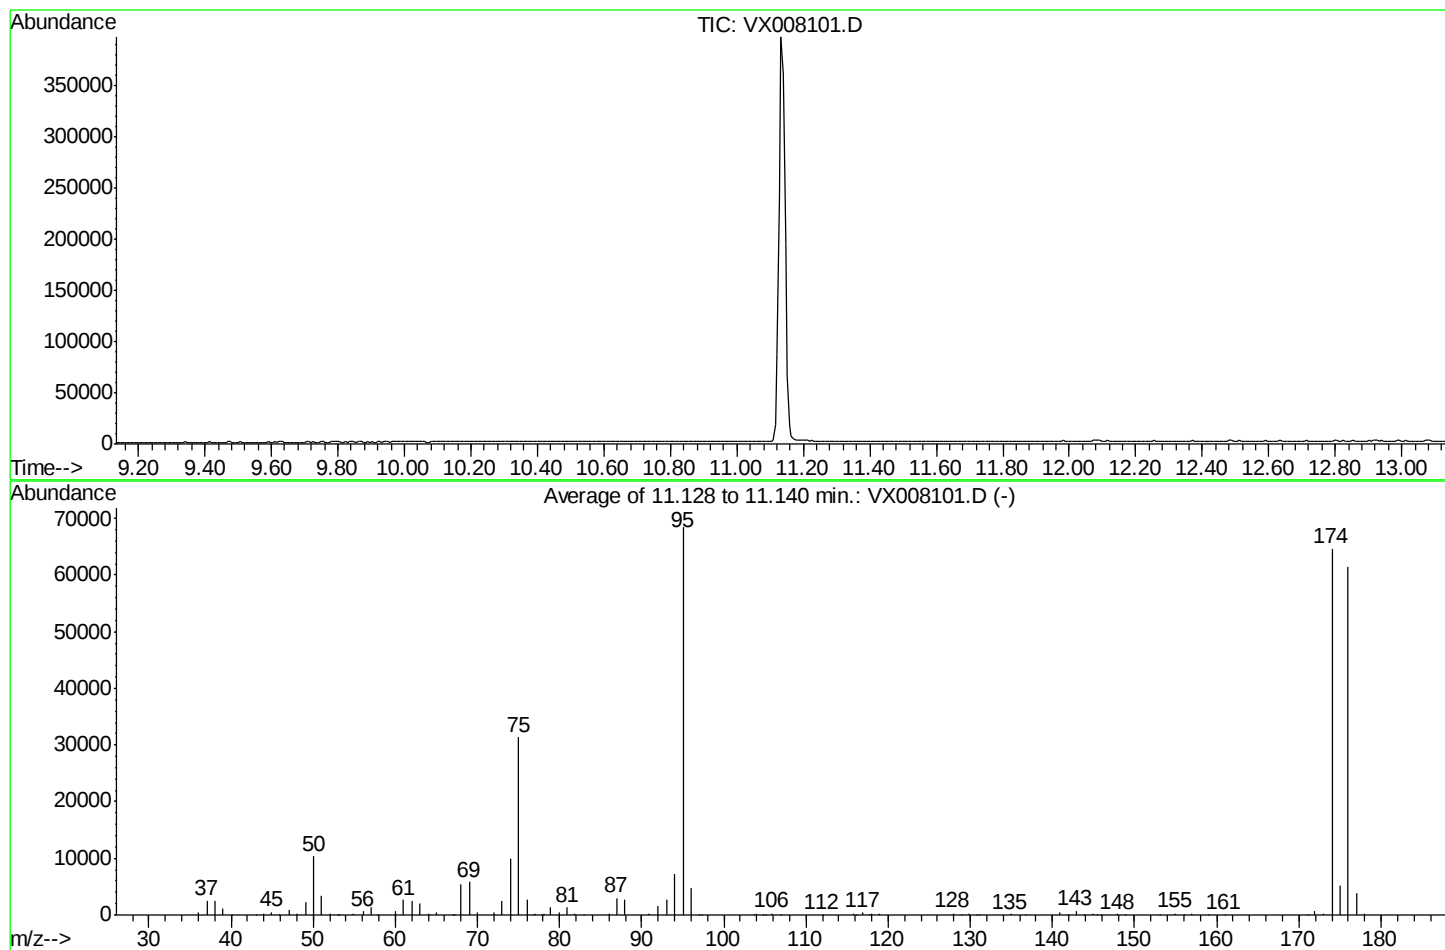

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.1	10334	PASS
75	95	30	60	45.8	31365	PASS
95	95	100	100	100.0	68416	PASS
96	95	5	9	7.0	4815	PASS
173	174	0.00	2	0.3	166	PASS
174	95	50	100	94.5	64650	PASS
175	174	5	9	7.9	5102	PASS
176	174	95	101	94.9	61362	PASS
177	176	5	9	6.3	3875	PASS