

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031521\
 Data File : VX021209.D
 Acq On : 15 Mar 2021 18:54
 Operator : JC/MD
 Sample : M1647-18
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Mar 16 03:04:54 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031521W.M
 Quant Title : SW846 8260
 QLast Update : Mon Mar 15 11:55:59 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.623	168	73162	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.829	114	135286	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.094	117	131377	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.059	152	59003	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.035	65	64924	52.04	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	104.08%
35) Dibromofluoromethane	5.470	113	47325	50.84	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	101.68%
50) Toluene-d8	8.694	98	169698	50.75	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	101.50%
62) 4-Bromofluorobenzene	11.118	95	68899	54.07	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	108.14%


Target Compounds						Qvalue
5) Bromomethane	1.640	94	164	0.30	ug/l #	51
11) Tert butyl alcohol	3.017	59	7702	35.44	ug/l #	89
13) Acrolein	2.281	56	84	0.63	ug/l #	64
14) Allyl chloride	2.687	41	382	0.22	ug/l #	25
16) Acetone	2.422	43	30487	60.80	ug/l	89
17) Carbon Disulfide	2.546	76	499	0.21	ug/l #	75
18) Methyl Acetate	2.752	43	30397	25.03	ug/l	90
20) Methylene Chloride	2.840	84	515	0.54	ug/l #	77
22) Diisopropyl ether	3.758	45	1370	0.44	ug/l #	15
25) 2-Butanone	4.634	43	6933	9.61	ug/l #	88
29) Tetrahydrofuran	5.082	42	135	0.29	ug/l #	27
36) 1,1-Dichloropropene	5.629	75	7093	5.00	ug/l #	49
37) Ethyl Acetate	4.793	43	620	0.40	ug/l #	64
38) Carbon Tetrachloride	5.629	117	8258	5.30	ug/l #	17
40) Benzene	6.111	78	42590	10.75	ug/l	99
42) 1,2-Dichloroethane	6.111	62	708	0.42	ug/l #	73
49) 1,4-Dioxane	7.717	88	1102	48.45	ug/l #	61
51) 4-Methyl-2-Pentanone	8.617	43	1644	1.10	ug/l	89
52) Toluene	8.764	92	57111	23.90	ug/l	99
55) 1,1,2-Trichloroethane	9.059	97	933	0.95	ug/l #	19
58) 2-Chloroethyl Vinyl ether	8.264	63	181	0.24	ug/l #	45
59) 2-Hexanone	9.470	43	558	0.50	ug/l	84
67) Ethyl Benzene	10.235	91	4294	0.85	ug/l	94
68) m/p-Xylenes	10.335	106	7435	4.11	ug/l	91
69) o-Xylene	10.682	106	3652	2.08	ug/l	88
70) Styrene	10.694	104	3622	1.22	ug/l #	77
76) 1,2,3-Trichloropropane	11.118	75	38834	26.54	ug/l #	39
80) 1,3,5-Trimethylbenzene	11.494	105	1003	0.26	ug/l	98
81) trans-1,4-Dichloro-2-b...	11.118	75	38834	75.34	ug/l #	12
84) 1,2,4-Trimethylbenzene	11.788	105	3205	0.83	ug/l	86
92) 1,2-Dibromo-3-Chloropr...	12.841	75	117	0.32	ug/l #	1
95) Naphthalene	13.818	128	29681	8.09	ug/l	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031521\
Data File : VX021209.D
Acq On : 15 Mar 2021 18:54
Operator : JC/MD
Sample : M1647-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampled :

Quant Time: Mar 16 03:04:54 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031521W.M
Quant Title : SW846 8260
QLast Update : Mon Mar 15 11:55:59 2021
Response via : Initial Calibration




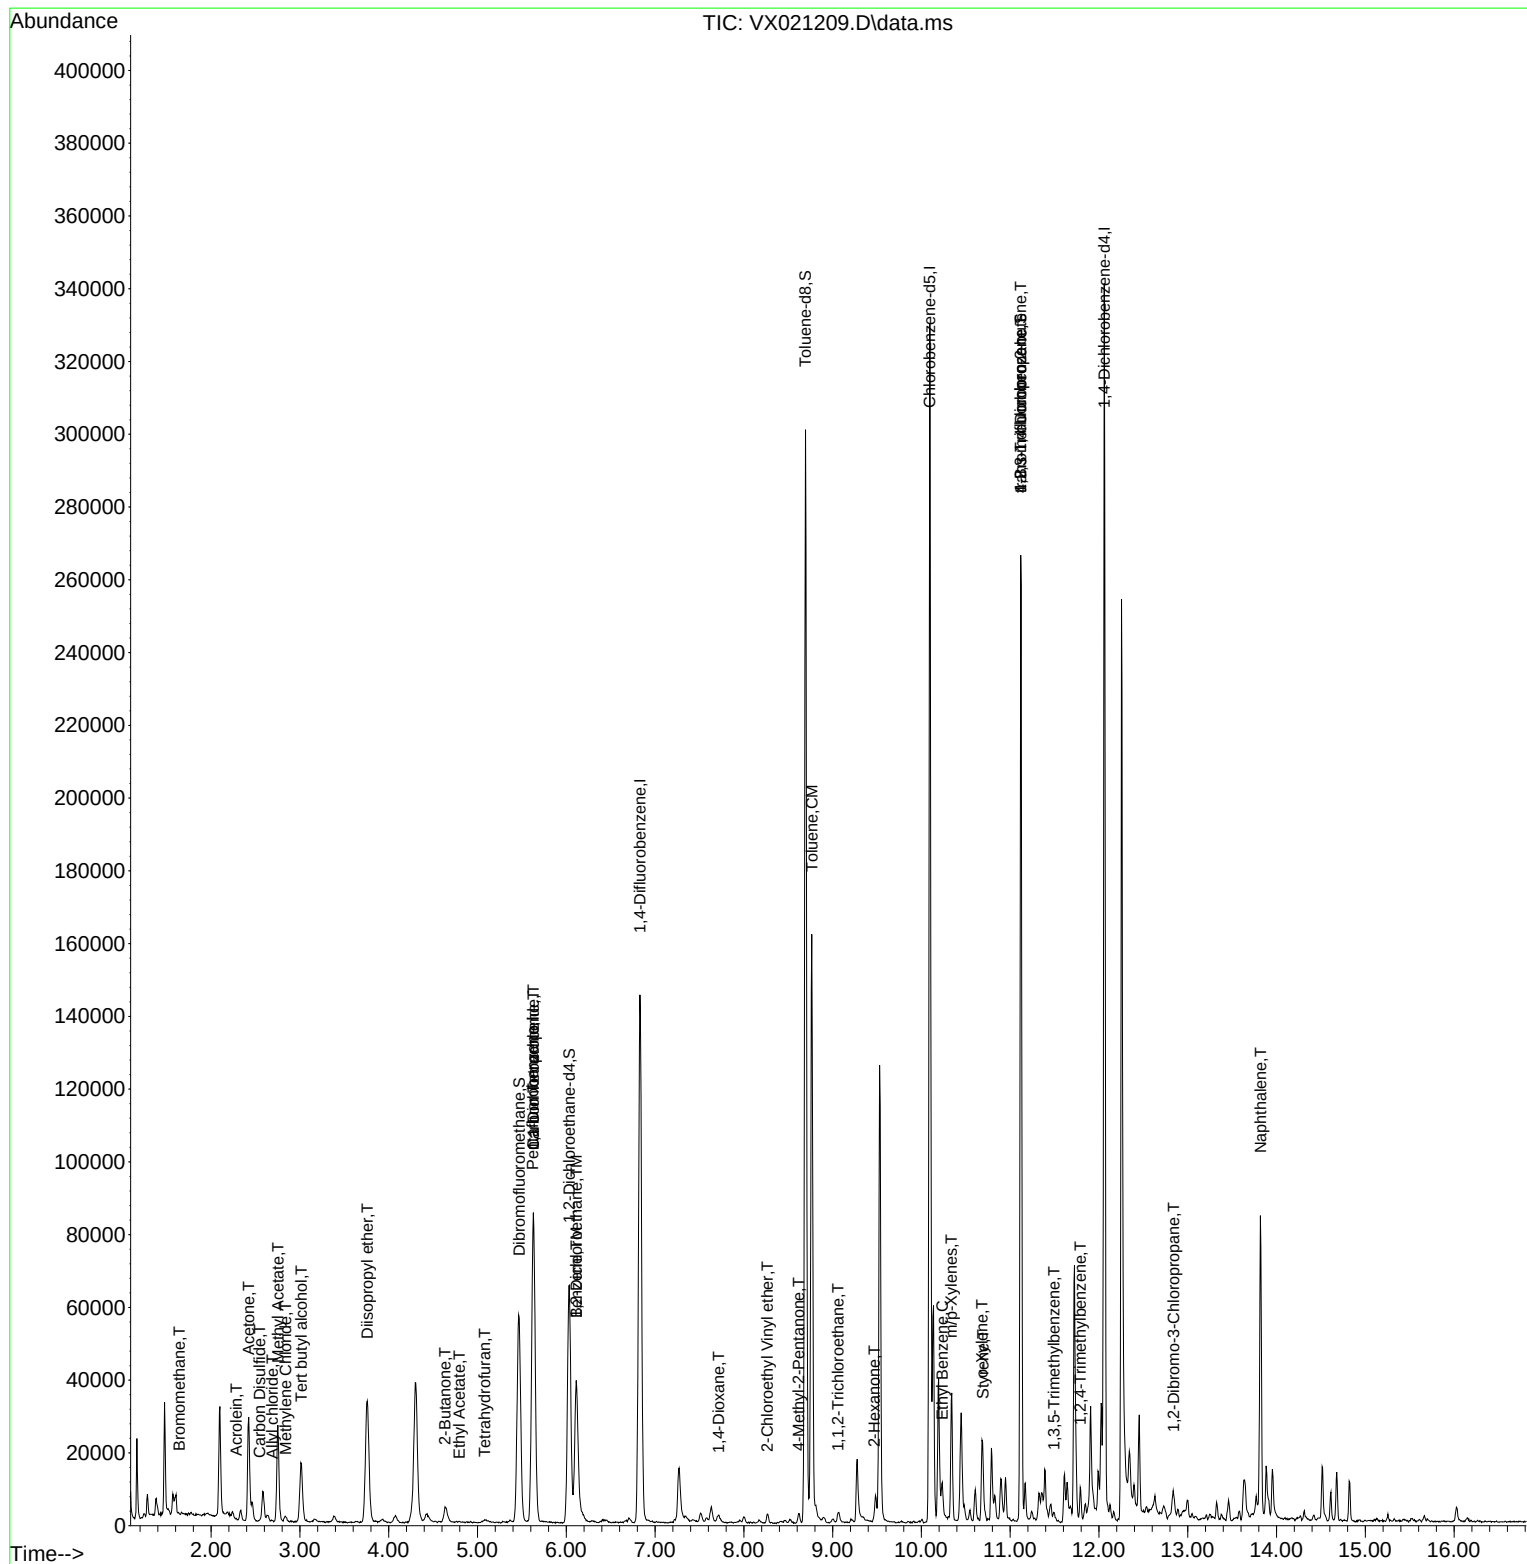




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.623 min Scan# 771
Delta R.T. -0.000 min
Lab File: VX021209.D
Acq: 15 Mar 2021 18:54




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:168 Resp: 73162
Ion Ratio Lower Upper
168 100
99 61.2 45.8 68.6

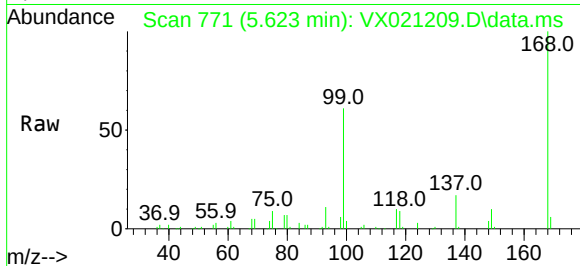

#5
Bromomethane
Concen: 0.30 ug/l
RT: 1.640 min Scan# 94
Delta R.T. 0.017 min
Lab File: VX021209.D
Acq: 15 Mar 2021 18:54

Tgt Ion: 94 Resp: 164
Ion Ratio Lower Upper
94 100
96 47.6 76.4 114.6#




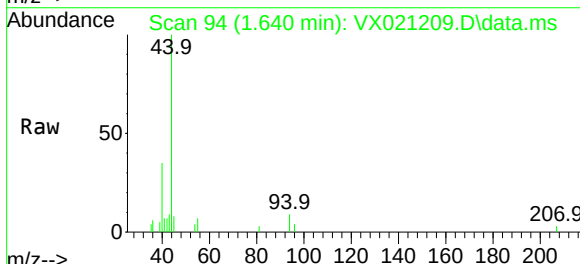




#11
Tert butyl alcohol
Concen: 35.44 ug/l
RT: 3.017 min Scan# 328
Delta R.T. -0.000 min
Lab File: VX021209.D
Acq: 15 Mar 2021 18:54




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 59 Resp: 7702
Ion Ratio Lower Upper
59 100
57 13.8 7.8 11.8#



#13
Acrolein
Concen: 0.63 ug/l
RT: 2.281 min Scan# 203
Delta R.T. 0.006 min
Lab File: VX021209.D
Acq: 15 Mar 2021 18:54


Tgt Ion: 56 Resp: 84
Ion Ratio Lower Upper
56 100
55 100.0 56.4 84.6#

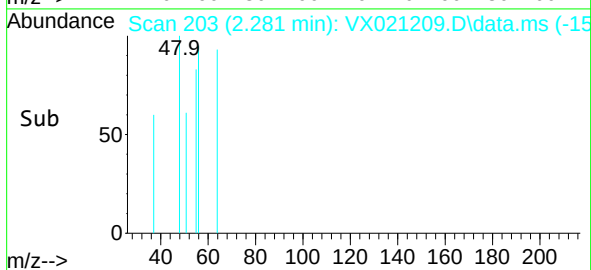






#14
 Allyl chloride
 Concen: 0.22 ug/l
 RT: 2.687 min Scan# 272
 Delta R.T. -0.018 min
 Lab File: VX021209.D
 Acq: 15 Mar 2021 18:54

Instrument :
 MSVOA_X
 ClientSampleId :







Tgt Ion: 41 Resp: 382
 Ion Ratio Lower Upper
 41 100
 39 0.0 51.6 77.4#
 76 0.0 30.5 45.7#

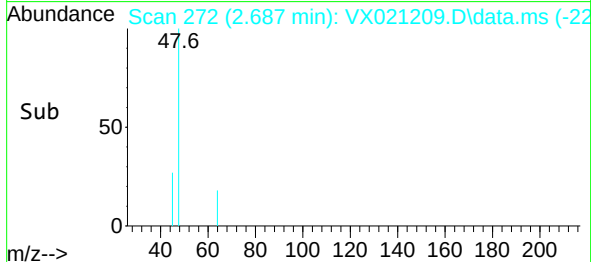

#16
 Acetone
 Concen: 60.80 ug/l
 RT: 2.422 min Scan# 227
 Delta R.T. -0.000 min
 Lab File: VX021209.D
 Acq: 15 Mar 2021 18:54

Tgt Ion: 43 Resp: 30487
 Ion Ratio Lower Upper
 43 100
 58 28.2 27.8 41.8


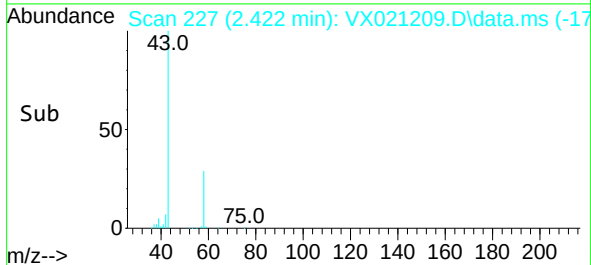

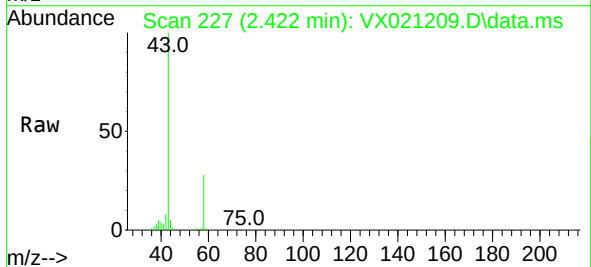




#17
Carbon Disulfide
Concen: 0.21 ug/l
RT: 2.546 min Scan# 248
Delta R.T. -0.000 min
Lab File: VX021209.D
Acq: 15 Mar 2021 18:54




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 76 Resp: 499
Ion Ratio Lower Upper
76 100
78 0.0 7.2 10.8#



#18
Methyl Acetate
Concen: 25.03 ug/l
RT: 2.752 min Scan# 283
Delta R.T. -0.000 min
Lab File: VX021209.D
Acq: 15 Mar 2021 18:54


Tgt Ion: 43 Resp: 30397
Ion Ratio Lower Upper
43 100
74 22.2 21.9 32.9

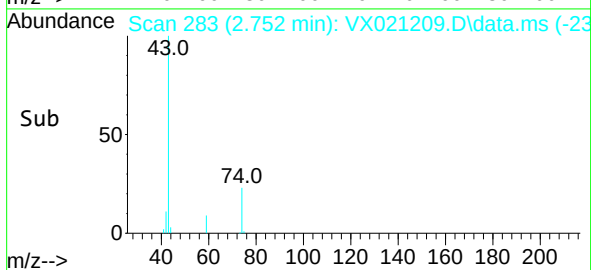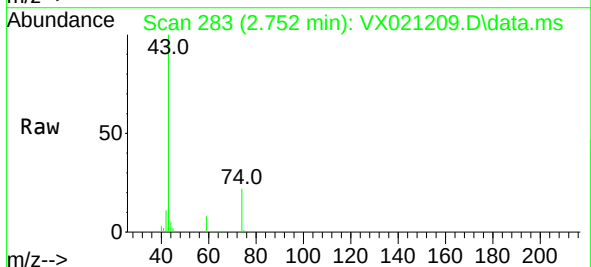



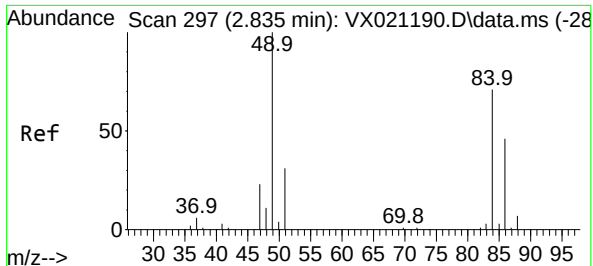


#20
Methylene Chloride
Concen: 0.54 ug/l
RT: 2.840 min Scan# 298
Delta R.T. 0.006 min
Lab File: VX021209.D
Acq: 15 Mar 2021 18:54

Instrument :
MSVOA_X
ClientSampled :



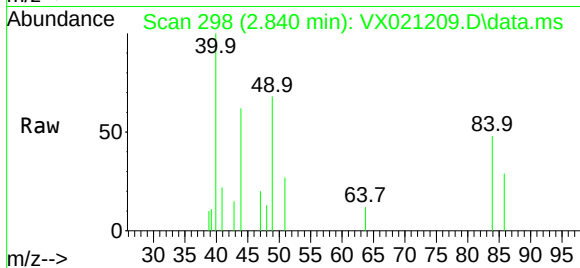



Tgt Ion: 84 Resp: 515
Ion Ratio Lower Upper
84 100
49 141.1 88.6 132.8#
51 56.3 27.0 40.6#
86 60.4 50.3 75.5

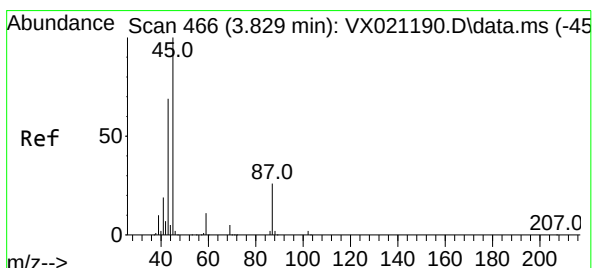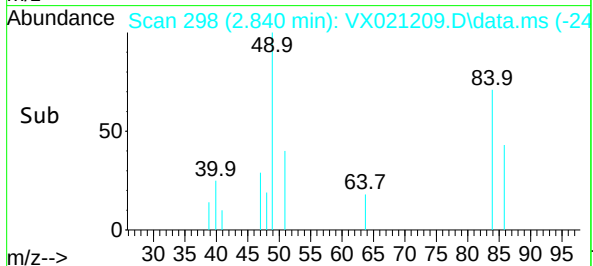

#22
Diisopropyl ether
Concen: 0.44 ug/l
RT: 3.758 min Scan# 454
Delta R.T. -0.071 min
Lab File: VX021209.D
Acq: 15 Mar 2021 18:54

Tgt Ion: 45 Resp: 1370
Ion Ratio Lower Upper
45 100
43 25.4 58.0 87.0#
87 0.0 25.4 38.0#
59 140.0 10.2 15.2#

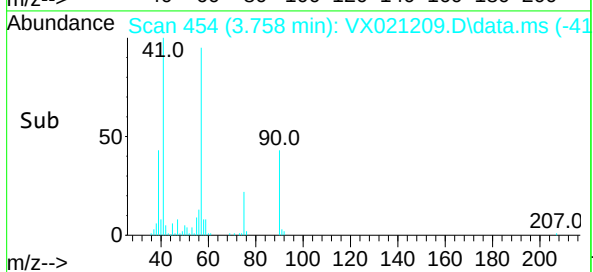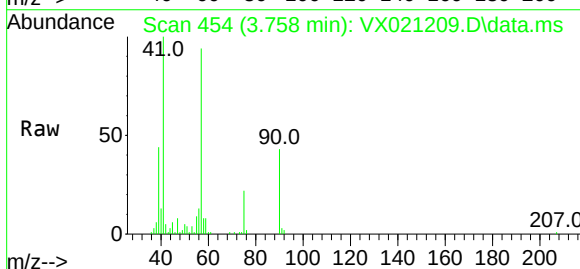

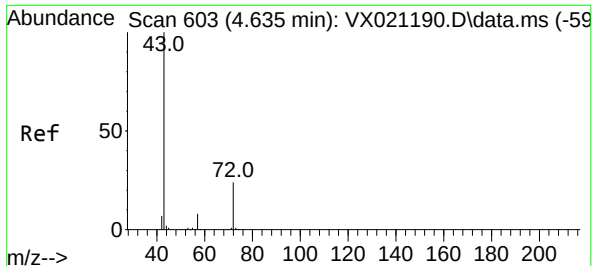

#25

2-Butanone

Concen: 9.61 ug/l

RT: 4.634 min Scan# 603

Delta R.T. -0.000 min





Lab File: VX021209.D

Acq: 15 Mar 2021 18:54

Tgt Ion: 43 Resp: 6933

Ion Ratio Lower Upper

43	100		
72	23.2	23.7	35.5#

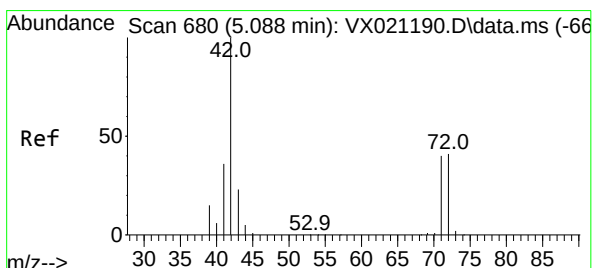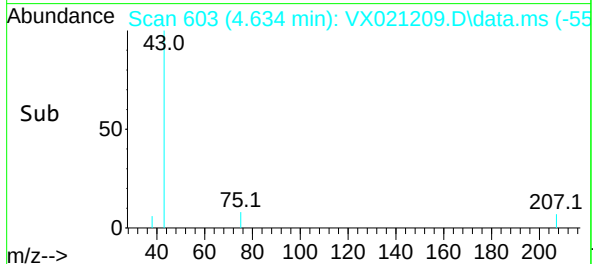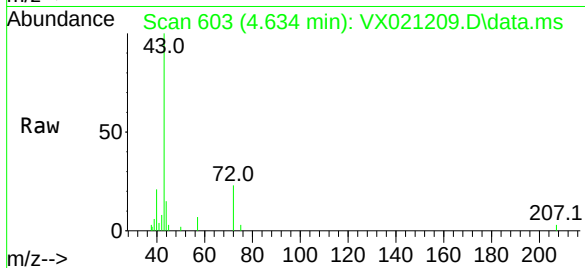

#29

Tetrahydrofuran

Concen: 0.29 ug/l

RT: 5.082 min Scan# 679

Delta R.T. -0.006 min




Lab File: VX021209.D


Acq: 15 Mar 2021 18:54

Tgt Ion: 42 Resp: 135

Ion Ratio Lower Upper

42	100		
72	0.0	41.7	62.5#
71	0.0	38.4	57.6#


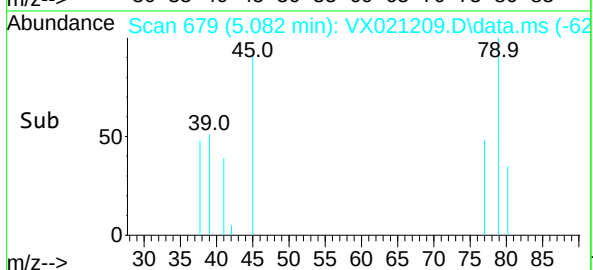

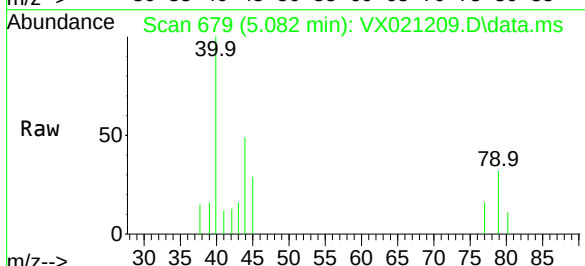




#33
1,2-Dichloroethane-d4
Concen: 52.04 ug/l
RT: 6.035 min Scan# 841
Delta R.T. 0.006 min
Lab File: VX021209.D
Acq: 15 Mar 2021 18:54




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 65 Resp: 64924
Ion Ratio Lower Upper
65 100
67 50.5 0.0 105.4



#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 6.829 min Scan# 976
Delta R.T. -0.000 min
Lab File: VX021209.D
Acq: 15 Mar 2021 18:54

Tgt Ion: 114 Resp: 135286
Ion Ratio Lower Upper
114 100
63 22.7 0.0 40.8
88 16.9 0.0 32.8


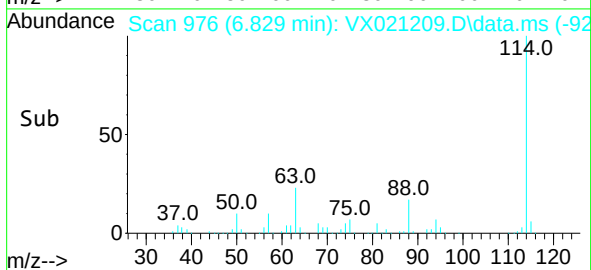

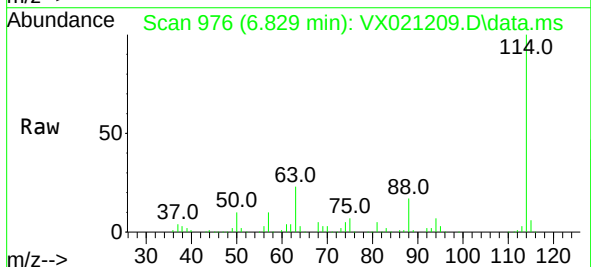




#35
Dibromofluoromethane
Concen: 50.84 ug/l
RT: 5.470 min Scan# 745
Delta R.T. 0.006 min
Lab File: VX021209.D
Acq: 15 Mar 2021 18:54




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion:113 Resp: 47325
Ion Ratio Lower Upper
113 100
111 102.9 81.9 122.9
192 17.8 16.7 25.1

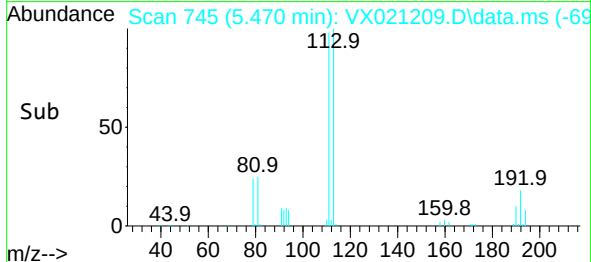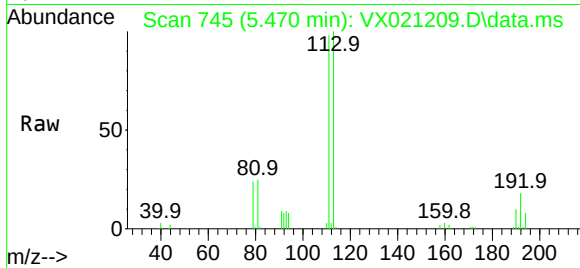

#36
1,1-Dichloropropene
Concen: 5.00 ug/l
RT: 5.629 min Scan# 772
Delta R.T. -0.141 min
Lab File: VX021209.D
Acq: 15 Mar 2021 18:54

Tgt Ion: 75 Resp: 7093
Ion Ratio Lower Upper
75 100
110 9.5 18.1 54.4#
77 0.0 25.3 37.9#

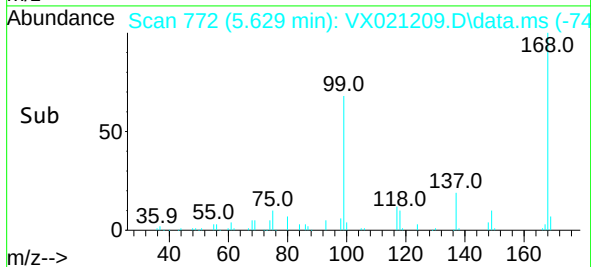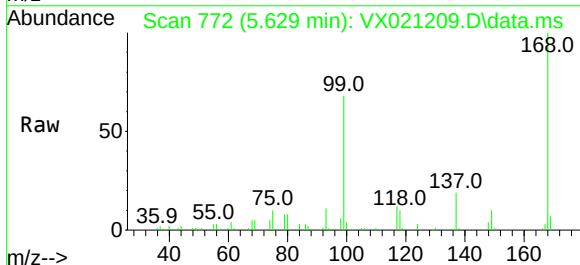



#37

Ethyl Acetate

Concen: 0.40 ug/l

RT: 4.793 min Scan# 630





Delta R.T. -0.000 min

Lab File: VX021209.D

Acq: 15 Mar 2021 18:54

Tgt Ion:	43	Resp:	620
Ion	Ratio	Lower	Upper
43	100		
61	0.0	12.8	19.2#
70	0.0	10.5	15.7#

Instrument :
MSVOA_X
ClientSampled :



#38

Carbon Tetrachloride

Concen: 5.30 ug/l




RT: 5.629 min Scan# 772


Delta R.T. -0.124 min

Lab File: VX021209.D

Acq: 15 Mar 2021 18:54

Tgt Ion:	117	Resp:	8258
Ion	Ratio	Lower	Upper
117	100		
119	6.3	76.2	114.2#
121	0.0	24.8	37.2#


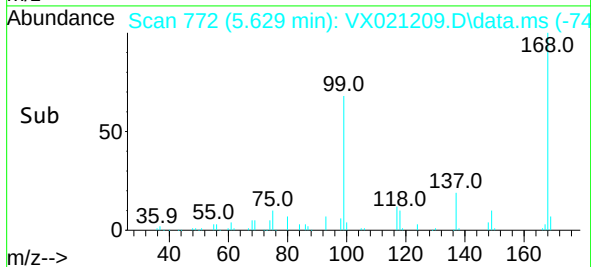

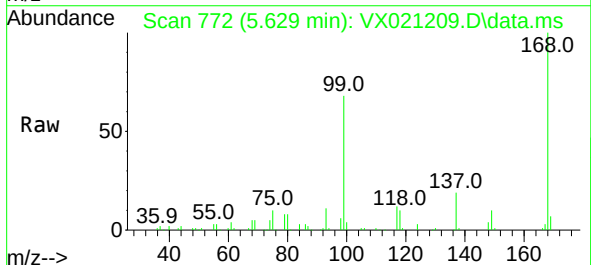




#40
Benzene
Concen: 10.75 ug/l
RT: 6.111 min Scan# 854
Delta R.T. -0.000 min
Lab File: VX021209.D
Acq: 15 Mar 2021 18:54




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 78 Resp: 42590
Ion Ratio Lower Upper
78 100
77 23.1 18.9 28.3



#42
1,2-Dichloroethane
Concen: 0.42 ug/l
RT: 6.111 min Scan# 854
Delta R.T. -0.047 min
Lab File: VX021209.D
Acq: 15 Mar 2021 18:54

Tgt Ion: 62 Resp: 708
Ion Ratio Lower Upper
62 100
98 0.0 0.0 20.2

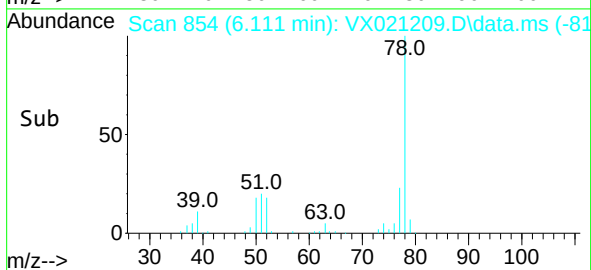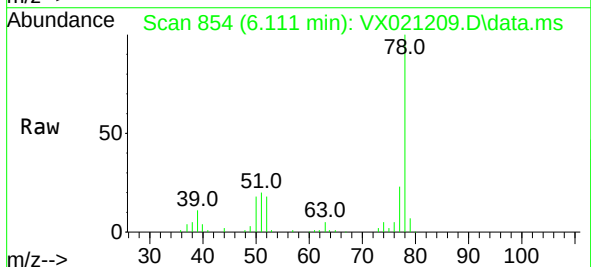

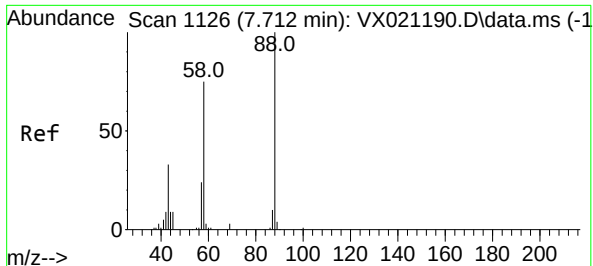

#49

1,4-Dioxane

Concen: 48.45 ug/l

RT: 7.717 min Scan# 1127

Delta R.T. 0.006 min

Lab File: VX021209.D

Acq: 15 Mar 2021 18:54





Tgt Ion: 88 Resp: 1102

Ion Ratio Lower Upper

88 100

43 74.8 23.2 34.8#

58 83.9 55.0 82.4#

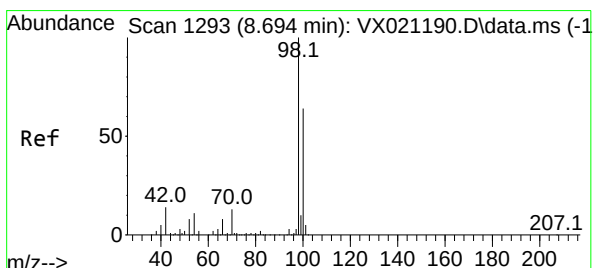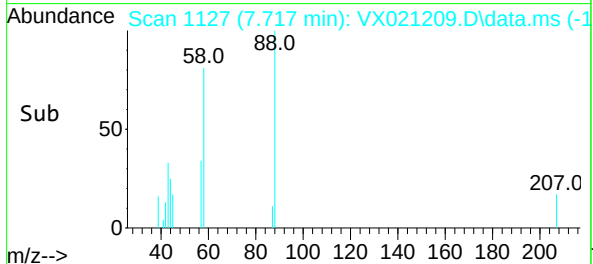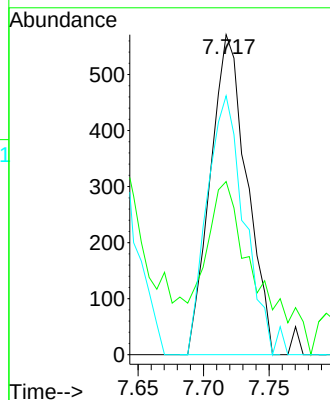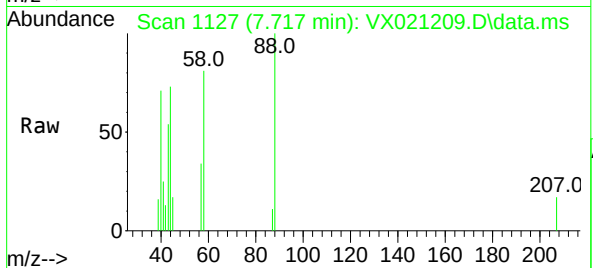

#50

Toluene-d8

Concen: 50.75 ug/l

RT: 8.694 min Scan# 1293

Delta R.T. -0.000 min

Lab File: VX021209.D




Acq: 15 Mar 2021 18:54


Tgt Ion: 98 Resp: 169698

Ion Ratio Lower Upper

98 100

100 64.6 51.9 77.9


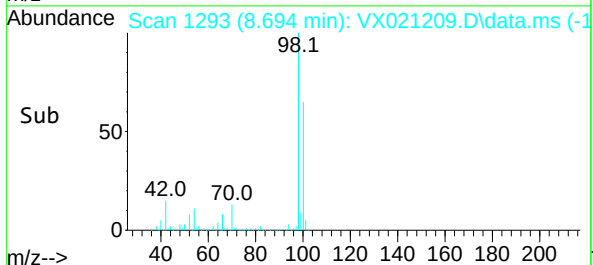
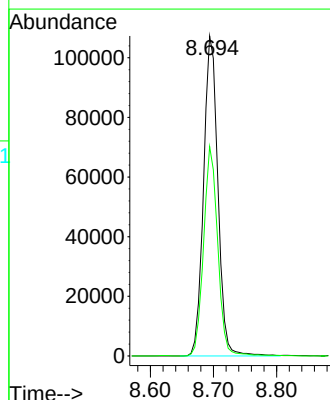
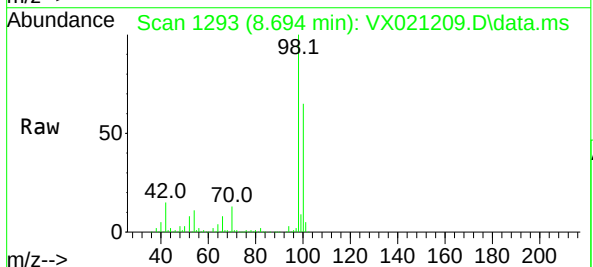




#51
4-Methyl-2-Pentanone
Concen: 1.10 ug/l
RT: 8.617 min Scan# 1280
Delta R.T. -0.000 min
Lab File: VX021209.D
Acq: 15 Mar 2021 18:54




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 43 Resp: 1644
Ion Ratio Lower Upper
43 100
58 36.9 35.4 53.0



#52
Toluene
Concen: 23.90 ug/l
RT: 8.764 min Scan# 1305
Delta R.T. -0.000 min
Lab File: VX021209.D
Acq: 15 Mar 2021 18:54


Tgt Ion: 92 Resp: 57111
Ion Ratio Lower Upper
92 100
91 173.2 137.1 205.7

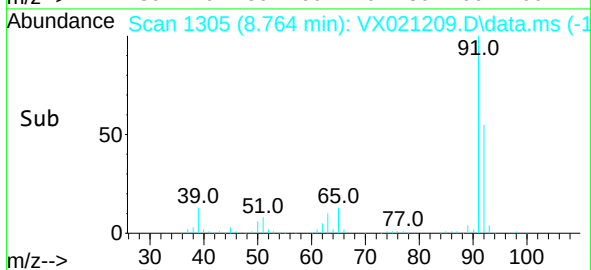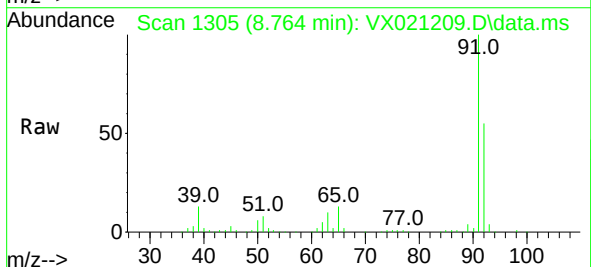






#55
1,1,2-Trichloroethane
Concen: 0.95 ug/l
RT: 9.059 min Scan# 1355
Delta R.T. -0.136 min
Lab File: VX021209.D
Acq: 15 Mar 2021 18:54

Instrument :
MSVOA_X
ClientSampled :



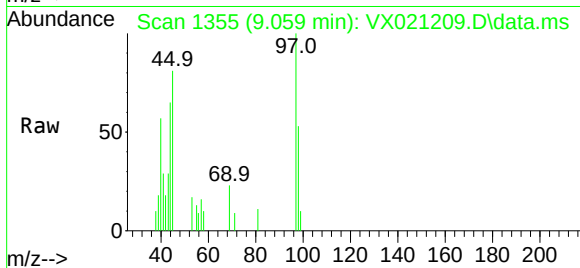



Tgt Ion:	97	Resp:	933
Ion	Ratio	Lower	Upper
97	100		
83	0.0	69.3	103.9#
85	0.0	44.3	66.5#
99	10.4	50.3	75.5#



#58
2-Chloroethyl Vinyl ether
Concen: 0.24 ug/l
RT: 8.264 min Scan# 1220
Delta R.T. -0.024 min
Lab File: VX021209.D
Acq: 15 Mar 2021 18:54

Tgt Ion:	63	Resp:	181
Ion	Ratio	Lower	Upper
63	100		
106	0.0	23.5	35.3#


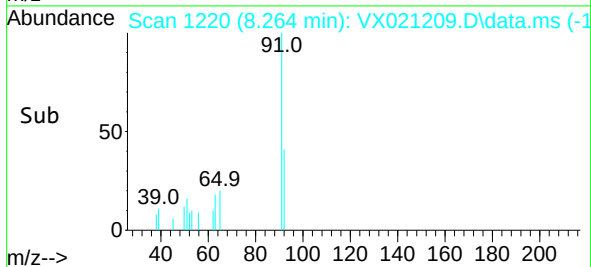

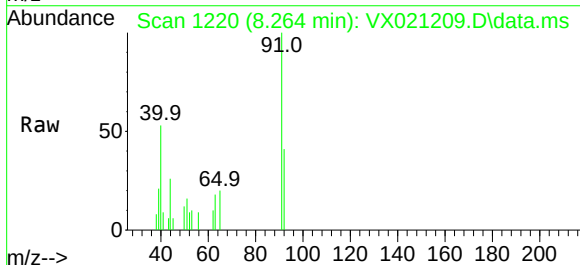




#59
2-Hexanone
Concen: 0.50 ug/l
RT: 9.470 min Scan# 1425
Delta R.T. -0.000 min
Lab File: VX021209.D
Acq: 15 Mar 2021 18:54




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 43 Resp: 558
Ion Ratio Lower Upper
43 100
58 74.2 30.9 92.8



#62
4-Bromofluorobenzene
Concen: 54.07 ug/l
RT: 11.118 min Scan# 1705
Delta R.T. -0.000 min
Lab File: VX021209.D
Acq: 15 Mar 2021 18:54

Tgt Ion: 95 Resp: 68899
Ion Ratio Lower Upper
95 100
174 69.3 0.0 154.6
176 70.5 0.0 155.8


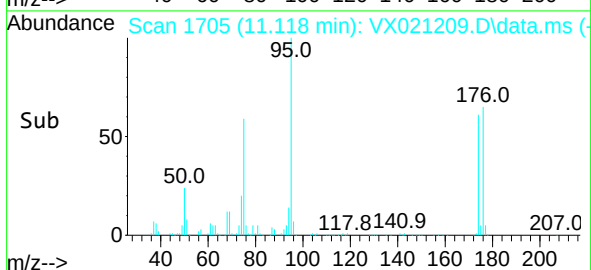






#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.094 min Scan# 1531
Delta R.T. -0.000 min
Lab File: VX021209.D
Acq: 15 Mar 2021 18:54




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion:117 Resp: 131377
Ion Ratio Lower Upper
117 100
82 60.9 47.4 71.2
119 31.8 26.6 39.8

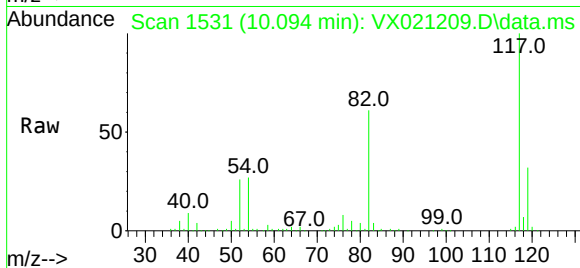

#67
Ethyl Benzene
Concen: 0.85 ug/l
RT: 10.235 min Scan# 1555
Delta R.T. 0.000 min
Lab File: VX021209.D
Acq: 15 Mar 2021 18:54

Tgt Ion: 91 Resp: 4294
Ion Ratio Lower Upper
91 100
106 27.4 24.6 37.0


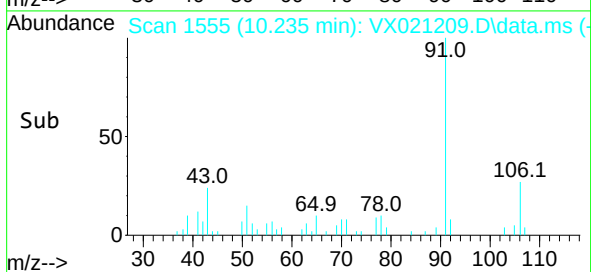

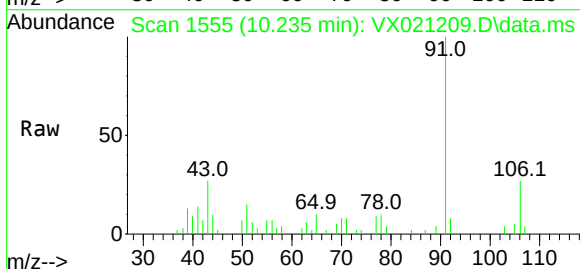




#68
m/p-Xylenes
Concen: 4.11 ug/l
RT: 10.335 min Scan# 1572
Delta R.T. -0.006 min
Lab File: VX021209.D
Acq: 15 Mar 2021 18:54




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion:106 Resp: 7435
Ion Ratio Lower Upper
106 100
91 217.7 162.8 244.2

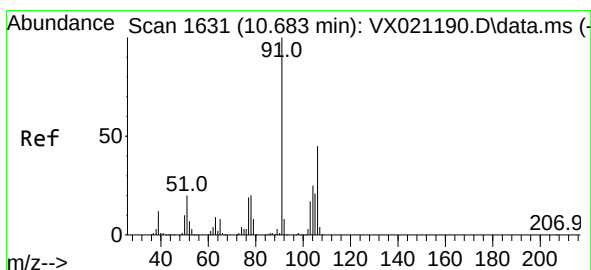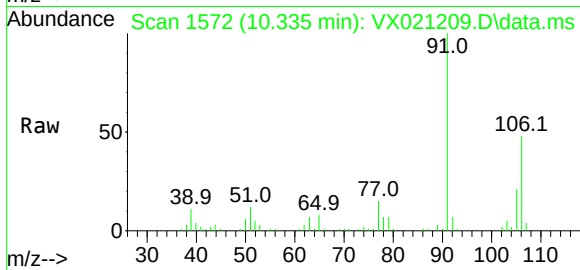

#69
o-Xylene
Concen: 2.08 ug/l
RT: 10.682 min Scan# 1631
Delta R.T. -0.001 min
Lab File: VX021209.D
Acq: 15 Mar 2021 18:54

Tgt Ion:106 Resp: 3652
Ion Ratio Lower Upper
106 100
91 234.9 108.1 324.2


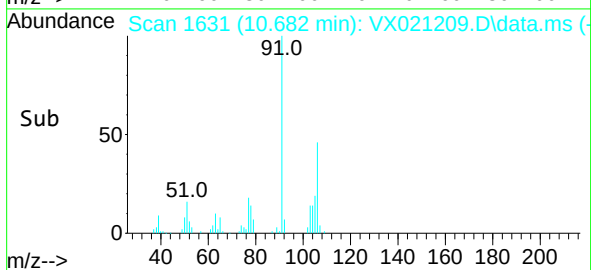

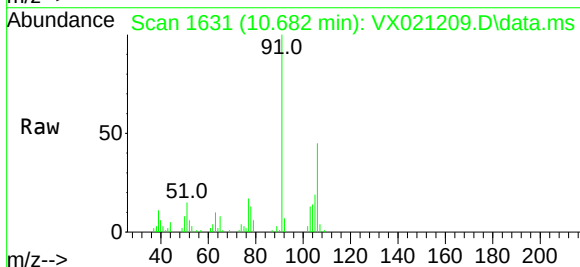


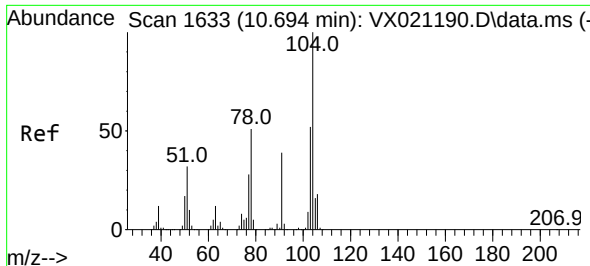

#70
Styrene
Concen: 1.22 ug/l
RT: 10.694 min Scan# 1633
Delta R.T. 0.000 min
Lab File: VX021209.D
Acq: 15 Mar 2021 18:54




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion:104 Resp: 3622
Ion Ratio Lower Upper
104 100
78 69.1 40.0 60.0#
103 67.5 43.4 65.0#

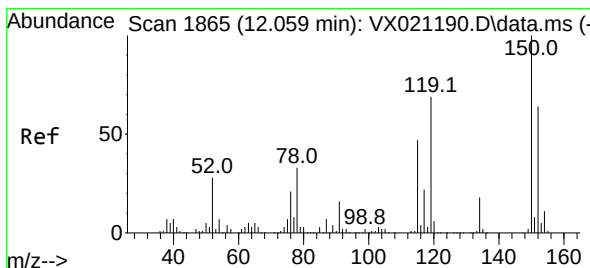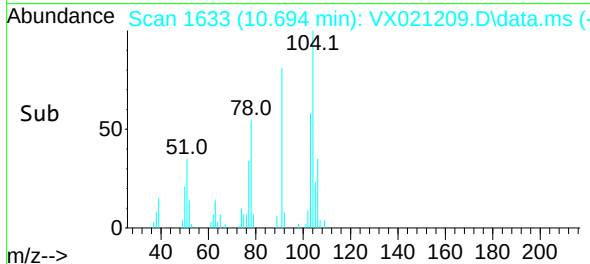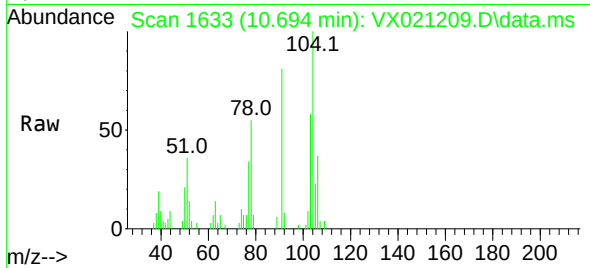

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.059 min Scan# 1865
Delta R.T. -0.006 min
Lab File: VX021209.D
Acq: 15 Mar 2021 18:54

Tgt Ion:152 Resp: 59003
Ion Ratio Lower Upper
152 100
115 67.8 41.1 123.3
150 159.0 0.0 349.0


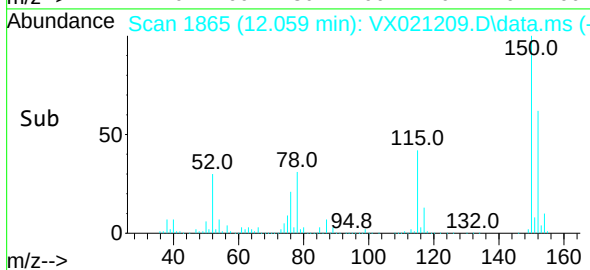

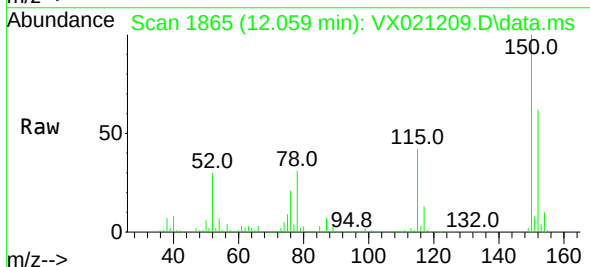


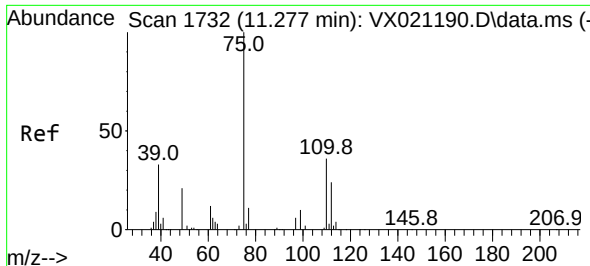

#76
1,2,3-Trichloropropane
Concen: 26.54 ug/l
RT: 11.118 min Scan# 1705
Delta R.T. -0.159 min
Lab File: VX021209.D
Acq: 15 Mar 2021 18:54




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 75 Resp: 38834
Ion Ratio Lower Upper
75 100
77 1.5 19.1 57.5#

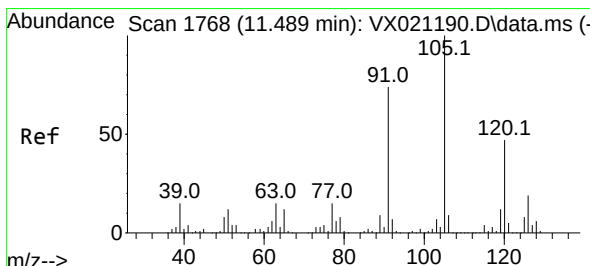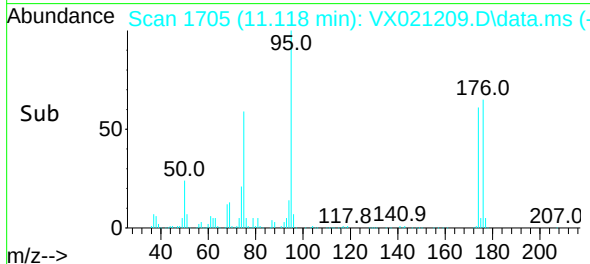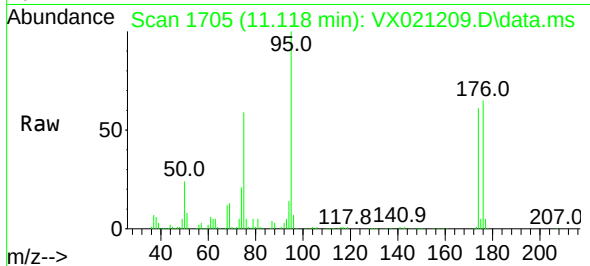

#80
1,3,5-Trimethylbenzene
Concen: 0.26 ug/l
RT: 11.494 min Scan# 1769
Delta R.T. 0.006 min
Lab File: VX021209.D
Acq: 15 Mar 2021 18:54


Tgt Ion: 105 Resp: 1003
Ion Ratio Lower Upper
105 100
120 46.4 23.8 71.5

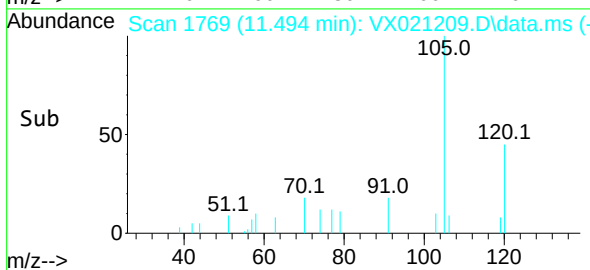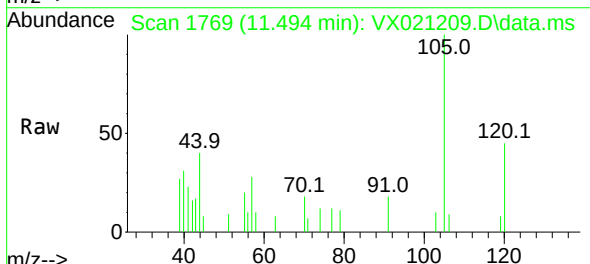



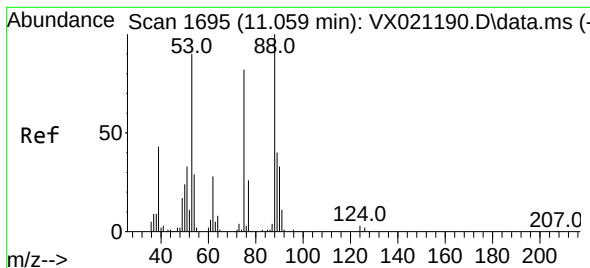


#81
trans-1,4-Dichloro-2-butene
Concen: 75.34 ug/l
RT: 11.118 min Scan# 1705
Delta R.T. 0.059 min
Lab File: VX021209.D
Acq: 15 Mar 2021 18:54


Instrument :
MSVOA_X
ClientSampleId :

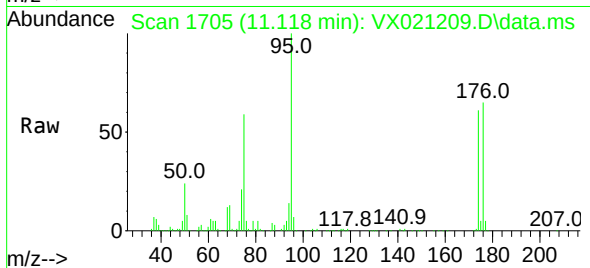



Tgt Ion: 75 Resp: 38834
Ion Ratio Lower Upper
75 100
53 0.0 74.5 111.7#
89 0.1 37.9 56.9#

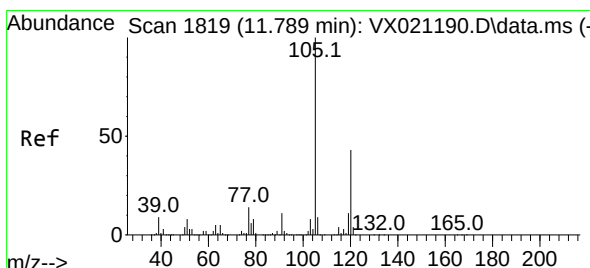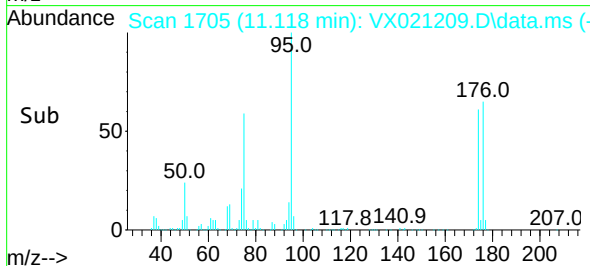


#84
1,2,4-Trimethylbenzene
Concen: 0.83 ug/l
RT: 11.788 min Scan# 1819
Delta R.T. -0.000 min
Lab File: VX021209.D
Acq: 15 Mar 2021 18:54

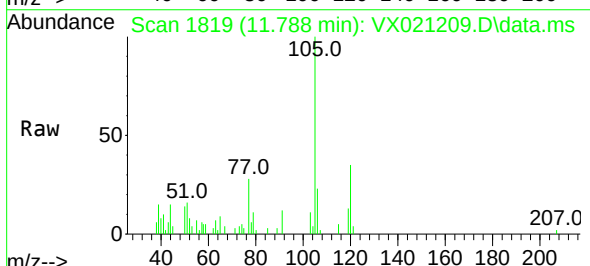


Tgt Ion: 105 Resp: 3205
Ion Ratio Lower Upper
105 100
120 35.6 22.4 67.3

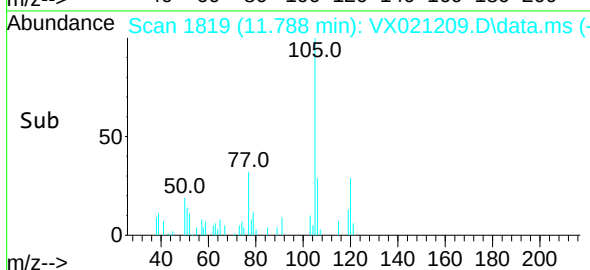






#92
1,2-Dibromo-3-Chloropropane
Concen: 0.32 ug/l
RT: 12.841 min Scan# 1998
Delta R.T. -0.141 min
Lab File: VX021209.D
Acq: 15 Mar 2021 18:54

Instrument :
MSVOA_X
ClientSampled :

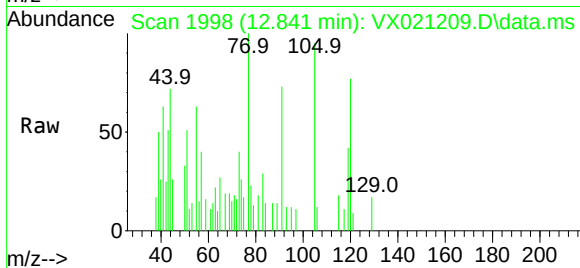

Tgt Ion: 75 Resp: 117
Ion Ratio Lower Upper
75 100
155 0.0 45.3 135.9#
157 0.0 57.7 173.1#



#95
Naphthalene
Concen: 8.09 ug/l
RT: 13.818 min Scan# 2164
Delta R.T. 0.000 min
Lab File: VX021209.D
Acq: 15 Mar 2021 18:54

Tgt Ion: 128 Resp: 29681
Ion Ratio Lower Upper
128 100
127 13.0 10.3 15.5
129 11.1 8.8 13.2

