


Bromoform

Response Ratio

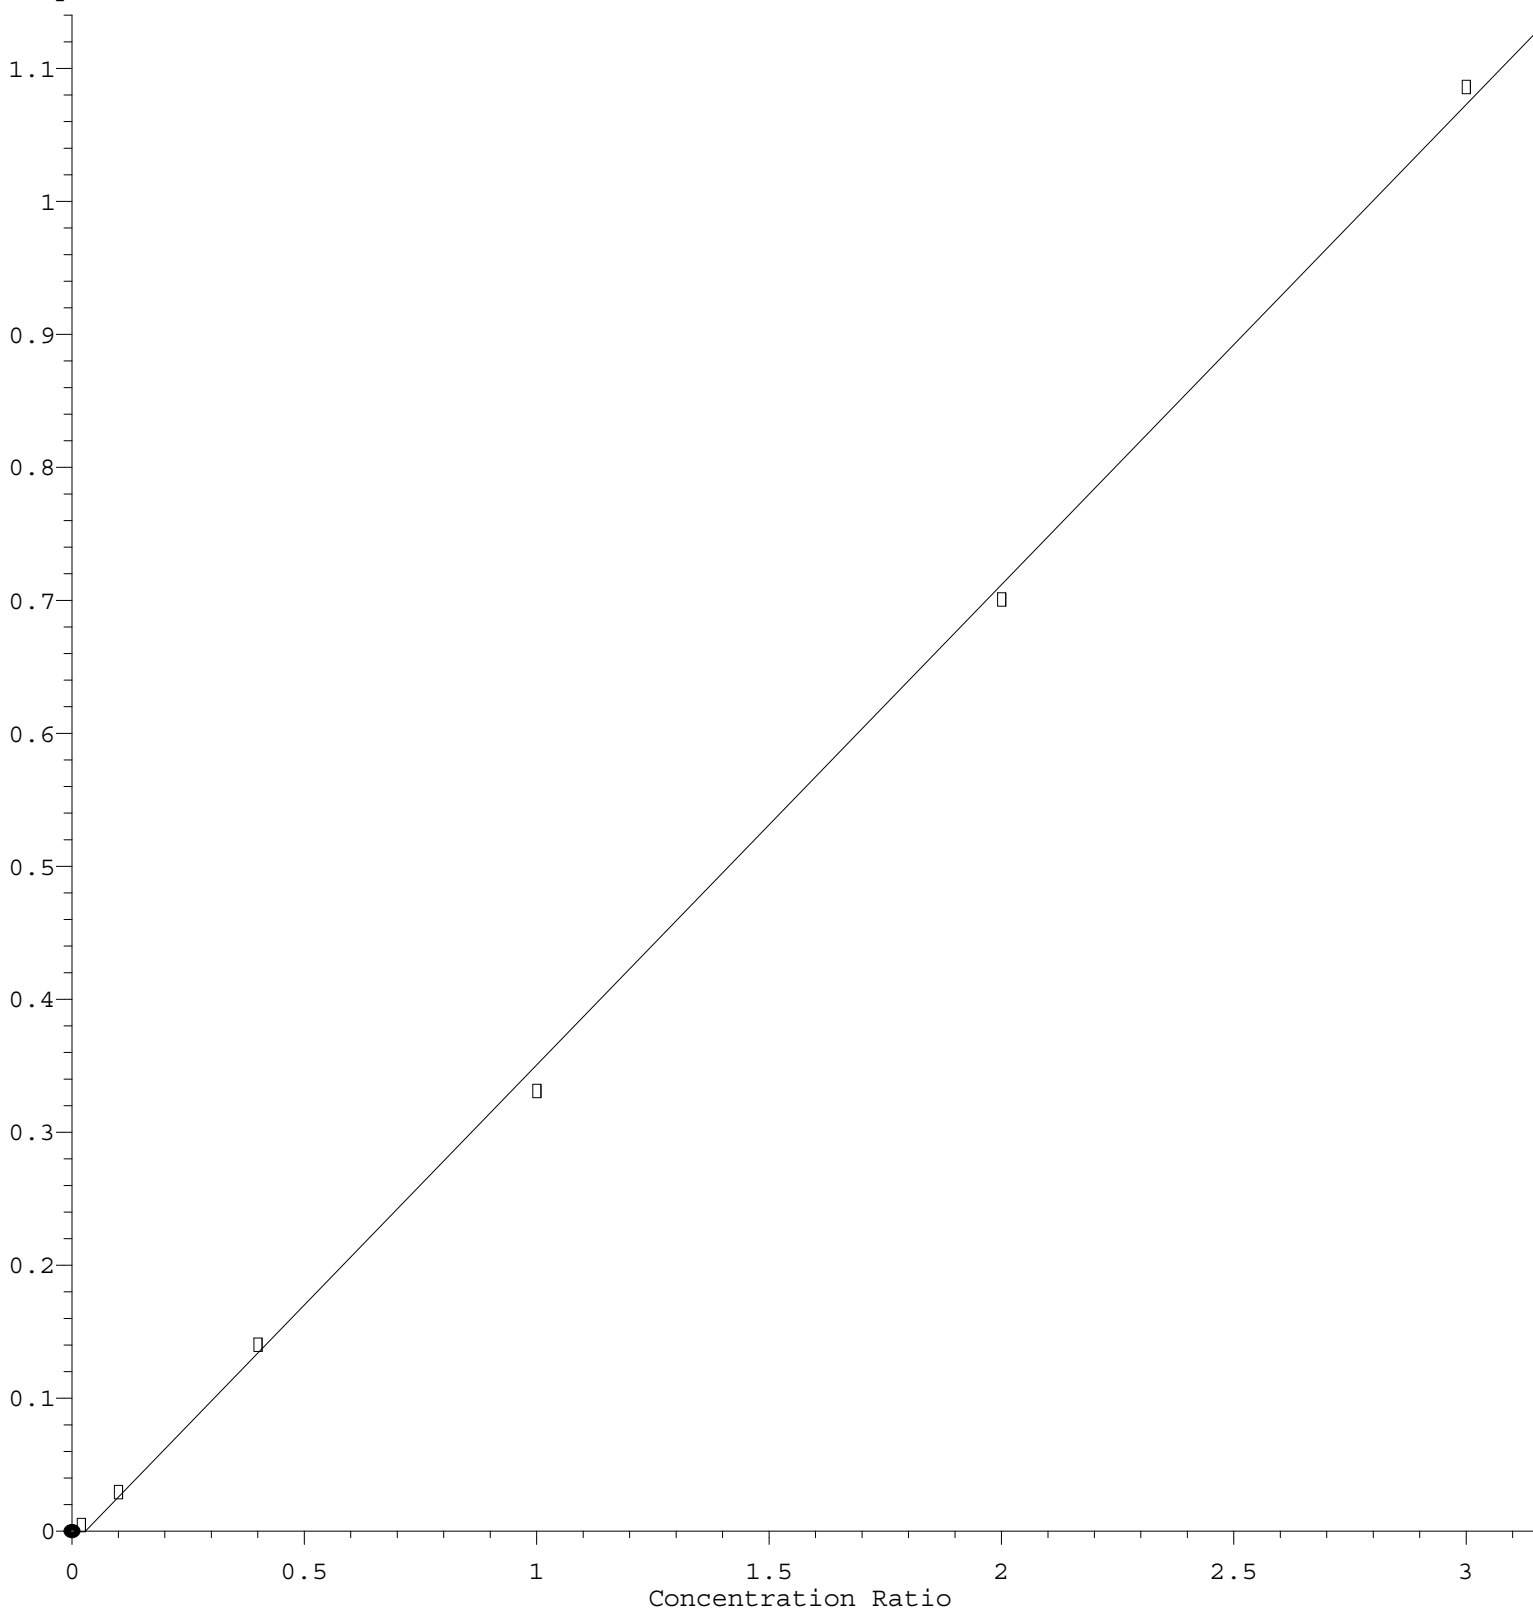

$$\text{Response} = 3.611\text{e-}001 * \text{Amt} - 1.050\text{e-}002$$


Coef of Det (r^2) = 0.999137 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X031521W.M

Calibration Table Last Updated: Mon Mar 15 11:55:59 2021

Naphthalene

Response Ratio

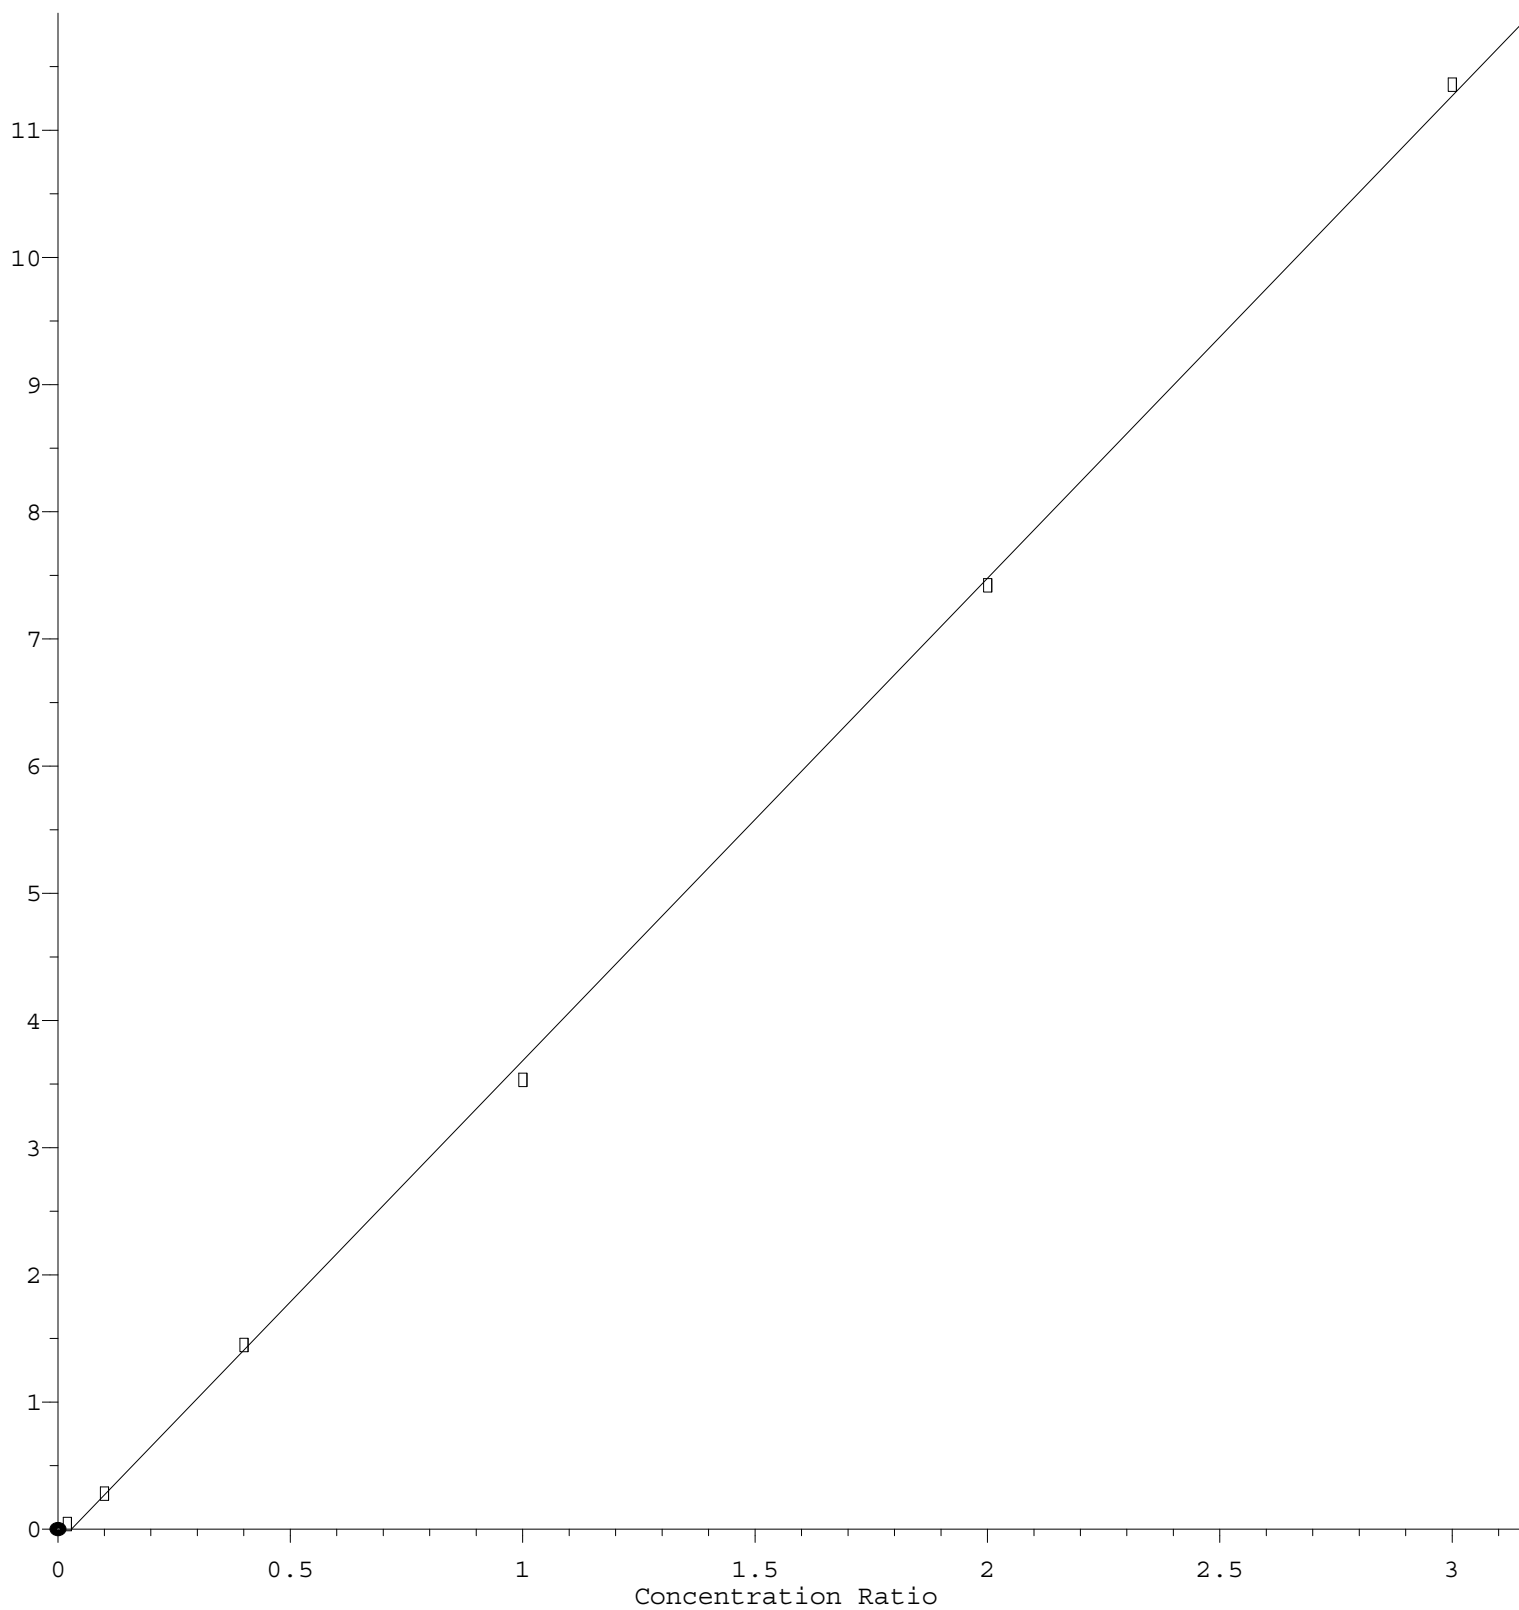

$$\text{Response} = 3.795\text{e}+000 * \text{Amt} - 1.112\text{e}-001$$


Coef of Det (r^2) = 0.999604 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X031521W.M

Calibration Table Last Updated: Mon Mar 15 11:55:59 2021

1,2,3-Trichlorobenzene

Response Ratio

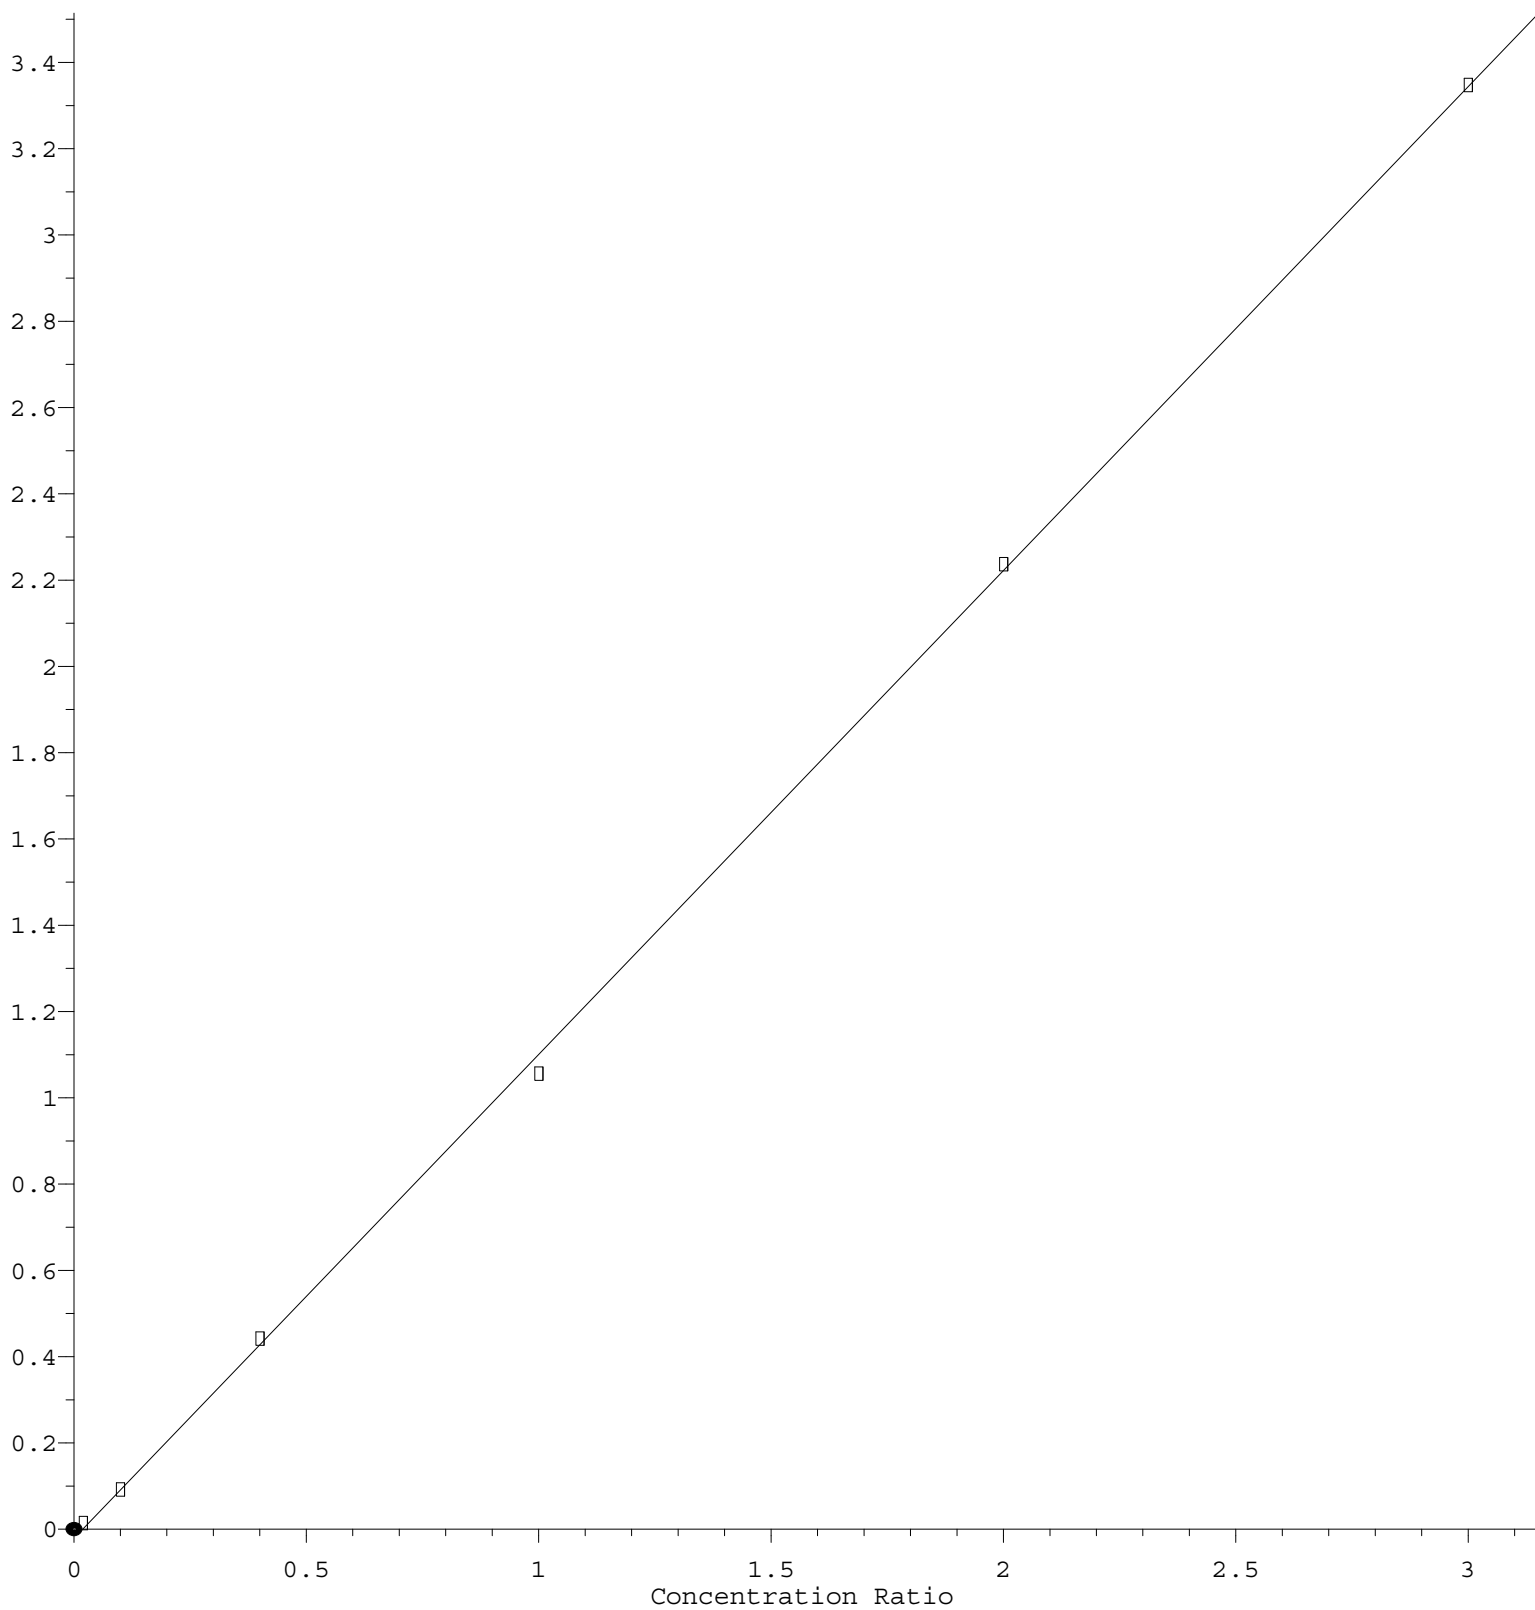

$$\text{Response} = 1.122\text{e}+000 * \text{Amt} - 2.084\text{e}-002$$

Coef of Det (r^2) = 0.999711 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X031521W.M

Calibration Table Last Updated: Mon Mar 15 11:55:59 2021