

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031521\
 Data File : VX021200.D
 Acq On : 15 Mar 2021 15:31
 Operator : JC/MD
 Sample : M1583-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-WATER-REF-4

Integration Parameters: RTEINT.P

Integrator: RTE

Smoother: ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031521W.M

Title : SW846 8260

Signal : TIC: VX021200.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	78	87	90	rBV5	4264	9065	1.87%	0.348%
2	2.234	190	195	206	rVB8	1761	5029	1.04%	0.193%
3	2.587	245	255	262	rBV	4418	9003	1.86%	0.346%
4	5.470	732	745	757	rBV2	58413	164404	33.91%	6.317%
5	5.635	760	773	786	rBV2	87856	245375	50.61%	9.428%
6	6.035	830	841	858	rVB	65430	174194	35.93%	6.693%
7	6.835	966	977	990	rBV	145776	350492	72.30%	13.467%
8	8.694	1286	1293	1317	rBV	302022	484797	100.00%	18.628%
9	10.094	1524	1531	1546	rBV	327405	440994	90.96%	16.945%
10	11.124	1699	1706	1716	rBV	259603	338409	69.80%	13.003%
11	12.059	1860	1865	1876	rBV	299159	380763	78.54%	14.631%




Sum of corrected areas: 2602525

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031521\
Data File : VX021200.D
Acq On : 15 Mar 2021 15:31
Operator : JC/MD
Sample : M1583-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031521W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

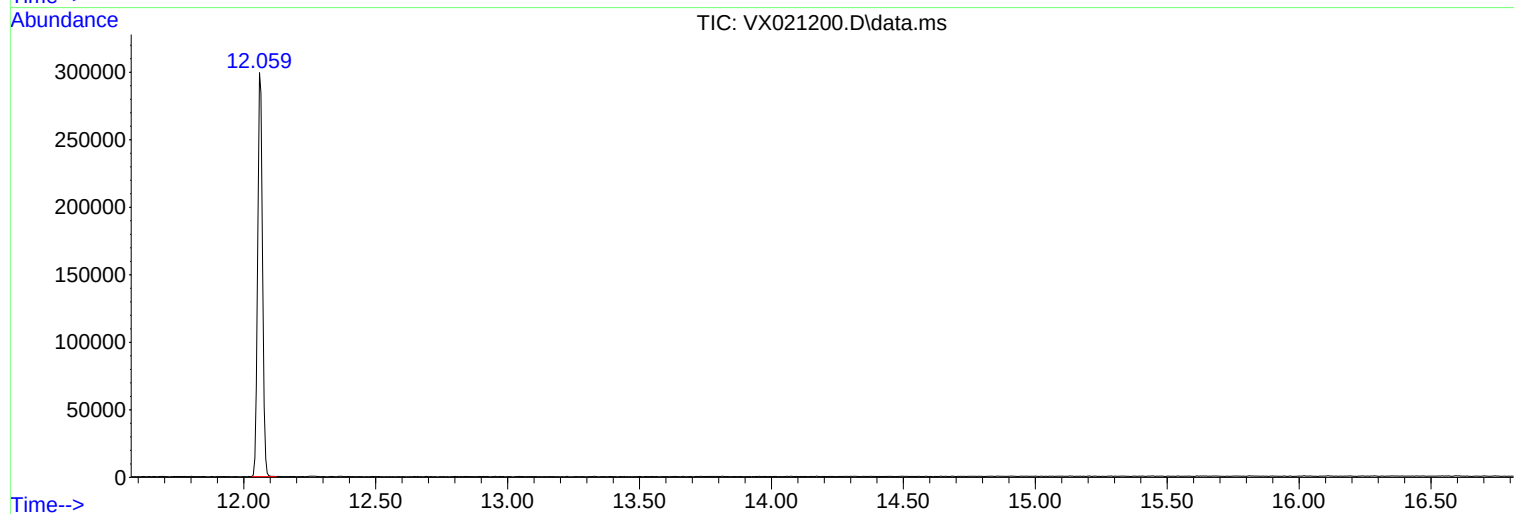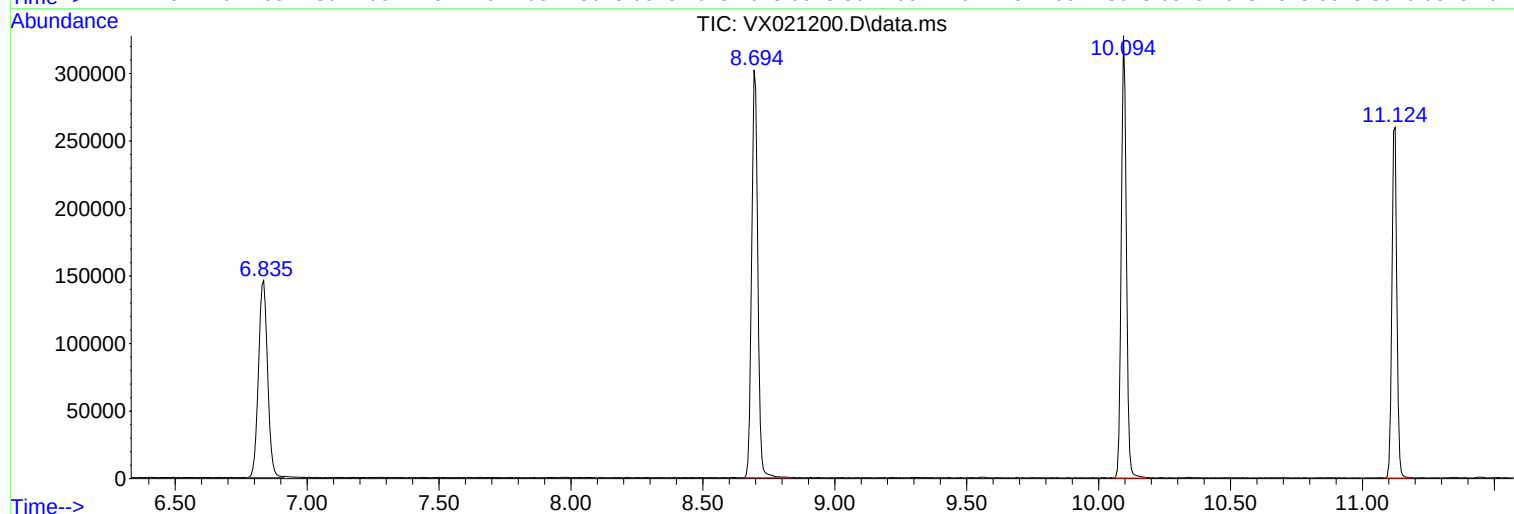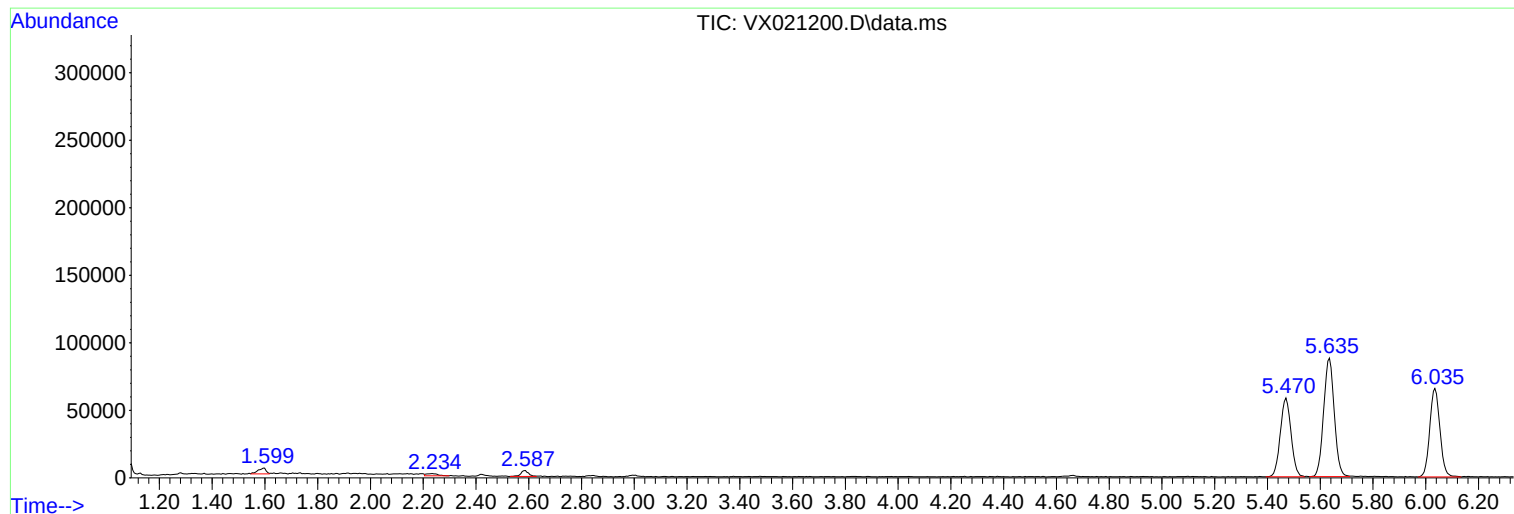

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031521\
Data File : VX021200.D
Acq On : 15 Mar 2021 15:31
Operator : JC/MD
Sample : M1583-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031521W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031521\
Data File : VX021200.D
Acq On : 15 Mar 2021 15:31
Operator : JC/MD
Sample : M1583-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031521W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------