

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031521\
 Data File : VX021221.D
 Acq On : 16 Mar 2021 00:21
 Operator : JC/MD
 Sample : M1645-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-WATER-REF-4

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031521W.M

Title : SW846 8260

Signal : TIC: VX021221.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.593	78	86	91	rVB3	4057	8428	1.75%	0.325%
2	2.581	247	254	263	rBV	6315	12238	2.54%	0.472%
3	2.999	319	325	334	rVB4	2176	5120	1.06%	0.198%
4	5.470	730	745	757	rBV	55058	160442	33.27%	6.191%
5	5.629	760	772	785	rBV	85673	241166	50.01%	9.305%
6	6.029	830	840	852	rBV	65037	168621	34.97%	6.506%
7	6.829	966	976	991	rBV	146017	344065	71.35%	13.276%
8	8.694	1285	1293	1307	rBV	309040	482241	100.00%	18.607%
9	10.094	1524	1531	1549	rVB	329148	444946	92.27%	17.168%
10	11.118	1700	1705	1715	rBV	256356	337965	70.08%	13.040%
11	12.059	1860	1865	1874	rBV	309790	386469	80.14%	14.912%




Sum of corrected areas: 2591701

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031521\
Data File : VX021221.D
Acq On : 16 Mar 2021 00:21
Operator : JC/MD
Sample : M1645-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031521W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

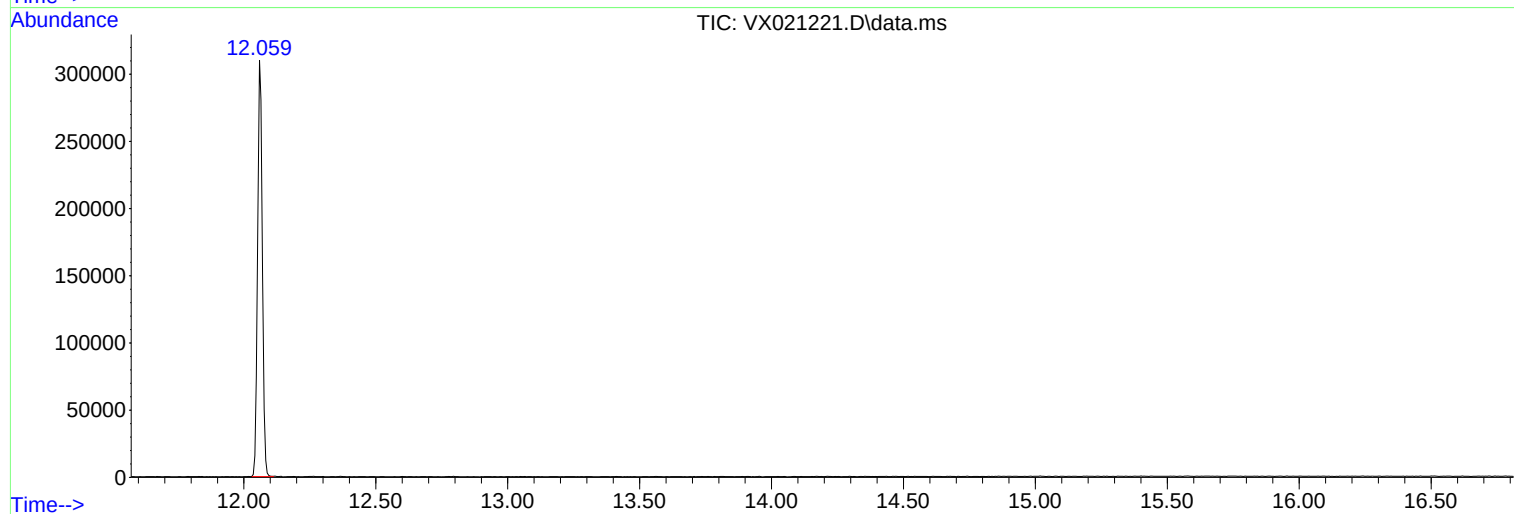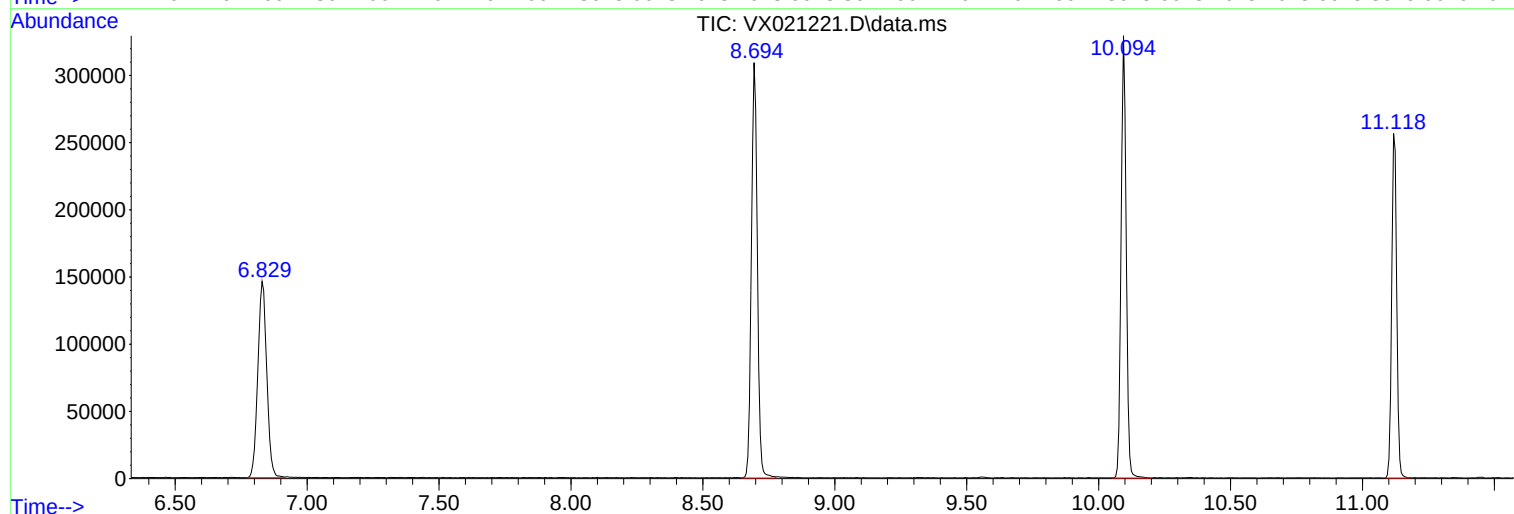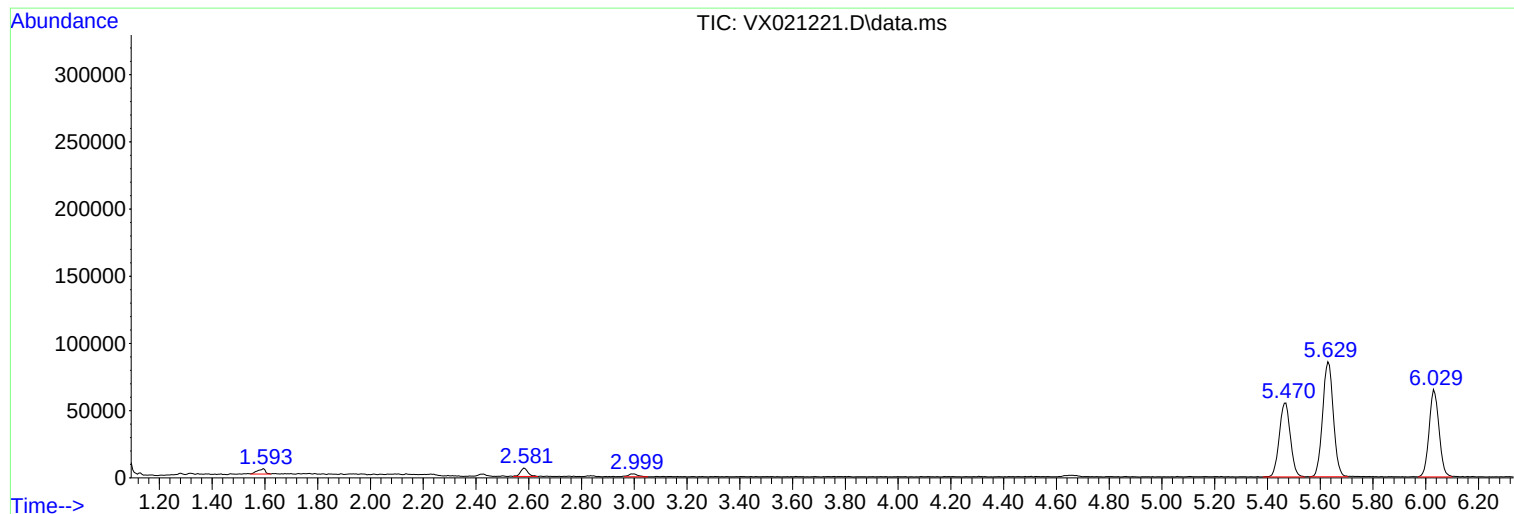

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031521\
Data File : VX021221.D
Acq On : 16 Mar 2021 00:21
Operator : JC/MD
Sample : M1645-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031521W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031521\
Data File : VX021221.D
Acq On : 16 Mar 2021 00:21
Operator : JC/MD
Sample : M1645-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031521W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
