
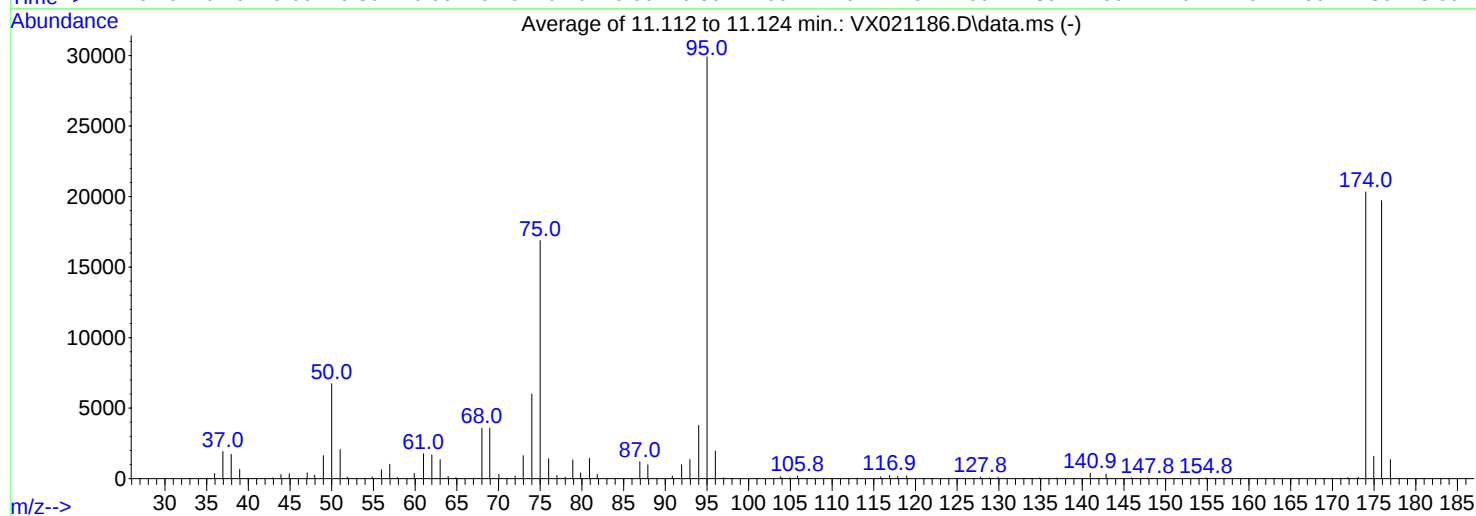


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031521\
 Data File : VX021186.D
 Acq On : 15 Mar 2021 08:54
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031521W.M
 Title : SW846 8260
 Last Update : Mon Mar 15 11:55:59 2021

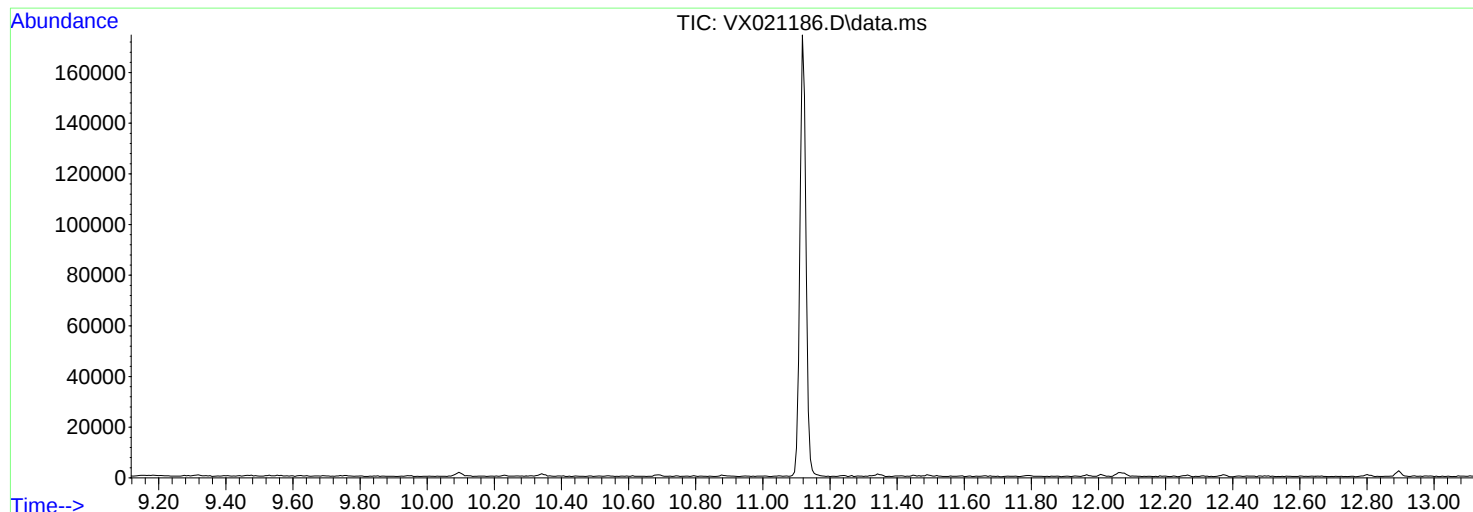

AutoFind: Scans 1704, 1705, 1706; Background Corrected with Scan 1698

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.5	6727	PASS
75	95	30	60	56.5	16883	PASS
95	95	100	100	100.0	29907	PASS
96	95	5	9	6.5	1946	PASS
173	174	0.00	2	0.4	91	PASS
174	95	50	100	68.0	20330	PASS
175	174	5	9	7.8	1585	PASS
176	174	95	101	97.0	19713	PASS
177	176	5	9	6.8	1349	PASS