


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031521\
Data File : VX021214.D
Acq On : 15 Mar 2021 21:14
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031521W.M
Title : SW846 8260
Last Update : Mon Mar 15 11:55:59 2021

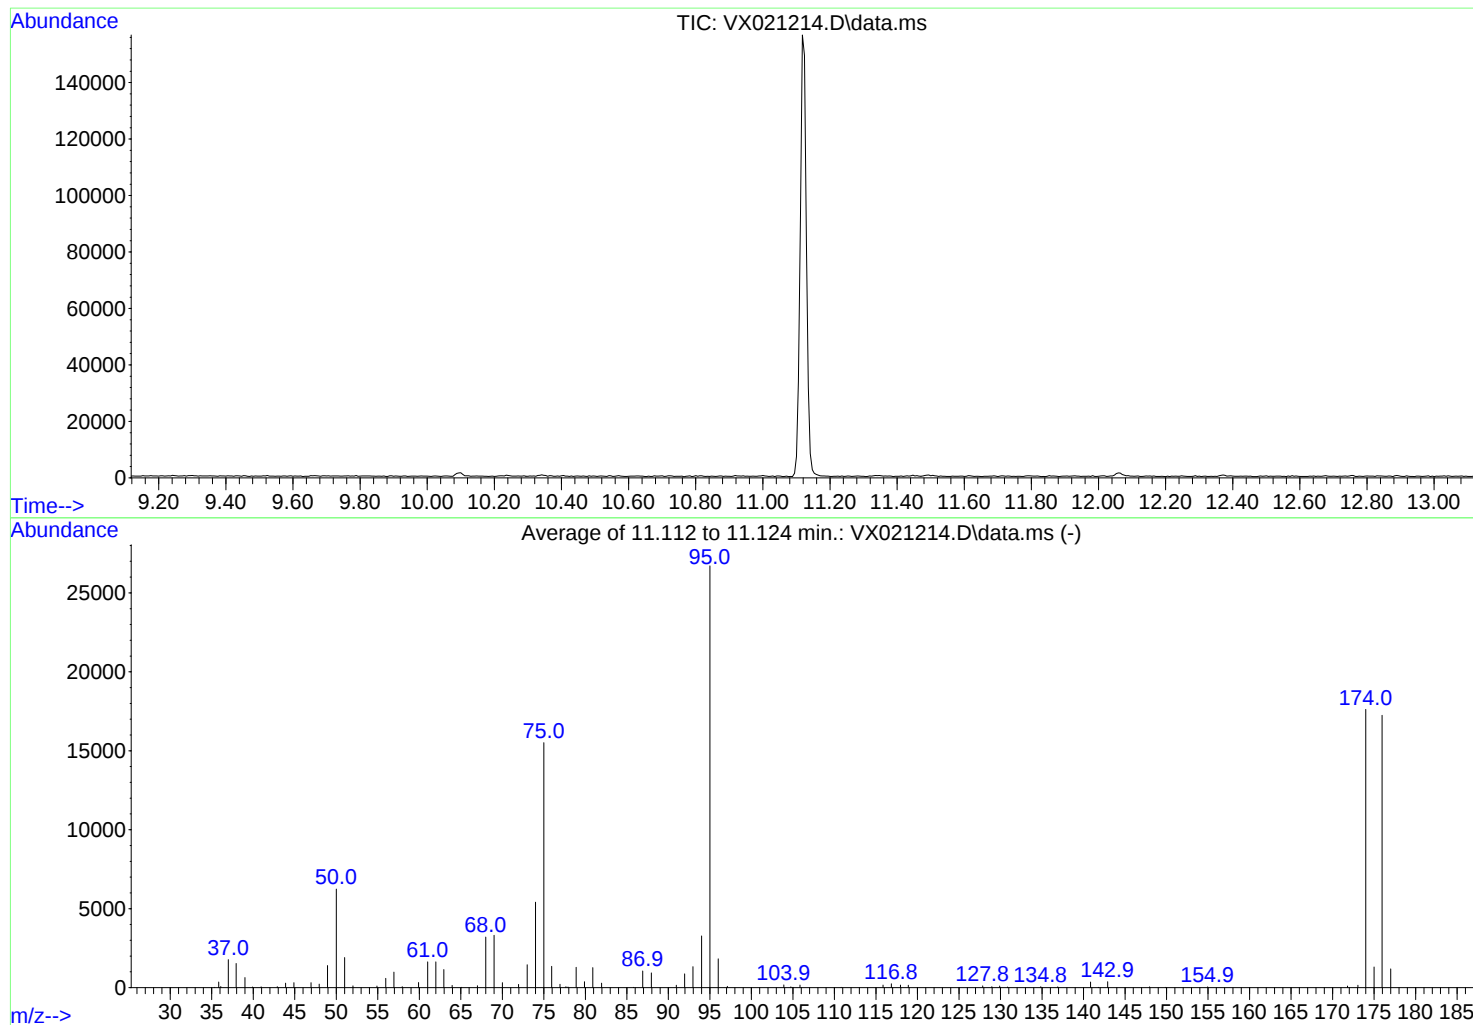

AutoFind: Scans 1704, 1705, 1706; Background Corrected with Scan 1698

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	23.4	6247	PASS
75	95	30	60	58.1	15517	PASS
95	95	100	100	100.0	26712	PASS
96	95	5	9	6.8	1827	PASS
173	174	0.00	2	0.9	152	PASS
174	95	50	100	66.0	17620	PASS
175	174	5	9	7.4	1309	PASS
176	174	95	101	97.9	17249	PASS
177	176	5	9	6.9	1190	PASS