

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031522\
 Data File : VX027453.D
 Acq On : 15 Mar 2022 17:32
 Operator : JC/MD
 Sample : N1950-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 31424

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X030822W.M
 Title : SW846 8260

Signal : TIC: VX027453.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	18	rVB2	42500	40826	2.27%	0.328%
2	1.264	22	29	32	rBV2	15189	28538	1.58%	0.229%
3	1.355	41	44	45	rBV	22241	19856	1.10%	0.159%
4	1.453	57	60	64	rVB	21063	22333	1.24%	0.179%
5	2.215	180	185	191	rVB3	9355	19380	1.08%	0.156%
6	2.380	206	212	229	rVB	146711	243153	13.50%	1.953%
7	2.538	229	238	246	rBV2	14253	27449	1.52%	0.220%
8	4.239	505	517	524	rBV5	6096	20955	1.16%	0.168%
9	4.574	564	572	586	rVB	6278	18990	1.05%	0.152%
10	5.391	694	706	719	rBV	222235	637994	35.41%	5.123%
11	5.556	722	733	750	rVB	372994	1055953	58.62%	8.480%
12	5.964	785	800	812	rBV	218812	592921	32.91%	4.761%
13	6.641	898	911	921	rBV	30216	80501	4.47%	0.646%
14	6.763	921	931	947	rVB	558622	1339069	74.33%	10.753%
15	6.964	954	964	974	rBV	28969	71381	3.96%	0.573%
16	7.464	1040	1046	1060	rVB	12725	29348	1.63%	0.236%
17	7.903	1113	1118	1127	rVB2	24150	50373	2.80%	0.405%
18	8.580	1222	1229	1234	rBV	13791	23188	1.29%	0.186%
19	8.653	1234	1241	1248	rVV	1130044	1801480	100.00%	14.466%
20	8.720	1248	1252	1261	rVB	87032	135264	7.51%	1.086%
21	8.805	1261	1266	1274	rBV	22522	36634	2.03%	0.294%
22	8.946	1281	1289	1294	rBV	14512	22373	1.24%	0.180%
23	9.244	1332	1338	1347	rBV	62734	97190	5.40%	0.780%
24	9.445	1365	1371	1377	rBV3	17176	31814	1.77%	0.255%
25	9.708	1404	1414	1424	rVB	16633	28991	1.61%	0.233%
26	9.836	1431	1435	1446	rVB	25936	37609	2.09%	0.302%
27	9.945	1446	1453	1461	rBV	54303	82681	4.59%	0.664%
28	10.055	1461	1471	1484	rVV	1203380	1619199	89.88%	13.003%
29	10.214	1490	1497	1503	rBV2	31206	56241	3.12%	0.452%
30	10.275	1503	1507	1509	rVV	32885	44891	2.49%	0.360%
31	10.299	1509	1511	1519	rVB	34983	48616	2.70%	0.390%
32	10.646	1562	1568	1573	rBV3	11229	19688	1.09%	0.158%
33	10.872	1598	1605	1607	rBV2	26866	47217	2.62%	0.379%
34	11.012	1623	1628	1632	rBV2	15193	20893	1.16%	0.168%
35	11.085	1634	1640	1650	rVV	945943	1286842	71.43%	10.334%
36	11.177	1650	1655	1660	rVB3	13610	21881	1.21%	0.176%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031522\
 Data File : VX027453.D
 Acq On : 15 Mar 2022 17:32
 Operator : JC/MD
 Sample : N1950-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 31424

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X030822W.M
 Title : SW846 8260

37	11.232	1660	1664	1669	rBV	12443	18765	1.04%	0.151%
38	11.354	1679	1684	1691	rBV7	9807	26918	1.49%	0.216%
39	11.457	1697	1701	1709	rVB	25591	40172	2.23%	0.323%
40	11.750	1743	1749	1754	rBV2	47767	65204	3.62%	0.524%
41	11.915	1767	1776	1780	rBV	17139	28701	1.59%	0.230%
42	11.976	1780	1786	1789	rBV	207480	277533	15.41%	2.229%
43	12.024	1789	1794	1806	rVB	1234515	1526319	84.73%	12.257%
44	12.122	1806	1810	1821	rVB	21000	40853	2.27%	0.328%
45	12.219	1821	1826	1828	rBV2	15663	20687	1.15%	0.166%
46	12.360	1839	1849	1855	rBV	58530	112760	6.26%	0.906%
47	12.920	1935	1941	1944	rBV4	10583	20826	1.16%	0.167%
48	13.006	1950	1955	1960	rVV4	17787	42579	2.36%	0.342%
49	13.055	1960	1963	1967	rVV	46698	69148	3.84%	0.555%
50	13.134	1971	1976	1983	rVB4	22111	39041	2.17%	0.314%
51	13.201	1983	1987	1990	rBV2	19488	28292	1.57%	0.227%
52	13.305	1999	2004	2011	rVB4	25412	48701	2.70%	0.391%
53	13.378	2011	2016	2021	rVV2	29833	53429	2.97%	0.429%
54	13.426	2021	2024	2029	rVV	32934	45488	2.53%	0.365%
55	13.585	2047	2050	2053	rBV3	14520	24961	1.39%	0.200%
56	13.622	2053	2056	2062	rVV	33445	64732	3.59%	0.520%
57	13.780	2078	2082	2085	rBV	18147	25172	1.40%	0.202%
58	13.920	2101	2105	2108	rBV4	14246	19839	1.10%	0.159%
59	14.146	2137	2142	2150	rBV9	10210	27248	1.51%	0.219%
60	14.371	2175	2179	2186	rBV7	9703	23695	1.32%	0.190%




Sum of corrected areas: 12452775

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031522\
Data File : VX027453.D
Acq On : 15 Mar 2022 17:32
Operator : JC/MD
Sample : N1950-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
31424

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X030822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

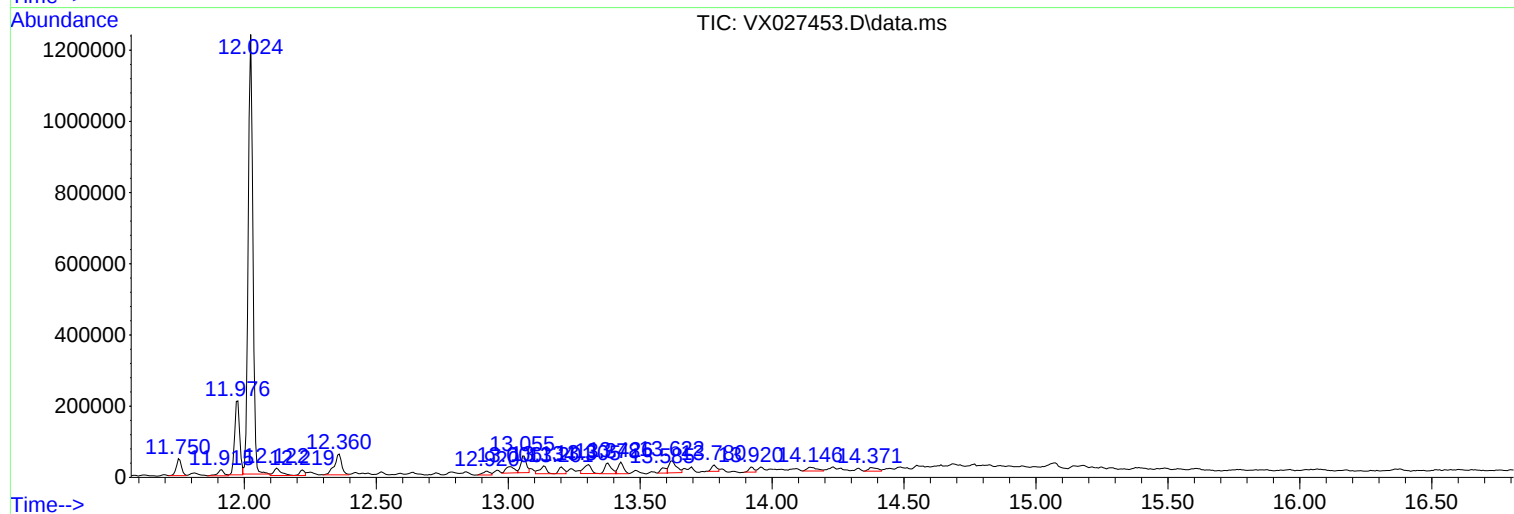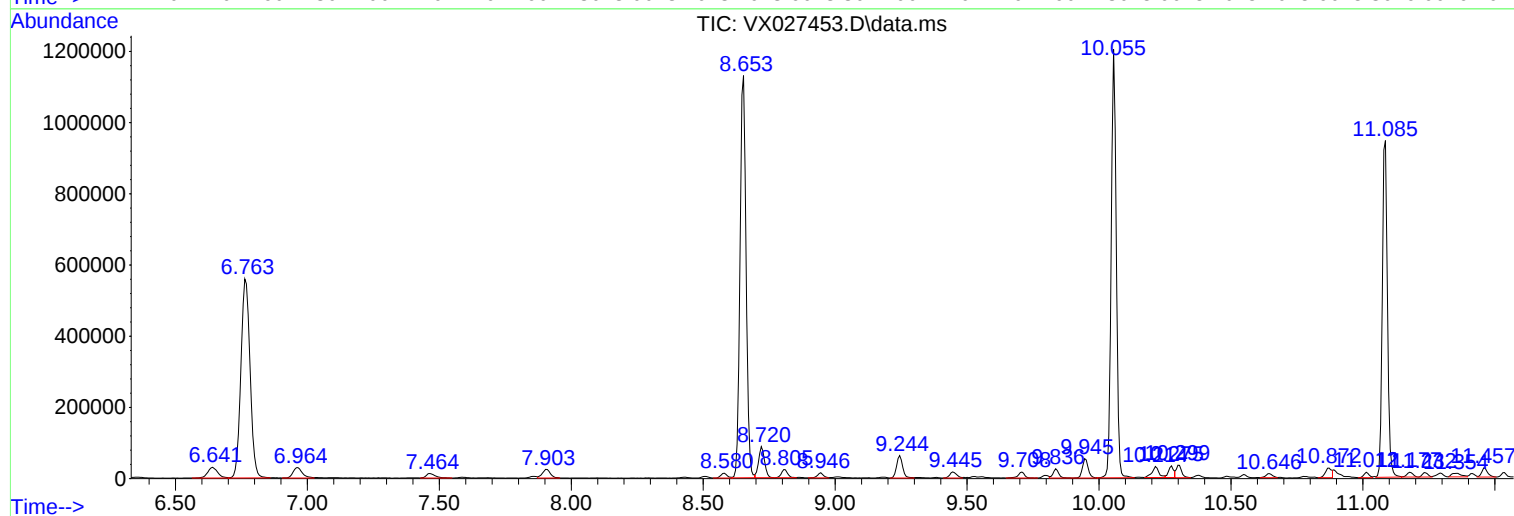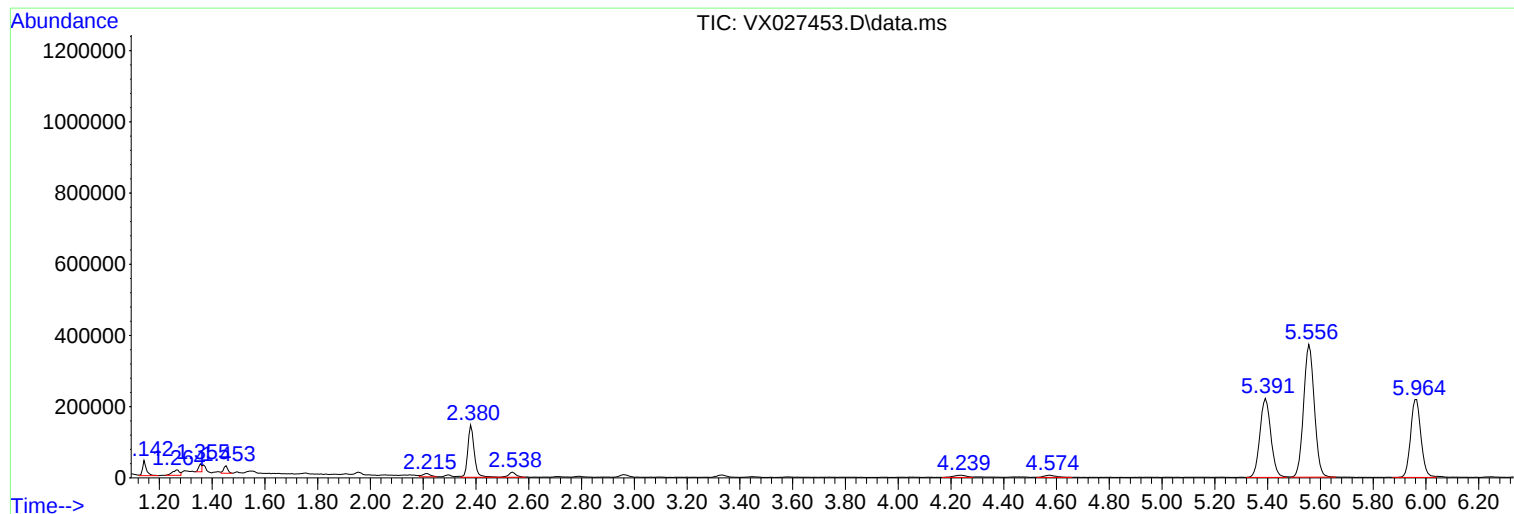

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031522\
Data File : VX027453.D
Acq On : 15 Mar 2022 17:32
Operator : JC/MD
Sample : N1950-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
31424

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X030822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031522\
Data File : VX027453.D
Acq On : 15 Mar 2022 17:32
Operator : JC/MD
Sample : N1950-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
31424

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X030822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------