

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031523\
 Data File : VX034511.D
 Acq On : 15 Mar 2023 16:22
 Operator : JC/MD
 Sample : 01892-01 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BOOM-030923

Quant Time: Mar 16 05:20:54 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
 Quant Title : SW846 8260
 QLast Update : Mon Mar 13 10:29:32 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	238383	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	404829	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	360881	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	167785	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	160998	46.424	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	92.840%
35) Dibromofluoromethane	5.385	113	124617	46.623	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	93.240%
50) Toluene-d8	8.647	98	491178	49.226	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	98.460%
62) 4-Bromofluorobenzene	11.079	95	193071	47.904	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	95.800%


Target Compounds					Qvalue	
3) Chloromethane	1.294	50	693	Below Cal		98
11) Tert butyl alcohol	2.940	59	3592	4.974 ug/l #		73
13) Acrolein	2.233	56	158	0.277 ug/l #		1
16) Acetone	2.373	43	10468	6.408 ug/l		98
20) Methylene Chloride	2.794	84	2790	0.880 ug/l #		71
25) 2-Butanone	4.574	43	3754	1.606 ug/l #		83
36) 1,1-Dichloropropene	5.550	75	19097	4.652 ug/l #		50
37) Ethyl Acetate	4.574	43	3754	0.837 ug/l #		71
38) Carbon Tetrachloride	5.550	117	23498	5.754 ug/l #		15
40) Benzene	6.044	78	11358	0.946 ug/l		96
52) Toluene	8.720	92	10692	1.438 ug/l		99
67) Ethyl Benzene	10.195	91	16963	1.197 ug/l		90
68) m/p-Xylenes	10.299	106	23441	4.305 ug/l		97
69) o-Xylene	10.640	106	17670	3.234 ug/l		97
70) Styrene	10.659	104	2699	0.306 ug/l #		6
73) Isopropylbenzene	10.963	105	8219	0.634 ug/l		92
76) 1,2,3-Trichloropropane	11.079	75	101837	26.434 ug/l #		35
78) n-propylbenzene	11.305	91	28336	1.892 ug/l		98
79) 2-Chlorotoluene	11.378	91	15864	1.715 ug/l #		42
80) 1,3,5-Trimethylbenzene	11.451	105	42128	3.873 ug/l		98
81) trans-1,4-Dichloro-2-b...	11.079	75	101837	71.511 ug/l #		9
82) 4-Chlorotoluene	11.451	91	5212	0.489 ug/l #		46
83) tert-Butylbenzene	11.750	119	25485	2.324 ug/l #		56
84) 1,2,4-Trimethylbenzene	11.750	105	218657	19.670 ug/l		98
85) sec-Butylbenzene	11.890	105	14878	1.110 ug/l		88
86) p-Isopropyltoluene	12.006	119	10899	0.967 ug/l		93
89) n-Butylbenzene	12.329	91	45694	4.562 ug/l #		40
90) Hexachloroethane	12.530	117	7620	3.655 ug/l #		15
92) 1,2-Dibromo-3-Chloropr...	12.926	75	757	0.770 ug/l #		9
95) Naphthalene	13.774	128	151085	12.230 ug/l		97
96) 1,2,3-Trichlorobenzene	13.975	180	766	0.213 ug/l #		1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031523\
Data File : VX034511.D
Acq On : 15 Mar 2023 16:22
Operator : JC/MD
Sample : 01892-01 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BOOM-030923

Quant Time: Mar 16 05:20:54 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260
QLast Update : Mon Mar 13 10:29:32 2023
Response via : Initial Calibration




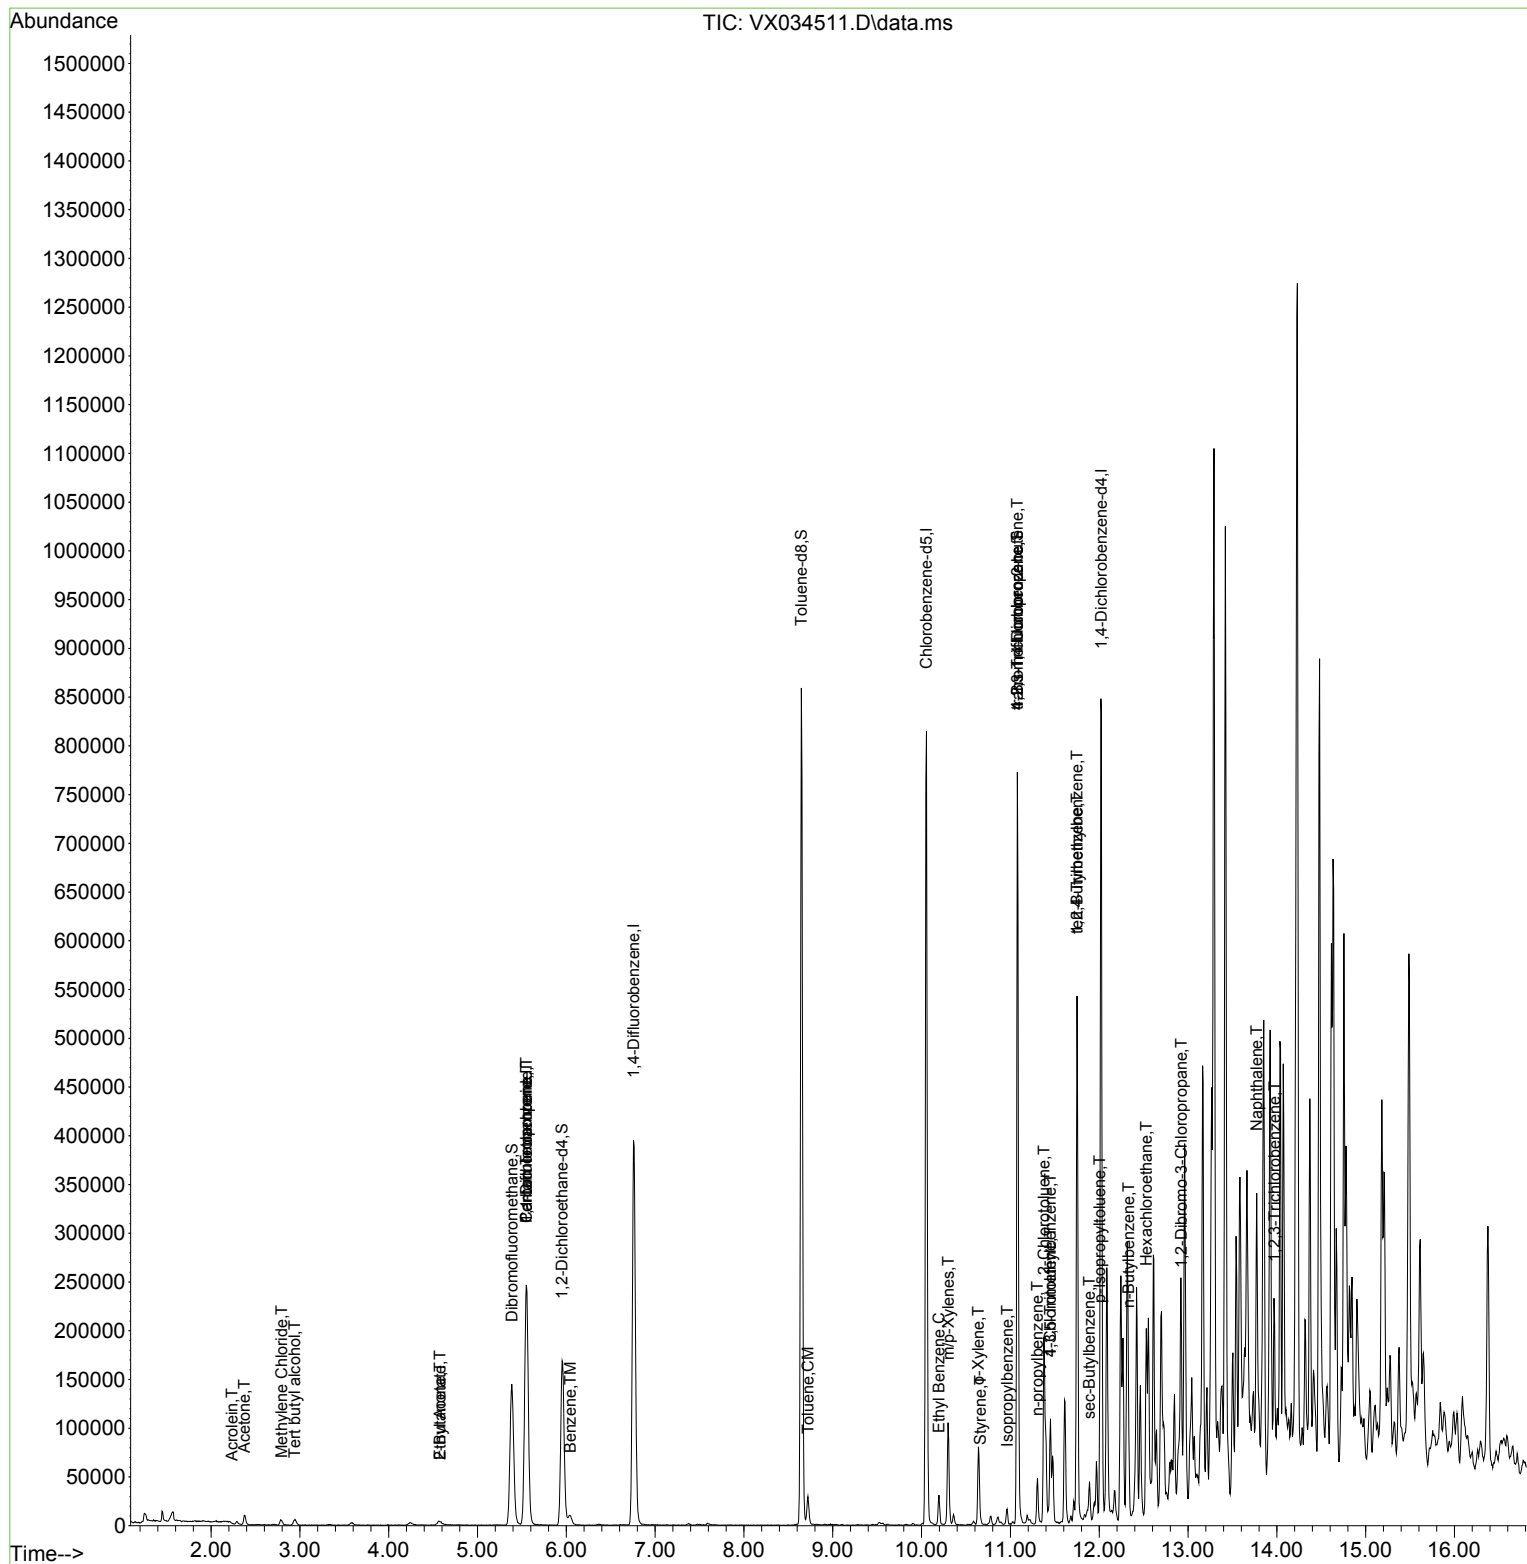




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX034511.D
Acq: 15 Mar 2023 16:22




Instrument :
MSVOA_X
ClientSampleId :
BOOM-030923

Tgt Ion:168 Resp: 238383
Ion Ratio Lower Upper
168 100
99 56.4 45.7 68.5

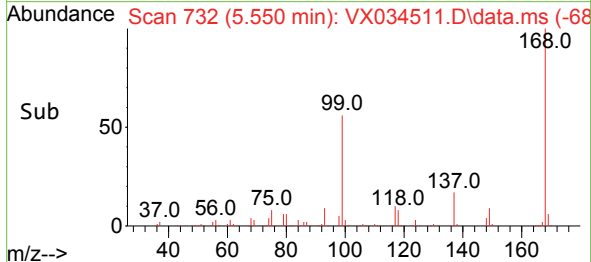

#3
Chloromethane
Concen: Below Cal
RT: 1.294 min Scan# 34
Delta R.T. -0.007 min
Lab File: VX034511.D
Acq: 15 Mar 2023 16:22

Tgt Ion: 50 Resp: 693
Ion Ratio Lower Upper
50 100
52 33.8 25.9 38.9





#11

Tert butyl alcohol

Concen: 4.974 ug/l

RT: 2.940 min Scan# 306

Delta R.T. -0.012 min

Lab File: VX034511.D

Acq: 15 Mar 2023 16:22

Instrument :

MSVOA_X

ClientSampleId :





BOOM-030923

Tgt Ion: 59 Resp: 3592

Ion Ratio Lower Upper

59 100

57 0.0 8.1 12.1#

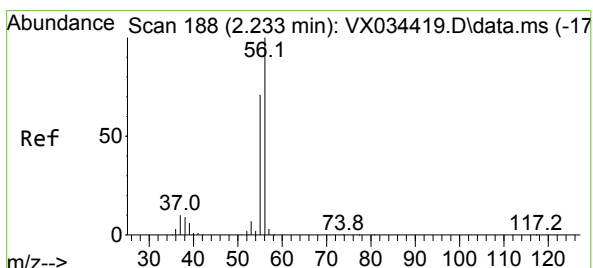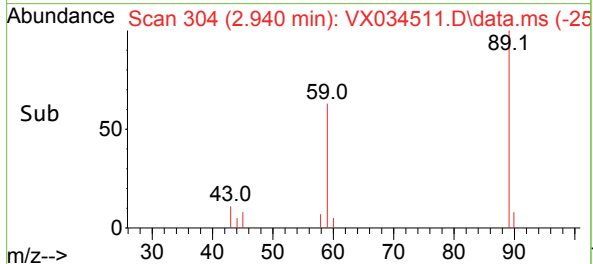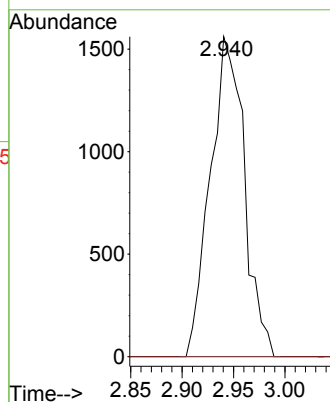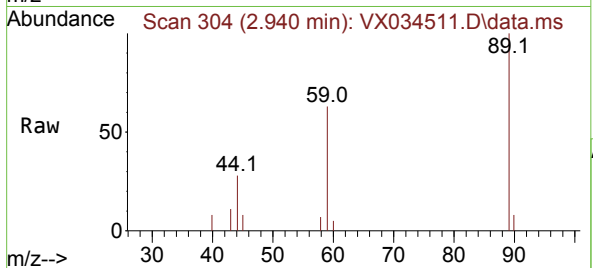

#13

Acrolein

Concen: 0.277 ug/l

RT: 2.233 min Scan# 188

Delta R.T. 0.000 min

Lab File: VX034511.D




Acq: 15 Mar 2023 16:22


Tgt Ion: 56 Resp: 158

Ion Ratio Lower Upper

56 100

55 177.2 56.6 85.0#


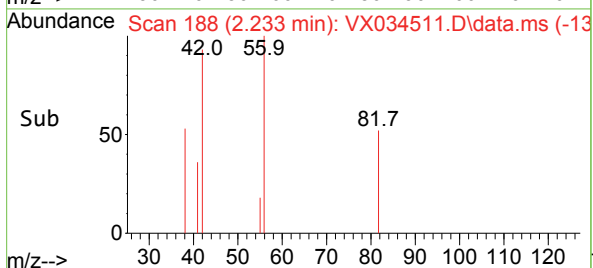

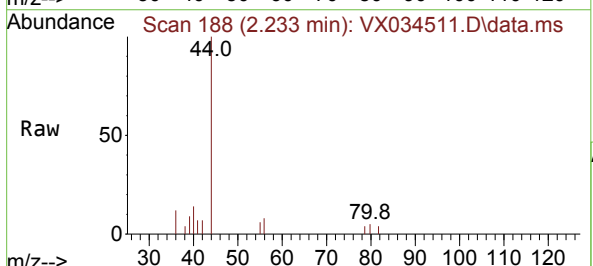




#16
Acetone
Concen: 6.408 ug/l
RT: 2.373 min Scan# 211
Delta R.T. 0.000 min
Lab File: VX034511.D
Acq: 15 Mar 2023 16:22




Instrument :
MSVOA_X
ClientSampleId :
BOOM-030923


Tgt Ion: 43 Resp: 10468
Ion Ratio Lower Upper
43 100
58 29.8 24.7 37.1

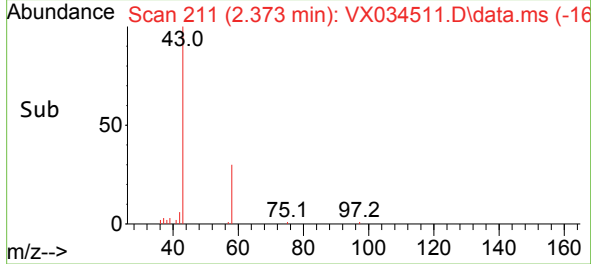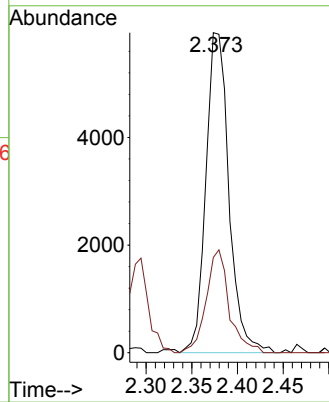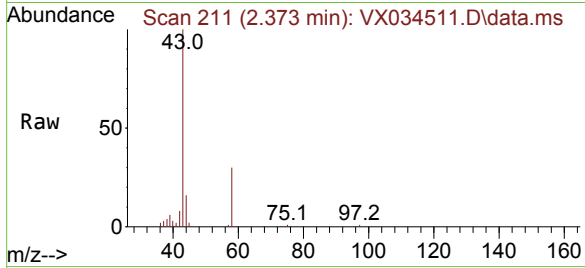

#20
Methylene Chloride
Concen: 0.880 ug/l
RT: 2.794 min Scan# 280
Delta R.T. 0.012 min
Lab File: VX034511.D
Acq: 15 Mar 2023 16:22

Tgt Ion: 84 Resp: 2790
Ion Ratio Lower Upper
84 100
49 89.2 103.8 155.8#
51 28.3 31.8 47.8#
86 45.3 51.4 77.2#


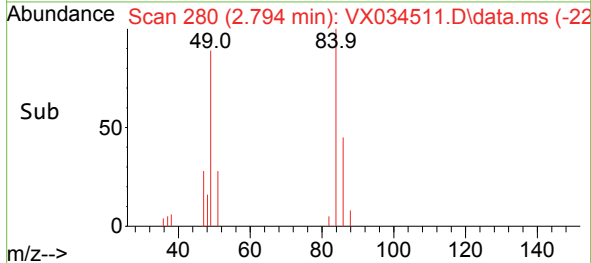
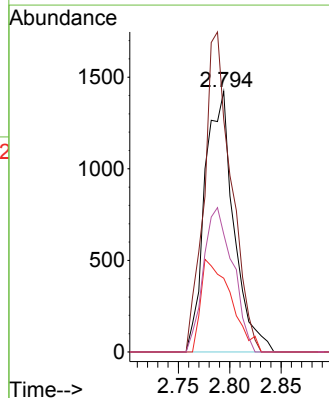
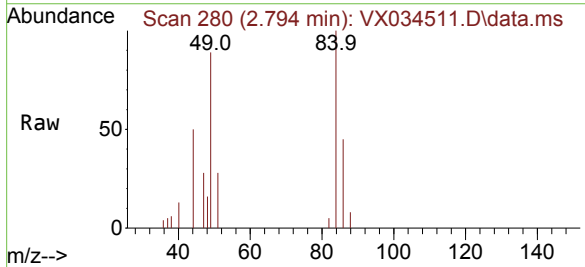




#25
2-Butanone
Concen: 1.606 ug/l
RT: 4.574 min Scan# 51
Delta R.T. 0.031 min
Lab File: VX034511.D
Acq: 15 Mar 2023 16:22




Instrument :
MSVOA_X
ClientSampleId :
BOOM-030923


Tgt Ion: 43 Resp: 3754
Ion Ratio Lower Upper
43 100
72 32.4 19.3 28.9#

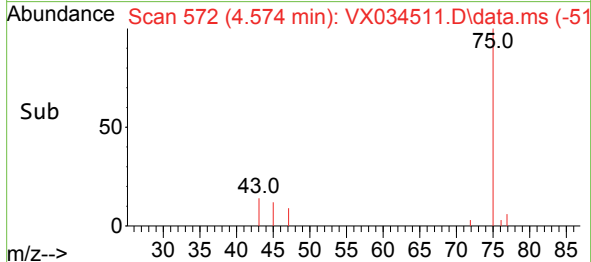

#33
1,2-Dichloroethane-d4
Concen: 46.424 ug/l
RT: 5.952 min Scan# 798
Delta R.T. 0.006 min
Lab File: VX034511.D
Acq: 15 Mar 2023 16:22

Tgt Ion: 65 Resp: 160998
Ion Ratio Lower Upper
65 100
67 52.5 0.0 104.0


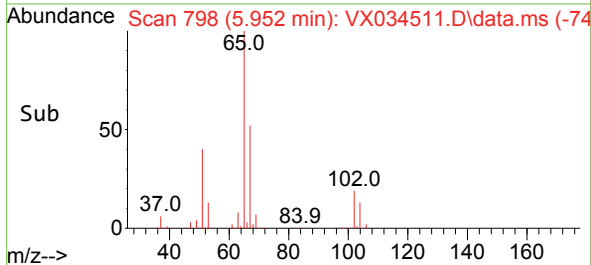






#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX034511.D
Acq: 15 Mar 2023 16:22




Instrument :
MSVOA_X
ClientSampleId :
BOOM-030923


Tgt Ion:114 Resp: 404829
Ion Ratio Lower Upper
114 100
63 20.8 0.0 42.2
88 16.8 0.0 33.2

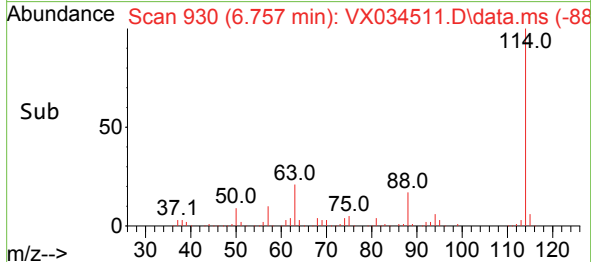

#35
Dibromofluoromethane
Concen: 46.623 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.006 min
Lab File: VX034511.D
Acq: 15 Mar 2023 16:22

Tgt Ion:113 Resp: 124617
Ion Ratio Lower Upper
113 100
111 105.2 83.7 125.5
192 19.4 15.4 23.2




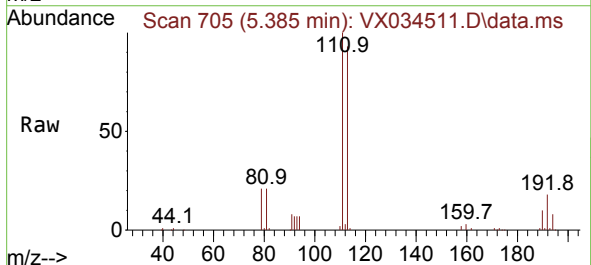




#36
1,1-Dichloropropene
Concen: 4.652 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.134 min
Lab File: VX034511.D
Acq: 15 Mar 2023 16:22




Instrument :
MSVOA_X
ClientSampleId :
BOOM-030923


Tgt Ion: 75 Resp: 19097
Ion Ratio Lower Upper
75 100
110 8.5 17.5 52.5#
77 0.0 24.3 36.5#

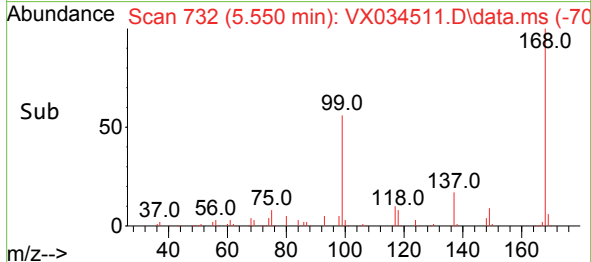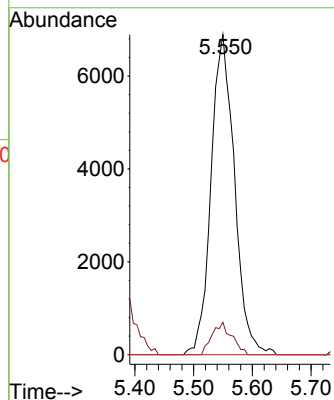

#37
Ethyl Acetate
Concen: 0.837 ug/l
RT: 4.574 min Scan# 572
Delta R.T. -0.128 min
Lab File: VX034511.D
Acq: 15 Mar 2023 16:22

Tgt Ion: 43 Resp: 3754
Ion Ratio Lower Upper
43 100
61 0.5 10.2 15.4#
70 0.0 8.2 12.4#


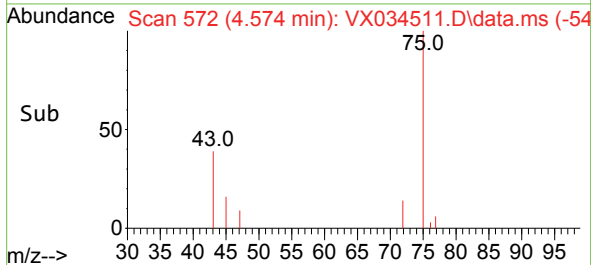
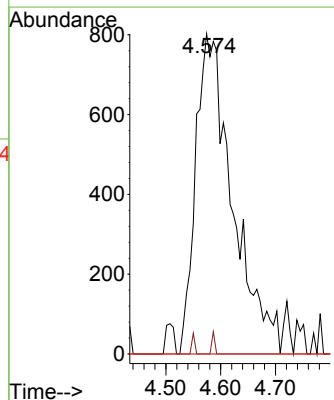



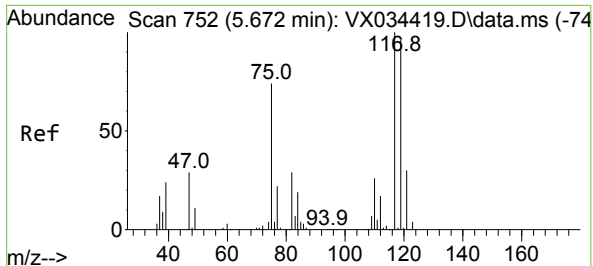

#38
Carbon Tetrachloride
Concen: 5.754 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.122 min
Lab File: VX034511.D
Acq: 15 Mar 2023 16:22




Instrument :
MSVOA_X
ClientSampleId :
BOOM-030923


Tgt Ion:117 Resp: 23498
Ion Ratio Lower Upper
117 100
119 4.1 76.6 114.8#
121 0.0 23.8 35.6#

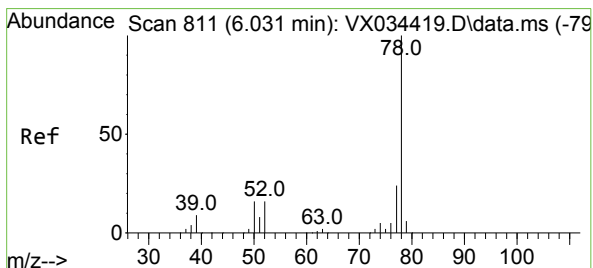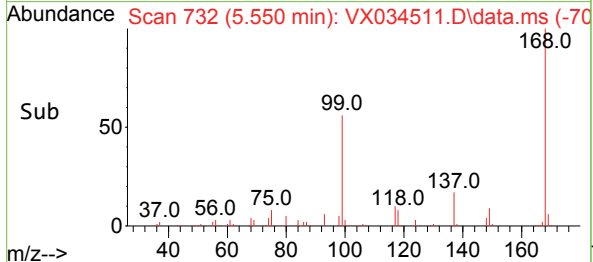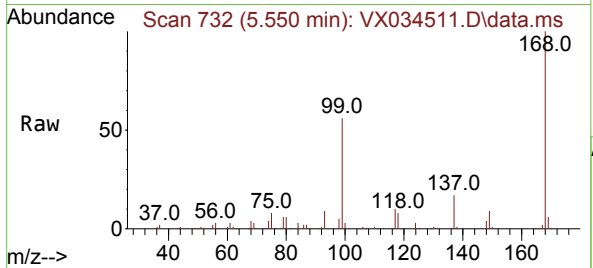

#40
Benzene
Concen: 0.946 ug/l
RT: 6.044 min Scan# 813
Delta R.T. 0.012 min
Lab File: VX034511.D
Acq: 15 Mar 2023 16:22

Tgt Ion: 78 Resp: 11358
Ion Ratio Lower Upper
78 100
77 21.7 19.0 28.4


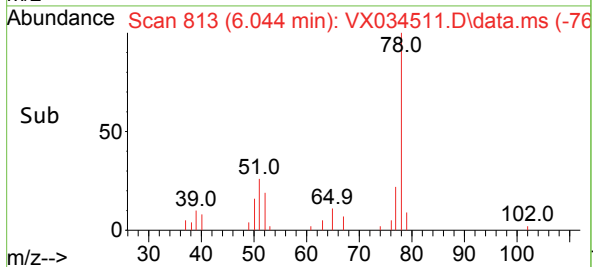

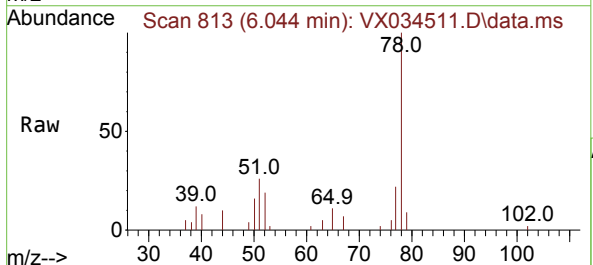




#50
Toluene-d8
Concen: 49.226 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX034511.D
Acq: 15 Mar 2023 16:22




Instrument :
MSVOA_X
ClientSampleId :
BOOM-030923


Tgt Ion: 98 Resp: 491178
Ion Ratio Lower Upper
98 100
100 65.9 52.5 78.7

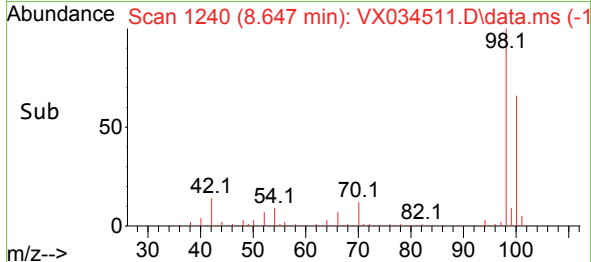

#52
Toluene
Concen: 1.438 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. 0.006 min
Lab File: VX034511.D
Acq: 15 Mar 2023 16:22

Tgt Ion: 92 Resp: 10692
Ion Ratio Lower Upper
92 100
91 171.8 136.8 205.2




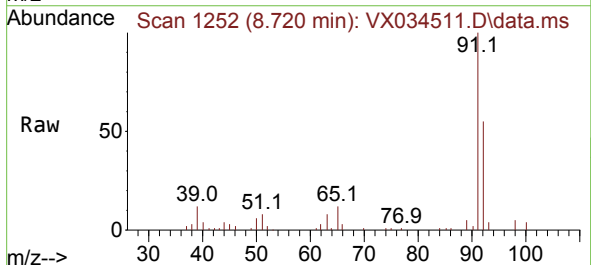




#62
4-Bromofluorobenzene
Concen: 47.904 ug/l
RT: 11.079 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX034511.D
Acq: 15 Mar 2023 16:22




Instrument :
MSVOA_X
ClientSampleId :
BOOM-030923


Tgt Ion: 95 Resp: 193071
Ion Ratio Lower Upper
95 100
174 76.2 0.0 147.4
176 73.3 0.0 140.6

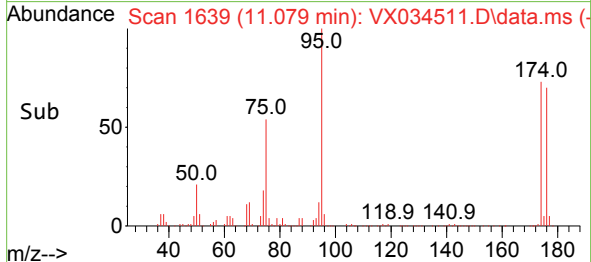

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX034511.D
Acq: 15 Mar 2023 16:22

Tgt Ion: 117 Resp: 360881
Ion Ratio Lower Upper
117 100
82 56.4 45.0 67.4
119 32.3 26.0 39.0


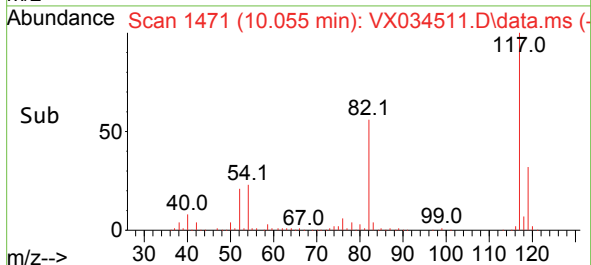
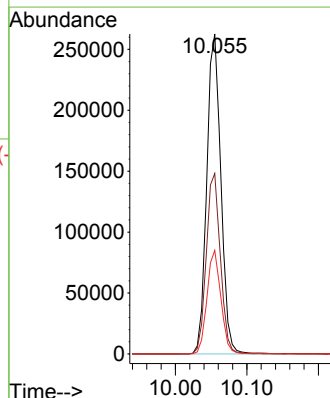
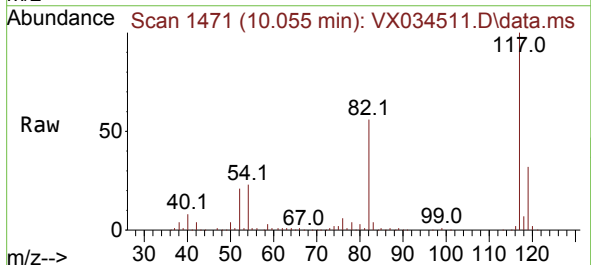




#67
Ethyl Benzene
Concen: 1.197 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX034511.D
Acq: 15 Mar 2023 16:22




Instrument :
MSVOA_X
ClientSampleId :
BOOM-030923


Tgt Ion: 91 Resp: 16963
Ion Ratio Lower Upper
91 100
106 26.7 25.6 38.4

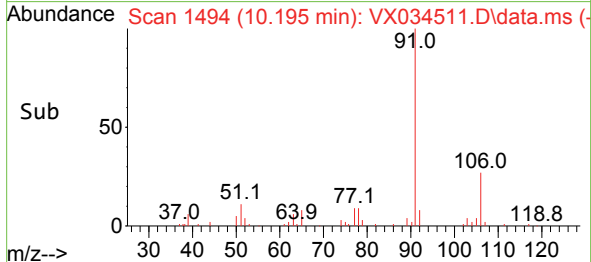

#68
m/p-Xylenes
Concen: 4.305 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. 0.000 min
Lab File: VX034511.D
Acq: 15 Mar 2023 16:22

Tgt Ion: 106 Resp: 23441
Ion Ratio Lower Upper
106 100
91 209.9 164.0 246.0

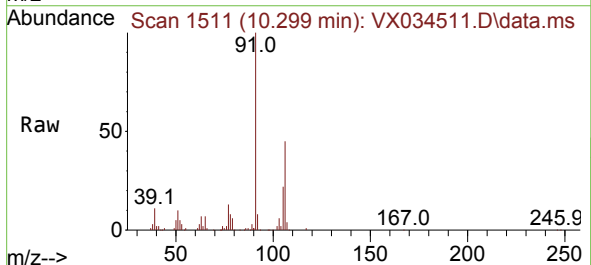

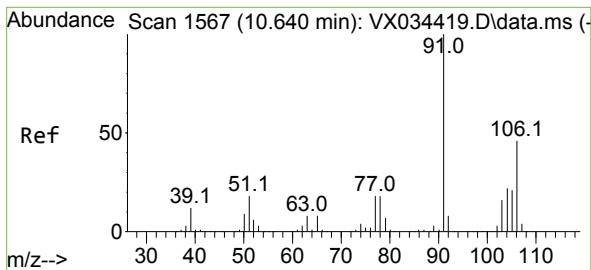

#69

o-Xylene

Concen: 3.234 ug/l

RT: 10.640 min Scan# 1567

Delta R.T. 0.000 min

Lab File: VX034511.D

Acq: 15 Mar 2023 16:22

Instrument :

MSVOA_X

ClientSampleId :





BOOM-030923

Tgt Ion:106 Resp: 17670

Ion Ratio Lower Upper

106 100

91 211.5 108.5 325.3

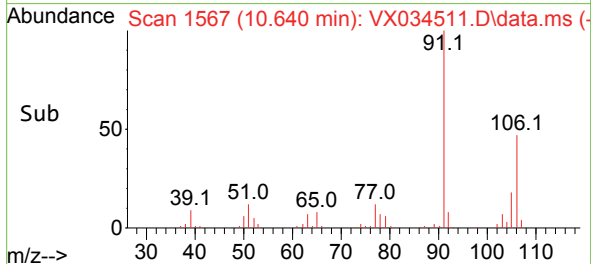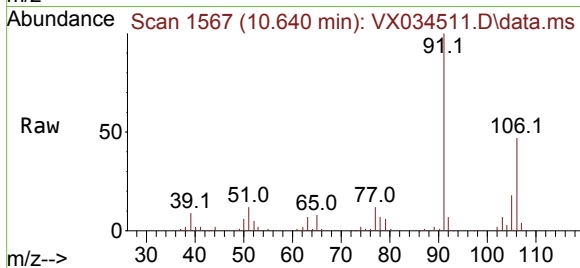

#70

Styrene

Concen: 0.306 ug/l

RT: 10.659 min Scan# 1570

Delta R.T. 0.006 min

Lab File: VX034511.D

Acq: 15 Mar 2023 16:22




Tgt Ion:104 Resp: 2699


Ion Ratio Lower Upper

104 100

78 124.3 43.4 65.2#

103 120.4 44.2 66.2#


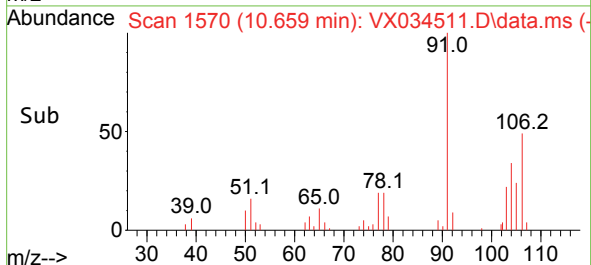
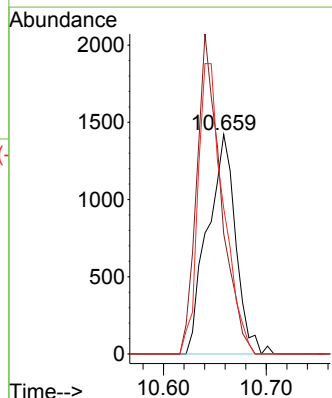
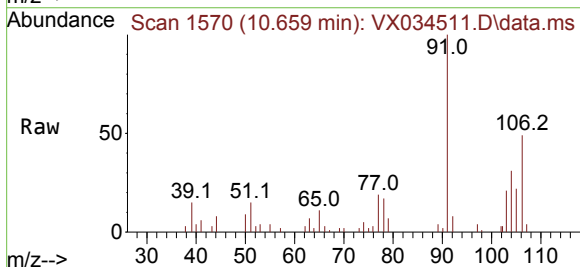




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX034511.D
Acq: 15 Mar 2023 16:22




Instrument :
MSVOA_X
ClientSampleId :
BOOM-030923


Tgt Ion:152 Resp: 167785
Ion Ratio Lower Upper
152 100
115 60.4 45.0 135.0
150 157.8 0.0 352.4

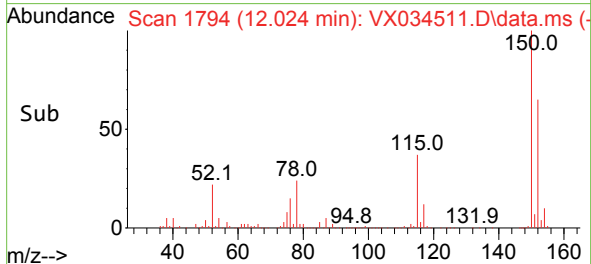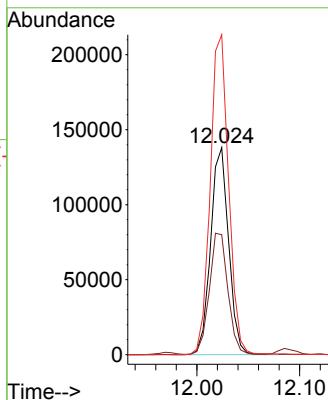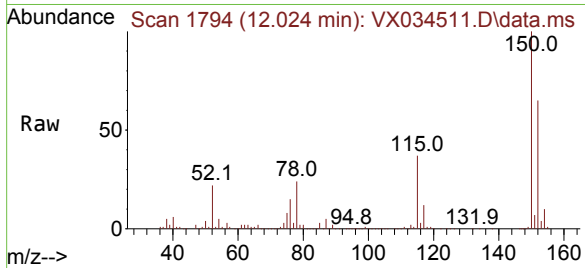

#73
Isopropylbenzene
Concen: 0.634 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. 0.000 min
Lab File: VX034511.D
Acq: 15 Mar 2023 16:22

Tgt Ion:105 Resp: 8219
Ion Ratio Lower Upper
105 100
120 22.7 13.3 39.9

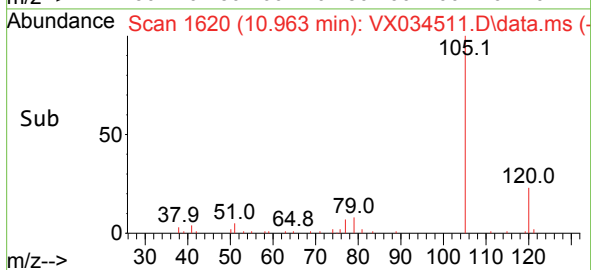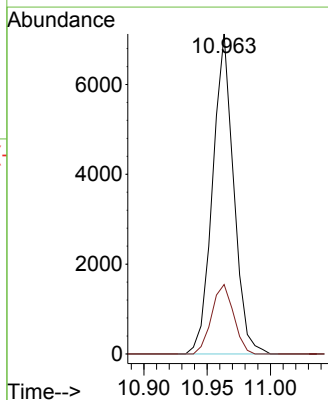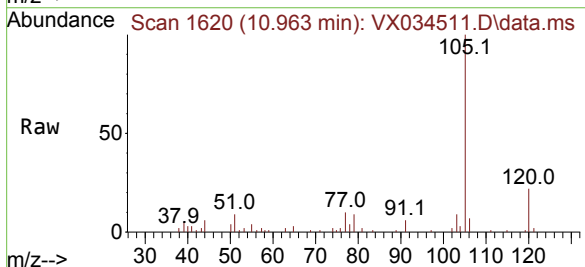



#76

1,2,3-Trichloropropane

Concen: 26.434 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.158 min

Lab File: VX034511.D

Acq: 15 Mar 2023 16:22

Instrument :

MSVOA_X

ClientSampleId :





BOOM-030923

Tgt Ion: 75 Resp: 101837

Ion Ratio Lower Upper

75 100

77 1.4 21.6 64.8#

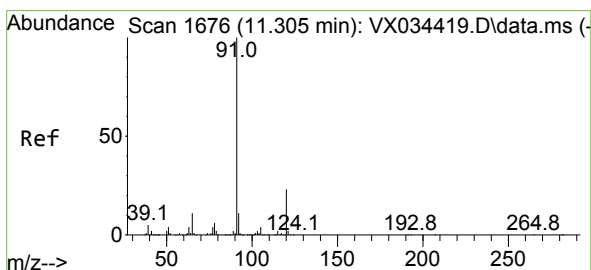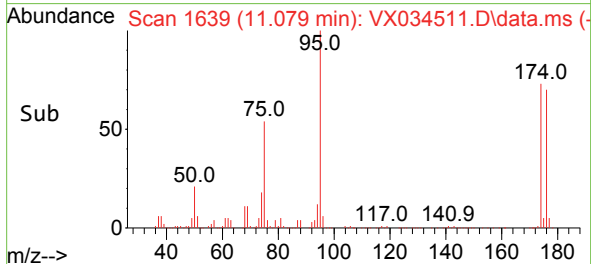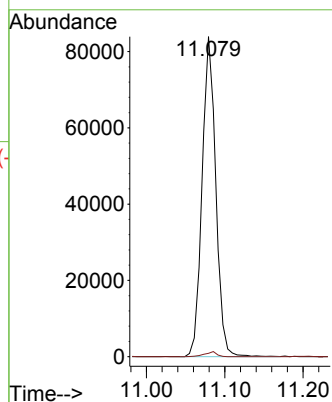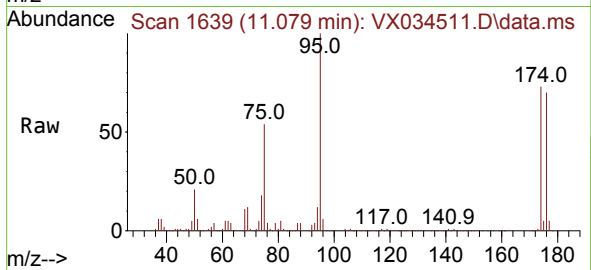

#78

n-propylbenzene

Concen: 1.892 ug/l

RT: 11.305 min Scan# 1676

Delta R.T. 0.000 min

Lab File: VX034511.D




Acq: 15 Mar 2023 16:22


Tgt Ion: 91 Resp: 28336

Ion Ratio Lower Upper

91 100

120 21.9 11.5 34.5





#79

2-Chlorotoluene

Concen: 1.715 ug/l

RT: 11.378 min Scan# 1

Delta R.T. 0.012 min

Lab File: VX034511.D

Acq: 15 Mar 2023 16:22

Instrument :

MSVOA_X

ClientSampleId :





BOOM-030923

Tgt Ion: 91 Resp: 15864

Ion Ratio Lower Upper

91 100

126 0.0 16.3 48.9#

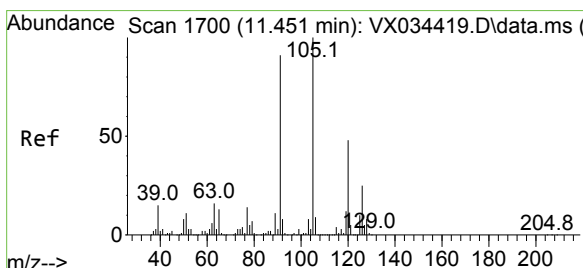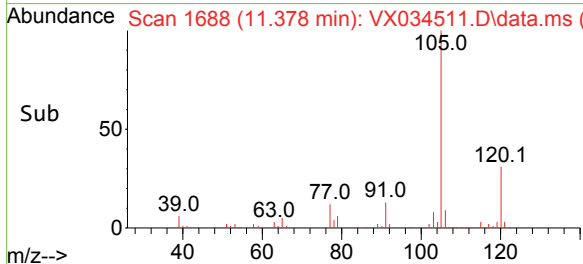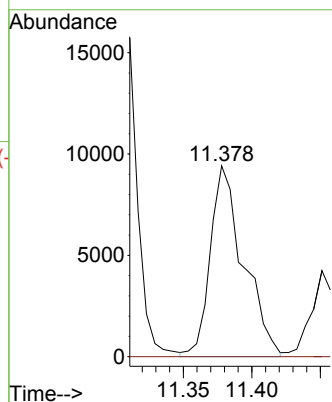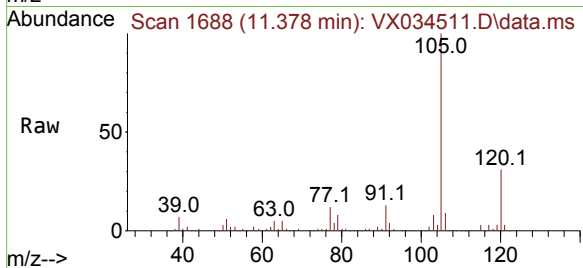

#80

1,3,5-Trimethylbenzene

Concen: 3.873 ug/l

RT: 11.451 min Scan# 1700

Delta R.T. 0.000 min

Lab File: VX034511.D




Acq: 15 Mar 2023 16:22


Tgt Ion: 105 Resp: 42128

Ion Ratio Lower Upper

105 100

120 48.9 23.7 71.1


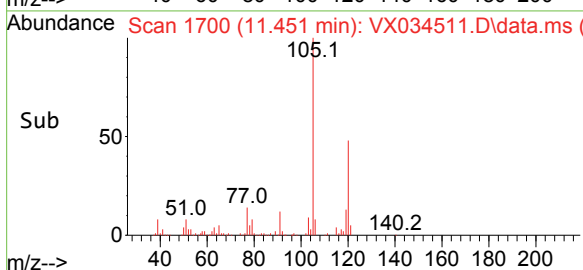

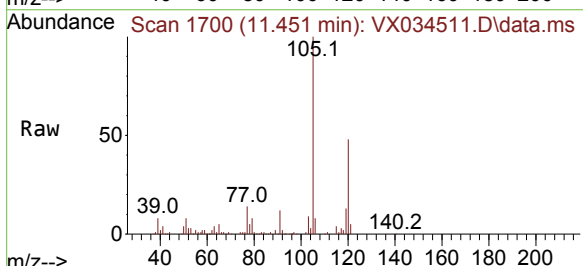




#81
trans-1,4-Dichloro-2-butene
Concen: 71.511 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX034511.D
Acq: 15 Mar 2023 16:22




Instrument :
MSVOA_X
ClientSampleId :
BOOM-030923


Tgt Ion: 75 Resp: 101837
Ion Ratio Lower Upper
75 100
53 0.2 82.6 124.0#
89 0.1 36.9 55.3#

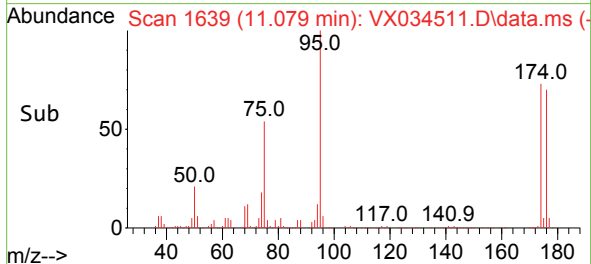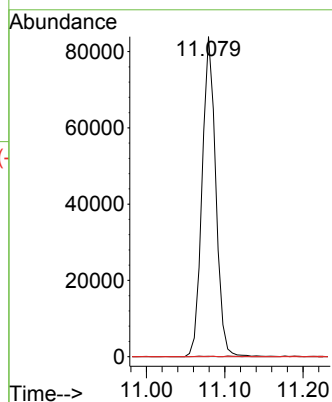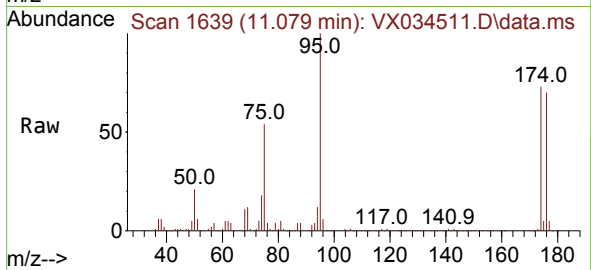

#82
4-Chlorotoluene
Concen: 0.489 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. 0.000 min
Lab File: VX034511.D
Acq: 15 Mar 2023 16:22

Tgt Ion: 91 Resp: 5212
Ion Ratio Lower Upper
91 100
126 0.0 14.2 42.6#

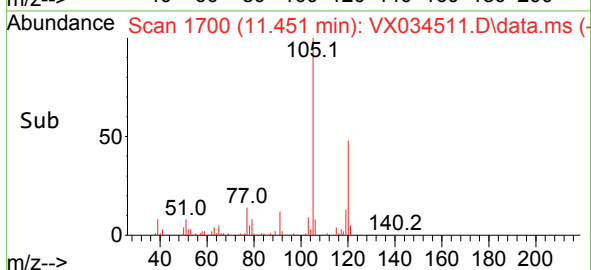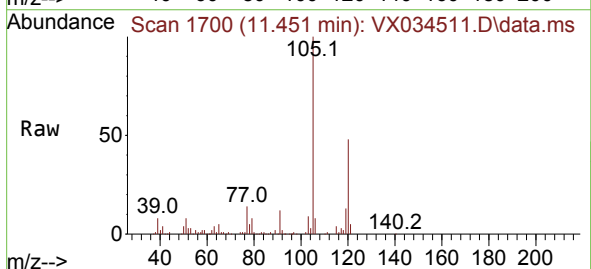



#83

tert-Butylbenzene

Concen: 2.324 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. 0.037 min

Lab File: VX034511.D

Acq: 15 Mar 2023 16:22

Instrument :

MSVOA_X

ClientSampleId :

BOOM-030923





Tgt Ion:119 Resp: 25485

Ion Ratio Lower Upper

119 100

91 93.6 30.6 92.0#

134 0.0 11.8 35.4#

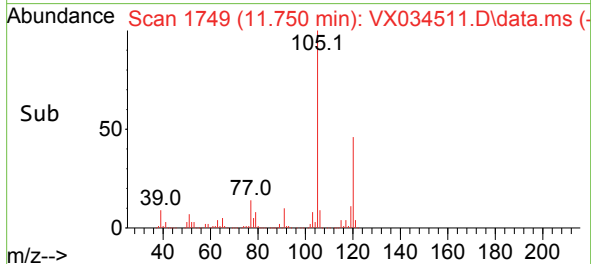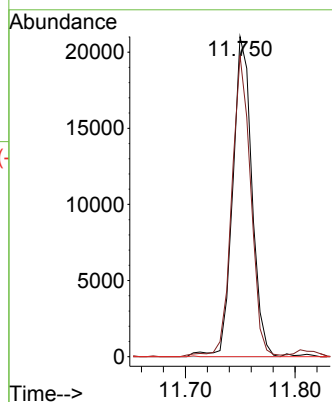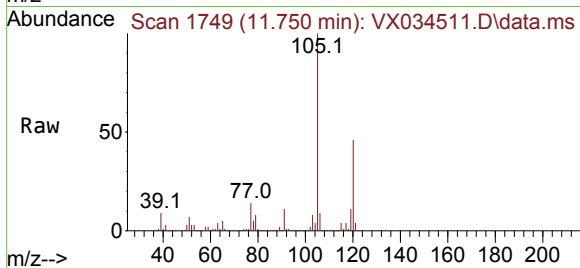

#84

1,2,4-Trimethylbenzene

Concen: 19.670 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. 0.000 min

Lab File: VX034511.D




Acq: 15 Mar 2023 16:22


Tgt Ion:105 Resp: 218657

Ion Ratio Lower Upper

105 100

120 45.8 22.4 67.0


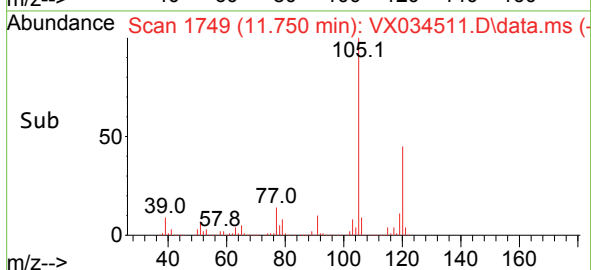

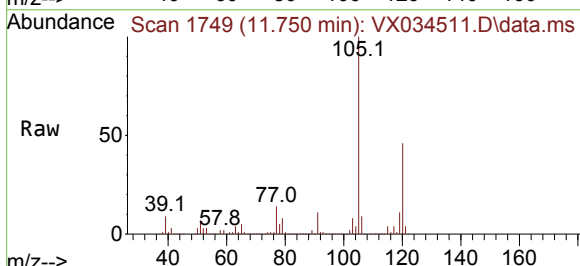




#85
 sec-Butylbenzene
 Concen: 1.110 ug/l
 RT: 11.890 min Scan# 1772
 Delta R.T. 0.000 min
 Lab File: VX034511.D
 Acq: 15 Mar 2023 16:22




Instrument :
 MSVOA_X
 ClientSampleId :
 BOOM-030923


Tgt Ion:105 Resp: 14878
 Ion Ratio Lower Upper
 105 100
 134 25.9 10.2 30.4

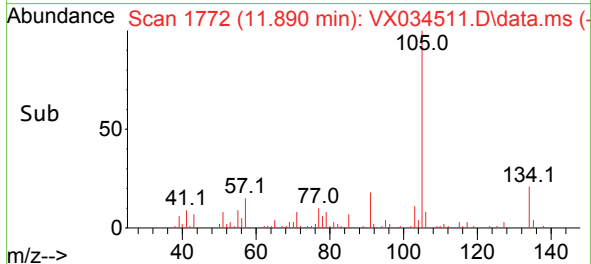

#86
 p-Isopropyltoluene
 Concen: 0.967 ug/l
 RT: 12.006 min Scan# 1791
 Delta R.T. 0.000 min
 Lab File: VX034511.D
 Acq: 15 Mar 2023 16:22

Tgt Ion:119 Resp: 10899
 Ion Ratio Lower Upper
 119 100
 134 30.1 13.2 39.5
 91 29.1 12.9 38.7


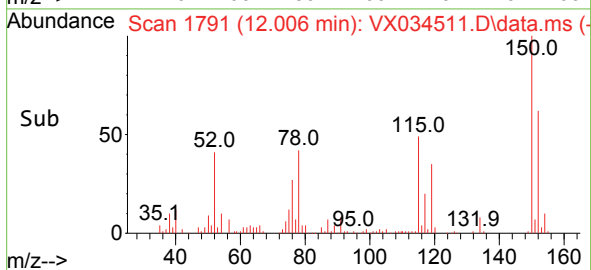






#89
n-Butylbenzene
Concen: 4.562 ug/l
RT: 12.329 min Scan# 1844
Delta R.T. 0.000 min
Lab File: VX034511.D
Acq: 15 Mar 2023 16:22




Instrument :
MSVOA_X
ClientSampleId :
BOOM-030923


Tgt Ion: 91 Resp: 45694
Ion Ratio Lower Upper
91 100
92 34.7 27.7 83.0
134 90.1 13.0 38.9#

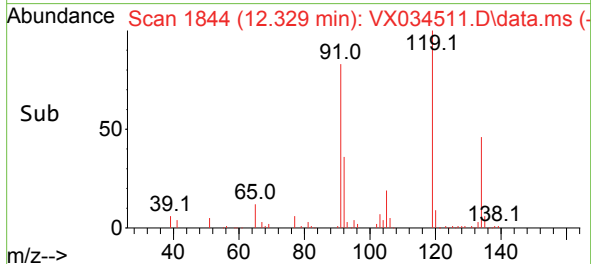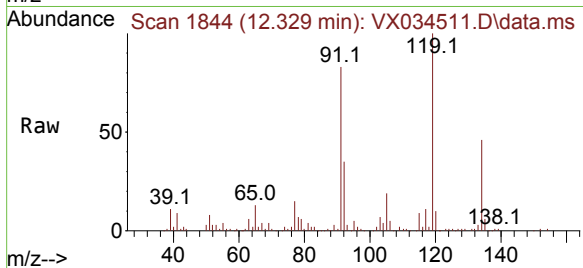

#90
Hexachloroethane
Concen: 3.655 ug/l
RT: 12.530 min Scan# 1877
Delta R.T. -0.006 min
Lab File: VX034511.D
Acq: 15 Mar 2023 16:22

Tgt Ion: 117 Resp: 7620
Ion Ratio Lower Upper
117 100
201 0.0 34.4 103.1#




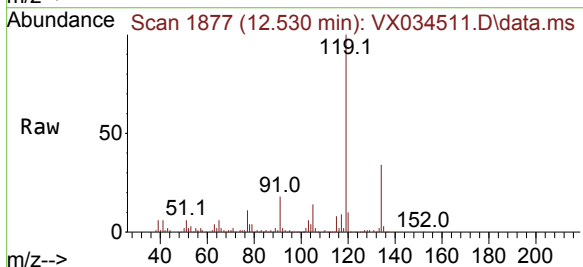




#92
1,2-Dibromo-3-Chloropropane
Concen: 0.770 ug/l
RT: 12.926 min Scan# 1942
Delta R.T. -0.012 min
Lab File: VX034511.D
Acq: 15 Mar 2023 16:22




Instrument :
MSVOA_X
ClientSampleId :
BOOM-030923


Tgt Ion: 75 Resp: 757
Ion Ratio Lower Upper
75 100
155 8.9 38.4 115.1#
157 0.0 49.9 149.7#

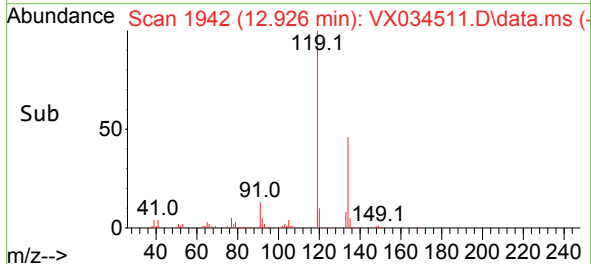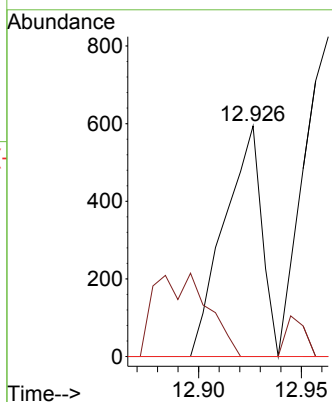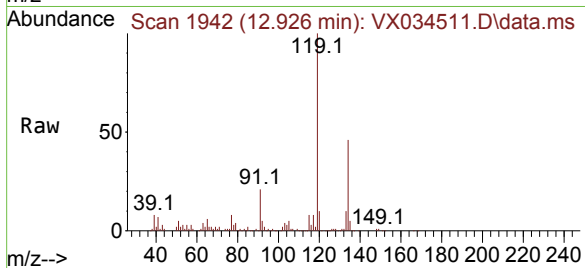

#95
Naphthalene
Concen: 12.230 ug/l
RT: 13.774 min Scan# 2081
Delta R.T. 0.000 min
Lab File: VX034511.D
Acq: 15 Mar 2023 16:22


Tgt Ion:128 Resp: 151085
Ion Ratio Lower Upper
128 100
127 13.5 10.2 15.4
129 12.3 8.6 13.0

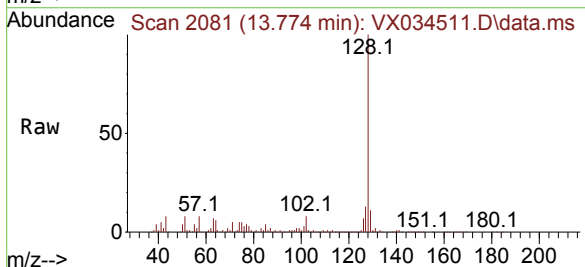



#96
 1,2,3-Trichlorobenzene
 Concen: 0.213 ug/l
 RT: 13.975 min Scan# 2114
 Delta R.T. 0.012 min
 Lab File: VX034511.D
 Acq: 15 Mar 2023 16:22

Instrument :
 MSVOA_X
 ClientSampleId :
 BOOM-030923

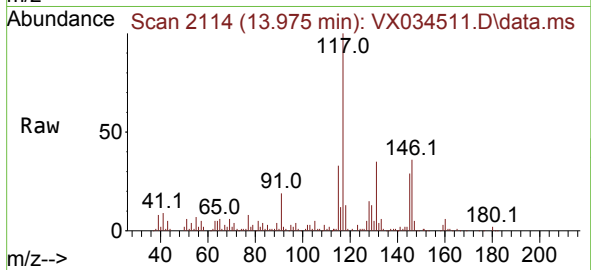

Tgt Ion:180 Resp: 766
 Ion Ratio Lower Upper
 180 100
 182 36.7 48.0 144.2#
 145 1895.0 17.7 53.1#

