

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031523\
Data File : VX034504.D
Acq On : 15 Mar 2023 13:33
Operator : JC/MD
Sample : VX0315MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0315MBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Title : SW846 8260

Signal : TIC: VX034504.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.563	70	78	80	rBV2	10252	17309	1.22%	0.234%
2	5.385	693	705	720	rBV	157092	464376	32.85%	6.275%
3	5.550	720	732	748	rVB2	262326	754161	53.35%	10.190%
4	5.952	786	798	815	rBV	182142	494484	34.98%	6.682%
5	6.757	920	930	945	rBV	433520	1022826	72.36%	13.821%
6	8.647	1233	1240	1257	rBV	914217	1413561	100.00%	19.100%
7	10.055	1465	1471	1484	rBV	865423	1204854	85.24%	16.280%
8	11.079	1634	1639	1650	rBV	731542	912870	64.58%	12.335%
9	12.024	1788	1794	1805	rBV	833183	1097232	77.62%	14.826%
10	13.725	2068	2073	2077	rBV2	15124	18989	1.34%	0.257%




Sum of corrected areas: 7400662

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031523\
Data File : VX034504.D
Acq On : 15 Mar 2023 13:33
Operator : JC/MD
Sample : VX0315MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0315MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

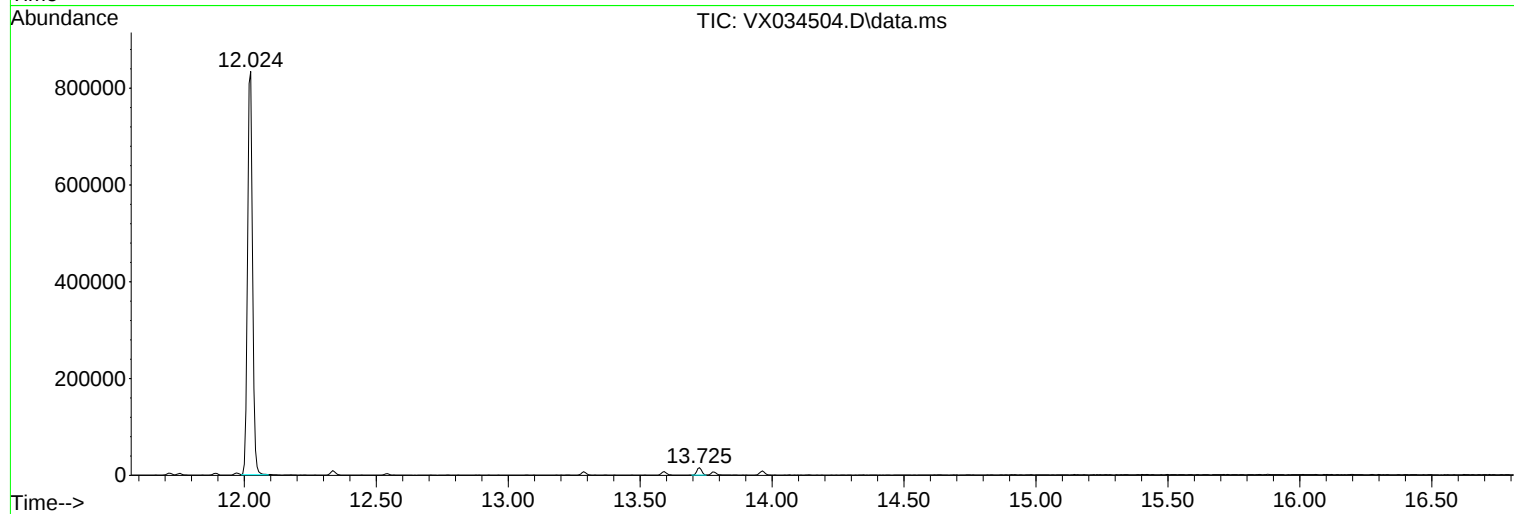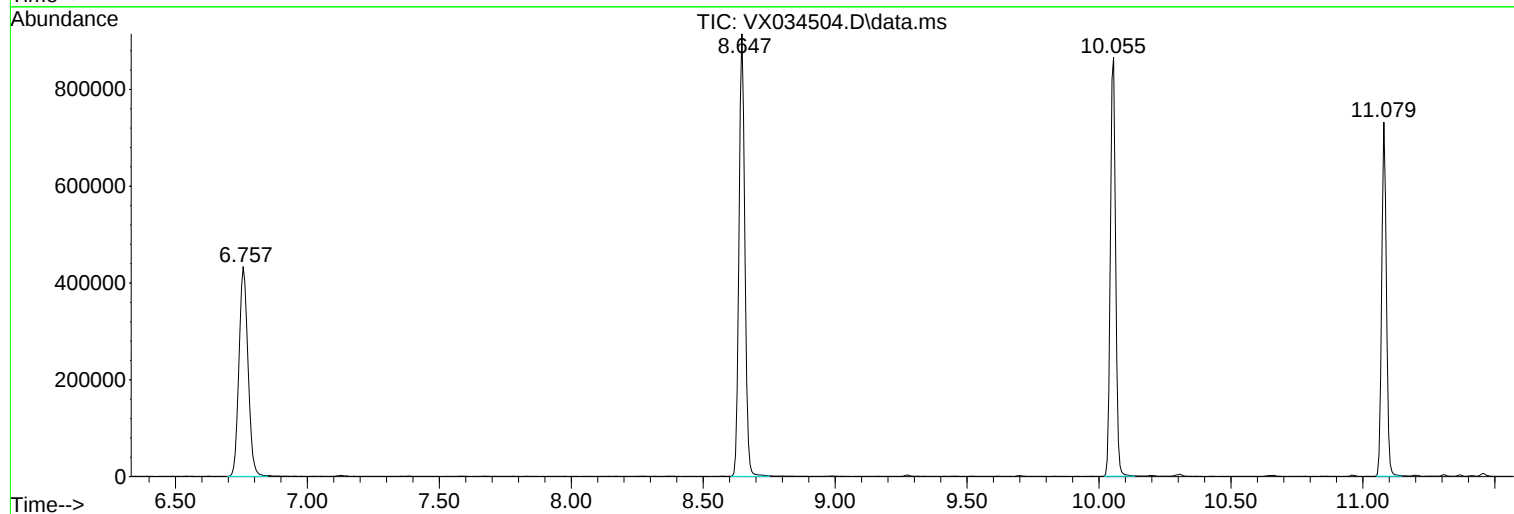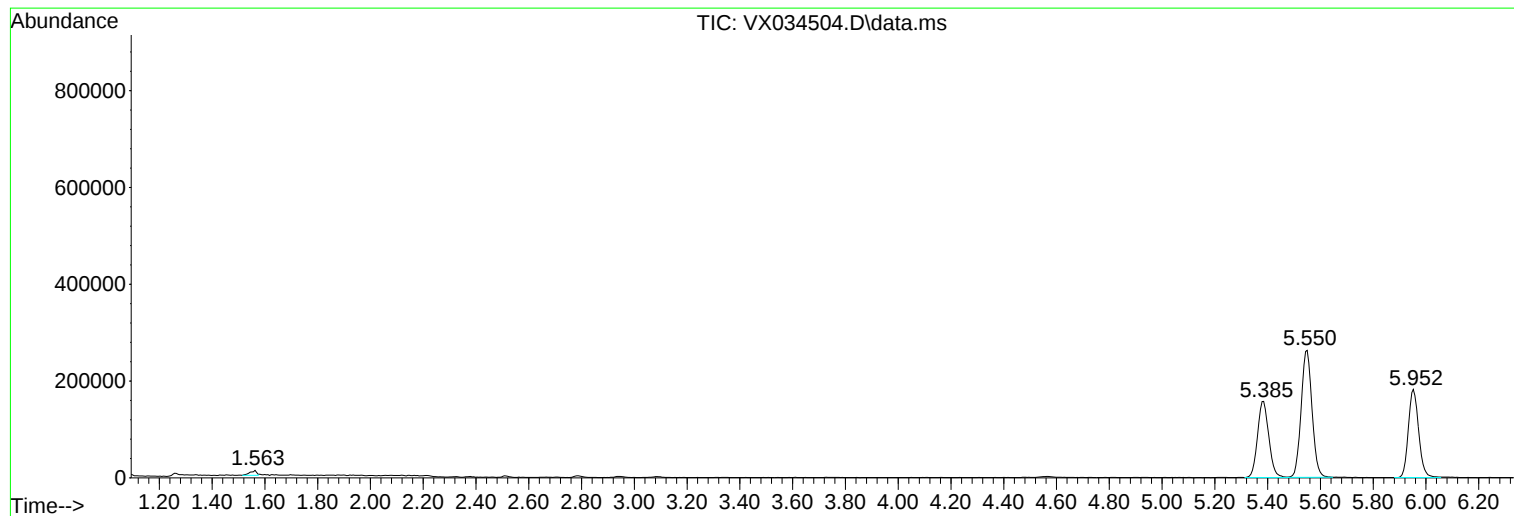

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031523\
Data File : VX034504.D
Acq On : 15 Mar 2023 13:33
Operator : JC/MD
Sample : VX0315MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0315MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031523\
Data File : VX034504.D
Acq On : 15 Mar 2023 13:33
Operator : JC/MD
Sample : VX0315MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0315MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc