

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031523\
Data File : VX034509.D
Acq On : 15 Mar 2023 15:35
Operator : JC/MD
Sample : 01922-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB-01-031423

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M

Title : SW846 8260

Signal : TIC: VX034509.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.245	22	26	32	rBV	14973	29761	2.27%	0.441%
2	1.562	71	78	82	rBV2	8171	13719	1.05%	0.203%
3	2.788	273	279	290	rVB2	7881	15064	1.15%	0.223%
4	5.385	694	705	721	rBV	143070	417137	31.79%	6.182%
5	5.550	721	732	748	rVB	245424	699559	53.32%	10.368%
6	5.952	787	798	812	rBV	165900	445768	33.97%	6.607%
7	6.763	920	931	947	rBV	396556	948470	72.29%	14.057%
8	8.647	1233	1240	1257	rBV	848298	1312081	100.00%	19.446%
9	10.055	1465	1471	1489	rBV	820159	1096092	83.54%	16.245%
10	11.079	1634	1639	1652	rBV	701799	871910	66.45%	12.922%
11	12.024	1788	1794	1803	rBV	689432	897800	68.43%	13.306%




Sum of corrected areas: 6747361

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031523\
Data File : VX034509.D
Acq On : 15 Mar 2023 15:35
Operator : JC/MD
Sample : 01922-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB-01-031423

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

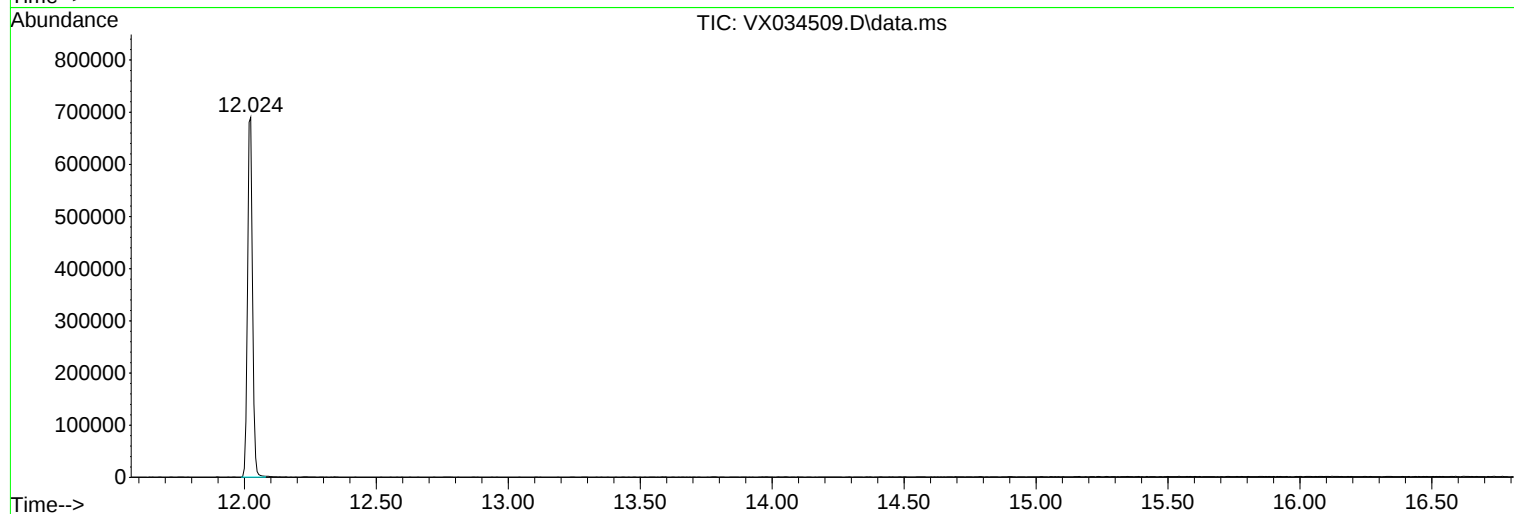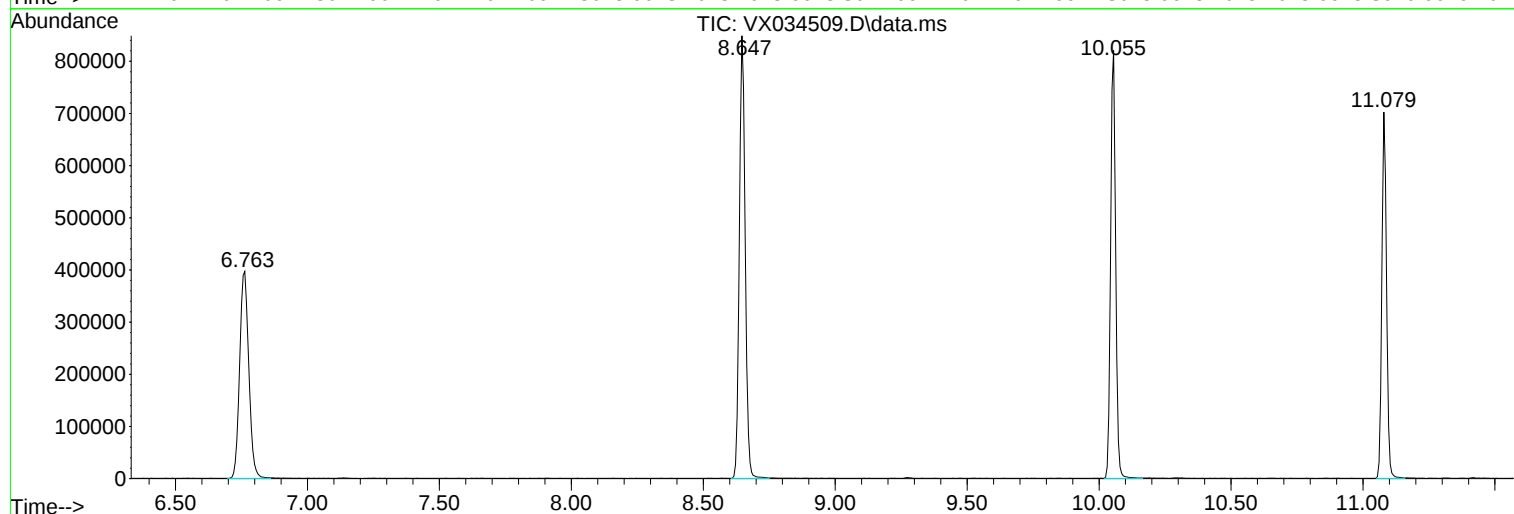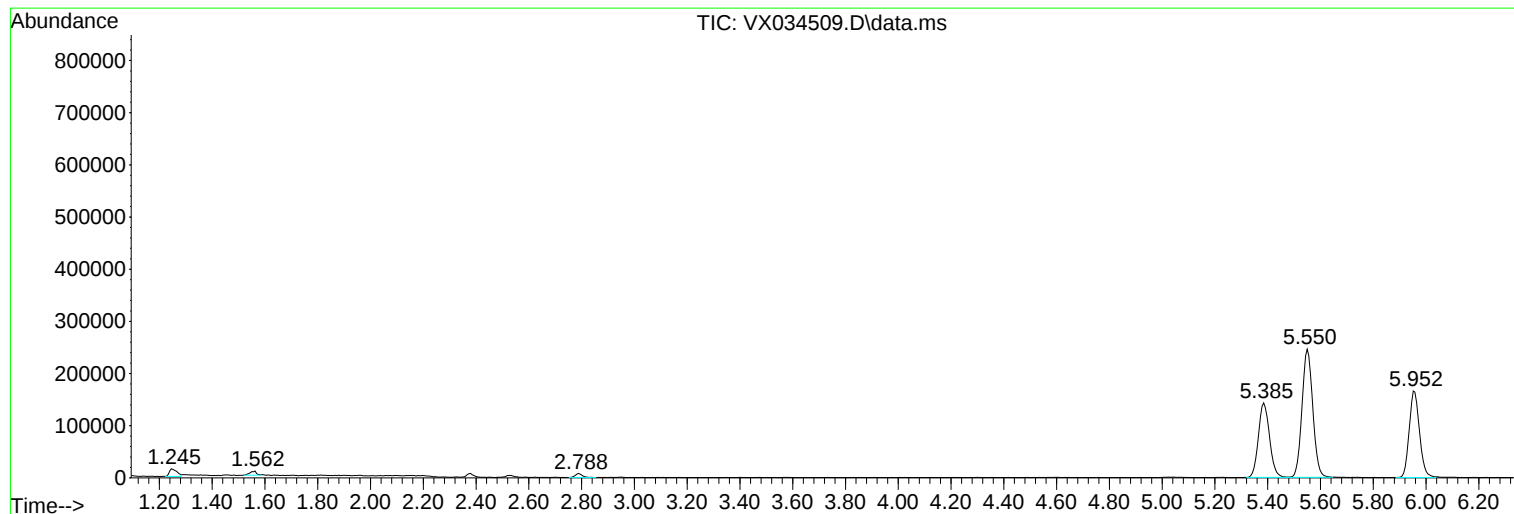

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031523\
Data File : VX034509.D
Acq On : 15 Mar 2023 15:35
Operator : JC/MD
Sample : 01922-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB-01-031423

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031523\
Data File : VX034509.D
Acq On : 15 Mar 2023 15:35
Operator : JC/MD
Sample : 01922-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB-01-031423

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------