

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031523\
 Data File : VX034515.D
 Acq On : 15 Mar 2023 17:56
 Operator : JC/MD
 Sample : 01909-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DS-01-031023-AM

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
 Title : SW846 8260

Signal : TIC: VX034515.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	34	rBV	16073	35988	2.59%	0.465%
2	5.385	693	705	720	rBV2	149973	439154	31.64%	5.673%
3	5.550	720	732	755	rVB	257744	735525	53.00%	9.502%
4	5.958	788	799	814	rBV	180079	478197	34.46%	6.178%
5	6.757	919	930	944	rBV	412760	994586	71.67%	12.849%
6	8.647	1233	1240	1253	rBV	895281	1387755	100.00%	17.929%
7	10.055	1465	1471	1483	rBV	860652	1180915	85.10%	15.256%
8	11.079	1634	1639	1650	rBV	786649	986698	71.10%	12.747%
9	12.024	1788	1794	1803	rBV	968222	1247579	89.90%	16.118%
10	12.226	1822	1827	1833	rBV2	10538	23691	1.71%	0.306%
11	14.231	2149	2156	2162	rVB4	13523	23637	1.70%	0.305%
12	14.481	2192	2197	2203	rBV2	11807	18431	1.33%	0.238%
13	14.615	2215	2219	2225	rBV5	17181	31192	2.25%	0.403%
14	14.908	2263	2267	2272	rBV4	9240	16261	1.17%	0.210%
15	15.182	2306	2312	2320	rBV2	25753	47468	3.42%	0.613%
16	15.377	2339	2344	2348	rBV6	11880	18156	1.31%	0.235%
17	15.481	2357	2361	2366	rVB4	15756	24350	1.75%	0.315%
18	15.615	2378	2383	2387	rVV5	18925	36202	2.61%	0.468%
19	15.652	2387	2389	2397	rVB7	7880	14673	1.06%	0.190%




Sum of corrected areas: 7740458

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031523\
Data File : VX034515.D
Acq On : 15 Mar 2023 17:56
Operator : JC/MD
Sample : 01909-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DS-01-031023-AM

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

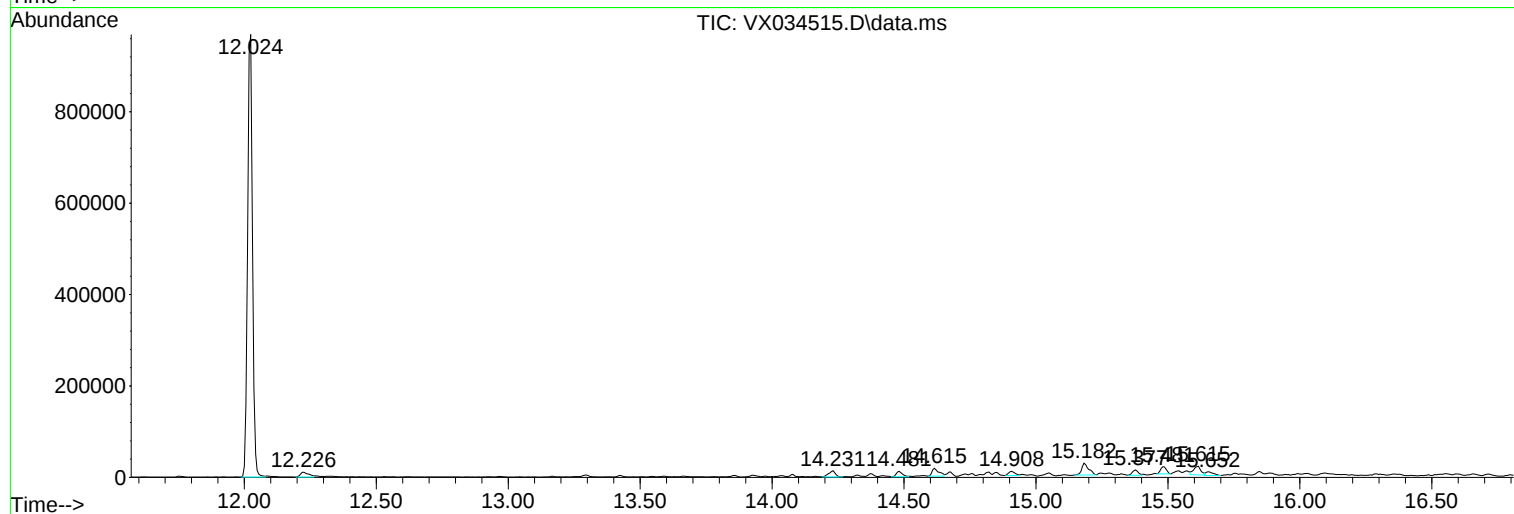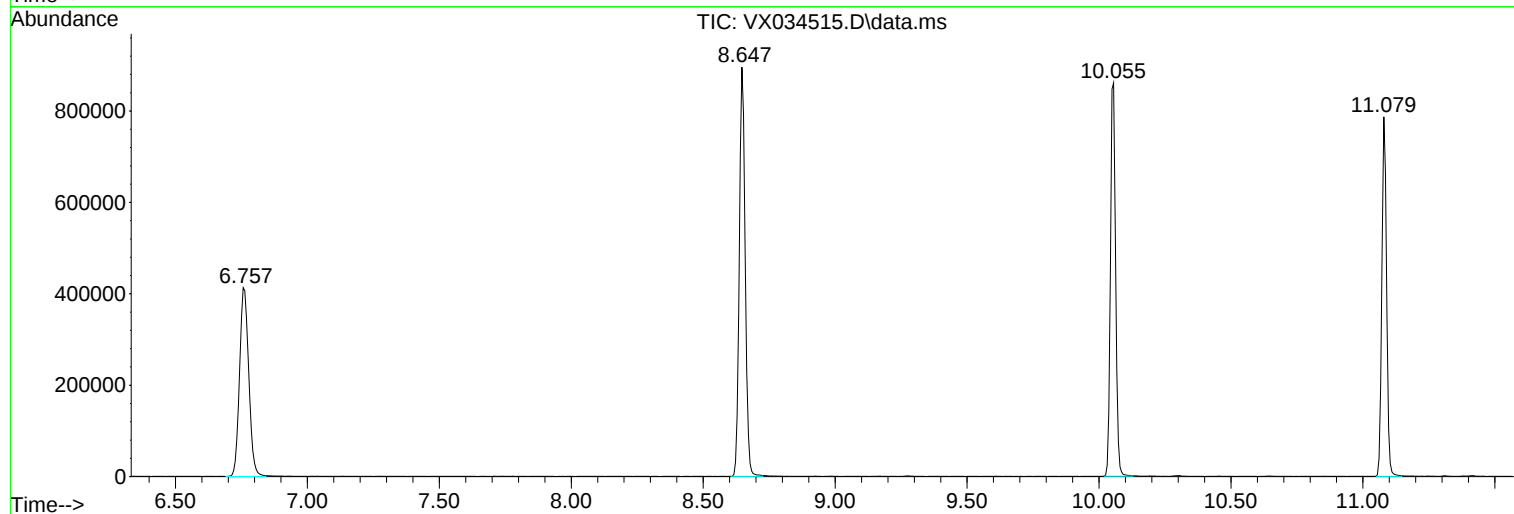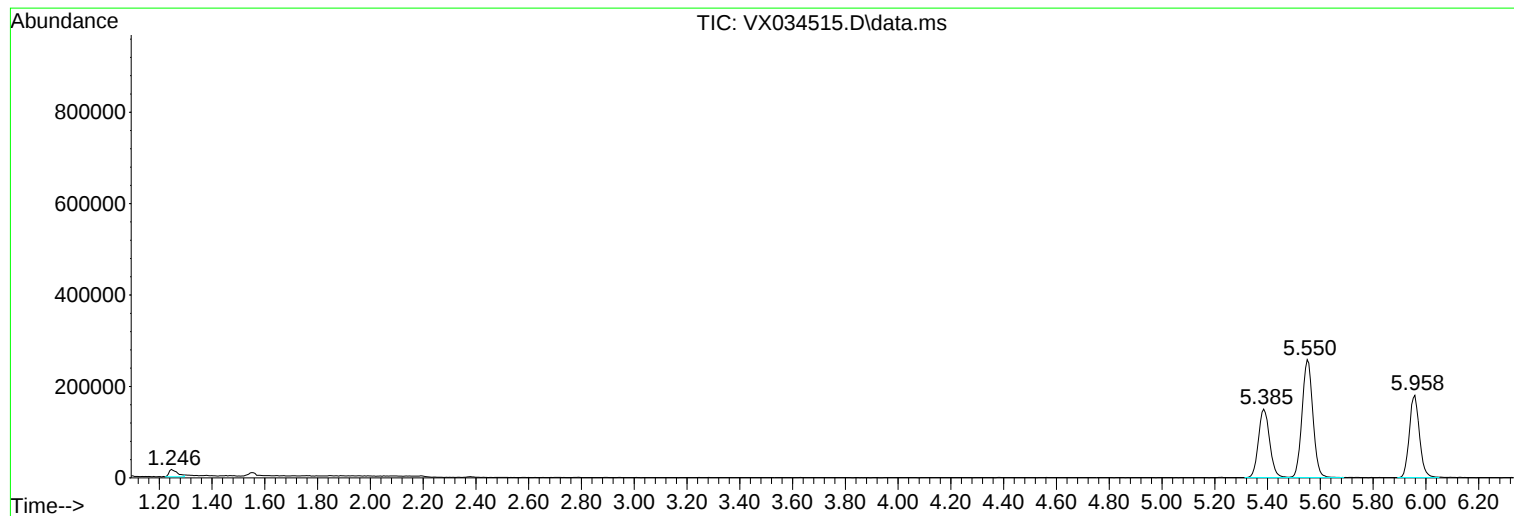

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031523\
Data File : VX034515.D
Acq On : 15 Mar 2023 17:56
Operator : JC/MD
Sample : 01909-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DS-01-031023-AM

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031523\
Data File : VX034515.D
Acq On : 15 Mar 2023 17:56
Operator : JC/MD
Sample : 01909-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DS-01-031023-AM

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------