

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031523\
Data File : VX034516.D
Acq On : 15 Mar 2023 18:19
Operator : JC/MD
Sample : 01909-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
UPS-01-031023-AM

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M

Title : SW846 8260

Signal : TIC: VX034516.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	33	rBV	15817	32629	2.32%	0.438%
2	1.557	69	77	80	rBV	8263	15306	1.09%	0.205%
3	5.385	694	705	721	rBV	152088	447441	31.75%	6.000%
4	5.550	721	732	750	rVB	261165	741732	52.63%	9.947%
5	5.952	787	798	811	rBV	176104	476435	33.80%	6.389%
6	6.763	920	931	948	rBV	420685	1010777	71.72%	13.555%
7	8.647	1233	1240	1256	rBV	909474	1409429	100.00%	18.901%
8	10.055	1465	1471	1485	rBV	900974	1209035	85.78%	16.214%
9	11.079	1634	1639	1657	rBV	805552	1006056	71.38%	13.492%
10	12.024	1788	1794	1803	rBV	870289	1108008	78.61%	14.859%




Sum of corrected areas: 7456848

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031523\
Data File : VX034516.D
Acq On : 15 Mar 2023 18:19
Operator : JC/MD
Sample : 01909-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
UPS-01-031023-AM

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

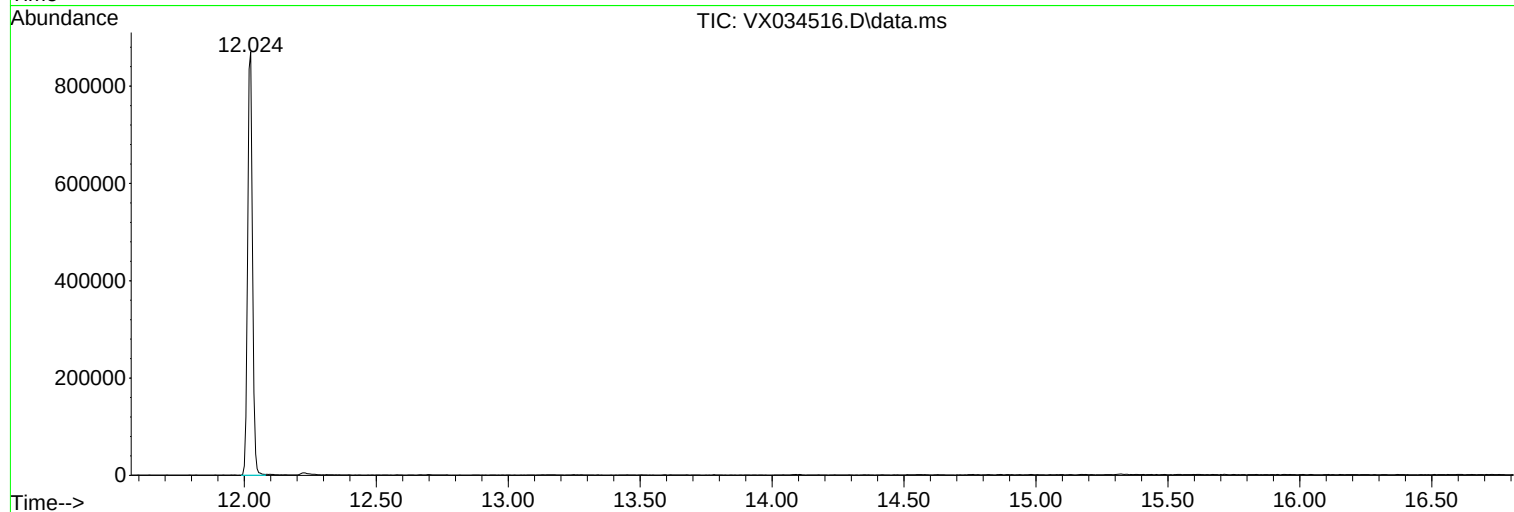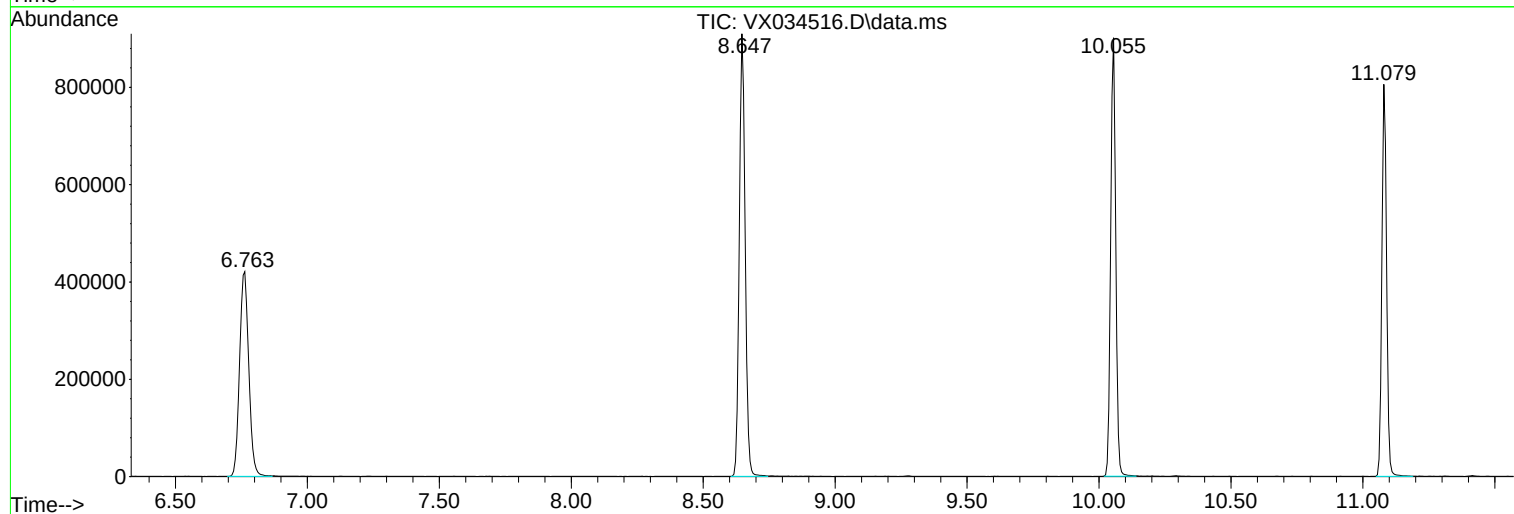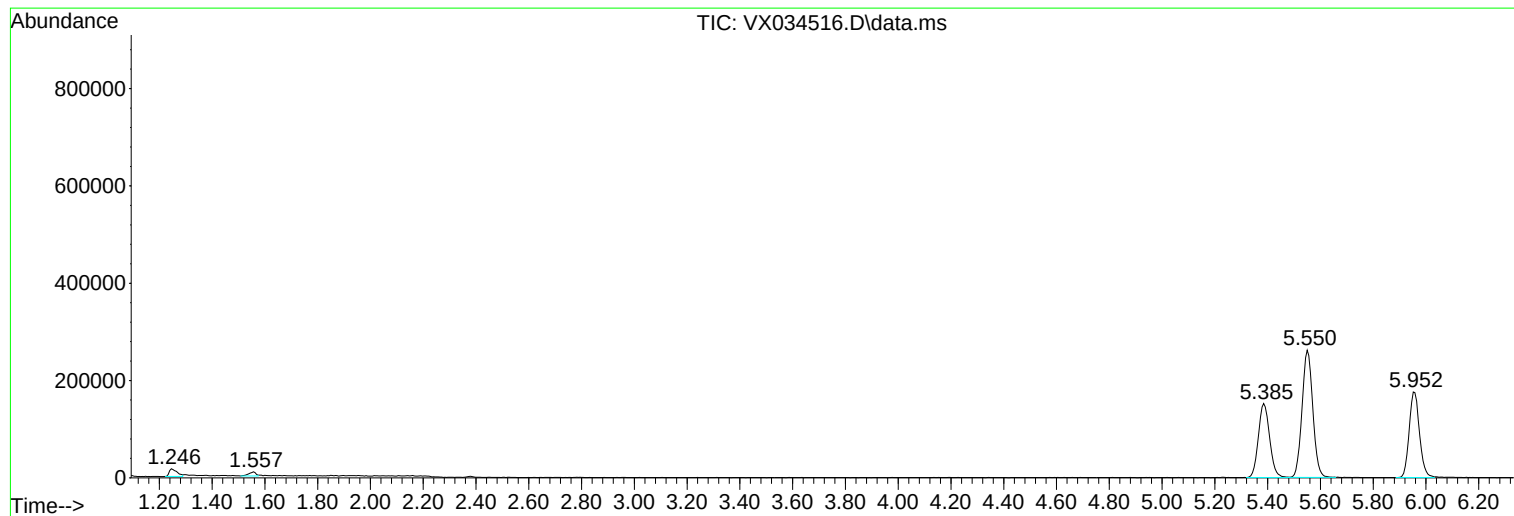

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031523\
Data File : VX034516.D
Acq On : 15 Mar 2023 18:19
Operator : JC/MD
Sample : 01909-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
UPS-01-031023-AM

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031523\
Data File : VX034516.D
Acq On : 15 Mar 2023 18:19
Operator : JC/MD
Sample : 01909-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
UPS-01-031023-AM

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc