

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031523\
 Data File : VX034517.D
 Acq On : 15 Mar 2023 18:43
 Operator : JC/MD
 Sample : 01880-16
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE125D3-20230310

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
 Title : SW846 8260

Signal : TIC: VX034517.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.251	23	27	38	rBV3	12680	33309	1.50%	0.300%
2	2.330	196	204	218	rVB	882732	1653142	74.56%	14.883%
3	4.495	549	559	568	rBV3	8567	24534	1.11%	0.221%
4	5.385	694	705	721	rBV	147916	426462	19.23%	3.839%
5	5.549	721	732	746	rVV	252027	711456	32.09%	6.405%
6	5.952	788	798	816	rBV	174000	462492	20.86%	4.164%
7	6.763	920	931	949	rBV	401204	972616	43.87%	8.757%
8	7.122	981	990	1014	rBV	1023010	2217254	100.00%	19.962%
9	8.646	1233	1240	1254	rBV	845623	1339547	60.41%	12.060%
10	9.274	1336	1343	1352	rBV	173999	262920	11.86%	2.367%
11	10.055	1465	1471	1481	rBV	846836	1125562	50.76%	10.134%
12	11.079	1634	1639	1653	rBV	712279	909652	41.03%	8.190%
13	12.024	1788	1794	1804	rBV	769788	968341	43.67%	8.718%




Sum of corrected areas: 11107287

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031523\
Data File : VX034517.D
Acq On : 15 Mar 2023 18:43
Operator : JC/MD
Sample : 01880-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE125D3-20230310

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

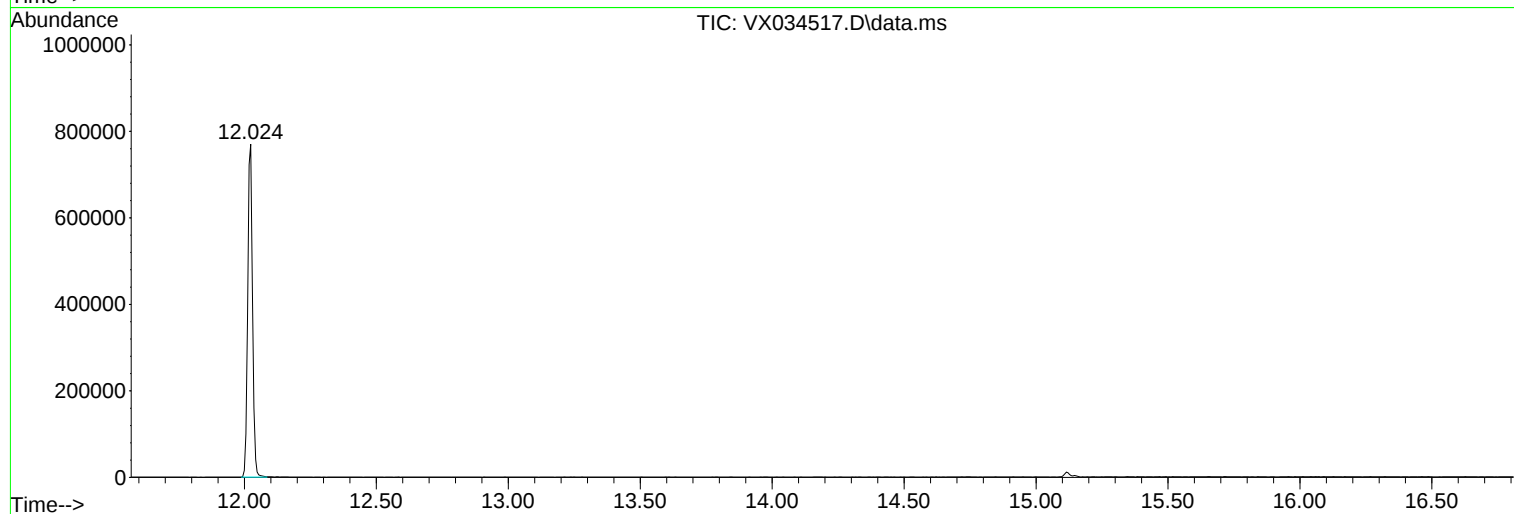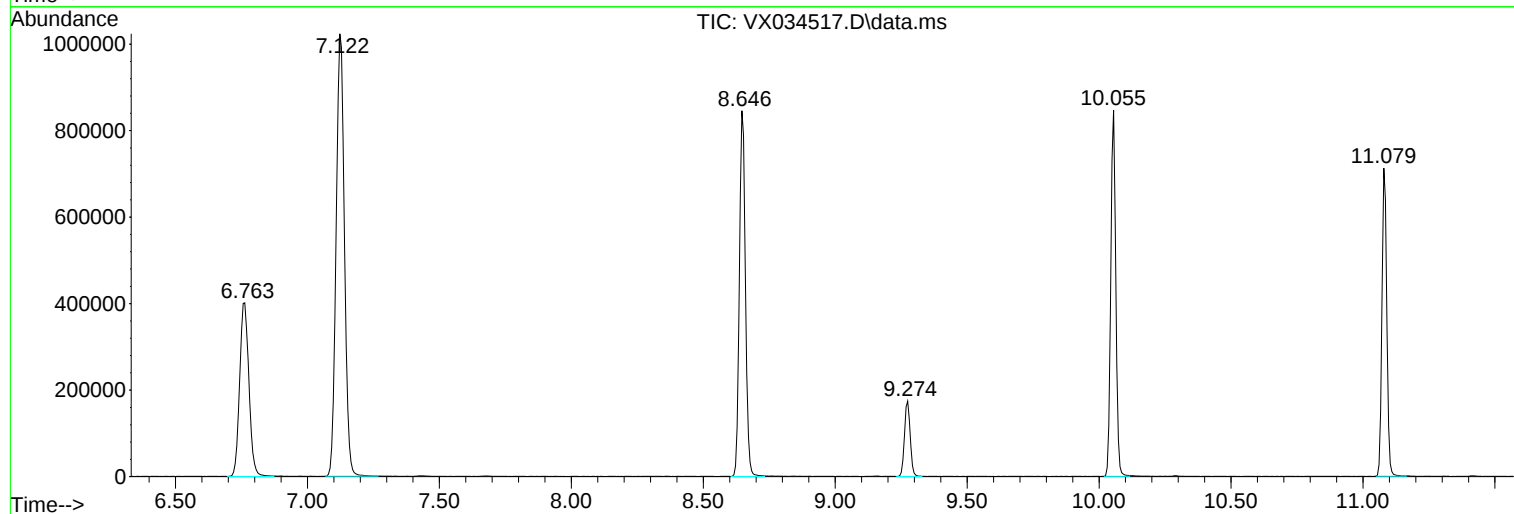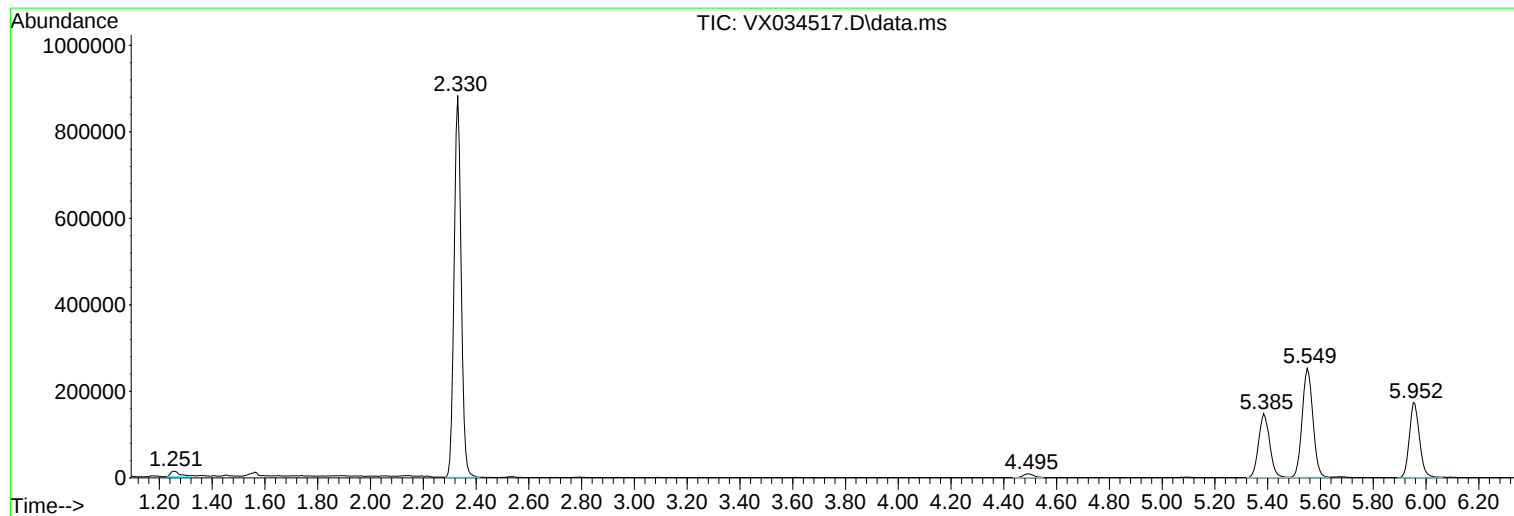

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031523\
Data File : VX034517.D
Acq On : 15 Mar 2023 18:43
Operator : JC/MD
Sample : 01880-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE125D3-20230310

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031523\
Data File : VX034517.D
Acq On : 15 Mar 2023 18:43
Operator : JC/MD
Sample : 01880-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE125D3-20230310

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------