

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031523\
 Data File : VX034518.D
 Acq On : 15 Mar 2023 19:06
 Operator : JC/MD
 Sample : 01903-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DUP05-20230312

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M

Title : SW846 8260

Signal : TIC: VX034518.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	21	27	32	rBV2	13740	29636	2.23%	0.359%
2	1.563	70	78	83	rBV2	7968	15829	1.19%	0.192%
3	5.001	629	642	663	rBV	411802	1280380	96.27%	15.525%
4	5.385	690	705	721	rBV	147000	429985	32.33%	5.214%
5	5.550	721	732	752	rVB	253174	711338	53.48%	8.625%
6	5.952	787	798	815	rBV	167789	457785	34.42%	5.551%
7	6.757	921	930	949	rBV	397826	963078	72.41%	11.678%
8	8.647	1233	1240	1251	rBV	832898	1329994	100.00%	16.127%
9	10.055	1465	1471	1483	rBV	835365	1127868	84.80%	13.676%
10	11.079	1634	1639	1649	rBV	736529	922430	69.36%	11.185%
11	12.024	1788	1794	1804	rBV	764501	978932	73.60%	11.870%




Sum of corrected areas: 8247255

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031523\
Data File : VX034518.D
Acq On : 15 Mar 2023 19:06
Operator : JC/MD
Sample : 01903-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP05-20230312

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

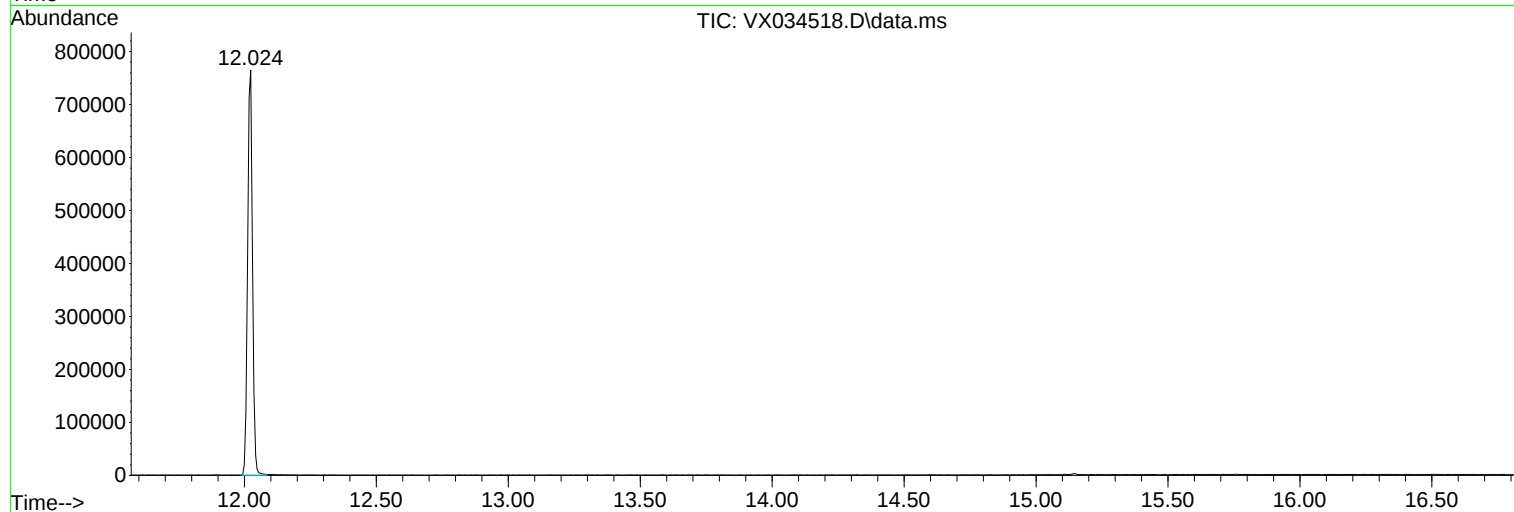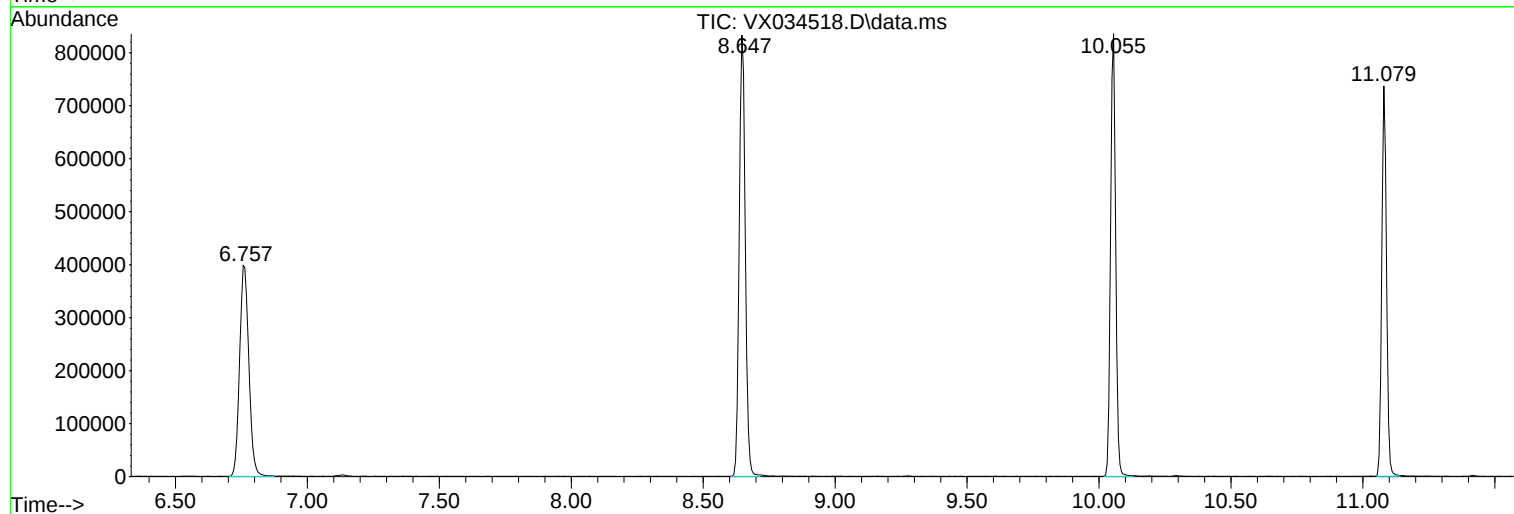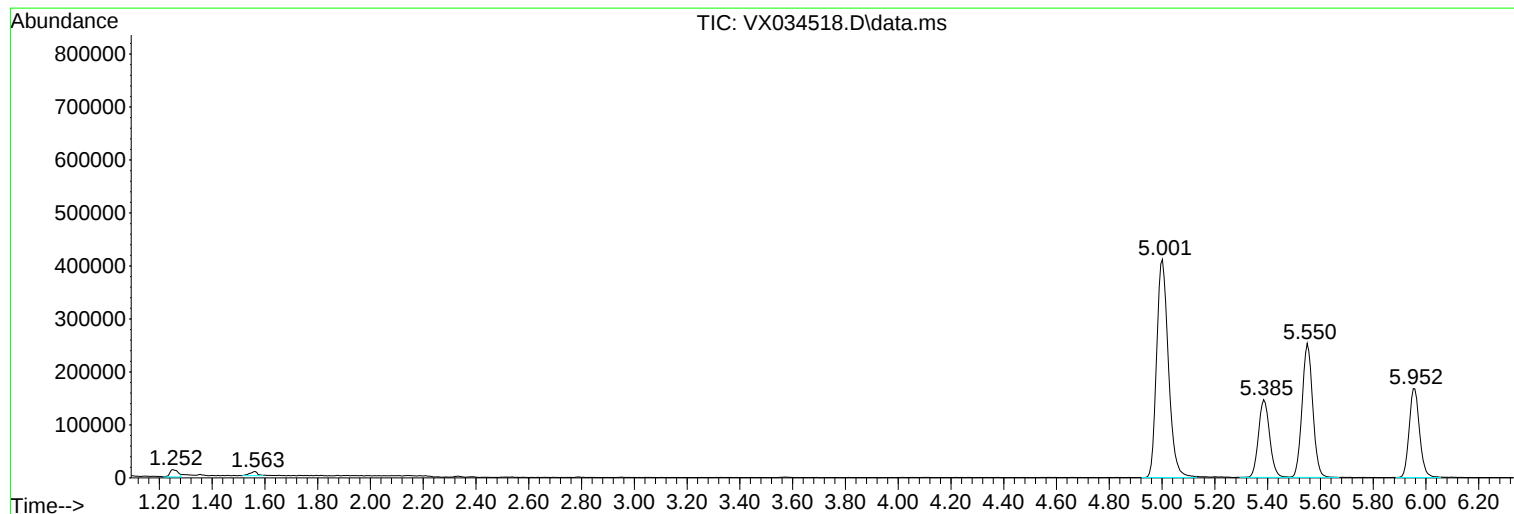

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031523\
Data File : VX034518.D
Acq On : 15 Mar 2023 19:06
Operator : JC/MD
Sample : 01903-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP05-20230312

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031523\
Data File : VX034518.D
Acq On : 15 Mar 2023 19:06
Operator : JC/MD
Sample : 01903-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP05-20230312

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------