

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031523\
Data File : VX034519.D
Acq On : 15 Mar 2023 19:30
Operator : JC/MD
Sample : 01903-21
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP06-20230312

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M

Title : SW846 8260

Signal : TIC: VX034519.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	23	27	39	rBV3	12786	36631	2.82%	0.530%
2	1.562	69	78	83	rBV3	8938	18914	1.45%	0.274%
3	5.013	634	644	656	rBV3	19397	62718	4.82%	0.908%
4	5.385	694	705	721	rBV3	140353	415002	31.91%	6.007%
5	5.550	721	732	749	rVB	241194	687893	52.89%	9.956%
6	5.952	789	798	817	rBV	164296	446268	34.31%	6.459%
7	6.763	920	931	951	rBV	389632	942538	72.46%	13.642%
8	8.647	1232	1240	1251	rBV	841111	1300710	100.00%	18.826%
9	10.055	1465	1471	1488	rBV	816228	1108109	85.19%	16.039%
10	11.079	1634	1639	1654	rBV	727668	917024	70.50%	13.273%
11	12.024	1788	1794	1804	rBV	761061	973213	74.82%	14.086%




Sum of corrected areas: 6909020

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031523\
Data File : VX034519.D
Acq On : 15 Mar 2023 19:30
Operator : JC/MD
Sample : 01903-21
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP06-20230312

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

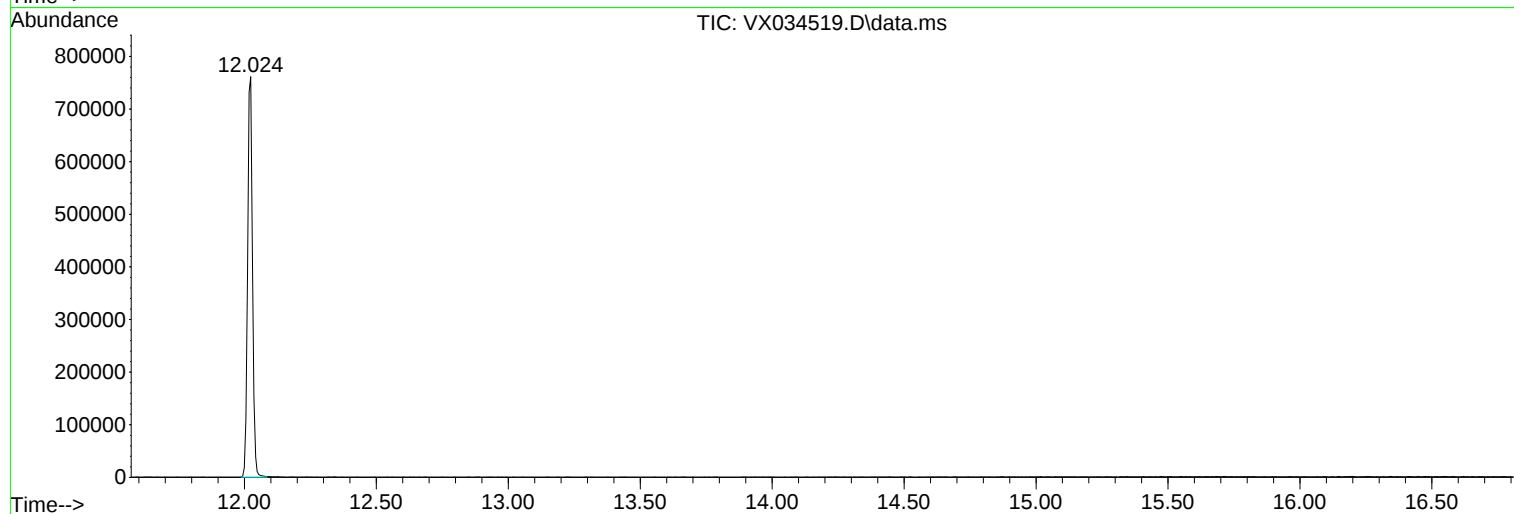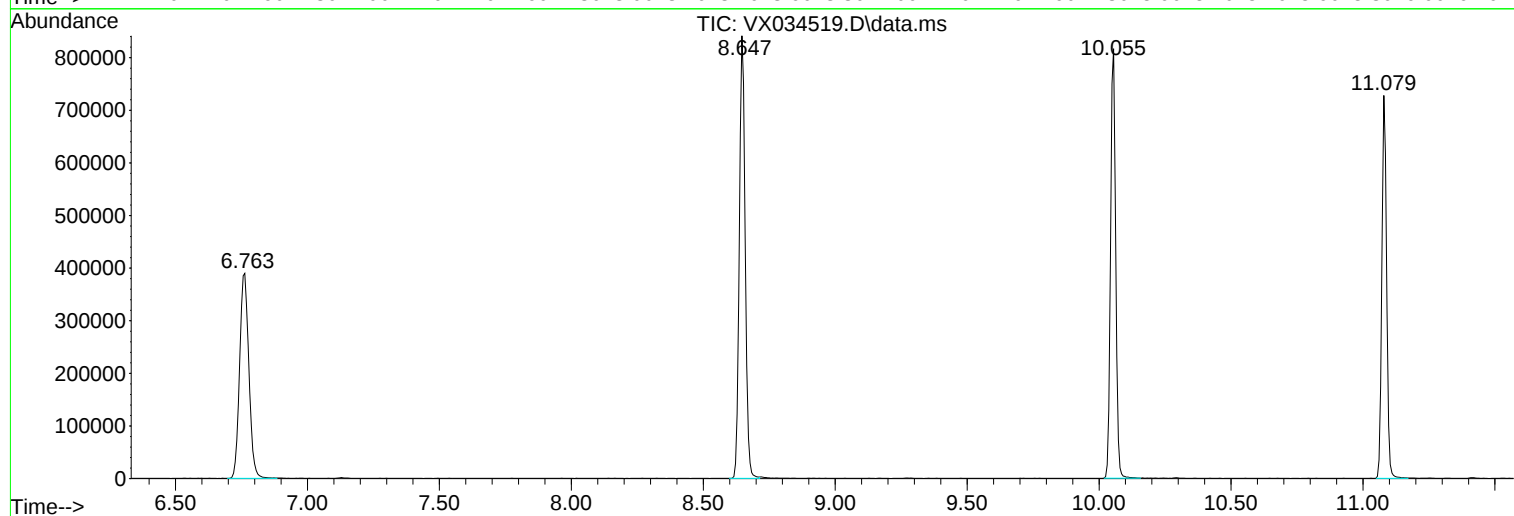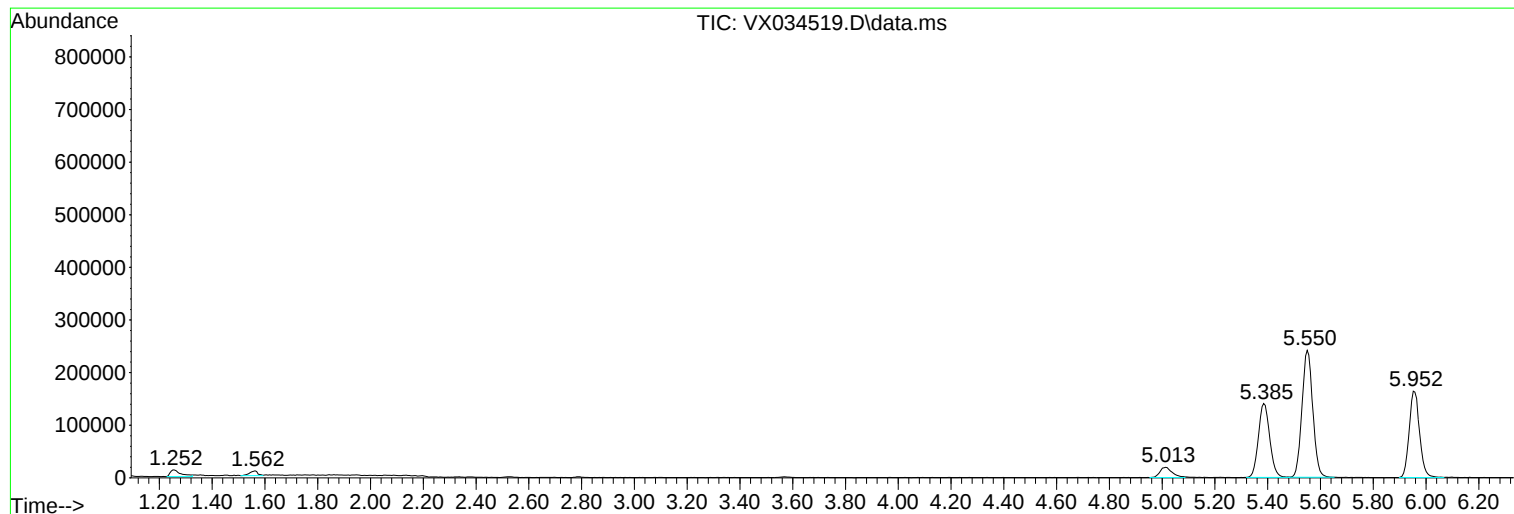

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031523\
Data File : VX034519.D
Acq On : 15 Mar 2023 19:30
Operator : JC/MD
Sample : 01903-21
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP06-20230312

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031523\
Data File : VX034519.D
Acq On : 15 Mar 2023 19:30
Operator : JC/MD
Sample : 01903-21
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP06-20230312

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------