

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX031523\  
 Data File : VX034521.D  
 Acq On : 15 Mar 2023 20:17  
 Operator : JC/MD  
 Sample : 01903-22  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 20 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 RW9-MW01D1-20230312

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X031023W.M  
 Title : SW846 8260

Signal : TIC: VX034521.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.245       | 22            | 26          | 36           | rBV2     | 15131          | 37907         | 2.45%           | 0.490%        |
| 2         | 1.556       | 70            | 77          | 84           | rBV4     | 8934           | 17759         | 1.15%           | 0.230%        |
| 3         | 5.013       | 635           | 644         | 655          | rBV2     | 12830          | 42072         | 2.72%           | 0.544%        |
| 4         | 5.385       | 694           | 705         | 720          | rBV2     | 145705         | 435576        | 28.20%          | 5.630%        |
| 5         | 5.550       | 720           | 732         | 747          | rVB      | 254384         | 726255        | 47.01%          | 9.387%        |
| 6         | 5.958       | 786           | 799         | 815          | rBV      | 173550         | 470491        | 30.46%          | 6.081%        |
| 7         | 6.763       | 921           | 931         | 946          | rBV      | 405640         | 979097        | 63.38%          | 12.655%       |
| 8         | 8.647       | 1233          | 1240        | 1250         | rBV      | 986971         | 1544750       | 100.00%         | 19.966%       |
| 9         | 9.275       | 1336          | 1343        | 1351         | rBV      | 25254          | 41186         | 2.67%           | 0.532%        |
| 10        | 10.055      | 1465          | 1471        | 1487         | rBV      | 918725         | 1283261       | 83.07%          | 16.586%       |
| 11        | 11.079      | 1634          | 1639        | 1650         | rBV      | 741411         | 947562        | 61.34%          | 12.247%       |
| 12        | 11.311      | 1672          | 1677        | 1682         | rBV      | 26857          | 42999         | 2.78%           | 0.556%        |
| 13        | 12.024      | 1788          | 1794        | 1802         | rBV      | 797429         | 1019092       | 65.97%          | 13.172%       |
| 14        | 13.274      | 1990          | 1999        | 2012         | rVB3     | 36589          | 149045        | 9.65%           | 1.926%        |


Sum of corrected areas: 7737052

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX031523\  
Data File : VX034521.D  
Acq On : 15 Mar 2023 20:17  
Operator : JC/MD  
Sample : 01903-22  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 20 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
RW9-MW01D1-20230312

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X031023W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

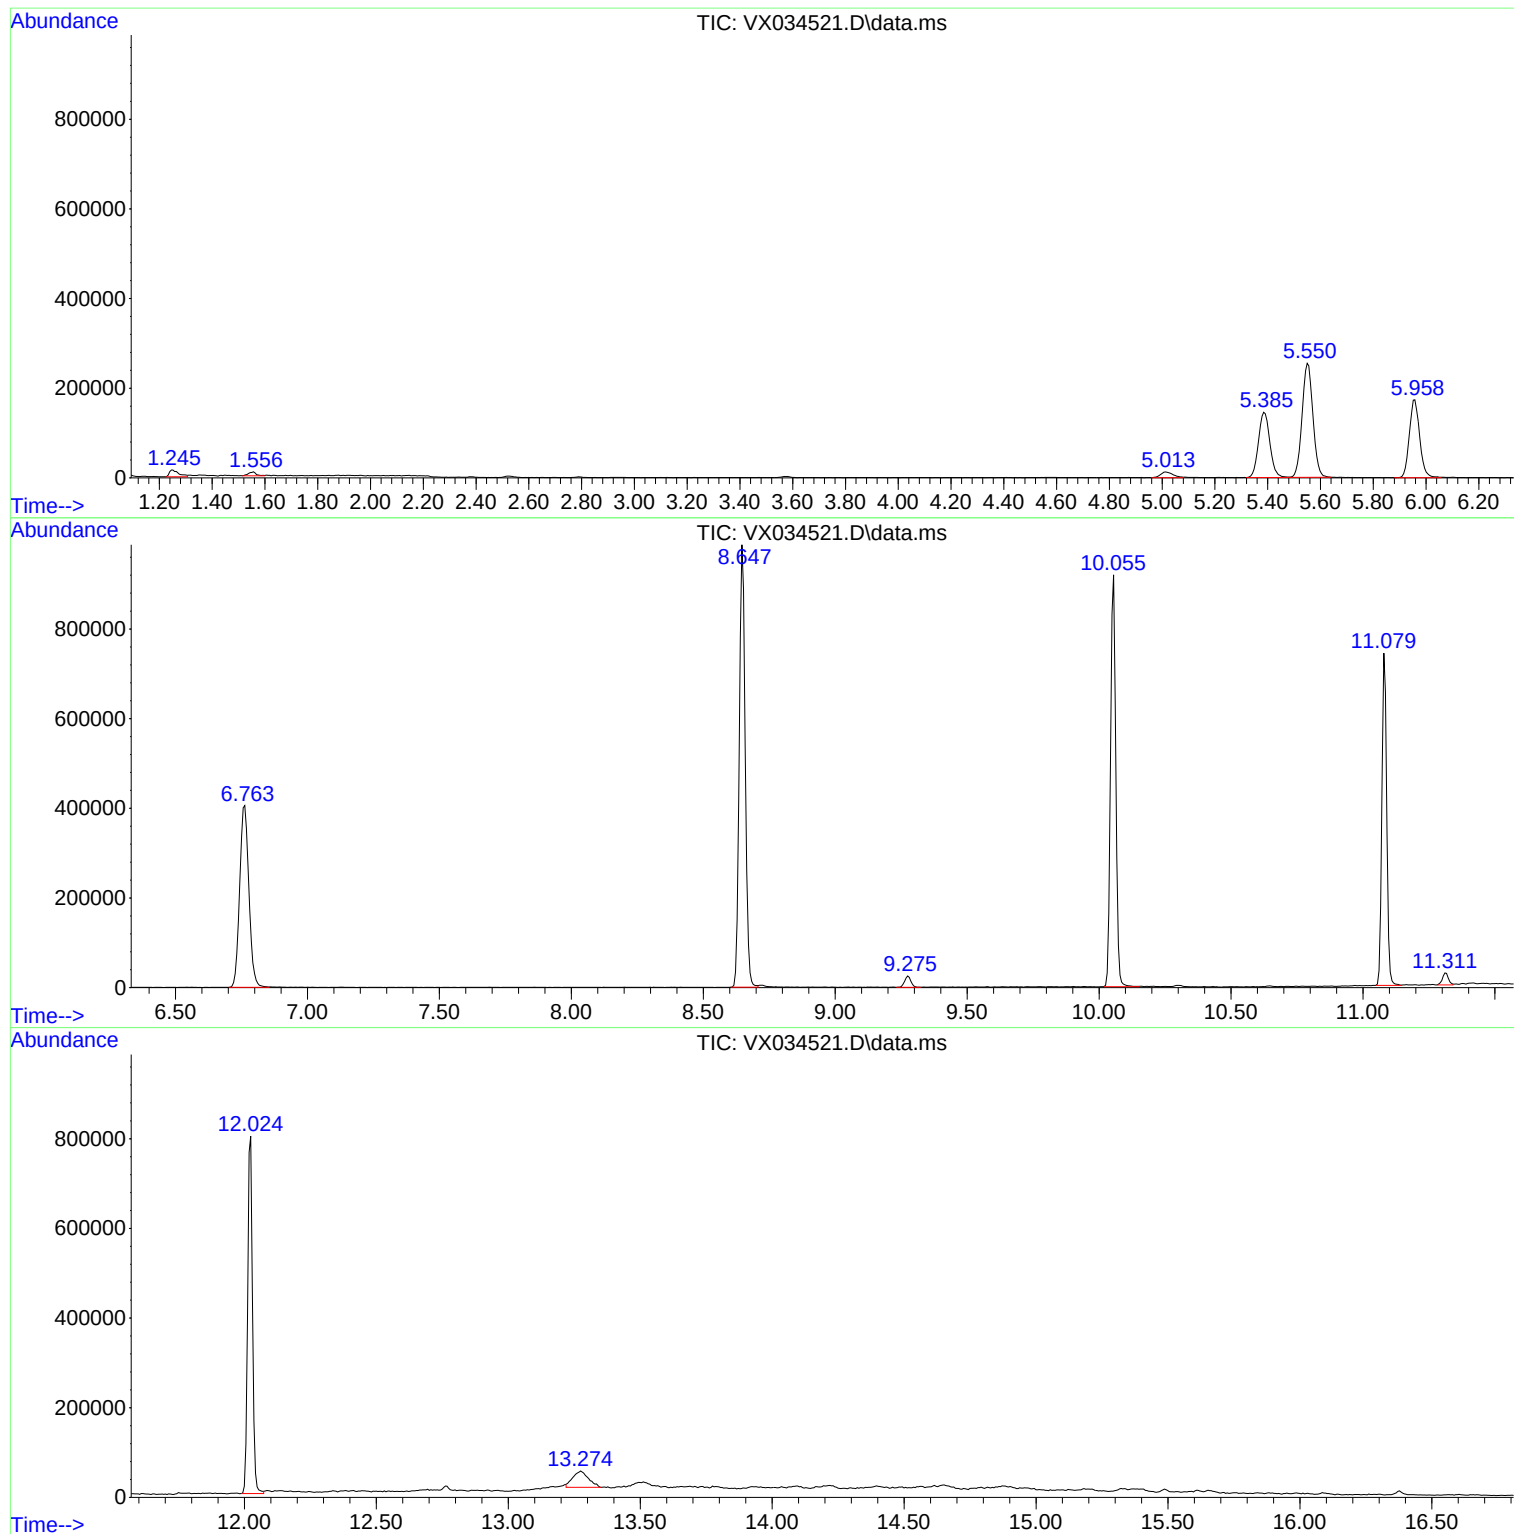

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX031523\  
Data File : VX034521.D  
Acq On : 15 Mar 2023 20:17  
Operator : JC/MD  
Sample : 01903-22  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 20 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
RW9-MW01D1-20230312

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X031023W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX031523\  
Data File : VX034521.D  
Acq On : 15 Mar 2023 20:17  
Operator : JC/MD  
Sample : 01903-22  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 20 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
RW9-MW01D1-20230312

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X031023W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|