

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031523\
 Data File : VX034523.D
 Acq On : 15 Mar 2023 21:04
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M

Title : SW846 8260

Signal : TIC: VX034523.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.557	69	77	83	rBV3	7311	14582	1.08%	0.212%
2	5.385	693	705	719	rBV2	147768	430578	31.97%	6.269%
3	5.550	721	732	746	rVB	255568	725374	53.86%	10.560%
4	5.958	788	799	815	rBV	169946	460110	34.17%	6.699%
5	6.757	921	930	942	rBV	407118	977923	72.62%	14.237%
6	7.129	983	991	999	rVB3	7596	17796	1.32%	0.259%
7	8.647	1233	1240	1258	rBV	871040	1346692	100.00%	19.606%
8	10.055	1465	1471	1489	rBV	820163	1120898	83.23%	16.319%
9	11.079	1634	1639	1648	rBV	635411	821858	61.03%	11.965%
10	12.018	1788	1793	1807	rBV	734000	952999	70.77%	13.874%




Sum of corrected areas: 6868810

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031523\
Data File : VX034523.D
Acq On : 15 Mar 2023 21:04
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

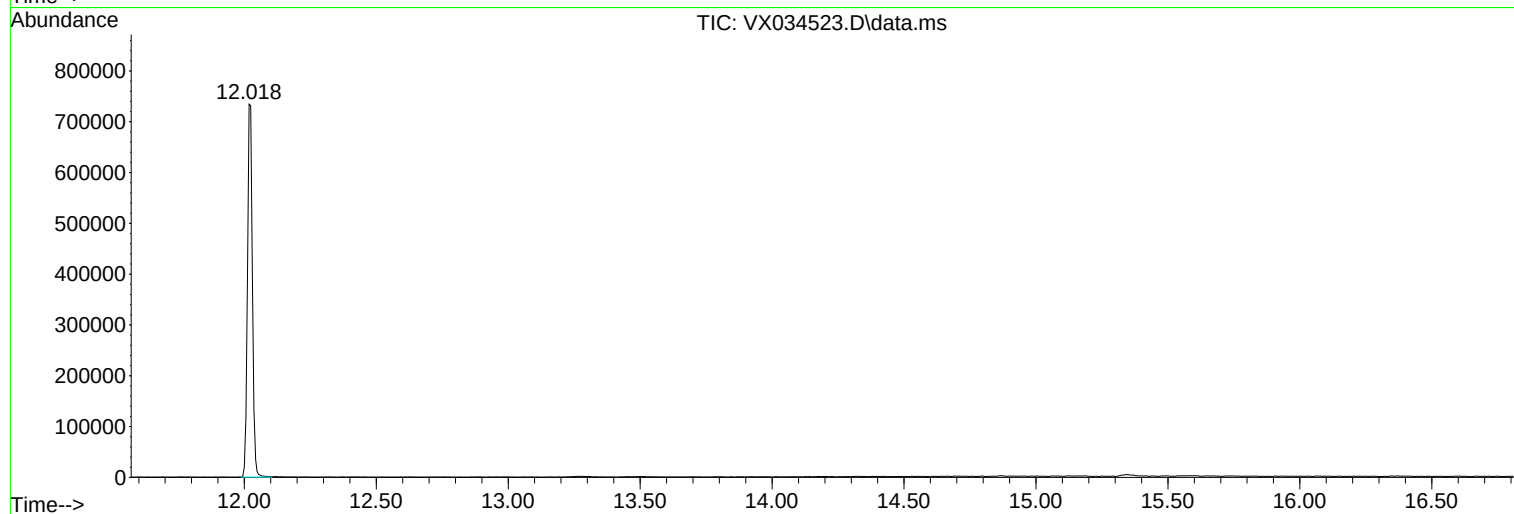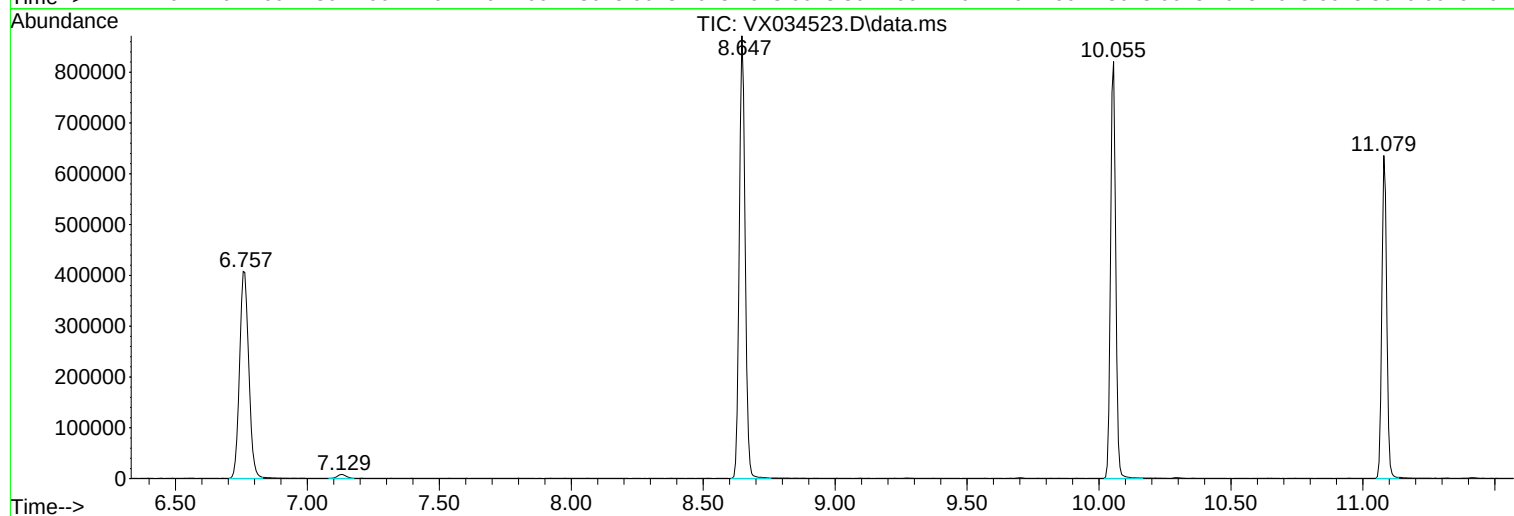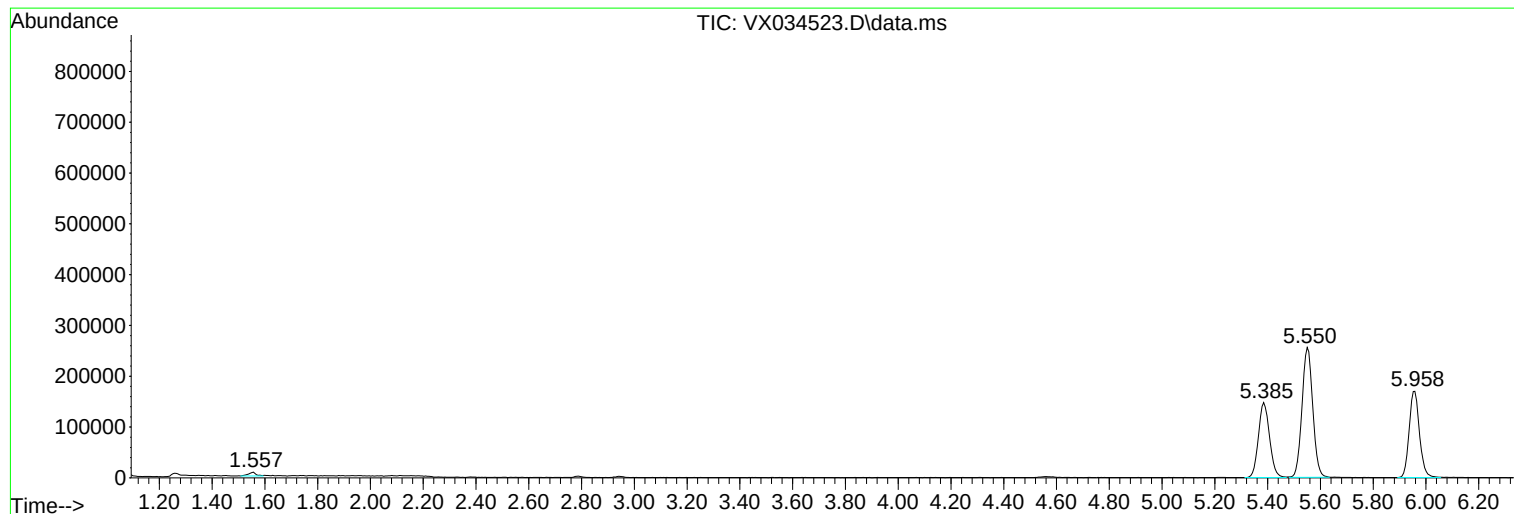

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031523\
Data File : VX034523.D
Acq On : 15 Mar 2023 21:04
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031523\
Data File : VX034523.D
Acq On : 15 Mar 2023 21:04
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------