

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX031523\  
Data File : VX034524.D  
Acq On : 15 Mar 2023 21:28  
Operator : JC/MD  
Sample : 01904-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 23 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
EB02-20230313

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X031023W.M

Title : SW846 8260

Signal : TIC: VX034524.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.258       | 23            | 28          | 38           | rBV3     | 9100           | 25846         | 1.98%           | 0.386%        |
| 2         | 1.355       | 41            | 44          | 49           | rVB      | 17213          | 16541         | 1.27%           | 0.247%        |
| 3         | 5.385       | 693           | 705         | 721          | rBV      | 143319         | 421597        | 32.28%          | 6.301%        |
| 4         | 5.550       | 721           | 732         | 748          | rVB      | 253733         | 702256        | 53.77%          | 10.496%       |
| 5         | 5.952       | 788           | 798         | 815          | rBV2     | 167022         | 454750        | 34.82%          | 6.797%        |
| 6         | 6.763       | 921           | 931         | 947          | rBV      | 396393         | 950469        | 72.78%          | 14.206%       |
| 7         | 8.647       | 1233          | 1240        | 1260         | rBV      | 821969         | 1305960       | 100.00%         | 19.519%       |
| 8         | 10.055      | 1465          | 1471        | 1481         | rBV      | 807707         | 1099109       | 84.16%          | 16.428%       |
| 9         | 11.079      | 1634          | 1639        | 1655         | rBV      | 625930         | 803781        | 61.55%          | 12.014%       |
| 10        | 12.024      | 1788          | 1794        | 1805         | rBV      | 699533         | 910323        | 69.71%          | 13.606%       |




Sum of corrected areas: 6690632

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX031523\  
Data File : VX034524.D  
Acq On : 15 Mar 2023 21:28  
Operator : JC/MD  
Sample : 01904-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 23 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
EB02-20230313

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X031023W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

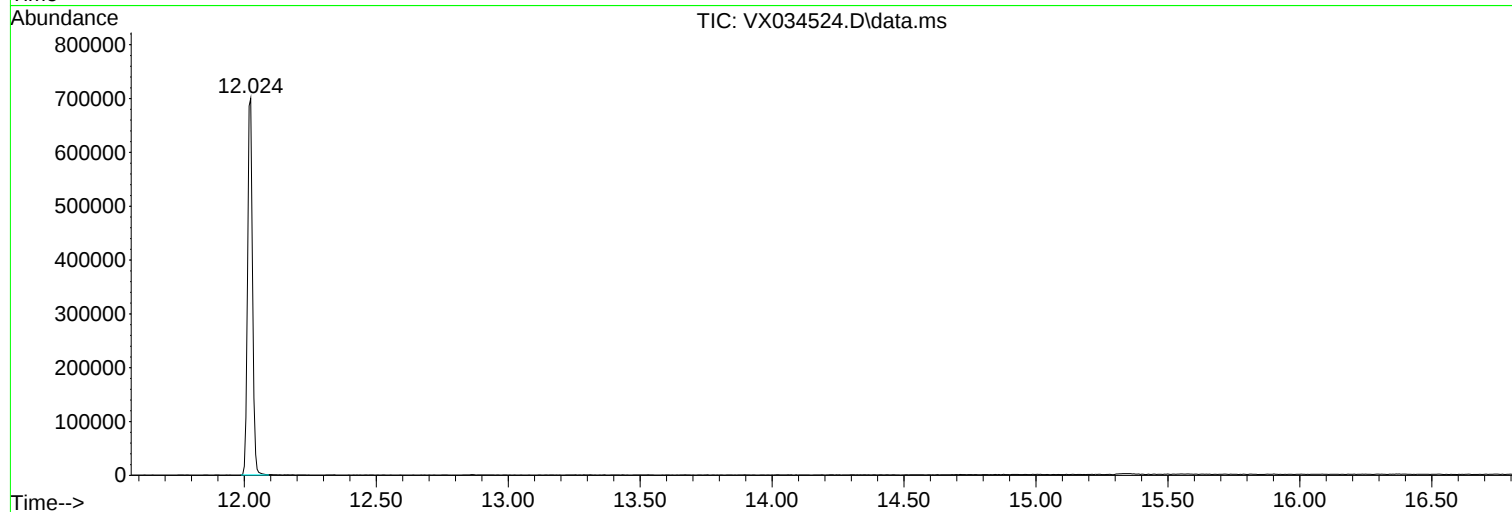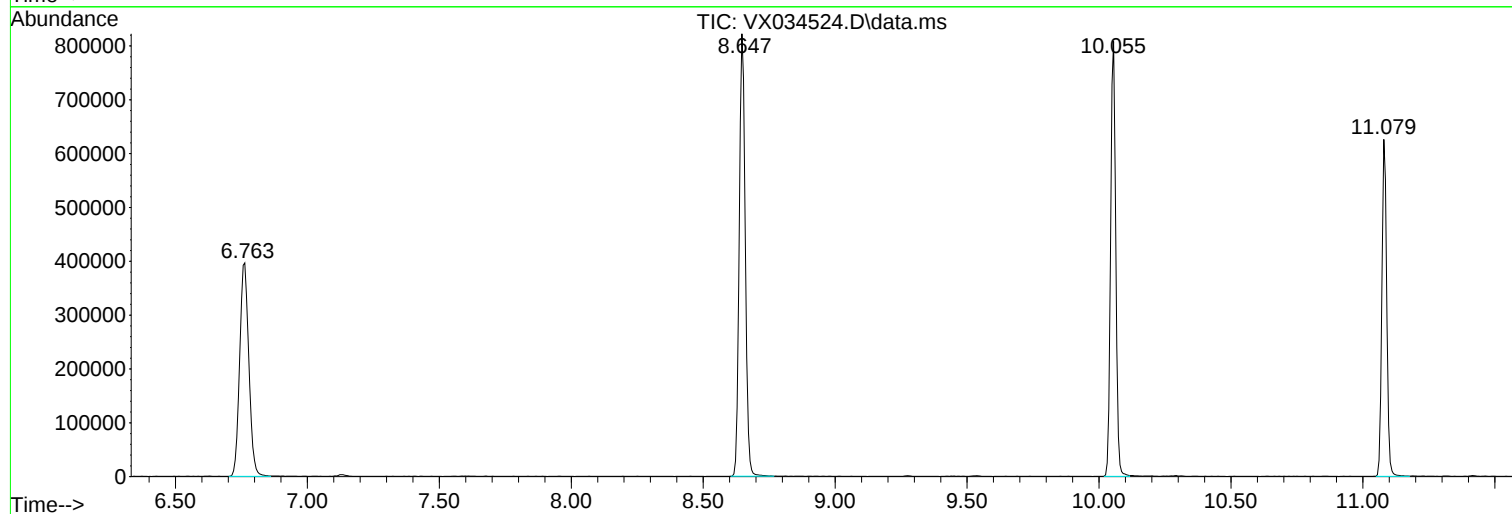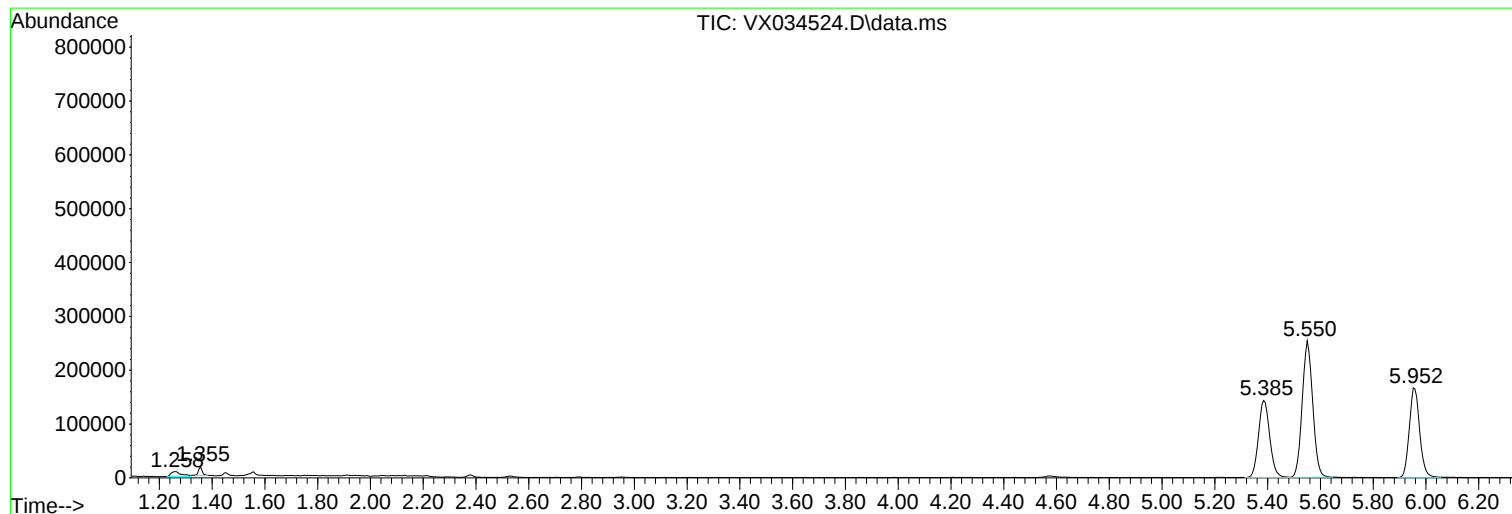

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX031523\  
Data File : VX034524.D  
Acq On : 15 Mar 2023 21:28  
Operator : JC/MD  
Sample : 01904-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 23 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
EB02-20230313

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X031023W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX031523\  
Data File : VX034524.D  
Acq On : 15 Mar 2023 21:28  
Operator : JC/MD  
Sample : 01904-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 23 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
EB02-20230313

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X031023W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|