

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX031523\  
 Data File : VX034525.D  
 Acq On : 15 Mar 2023 21:51  
 Operator : JC/MD  
 Sample : 01904-02  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 24 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 FB02-20230313

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X031023W.M

Title : SW846 8260

Signal : TIC: VX034525.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.264       | 22            | 29          | 32           | rBV3     | 8786           | 17820         | 1.35%           | 0.252%        |
| 2         | 1.356       | 41            | 44          | 50           | rVB      | 17611          | 18756         | 1.42%           | 0.266%        |
| 3         | 5.385       | 693           | 705         | 721          | rBV      | 144910         | 427278        | 32.32%          | 6.054%        |
| 4         | 5.550       | 721           | 732         | 748          | rVB      | 248499         | 707732        | 53.53%          | 10.028%       |
| 5         | 5.952       | 787           | 798         | 814          | rBV      | 170054         | 460479        | 34.83%          | 6.525%        |
| 6         | 6.763       | 921           | 931         | 946          | rBV      | 396056         | 957109        | 72.39%          | 13.562%       |
| 7         | 8.647       | 1232          | 1240        | 1253         | rBV      | 845292         | 1322225       | 100.00%         | 18.735%       |
| 8         | 10.055      | 1465          | 1471        | 1483         | rBV      | 911456         | 1250605       | 94.58%          | 17.720%       |
| 9         | 11.079      | 1634          | 1639        | 1656         | rBV      | 770879         | 975157        | 73.75%          | 13.817%       |
| 10        | 12.018      | 1788          | 1793        | 1808         | rBV      | 696849         | 920365        | 69.61%          | 13.041%       |


Sum of corrected areas: 7057526

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX031523\  
Data File : VX034525.D  
Acq On : 15 Mar 2023 21:51  
Operator : JC/MD  
Sample : 01904-02  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 24 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
FB02-20230313

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X031023W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

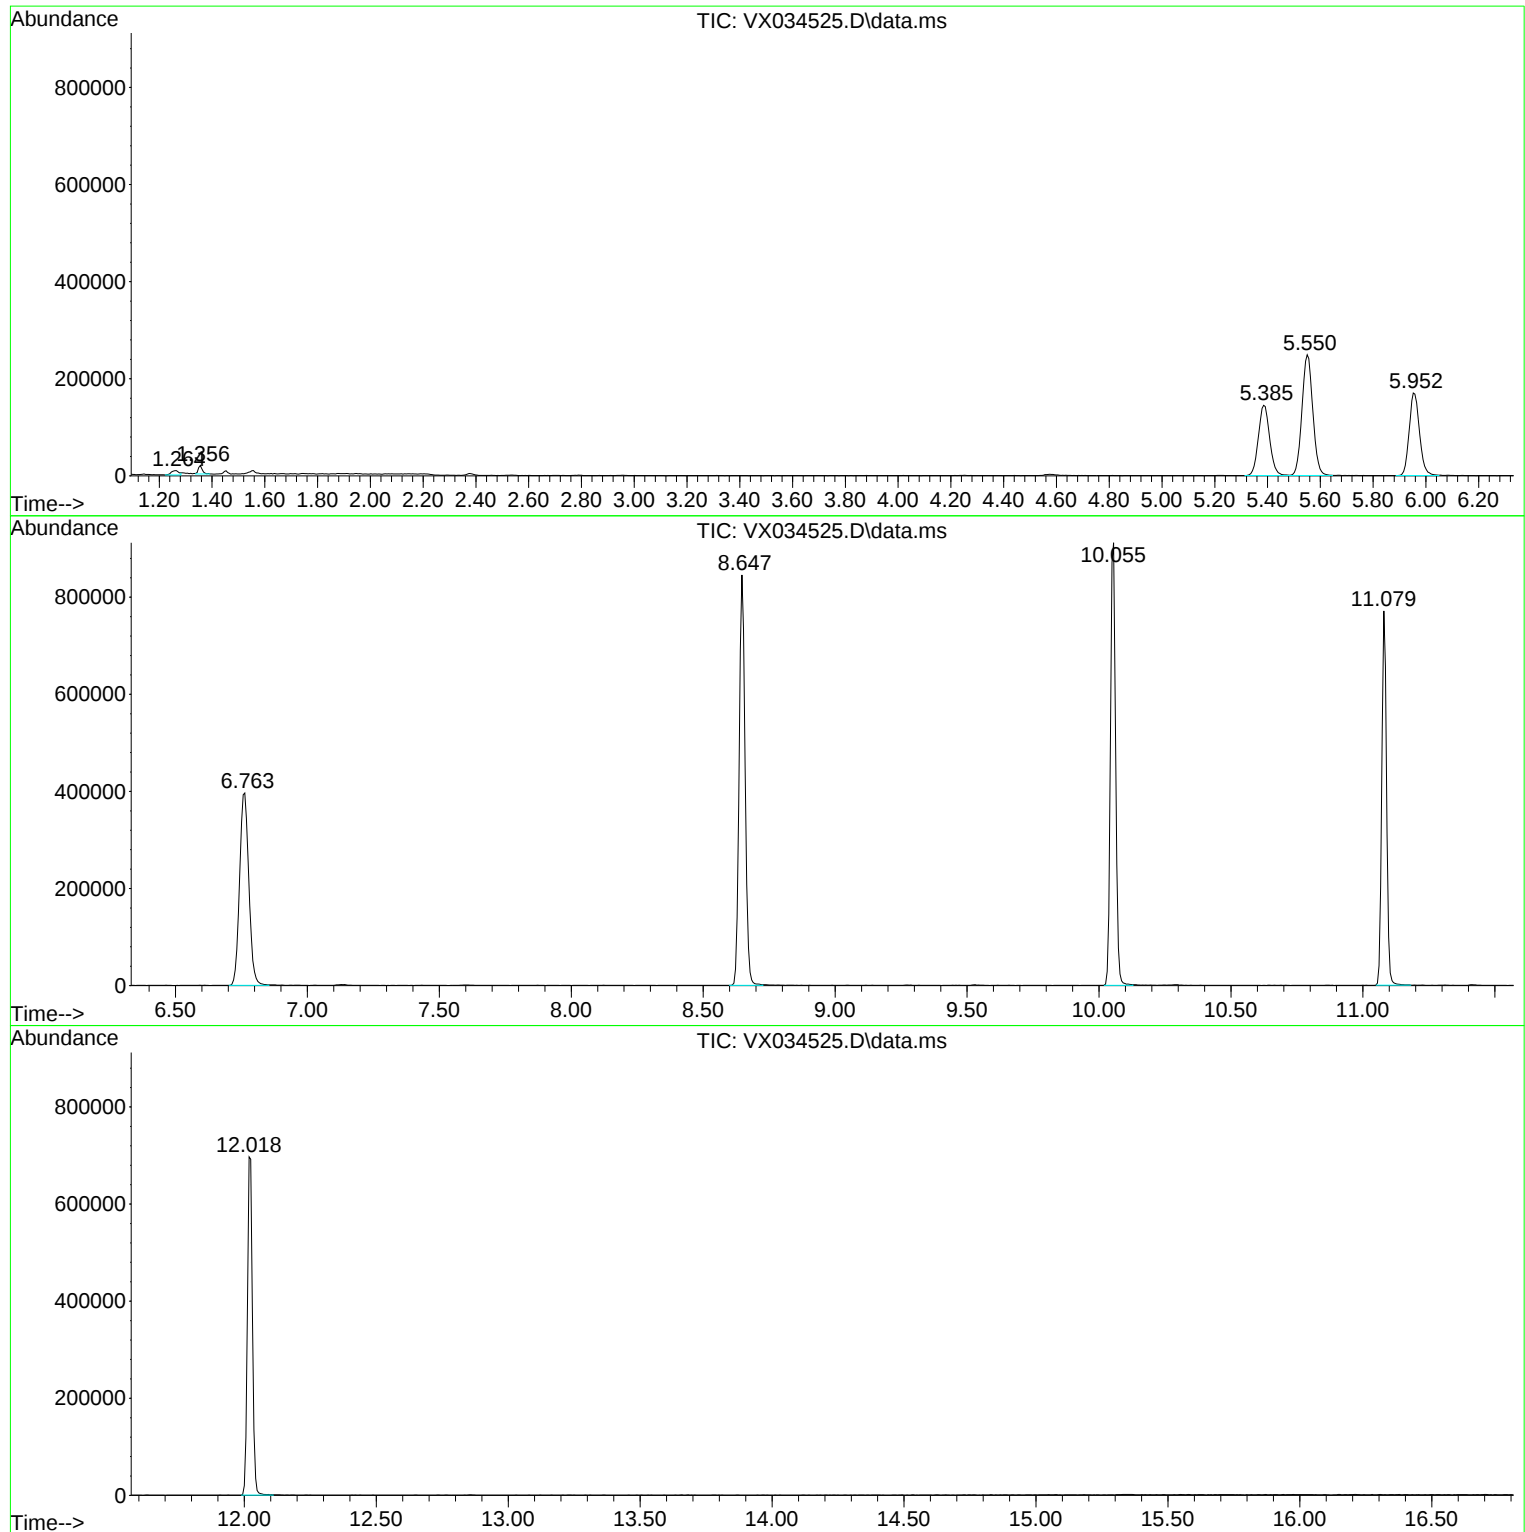

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX031523\  
Data File : VX034525.D  
Acq On : 15 Mar 2023 21:51  
Operator : JC/MD  
Sample : 01904-02  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 24 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
FB02-20230313

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X031023W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX031523\  
Data File : VX034525.D  
Acq On : 15 Mar 2023 21:51  
Operator : JC/MD  
Sample : 01904-02  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 24 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
FB02-20230313

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X031023W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|