
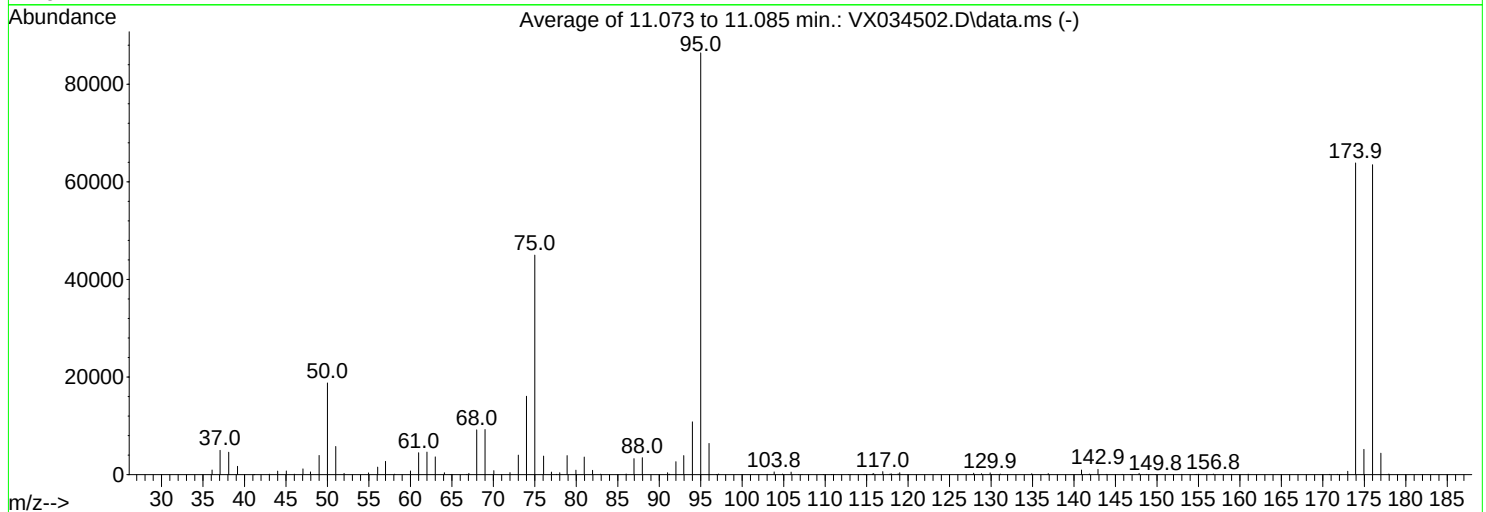


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031523\
Data File : VX034502.D
Acq On : 15 Mar 2023 12:35
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Title : SW846 8260
Last Update : Mon Mar 13 10:29:32 2023

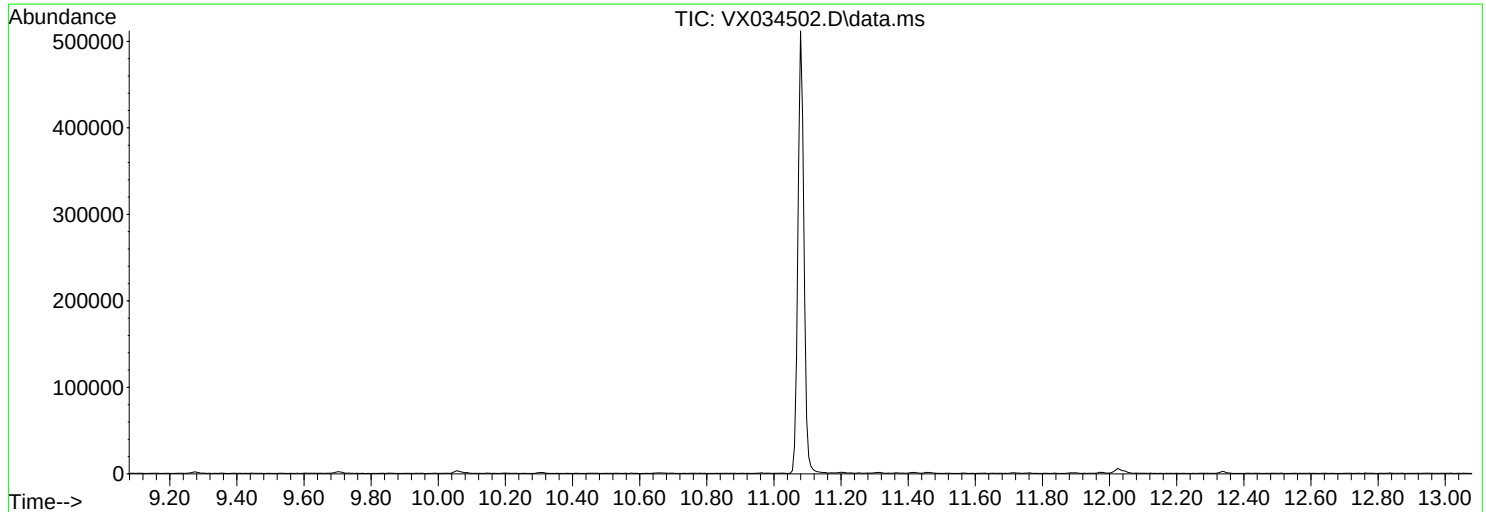

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.7	18779	PASS
75	95	30	60	52.1	45003	PASS
95	95	100	100	100.0	86445	PASS
96	95	5	9	7.4	6404	PASS
173	174	0.00	2	1.1	694	PASS
174	95	50	100	73.9	63867	PASS
175	174	5	9	8.1	5195	PASS
176	174	95	101	99.5	63531	PASS
177	176	5	9	6.9	4406	PASS