

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
 Data File : VX040668.D
 Acq On : 15 Mar 2024 21:21
 Operator : JC/MD
 Sample : P1754-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Mar 16 05:53:13 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 16 05:02:38 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	148347	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	139975	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	59873	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	47861	36.805	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	73.620%
7) Chloroethane-d5	1.666	69	43772	42.162	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	84.320%
11) 1,1-Dichloroethene-d2	2.306	65	21948	36.665	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	73.320%
21) 2-Butanone-d5	4.452	46	99656	99.867	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	99.870%
24) Chloroform-d	5.056	84	111563	46.197	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.400%
26) 1,2-Dichloroethane-d4	5.952	65	83685	46.415	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.820%
32) Benzene-d6	5.977	84	190176	44.285	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.560%
36) 1,2-Dichloropropane-d6	7.312	67	63407	47.641	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	95.280%
41) Toluene-d8	8.647	98	167146	40.388	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	80.780%
43) trans-1,3-Dichloroprop...	8.952	79	30774	43.443	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	86.880%
47) 2-Hexanone-d5	9.384	63	71472	97.323	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	97.320%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	87898	44.110	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	88.220%
66) 1,2-Dichlorobenzene-d4	12.317	152	62049	49.480	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.960%
Target Compounds						
					Qvalue	
12) 1,1-Dichloroethene	2.319	96	1537	1.700	ug/L #	1
13) Acetone	2.380	43	145326	203.940	ug/L	99
19) 1,1-Dichloroethane	3.611	63	5477	3.037	ug/L	93
22) 2-Butanone	4.562	43	3983	4.221	ug/L #	74
39) cis-1,3-Dichloropropene	8.318	75	2438	1.455	ug/L	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
Data File : VX040668.D
Acq On : 15 Mar 2024 21:21
Operator : JC/MD
Sample : P1754-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Mar 16 05:53:13 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 16 05:02:38 2024
Response via : Initial Calibration

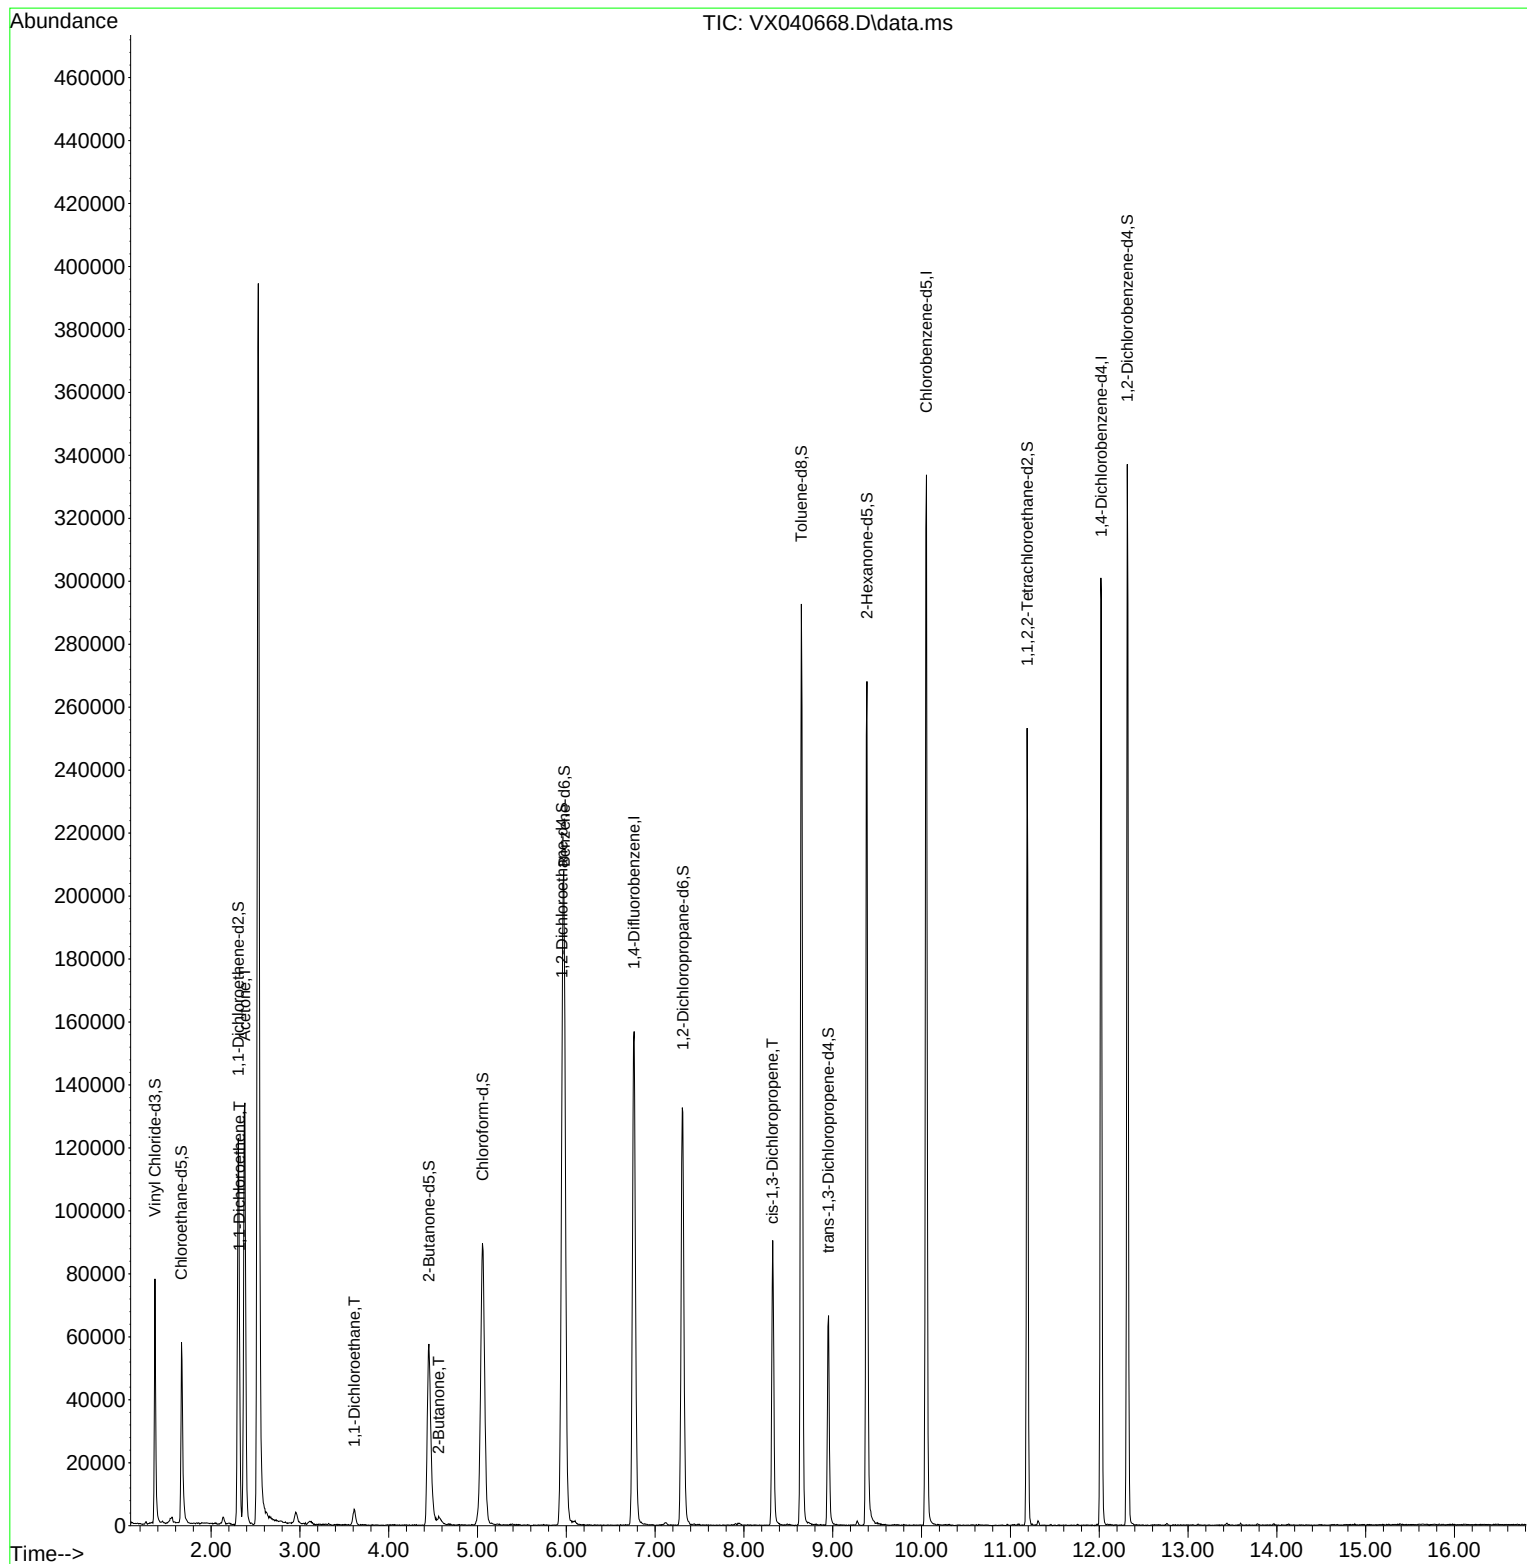



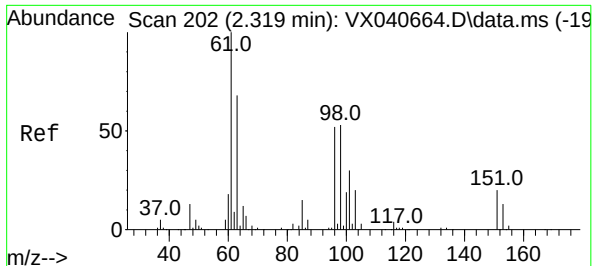


#12
1,1-Dichloroethene
Concen: 1.700 ug/L
RT: 2.319 min Scan# 202
Delta R.T. -0.000 min
Lab File: VX040668.D
Acq: 15 Mar 2024 21:21

Instrument :
MSVOA_X
ClientSampleId :



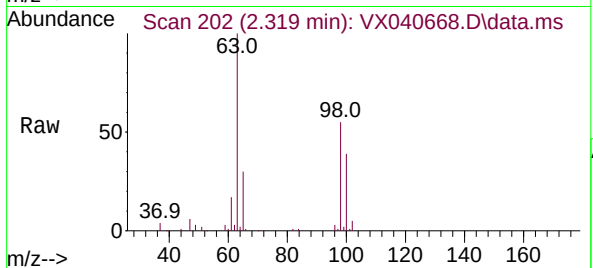



Tgt Ion: 96 Resp: 1537
Ion Ratio Lower Upper
96 100
61 515.8 134.8 250.4#
63 2952.5 92.5 171.9#

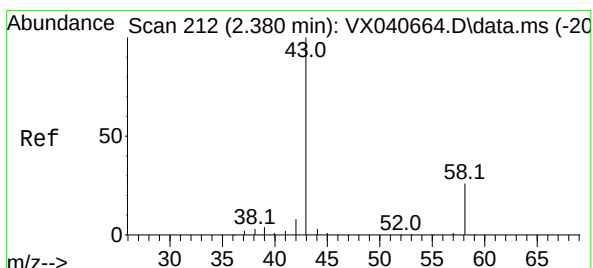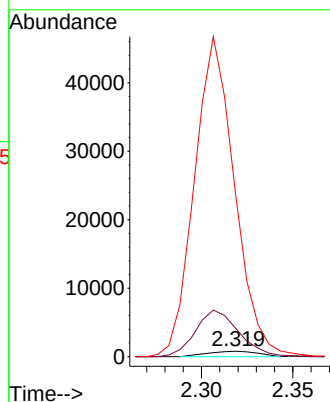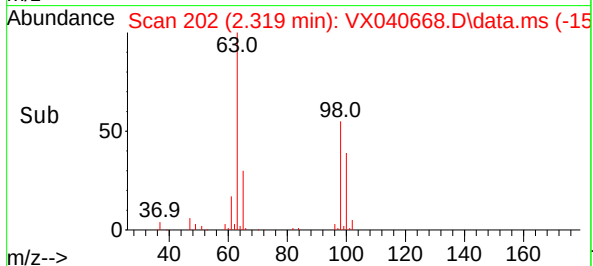

#13
Acetone
Concen: 203.940 ug/L
RT: 2.380 min Scan# 212
Delta R.T. -0.000 min
Lab File: VX040668.D
Acq: 15 Mar 2024 21:21

Tgt Ion: 43 Resp: 145326
Ion Ratio Lower Upper
43 100
58 26.8 0.0 54.6

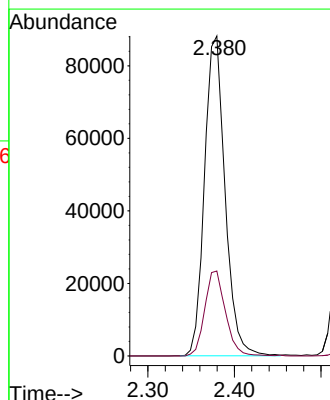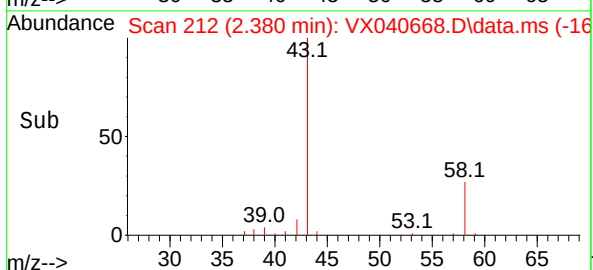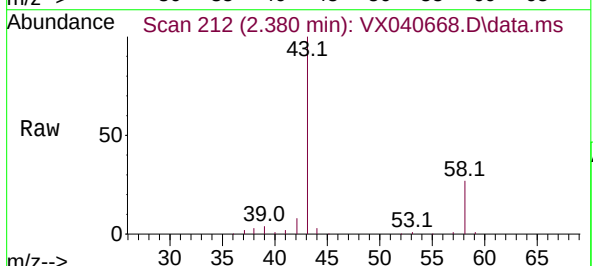

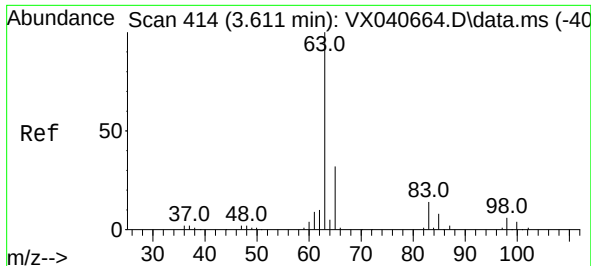

#19

1,1-Dichloroethane

Concen: 3.037 ug/L

RT: 3.611 min Scan# 41

Delta R.T. -0.000 min


Lab File: VX040668.D

Acq: 15 Mar 2024 21:21

Instrument :

MSVOA_X

ClientSampleId :

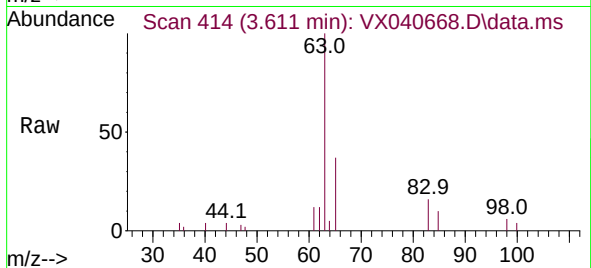




Tgt Ion: 63 Resp: 5477

Ion Ratio Lower Upper

63 100

65 37.5 23.1 42.9

83 16.0 9.9 18.5

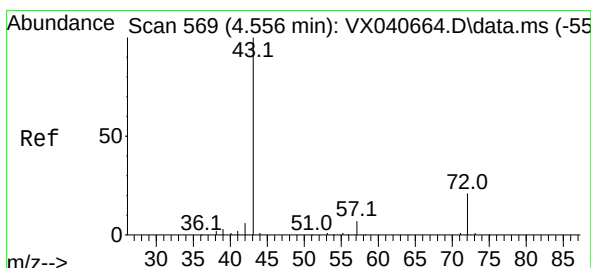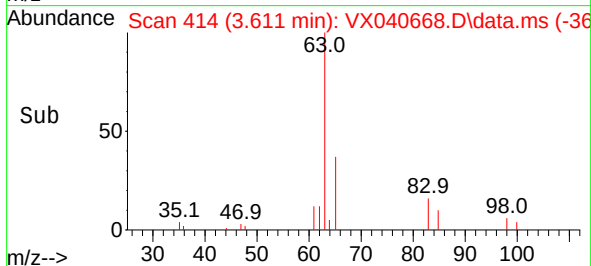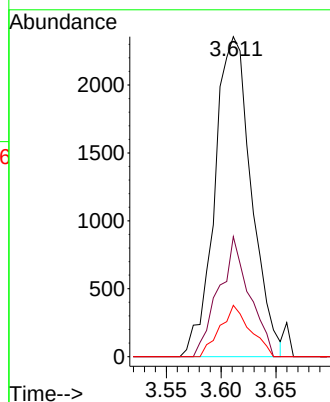

#22

2-Butanone

Concen: 4.221 ug/L

RT: 4.562 min Scan# 570

Delta R.T. 0.006 min

Lab File: VX040668.D




Acq: 15 Mar 2024 21:21


Tgt Ion: 43 Resp: 3983

Ion Ratio Lower Upper

43 100

72 11.9 12.4 37.2#

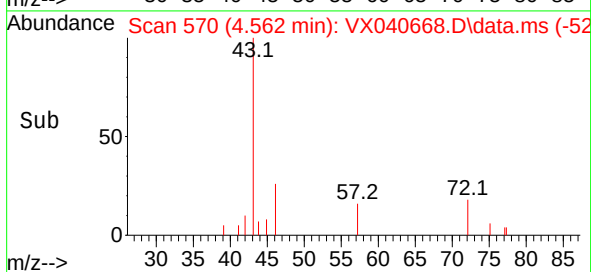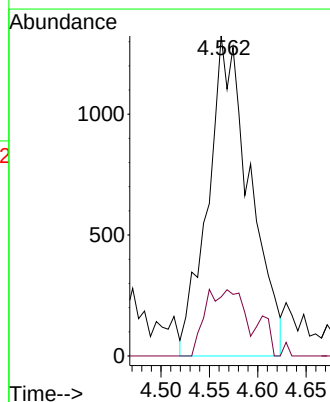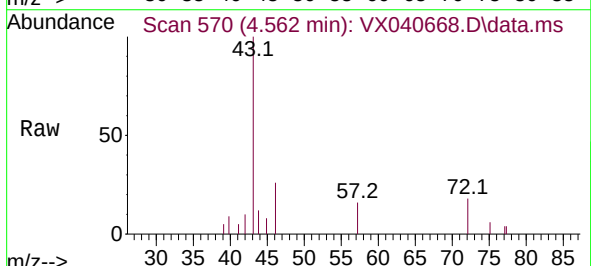

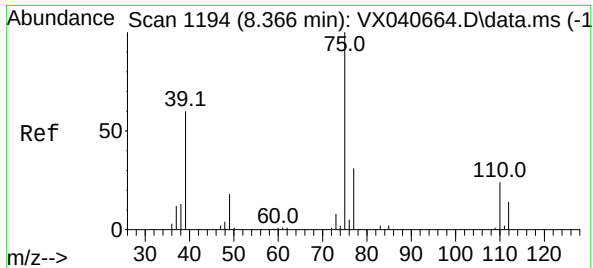

#39
 cis-1,3-Dichloropropene
 Concen: 1.455 ug/L
 RT: 8.318 min Scan# 11
 Delta R.T. -0.049 min
 Lab File: VX040668.D
 Acq: 15 Mar 2024 21:21

Instrument :
 MSVOA_X
 ClientSampleId :

Tgt Ion: 75 Resp: 2438
 Ion Ratio Lower Upper
 75 100
 77 38.0 21.1 39.3

