

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
 Data File : VX040656.D
 Acq On : 15 Mar 2024 16:01
 Operator : JC/MD
 Sample : P1753-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YCKY6

Quant Time: Mar 16 02:54:07 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 16 01:57:16 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	148560	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	141347	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	67534	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	46668	35.836	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	71.680%
7) Chloroethane-d5	1.666	69	42531	40.908	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	81.820%
11) 1,1-Dichloroethene-d2	2.306	65	22713	37.888	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	75.780%
21) 2-Butanone-d5	4.446	46	96435	96.501	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	96.500%
24) Chloroform-d	5.056	84	108642	44.923	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.840%
26) 1,2-Dichloroethane-d4	5.958	65	81529	45.154	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.300%
32) Benzene-d6	5.970	84	190136	43.846	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.700%
36) 1,2-Dichloropropane-d6	7.305	67	62003	46.134	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	92.260%
41) Toluene-d8	8.647	98	167958	40.190	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	80.380%
43) trans-1,3-Dichloroprop...	8.945	79	30183	42.196	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	84.400%
47) 2-Hexanone-d5	9.384	63	69299	93.448	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	93.450%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	94940	47.181	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	94.360%
66) 1,2-Dichlorobenzene-d4	12.323	152	66817	47.238	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.480%
Target Compounds						
					Qvalue	
13) Acetone	2.379	43	156353	219.099	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
Data File : VX040656.D
Acq On : 15 Mar 2024 16:01
Operator : JC/MD
Sample : P1753-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YCKY6

Quant Time: Mar 16 02:54:07 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 16 01:57:16 2024
Response via : Initial Calibration

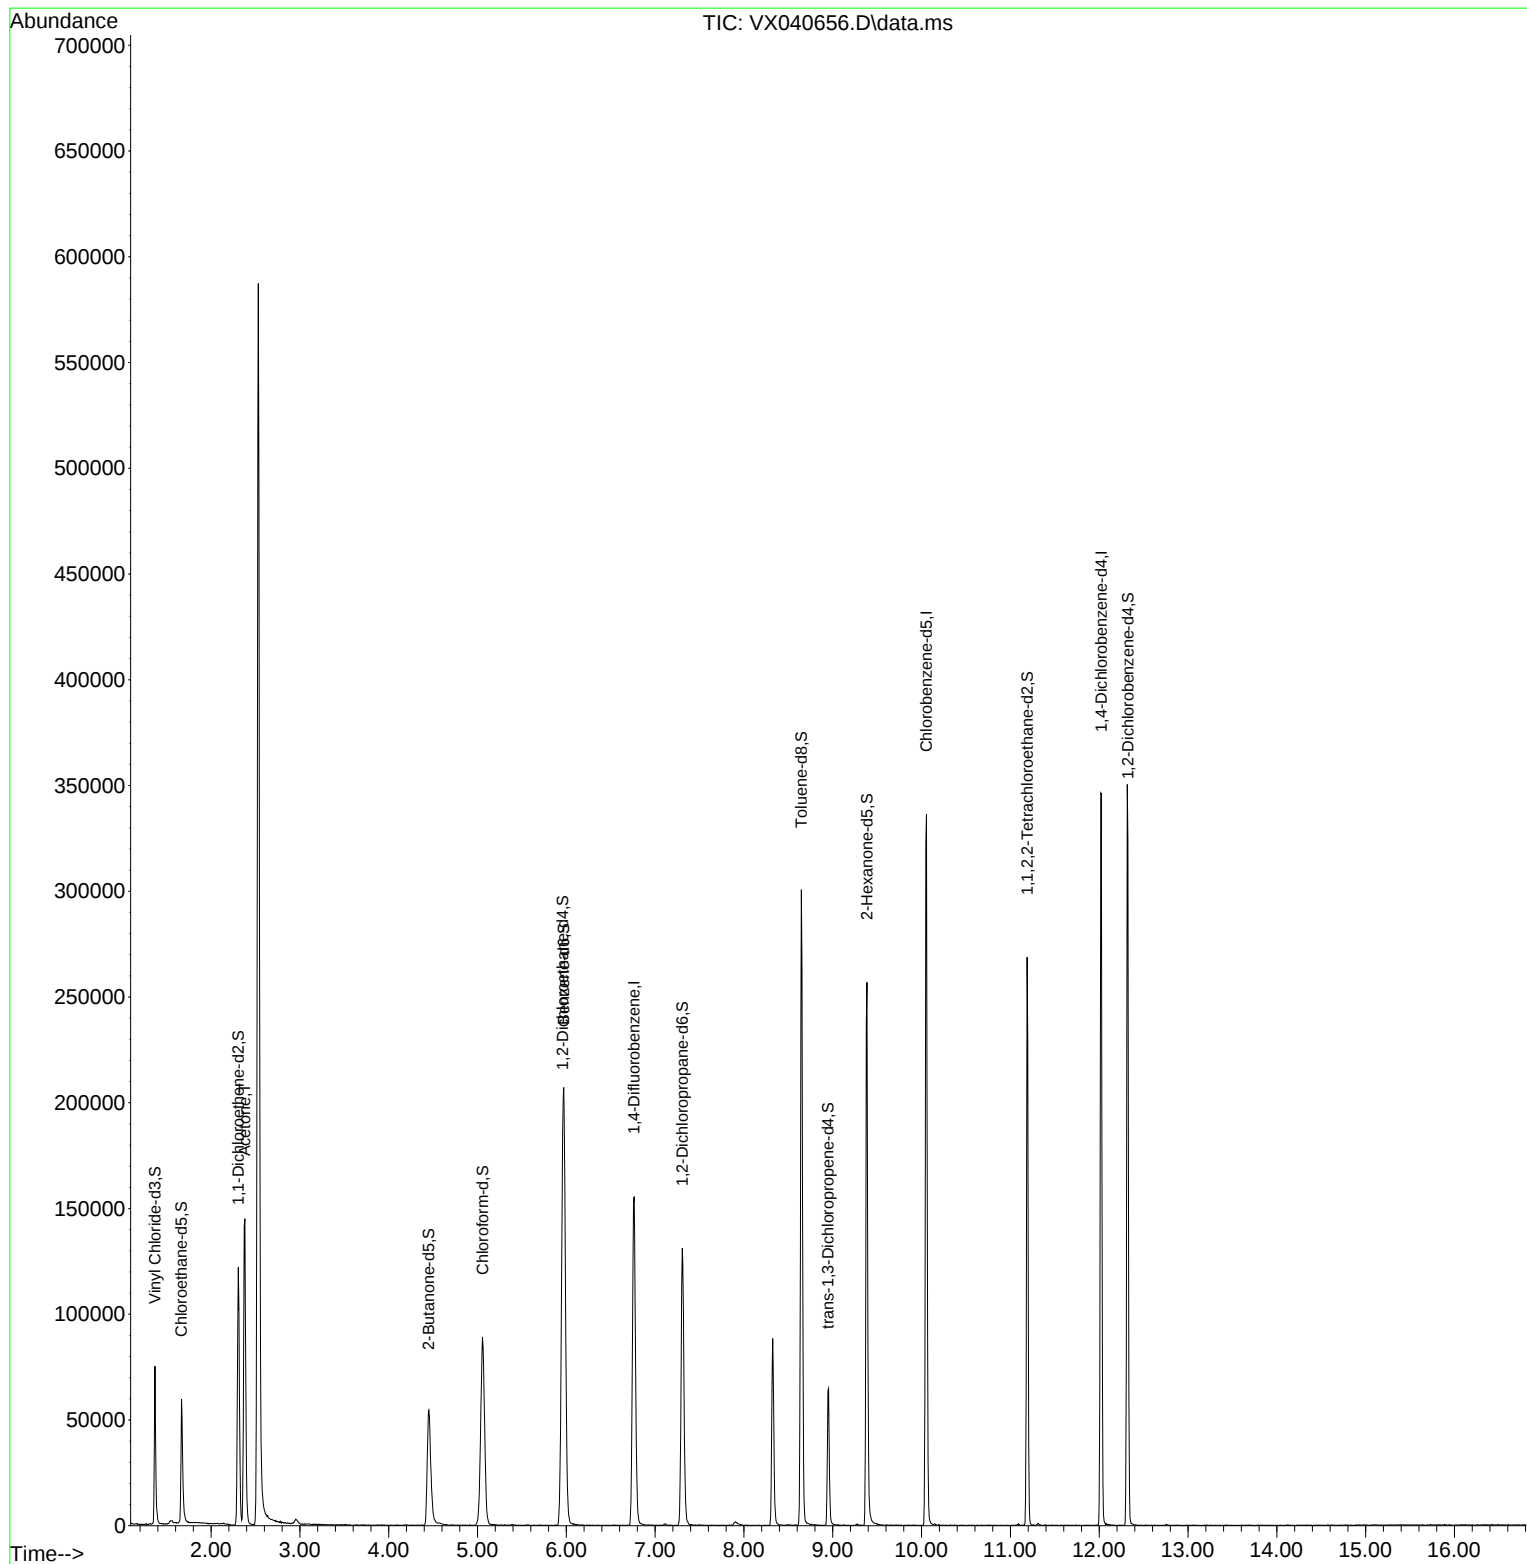

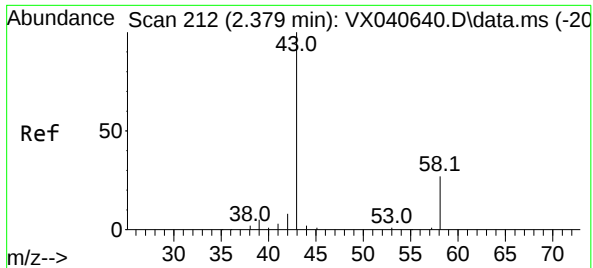

#13
 Acetone
 Concen: 219.099 ug/L
 RT: 2.379 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: VX040656.D
 Acq: 15 Mar 2024 16:01

Instrument :
 MSVOA_X
 ClientSampleId :
 YCKY6

Tgt Ion: 43 Resp: 156353
 Ion Ratio Lower Upper
 43 100
 58 26.6 0.0 54.6

