

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
 Data File : VX040658.D
 Acq On : 15 Mar 2024 16:47
 Operator : JC/MD
 Sample : P1753-17
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YCKY8

Quant Time: Mar 16 02:54:35 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 16 01:57:16 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	147576	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	138211	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	63798	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	46896	36.251	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	72.500%
7) Chloroethane-d5	1.666	69	42654	41.300	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	82.600%
11) 1,1-Dichloroethene-d2	2.306	65	21348	35.849	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	71.700%
21) 2-Butanone-d5	4.446	46	93859	94.550	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	94.550%
24) Chloroform-d	5.056	84	106681	44.406	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.820%
26) 1,2-Dichloroethane-d4	5.952	65	80396	44.824	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.640%
32) Benzene-d6	5.976	84	185227	43.683	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.360%
36) 1,2-Dichloropropane-d6	7.305	67	60422	45.977	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	91.960%
41) Toluene-d8	8.647	98	165670	40.542	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	81.080%
43) trans-1,3-Dichloroprop...	8.951	79	29667	42.415	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	84.840%
47) 2-Hexanone-d5	9.384	63	67689	93.348	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	93.350%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	95308	48.439	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	96.880%
66) 1,2-Dichlorobenzene-d4	12.323	152	59933	44.853	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	89.700%
Target Compounds						
					Qvalue	
13) Acetone	2.373	43	116273	164.021	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
Data File : VX040658.D
Acq On : 15 Mar 2024 16:47
Operator : JC/MD
Sample : P1753-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YCKY8

Quant Time: Mar 16 02:54:35 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM030724WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 16 01:57:16 2024
Response via : Initial Calibration

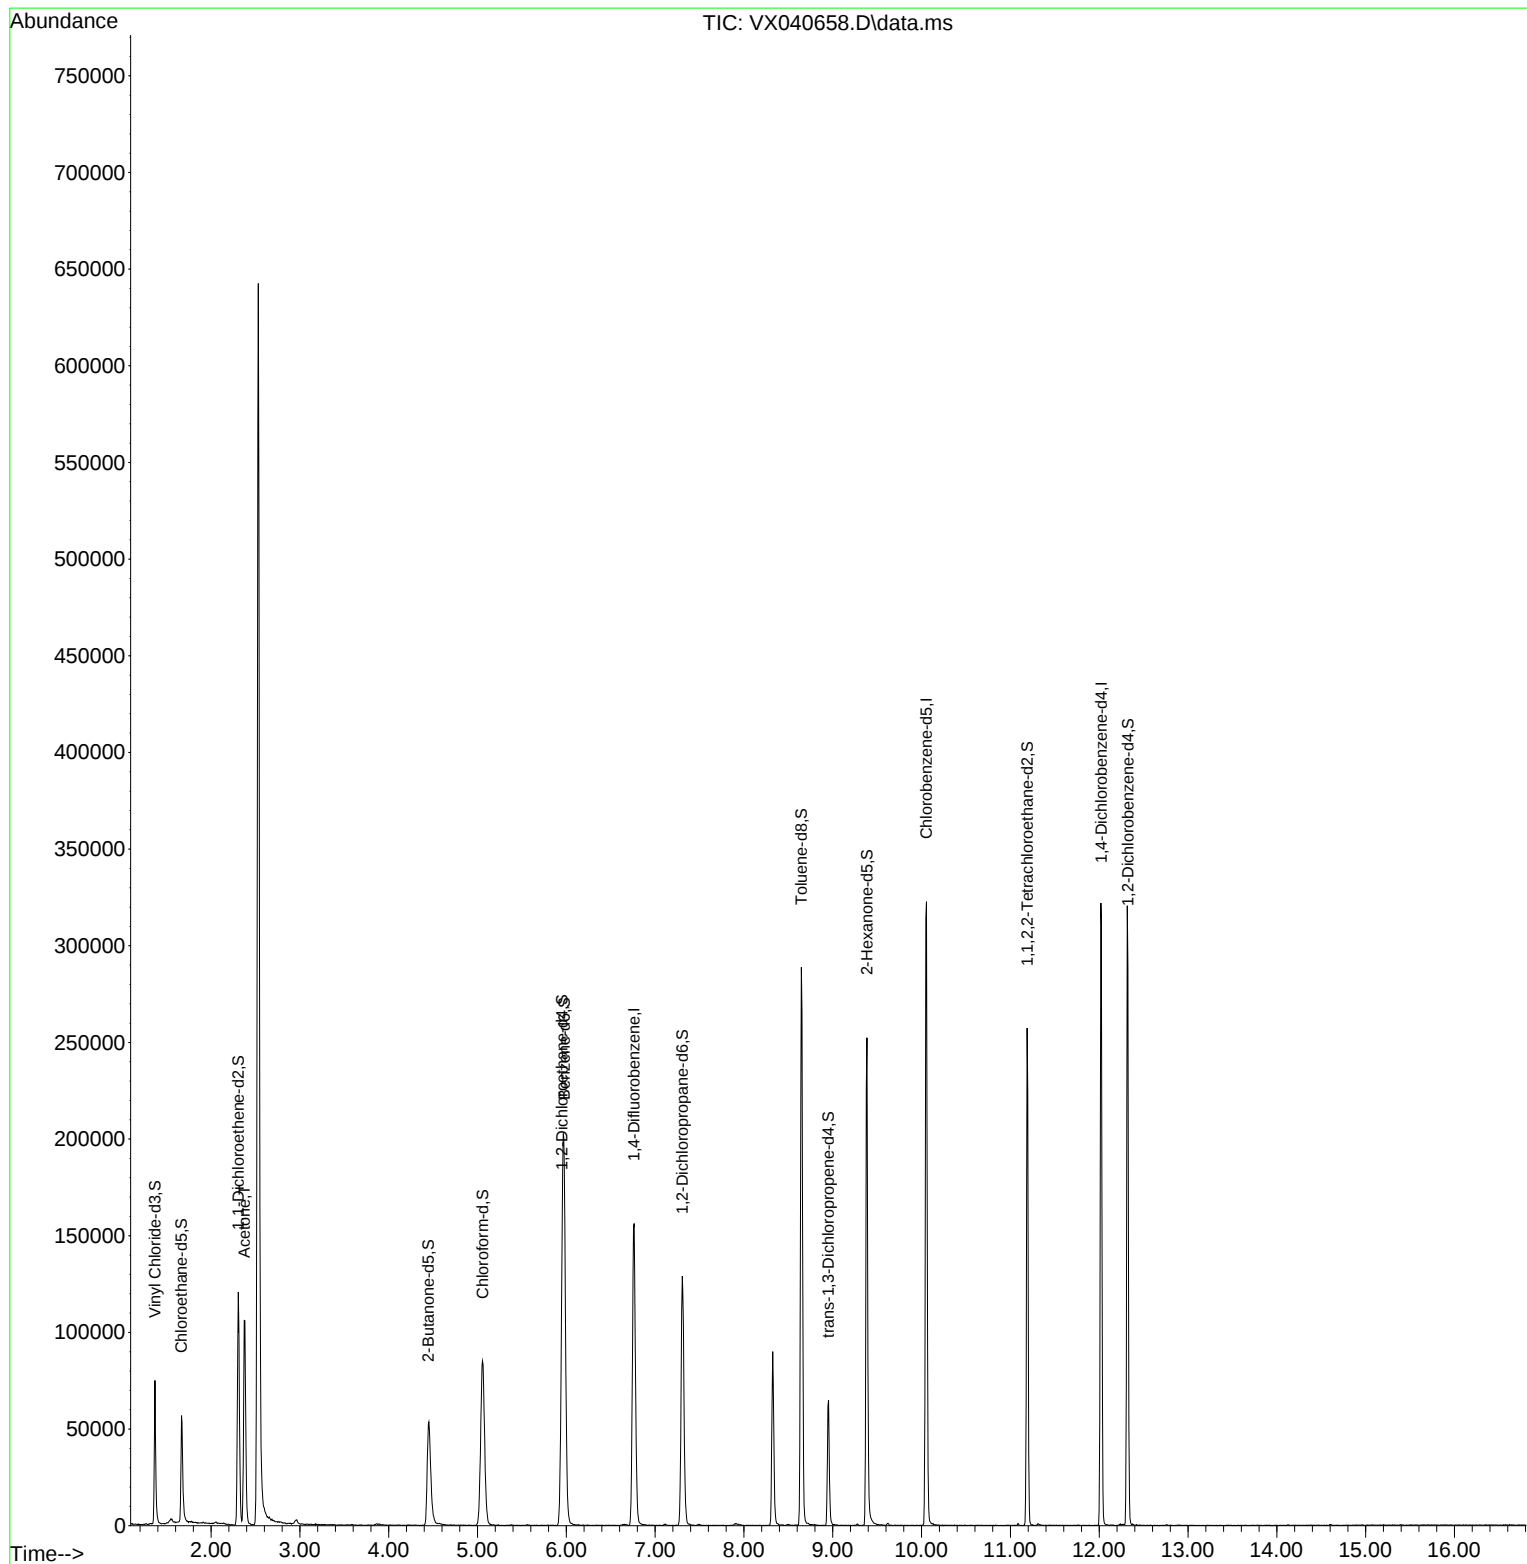

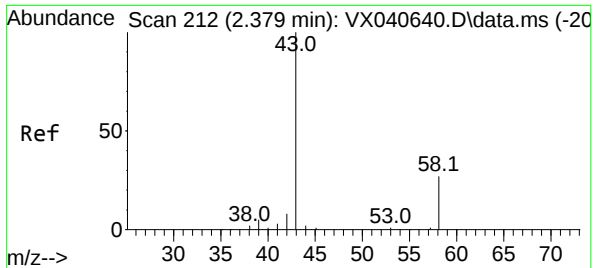

#13
 Acetone
 Concen: 164.021 ug/L
 RT: 2.373 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: VX040658.D
 Acq: 15 Mar 2024 16:47

Instrument :
 MSVOA_X
 ClientSampleId :
 YCKY8

Tgt Ion: 43 Resp: 116273
 Ion Ratio Lower Upper
 43 100
 58 26.4 0.0 54.6

