

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
 Data File : VX040674.D
 Acq On : 15 Mar 2024 23:38
 Operator : JC/MD
 Sample : P1754-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YCL21

Manual Integrations
 APPROVED

Reviewed By : John Carlone 03/18/2024
 Supervised By : Semsettin Yesilyurt 03/19/2024

Quant Time: Mar 16 05:54:41 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 16 05:02:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	147240	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	139551	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	61008	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	43798	33.934	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	67.860%		
7) Chloroethane-d5	1.666	69	41752	40.519	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	81.040%		
11) 1,1-Dichloroethene-d2	2.306	65	21217	35.710	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	71.420%		
21) 2-Butanone-d5	4.452	46	98582	99.534	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	99.530%		
24) Chloroform-d	5.056	84	108546	45.286	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	90.580%		
26) 1,2-Dichloroethane-d4	5.952	65	81330	45.448	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	90.900%		
32) Benzene-d6	5.976	84	183881	42.949	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	85.900%		
36) 1,2-Dichloropropane-d6	7.305	67	59657	44.959	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	89.920%		
41) Toluene-d8	8.647	98	161375	39.112	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	78.220%#		
43) trans-1,3-Dichloroprop...	8.952	79	28887	40.903	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	81.800%		
47) 2-Hexanone-d5	9.384	63	68866	94.059	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	94.060%		
56) 1,1,2,2-Tetrachloroeth...	11.189	84	95923	48.283	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	96.560%		
66) 1,2-Dichlorobenzene-d4	12.323	152	60220	47.128	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	94.260%		
Target Compounds						Qvalue
12) 1,1-Dichloroethene	2.319	96	38647	43.061	ug/L	98
13) Acetone	2.380	43	28062	39.676	ug/L	98
19) 1,1-Dichloroethane	3.611	63	6974	3.896	ug/L	97
20) cis-1,2-Dichloroethene	4.489	96	11736	11.359	ug/L	95
30) 1,1,1-Trichloroethane	5.391	97	5178m	2.979	ug/L	
34) Trichloroethene	7.123	95	38504	34.792	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
Data File : VX040674.D
Acq On : 15 Mar 2024 23:38
Operator : JC/MD
Sample : P1754-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 38 Sample Multiplier: 1


Instrument :
MSVOA_X
ClientSampleId :
YCL21

Quant Time: Mar 16 05:54:41 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 16 05:02:38 2024
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :John Carlone 03/18/2024
Supervised By :Semsettin Yesilyurt 03/19/2024

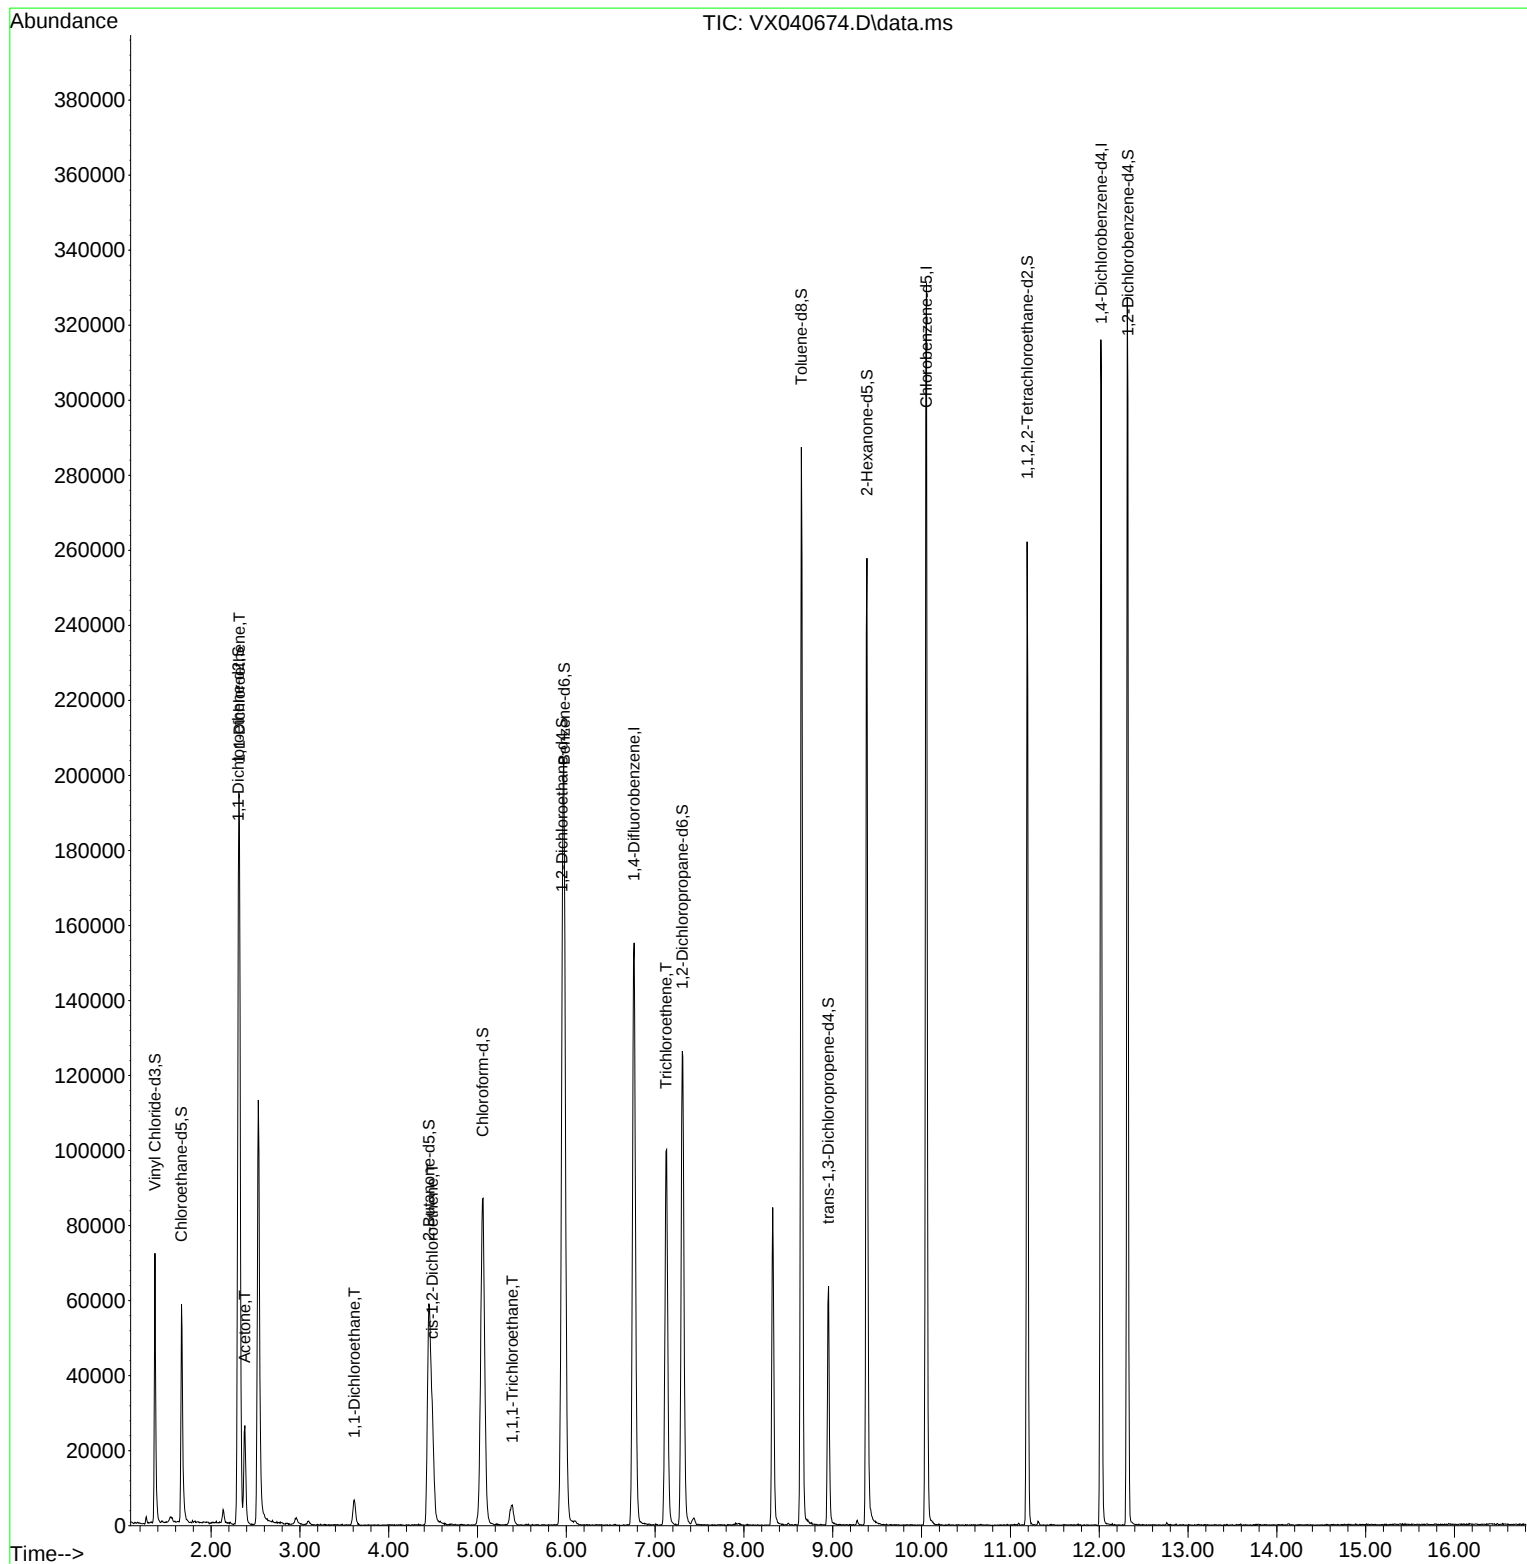

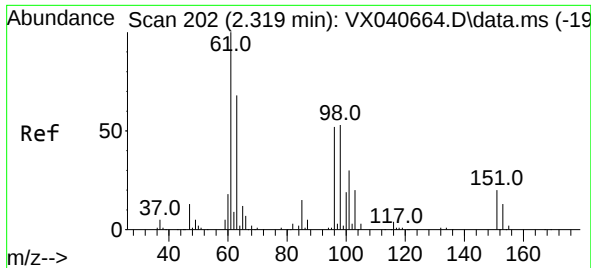





#12
1,1-Dichloroethene
Concen: 43.061 ug/L
RT: 2.319 min Scan# 202
Delta R.T. -0.000 min
Lab File: VX040674.D
Acq: 15 Mar 2024 23:38

Instrument :
MSVOA_X
ClientSampleId :
YCL21

Tgt Ion: 96 Resp: 3864
Ion Ratio Lower Upper
96 100
61 189.3 134.8 250.4
63 134.9 92.5 171.9




Manual Integrations
APPROVED


Reviewed By :John Carlone 03/18/2024
Supervised By :Semsettin Yesilyurt 03/19/2024

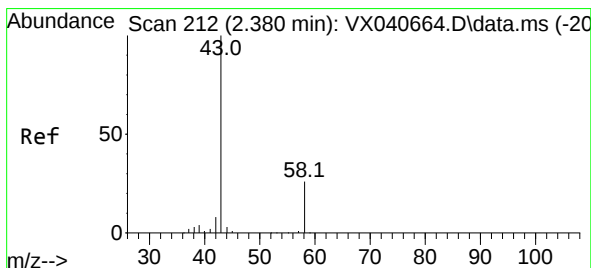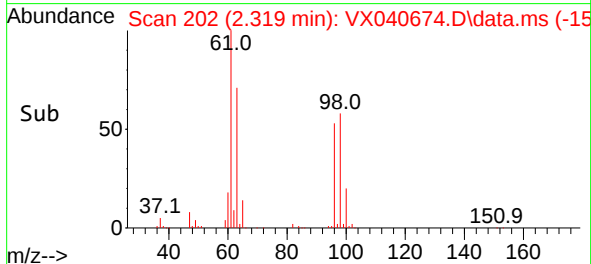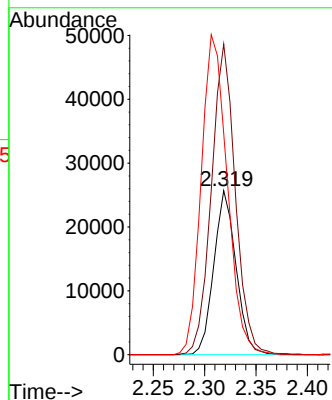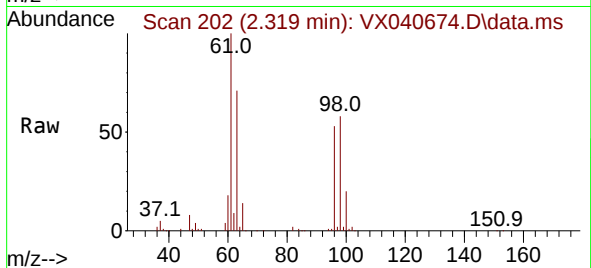

#13
Acetone
Concen: 39.676 ug/L
RT: 2.380 min Scan# 212
Delta R.T. -0.000 min
Lab File: VX040674.D
Acq: 15 Mar 2024 23:38

Tgt Ion: 43 Resp: 28062
Ion Ratio Lower Upper
43 100
58 26.3 0.0 54.6

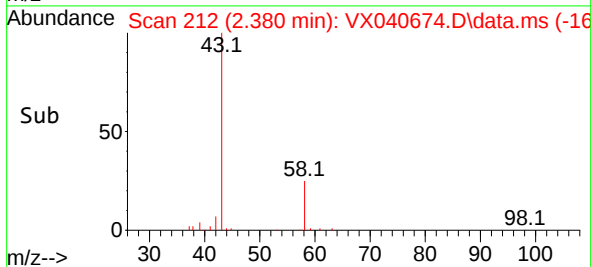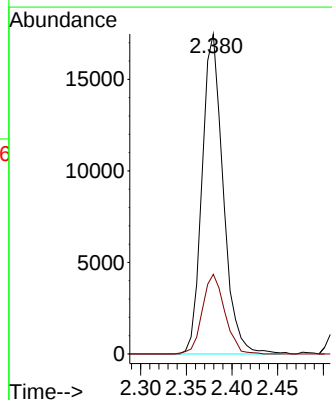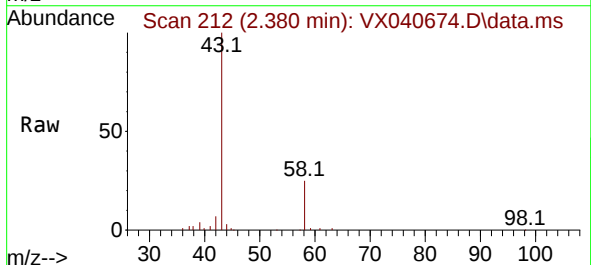

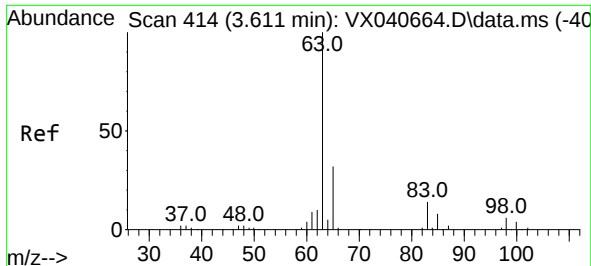

#19

1,1-Dichloroethane

Concen: 3.896 ug/L

RT: 3.611 min Scan# 414

Delta R.T. -0.000 min

Lab File: VX040674.D

Acq: 15 Mar 2024 23:38

Instrument :

MSVOA_X

ClientSampleId :

YCL21

Tgt Ion: 63 Resp: 6974





Ion	Ratio	Lower	Upper
63	100		
65	33.6	23.1	42.9
83	11.1	9.9	18.5

Manual Integrations

APPROVED

Reviewed By :John Carlone 03/18/2024

Supervised By :Semsettin Yesilyurt 03/19/2024

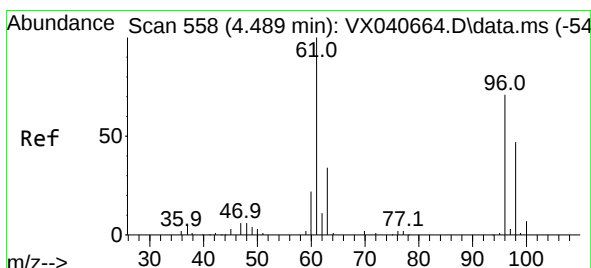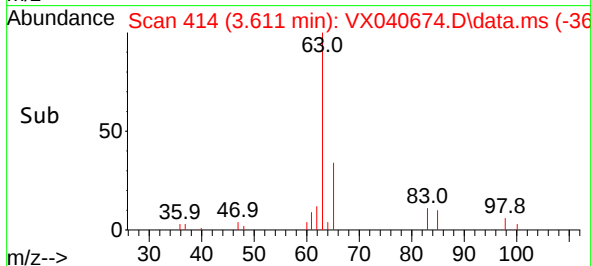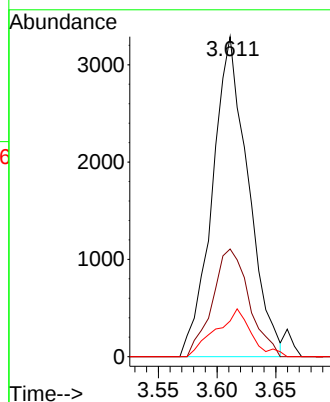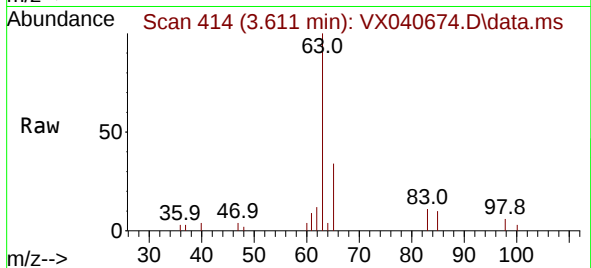

#20

cis-1,2-Dichloroethene

Concen: 11.359 ug/L

RT: 4.489 min Scan# 558




Delta R.T. -0.000 min


Lab File: VX040674.D

Acq: 15 Mar 2024 23:38

Tgt Ion: 96 Resp: 11736

Ion	Ratio	Lower	Upper
96	100		
61	138.7	93.0	172.8
98	63.3	42.4	78.6

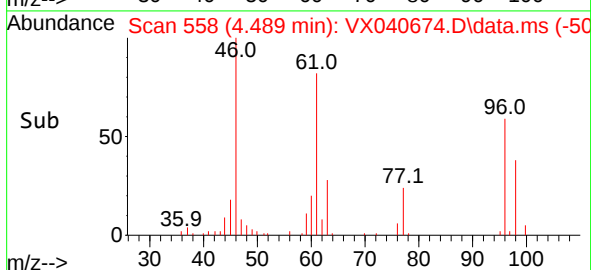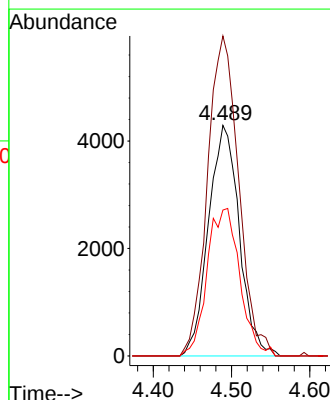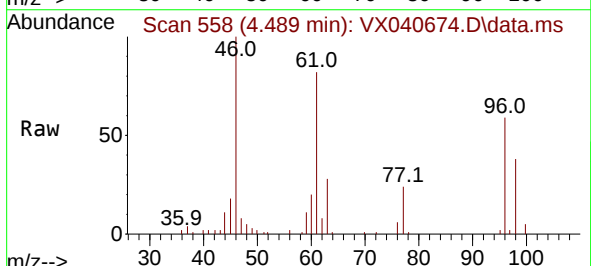

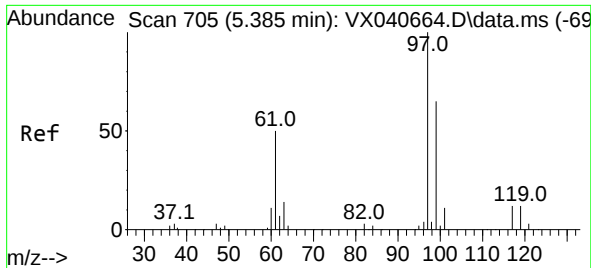





#30
1,1,1-Trichloroethane
Concen: 2.979 ug/L m
RT: 5.391 min Scan# 705
Delta R.T. 0.006 min
Lab File: VX040674.D
Acq: 15 Mar 2024 23:38

Instrument :
MSVOA_X
ClientSampleId :
YCL21

Tgt Ion: 97 Resp: 5178
Ion Ratio Lower Upper
97 100
99 57.9 52.1 78.1
61 32.0 38.3 57.5

Manual Integrations
APPROVED

Reviewed By :John Carlone 03/18/2024
Supervised By :Semsettin Yesilyurt 03/19/2024

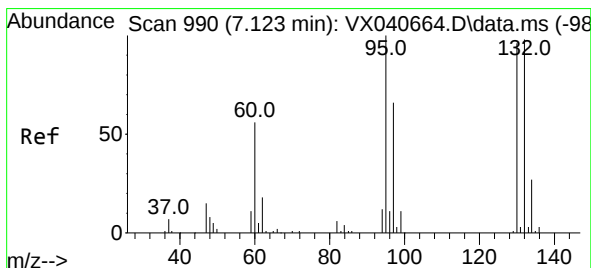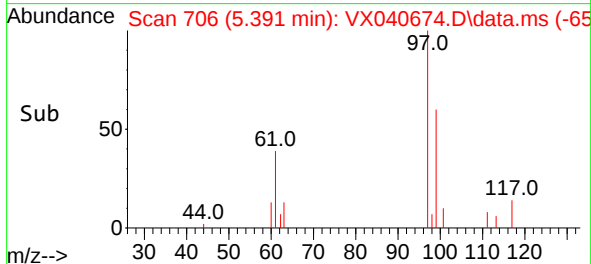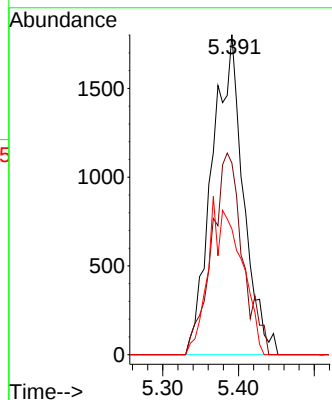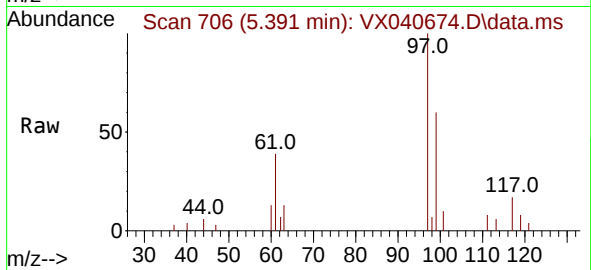

#34
Trichloroethene
Concen: 34.792 ug/L
RT: 7.123 min Scan# 990
Delta R.T. -0.000 min
Lab File: VX040674.D
Acq: 15 Mar 2024 23:38

Tgt Ion: 95 Resp: 38504
Ion Ratio Lower Upper
95 100
97 62.0 44.7 83.1
132 81.6 61.5 114.3
130 87.2 66.9 124.3

