

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
 Data File : VX040644.D
 Acq On : 15 Mar 2024 11:26
 Operator : JC/MD
 Sample : P1753-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YCKZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
 Title : VOC Analysis

Signal : TIC: VX040644.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	7	9	11	rBV2	547	492	0.05%	0.008%
2	1.368	41	46	52	rBV	84787	92161	8.93%	1.432%
3	1.557	70	77	80	rBV5	1553	2986	0.29%	0.046%
4	1.666	91	95	108	rVB	60439	86214	8.36%	1.339%
5	2.136	168	172	178	rBV5	2231	3482	0.34%	0.054%
6	2.252	190	191	194	rBV2	200	242	0.02%	0.004%
7	2.306	194	200	206	rVV	132146	203318	19.71%	3.159%
8	2.380	206	212	226	rVB	127056	212303	20.58%	3.298%
9	2.532	230	237	260	rBV	583346	1031578	100.00%	16.026%
10	3.434	383	385	386	rBV2	278	255	0.02%	0.004%
11	3.617	406	415	421	rBV4	1031	2487	0.24%	0.039%
12	3.794	441	444	445	rBV2	285	253	0.02%	0.004%
13	3.904	459	462	464	rBV2	233	248	0.02%	0.004%
14	3.953	467	470	473	rVB2	255	413	0.04%	0.006%
15	4.001	473	478	482	rBV3	275	630	0.06%	0.010%
16	4.142	498	501	503	rBV3	234	305	0.03%	0.005%
17	4.166	503	505	509	rVB	228	215	0.02%	0.003%
18	4.209	509	512	513	rBV	178	237	0.02%	0.004%
19	4.300	524	527	530	rBV2	238	338	0.03%	0.005%
20	4.452	543	552	566	rBV	56839	161169	15.62%	2.504%
21	4.715	594	595	599	rBV2	179	215	0.02%	0.003%
22	4.776	601	605	606	rBV2	178	218	0.02%	0.003%
23	5.056	635	651	668	rBV	91491	293540	28.46%	4.560%
24	5.330	694	696	700	rBV2	213	310	0.03%	0.005%
25	5.373	700	703	704	rBV2	554	606	0.06%	0.009%
26	5.550	729	732	734	rBV3	484	577	0.06%	0.009%
27	5.666	747	751	752	rBV2	399	446	0.04%	0.007%
28	5.964	789	800	817	rBV2	216397	657191	63.71%	10.210%
29	6.294	852	854	857	rVB2	229	233	0.02%	0.004%
30	6.330	857	860	862	rBV	273	295	0.03%	0.005%
31	6.476	881	884	885	rVB	290	291	0.03%	0.005%
32	6.507	885	889	890	rBV	219	236	0.02%	0.004%
33	6.623	905	908	915	rVB2	232	398	0.04%	0.006%
34	6.757	918	930	947	rBV	159707	383741	37.20%	5.962%
35	7.031	973	975	976	rBV2	250	220	0.02%	0.003%
36	7.129	982	991	1000	rBV4	8768	19922	1.93%	0.310%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
 Data File : VX040644.D
 Acq On : 15 Mar 2024 11:26
 Operator : JC/MD
 Sample : P1753-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YCKZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
 Title : VOC Analysis

37	7.306	1012	1020	1037	rBV2	133973	302121	29.29%	4.694%
38	7.434	1037	1041	1046	rVB4	1939	3554	0.34%	0.055%
39	7.580	1061	1065	1067	rBV	285	336	0.03%	0.005%
40	7.903	1113	1118	1122	rBV3	795	1688	0.16%	0.026%
41	8.324	1180	1187	1201	rBV	96049	158982	15.41%	2.470%
42	8.494	1212	1215	1218	rBV3	379	502	0.05%	0.008%
43	8.580	1225	1229	1234	rBV4	1041	1854	0.18%	0.029%
44	8.647	1234	1240	1249	rVV	317899	496064	48.09%	7.707%
45	8.714	1249	1251	1258	rVB3	1963	3064	0.30%	0.048%
46	8.952	1284	1290	1302	rVV	70738	109687	10.63%	1.704%
47	9.159	1320	1324	1329	rVB3	747	899	0.09%	0.014%
48	9.275	1339	1343	1348	rVB3	2822	4071	0.39%	0.063%
49	9.336	1348	1353	1355	rBV	210	292	0.03%	0.005%
50	9.384	1355	1361	1381	rBV	258933	383137	37.14%	5.952%
51	9.848	1432	1437	1439	rVB3	362	350	0.03%	0.005%
52	9.878	1439	1442	1444	rVB2	258	268	0.03%	0.004%
53	9.909	1444	1447	1448	rBV	177	206	0.02%	0.003%
54	10.055	1465	1471	1483	rBV	330460	474589	46.01%	7.373%
55	10.195	1491	1494	1500	rVB2	1554	2200	0.21%	0.034%
56	10.299	1508	1511	1518	rVB2	1441	2223	0.22%	0.035%
57	10.646	1563	1568	1570	rBV4	1936	2781	0.27%	0.043%
58	10.799	1591	1593	1596	rVB	351	335	0.03%	0.005%
59	10.860	1599	1603	1604	rBV2	172	212	0.02%	0.003%
60	10.963	1617	1620	1625	rVB	1307	1725	0.17%	0.027%
61	11.091	1638	1641	1646	rVB2	1159	1469	0.14%	0.023%
62	11.189	1652	1657	1672	rVB	275883	349992	33.93%	5.437%
63	11.311	1674	1677	1682	rVB	1791	2183	0.21%	0.034%
64	11.451	1696	1700	1705	rBV2	1362	1763	0.17%	0.027%
65	11.530	1708	1713	1714	rBV2	168	290	0.03%	0.005%
66	11.756	1746	1750	1754	rVV2	1628	1987	0.19%	0.031%
67	11.975	1782	1786	1788	rBV2	1370	1680	0.16%	0.026%
68	12.018	1788	1793	1803	rVV	359933	466039	45.18%	7.240%
69	12.189	1819	1821	1824	rVB	237	245	0.02%	0.004%
70	12.317	1837	1842	1851	rBV	385833	488238	47.33%	7.585%
71	12.597	1886	1888	1890	rBV	229	224	0.02%	0.003%
72	12.683	1899	1902	1904	rVV2	186	232	0.02%	0.004%
73	12.762	1912	1915	1920	rVB2	596	817	0.08%	0.013%
74	12.866	1930	1932	1936	rVV	299	375	0.04%	0.006%
75	13.109	1969	1972	1976	rBV2	926	1110	0.11%	0.017%
76	13.341	2007	2010	2014	rBV2	248	366	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
 Data File : VX040644.D
 Acq On : 15 Mar 2024 11:26
 Operator : JC/MD
 Sample : P1753-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YCKZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
 Title : VOC Analysis

77	13.591	2047	2051	2055	rVB3	1012	1237	0.12%	0.019%
78	13.780	2077	2082	2090	rVV2	1253	1746	0.17%	0.027%
79	13.932	2102	2107	2108	rBV	152	212	0.02%	0.003%
80	13.963	2108	2112	2117	rVB2	1017	1553	0.15%	0.024%
81	14.085	2129	2132	2134	rBV2	215	301	0.03%	0.005%
82	14.128	2137	2139	2143	rVB3	535	580	0.06%	0.009%
83	14.292	2163	2166	2169	rBV2	225	381	0.04%	0.006%
84	14.329	2169	2172	2174	rBV	342	282	0.03%	0.004%
85	14.463	2190	2194	2197	rBV2	228	372	0.04%	0.006%
86	14.609	2215	2218	2222	rBV2	278	396	0.04%	0.006%
87	14.701	2229	2233	2236	rBV2	273	343	0.03%	0.005%
88	14.871	2257	2261	2262	rVB	302	308	0.03%	0.005%
89	14.932	2269	2271	2274	rVB	239	207	0.02%	0.003%
90	15.255	2322	2324	2326	rBV	294	282	0.03%	0.004%
91	15.280	2326	2328	2330	rVV	240	226	0.02%	0.004%
92	15.396	2345	2347	2350	rVB	324	226	0.02%	0.004%
93	15.646	2386	2388	2390	rVV2	204	204	0.02%	0.003%
94	15.774	2405	2409	2411	rVB2	310	349	0.03%	0.005%
95	15.932	2433	2435	2436	rVB	438	246	0.02%	0.004%
96	15.963	2436	2440	2441	rBV2	237	318	0.03%	0.005%
97	16.036	2451	2452	2454	rBV	325	211	0.02%	0.003%
98	16.139	2466	2469	2472	rBV2	335	467	0.05%	0.007%
99	16.164	2472	2473	2476	rVV3	283	238	0.02%	0.004%
100	16.615	2544	2547	2548	rBV2	216	223	0.02%	0.003%




Sum of corrected areas: 6436823

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
Data File : VX040644.D
Acq On : 15 Mar 2024 11:26
Operator : JC/MD
Sample : P1753-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YCKZ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

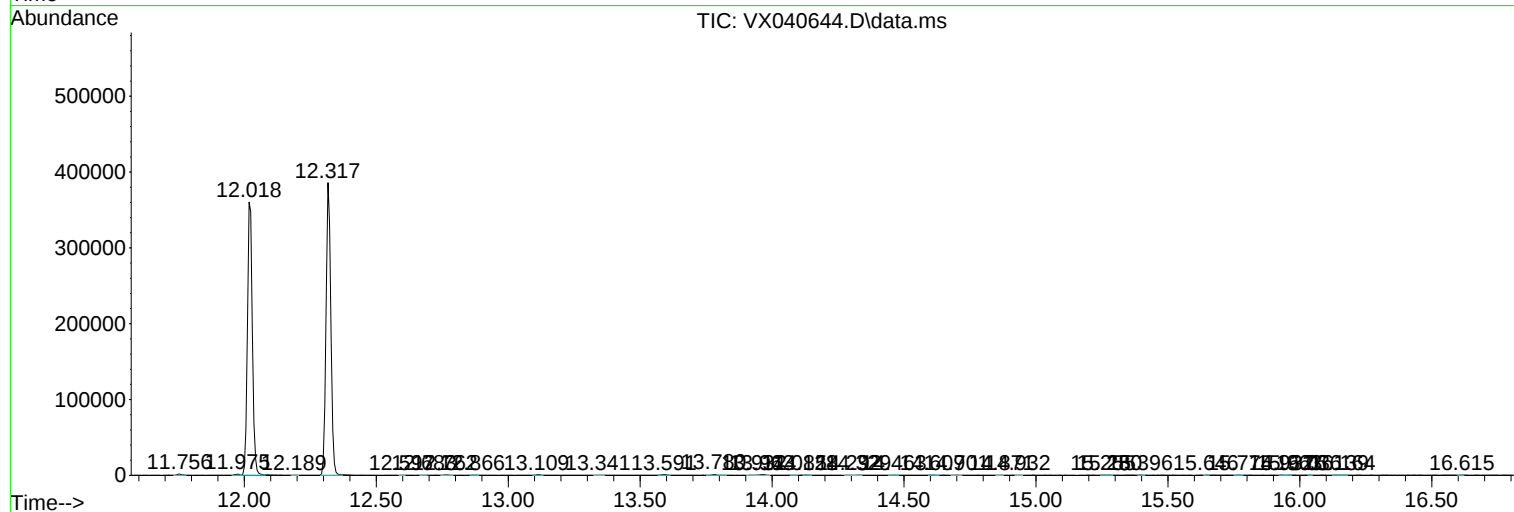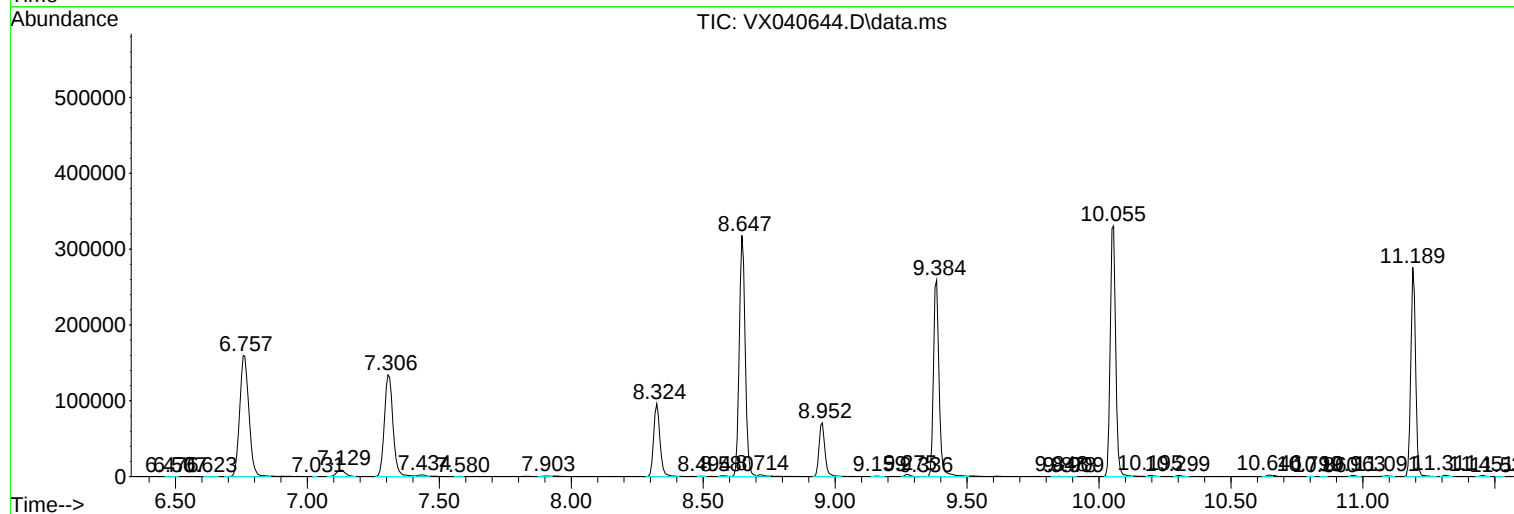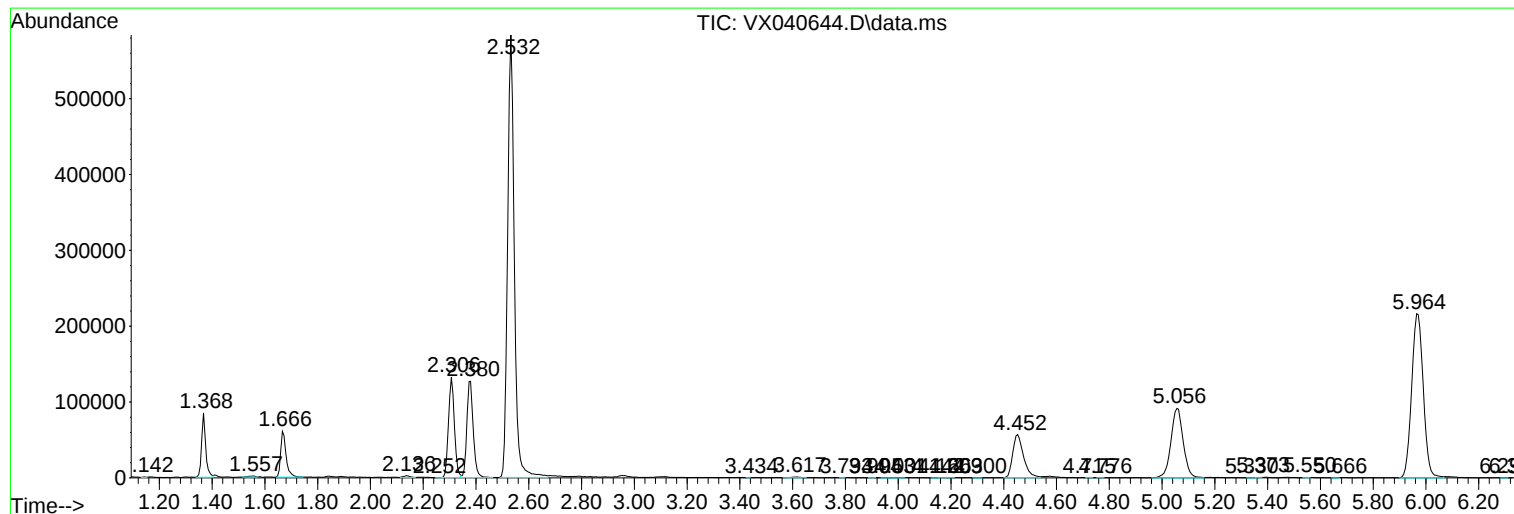

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
Data File : VX040644.D
Acq On : 15 Mar 2024 11:26
Operator : JC/MD
Sample : P1753-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YCKZ3










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.532	134.41 ug/L	1031580	1,4-Difluorobenzene	6.763

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	83
2			Isopropyl Alcohol	60	C3H8O	000067-63-0	78
3			Isopropyl Alcohol	60	C3H8O	000067-63-0	64
4			Hydrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	9
5			Hydrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	9

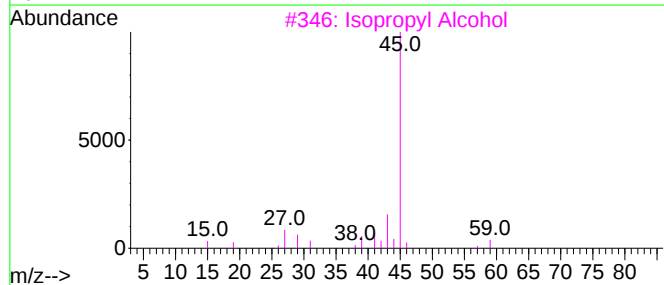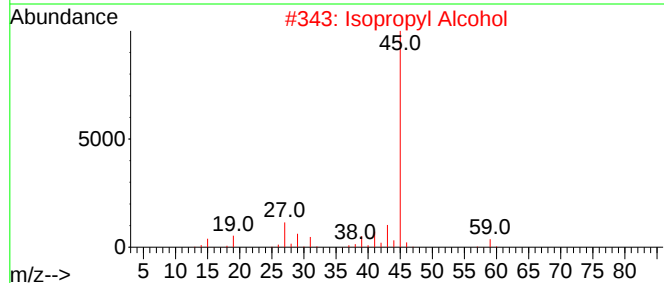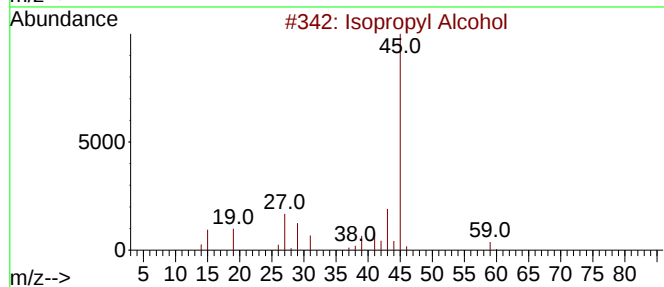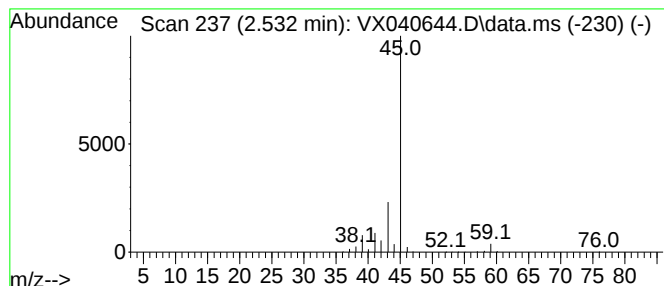

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
Data File : VX040644.D
Acq On : 15 Mar 2024 11:26
Operator : JC/MD
Sample : P1753-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YCKZ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.532	134.4	ug/L	1031580	1	6.763	383741	50.0