

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
 Data File : VX040652.D
 Acq On : 15 Mar 2024 14:29
 Operator : JC/MD
 Sample : P1753-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YCKW6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
 Title : VOC Analysis

Signal : TIC: VX040652.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.270	27	30	32	rBV2	1093	1025	0.16%	0.019%
2	1.368	41	46	57	rVB	79983	93201	14.74%	1.698%
3	1.666	91	95	107	rBV	57621	82373	13.03%	1.501%
4	2.136	168	172	178	rVB5	3649	5944	0.94%	0.108%
5	2.313	194	201	207	rBV2	155316	288310	45.60%	5.254%
6	2.374	207	211	223	rVB	180253	295673	46.76%	5.388%
7	2.532	230	237	254	rBV	96805	183254	28.98%	3.339%
8	3.379	373	376	379	rBV2	172	271	0.04%	0.005%
9	3.617	403	415	425	rVB2	7909	19035	3.01%	0.347%
10	3.690	425	427	429	rBV2	140	178	0.03%	0.003%
11	3.776	439	441	443	rBV	144	172	0.03%	0.003%
12	3.812	446	447	449	rBV	331	231	0.04%	0.004%
13	4.452	543	552	565	rBV	54611	174988	27.67%	3.189%
14	4.745	598	600	602	rVB	219	189	0.03%	0.003%
15	4.922	627	629	631	rVB	197	184	0.03%	0.003%
16	4.940	631	632	633	rBV	261	138	0.02%	0.003%
17	5.056	635	651	665	rBV	89014	279965	44.28%	5.101%
18	5.208	674	676	677	rVB	270	150	0.02%	0.003%
19	5.263	683	685	687	rBV2	285	244	0.04%	0.004%
20	5.294	687	690	691	rBV	160	192	0.03%	0.003%
21	5.379	697	704	706	rBV2	3655	6513	1.03%	0.119%
22	5.532	728	729	732	rBV	167	205	0.03%	0.004%
23	5.641	744	747	748	rBV2	144	144	0.02%	0.003%
24	5.702	756	757	759	rBV2	188	173	0.03%	0.003%
25	5.745	762	764	766	rVV	330	266	0.04%	0.005%
26	5.970	789	801	814	rBV2	211055	632326	100.00%	11.522%
27	6.281	848	852	853	rBV	173	179	0.03%	0.003%
28	6.367	864	866	868	rBV	159	144	0.02%	0.003%
29	6.403	870	872	874	rVB2	184	159	0.03%	0.003%
30	6.440	874	878	879	rBV2	167	237	0.04%	0.004%
31	6.544	889	895	899	rVB2	245	422	0.07%	0.008%
32	6.623	906	908	913	rVB2	200	336	0.05%	0.006%
33	6.763	922	931	949	rBV	158724	379552	60.02%	6.916%
34	7.019	969	973	974	rBV2	158	240	0.04%	0.004%
35	7.117	986	989	993	rVB2	701	1049	0.17%	0.019%
36	7.196	998	1002	1004	rBV	242	339	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
 Data File : VX040652.D
 Acq On : 15 Mar 2024 14:29
 Operator : JC/MD
 Sample : P1753-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YCKW6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
 Title : VOC Analysis

37	7.306	1012	1020	1035	rBV	130996	291163	46.05%	5.306%
38	7.476	1047	1048	1055	rVB3	500	834	0.13%	0.015%
39	7.549	1058	1060	1063	rBV2	145	150	0.02%	0.003%
40	7.702	1083	1085	1087	rBV	203	160	0.03%	0.003%
41	7.860	1110	1111	1114	rBV	213	233	0.04%	0.004%
42	7.909	1114	1119	1124	rVV5	1403	3047	0.48%	0.056%
43	8.007	1134	1135	1138	rBV2	134	166	0.03%	0.003%
44	8.324	1180	1187	1198	rBV	89825	149345	23.62%	2.721%
45	8.647	1234	1240	1250	rBV	306888	476169	75.30%	8.677%
46	8.952	1284	1290	1302	rBV	67991	102160	16.16%	1.862%
47	9.074	1308	1310	1312	rBV2	275	203	0.03%	0.004%
48	9.281	1339	1344	1348	rVB2	586	983	0.16%	0.018%
49	9.384	1355	1361	1384	rBV	249927	368464	58.27%	6.714%
50	9.701	1412	1413	1416	rBV2	249	205	0.03%	0.004%
51	10.055	1465	1471	1485	rVV	338182	470912	74.47%	8.581%
52	10.195	1493	1494	1496	rVV2	330	159	0.03%	0.003%
53	10.232	1499	1500	1503	rBV	211	210	0.03%	0.004%
54	10.640	1564	1567	1568	rBV	193	209	0.03%	0.004%
55	10.653	1568	1569	1572	rVV2	263	177	0.03%	0.003%
56	10.750	1583	1585	1587	rVB2	247	164	0.03%	0.003%
57	10.781	1587	1590	1591	rVB	233	225	0.04%	0.004%
58	10.799	1591	1593	1594	rBV	205	157	0.02%	0.003%
59	10.915	1609	1612	1614	rBV	195	217	0.03%	0.004%
60	10.970	1619	1621	1623	rBV	150	153	0.02%	0.003%
61	11.085	1637	1640	1644	rBV3	515	702	0.11%	0.013%
62	11.189	1652	1657	1674	rVV	250910	312410	49.41%	5.693%
63	11.311	1674	1677	1682	rVV3	1007	1233	0.19%	0.022%
64	11.409	1688	1693	1694	rBV	187	222	0.04%	0.004%
65	11.561	1715	1718	1720	rBV	202	265	0.04%	0.005%
66	11.622	1726	1728	1729	rBV	178	140	0.02%	0.003%
67	11.713	1742	1743	1744	rBV	272	141	0.02%	0.003%
68	11.860	1764	1767	1771	rBV	145	222	0.04%	0.004%
69	11.902	1772	1774	1776	rVV2	161	142	0.02%	0.003%
70	11.969	1783	1785	1788	rVB2	250	229	0.04%	0.004%
71	12.018	1788	1793	1802	rBV	323615	422546	66.82%	7.700%
72	12.189	1818	1821	1823	rVB	198	185	0.03%	0.003%
73	12.317	1837	1842	1851	rBV	329301	429173	67.87%	7.820%
74	12.396	1853	1855	1857	rVB2	388	244	0.04%	0.004%
75	12.469	1864	1867	1871	rVB2	241	315	0.05%	0.006%
76	12.518	1871	1875	1876	rBV	221	243	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
 Data File : VX040652.D
 Acq On : 15 Mar 2024 14:29
 Operator : JC/MD
 Sample : P1753-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YCKW6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
 Title : VOC Analysis

77	12.579	1884	1885	1888	rBV	200	137	0.02%	0.002%
78	12.616	1888	1891	1892	rBV2	154	148	0.02%	0.003%
79	12.762	1912	1915	1918	rVB2	489	582	0.09%	0.011%
80	12.994	1950	1953	1954	rBV	184	181	0.03%	0.003%
81	13.048	1960	1962	1964	rBV	161	139	0.02%	0.003%
82	13.195	1983	1986	1988	rBV2	171	230	0.04%	0.004%
83	13.262	1995	1997	2000	rBV	203	274	0.04%	0.005%
84	13.829	2087	2090	2093	rBV2	157	225	0.04%	0.004%
85	13.975	2113	2114	2118	rBV	203	218	0.03%	0.004%
86	14.128	2136	2139	2142	rBV3	312	426	0.07%	0.008%
87	14.286	2162	2165	2167	rBV	191	235	0.04%	0.004%
88	14.469	2193	2195	2196	rBV	231	165	0.03%	0.003%
89	14.530	2204	2205	2208	rVB2	274	137	0.02%	0.002%
90	14.609	2216	2218	2220	rVB2	440	337	0.05%	0.006%
91	14.762	2241	2243	2244	rBV	232	164	0.03%	0.003%
92	15.042	2287	2289	2292	rBV2	162	158	0.02%	0.003%
93	15.182	2311	2312	2314	rBV2	283	265	0.04%	0.005%
94	15.377	2340	2344	2345	rBV	227	303	0.05%	0.006%
95	15.572	2375	2376	2378	rBV	246	211	0.03%	0.004%
96	15.676	2392	2393	2398	rVB2	274	247	0.04%	0.005%
97	15.883	2426	2427	2430	rBV2	331	330	0.05%	0.006%
98	16.298	2493	2495	2496	rBV	218	142	0.02%	0.003%
99	16.481	2524	2525	2527	rBV	278	192	0.03%	0.003%
100	16.627	2547	2549	2550	rBV	247	187	0.03%	0.003%




Sum of corrected areas: 5487911

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
Data File : VX040652.D
Acq On : 15 Mar 2024 14:29
Operator : JC/MD
Sample : P1753-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YCKW6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

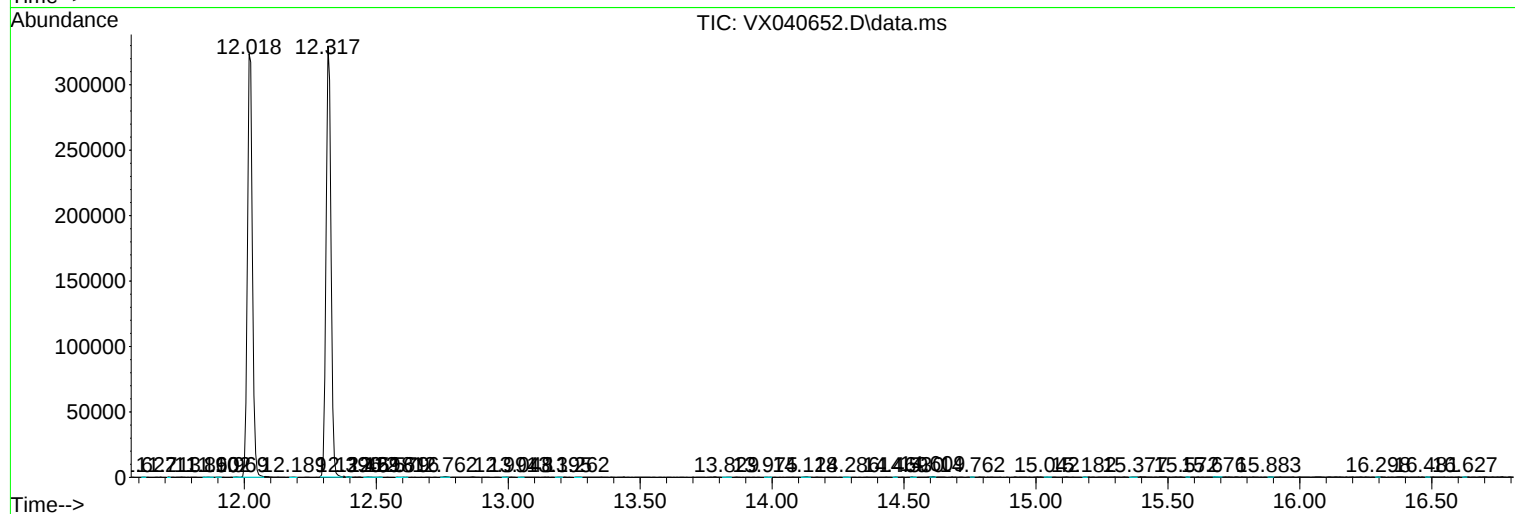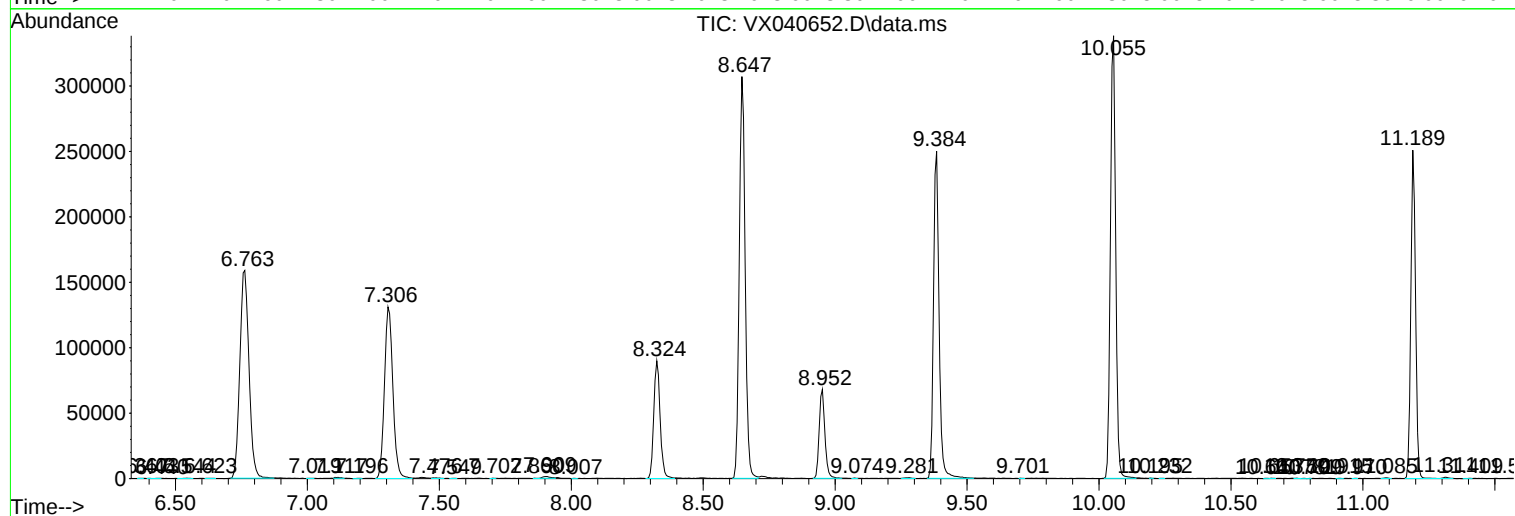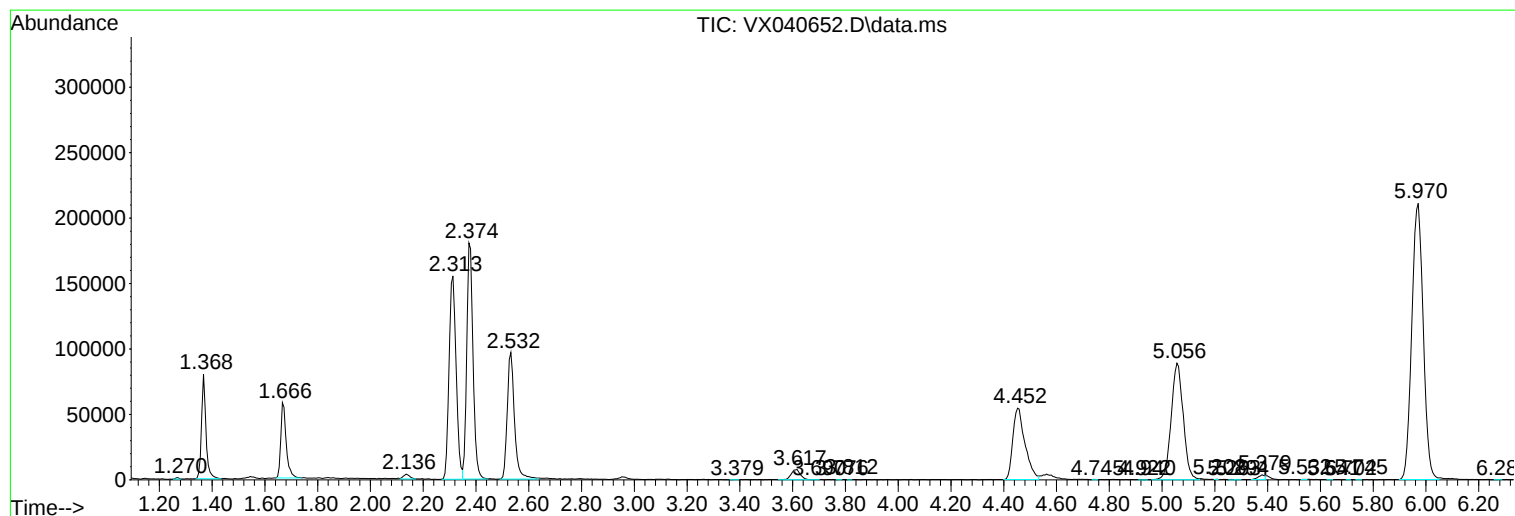

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
Data File : VX040652.D
Acq On : 15 Mar 2024 14:29
Operator : JC/MD
Sample : P1753-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YCKW6










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.532	24.14 ug/L	183254	1,4-Difluorobenzene	6.763

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	78
2			Isopropyl Alcohol	60	C3H8O	000067-63-0	56
3			Hydrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	9
4			Isopropyl Alcohol	60	C3H8O	000067-63-0	9
5			Hydrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	9

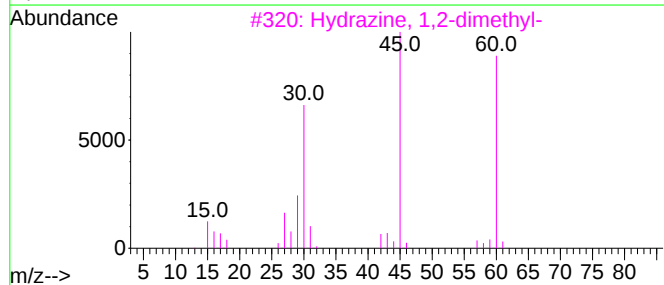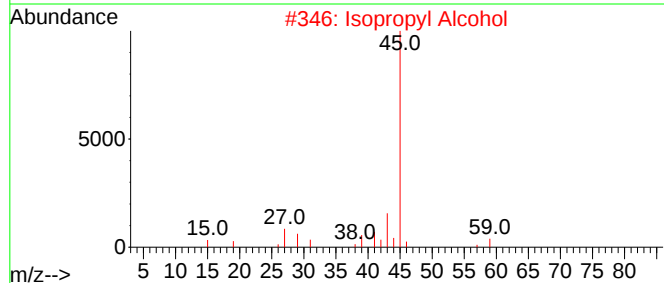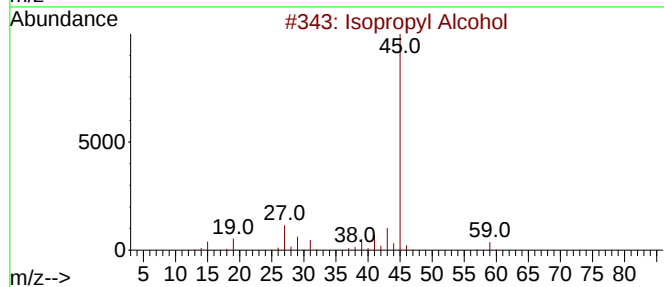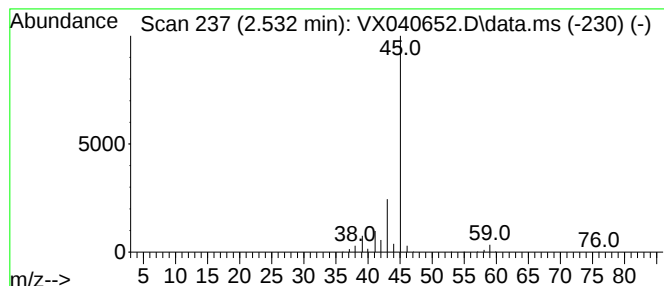

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
Data File : VX040652.D
Acq On : 15 Mar 2024 14:29
Operator : JC/MD
Sample : P1753-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YCKW6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.532	24.1	ug/L	183254	1	6.763	379552	50.0