

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
 Data File : VX040656.D
 Acq On : 15 Mar 2024 16:01
 Operator : JC/MD
 Sample : P1753-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YCKY6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
 Title : VOC Analysis

Signal : TIC: VX040656.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	55	rVB	74382	78154	7.58%	1.272%
2	1.666	91	95	107	rVB	58200	79565	7.72%	1.295%
3	2.306	194	200	206	rBV	121738	185429	17.99%	3.017%
4	2.379	206	212	224	rVB	144579	237773	23.06%	3.869%
5	2.532	229	237	253	rBV	586962	1030909	100.00%	16.773%
6	3.507	394	397	398	rBV	386	293	0.03%	0.005%
7	3.526	398	400	403	rVB3	302	267	0.03%	0.004%
8	3.678	422	425	426	rBV2	218	292	0.03%	0.005%
9	3.733	432	434	435	rBV	339	247	0.02%	0.004%
10	3.769	438	440	443	rVB2	196	234	0.02%	0.004%
11	4.263	519	521	525	rBV2	213	353	0.03%	0.006%
12	4.373	538	539	541	rBV2	213	171	0.02%	0.003%
13	4.452	543	552	567	rBV2	54257	155009	15.04%	2.522%
14	4.910	625	627	630	rBV	367	330	0.03%	0.005%
15	5.056	638	651	664	rBV	88932	270794	26.27%	4.406%
16	5.385	703	705	707	rBV2	317	264	0.03%	0.004%
17	5.544	729	731	732	rBV	273	259	0.03%	0.004%
18	5.970	789	801	817	rBV2	207162	626250	60.75%	10.189%
19	6.537	892	894	896	rBV	223	180	0.02%	0.003%
20	6.690	917	919	922	rVB	208	174	0.02%	0.003%
21	6.763	922	931	945	rBV	155546	375026	36.38%	6.102%
22	7.007	969	971	973	rBV2	265	278	0.03%	0.005%
23	7.049	975	978	982	rBV	220	303	0.03%	0.005%
24	7.116	982	989	995	rVV5	765	1652	0.16%	0.027%
25	7.305	1011	1020	1034	rVV	131125	287574	27.90%	4.679%
26	7.427	1038	1040	1042	rVB2	212	172	0.02%	0.003%
27	7.494	1047	1051	1053	rBV	326	527	0.05%	0.009%
28	7.641	1073	1075	1080	rBV2	232	459	0.04%	0.007%
29	7.720	1087	1088	1089	rBV2	261	154	0.01%	0.003%
30	7.903	1112	1118	1128	rBV6	1641	4812	0.47%	0.078%
31	8.165	1159	1161	1164	rVB	221	247	0.02%	0.004%
32	8.324	1181	1187	1201	rVV	88330	146262	14.19%	2.380%
33	8.573	1226	1228	1231	rBV	276	269	0.03%	0.004%
34	8.647	1234	1240	1250	rBV	300258	463719	44.98%	7.545%
35	8.951	1284	1290	1304	rVV	64554	98363	9.54%	1.600%
36	9.116	1314	1317	1318	rBV2	176	207	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
 Data File : VX040656.D
 Acq On : 15 Mar 2024 16:01
 Operator : JC/MD
 Sample : P1753-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YCKY6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
 Title : VOC Analysis

37	9.275	1335	1343	1349	rBV2	817	1529	0.15%	0.025%
38	9.317	1349	1350	1352	rBV	299	226	0.02%	0.004%
39	9.384	1355	1361	1377	rBV	256733	370026	35.89%	6.020%
40	9.640	1401	1403	1405	rBV	212	172	0.02%	0.003%
41	9.695	1408	1412	1414	rBV2	161	243	0.02%	0.004%
42	9.817	1429	1432	1433	rVB	170	147	0.01%	0.002%
43	9.848	1433	1437	1439	rBV	292	330	0.03%	0.005%
44	10.055	1465	1471	1484	rVV	336060	465104	45.12%	7.567%
45	10.195	1492	1494	1496	rVB	454	236	0.02%	0.004%
46	10.323	1512	1515	1516	rBV	254	256	0.02%	0.004%
47	10.372	1521	1523	1526	rVV2	221	227	0.02%	0.004%
48	10.567	1551	1555	1557	rBV2	235	335	0.03%	0.005%
49	10.628	1562	1565	1568	rVB	281	250	0.02%	0.004%
50	10.671	1568	1572	1574	rVB	252	294	0.03%	0.005%
51	10.689	1574	1575	1578	rBV2	148	180	0.02%	0.003%
52	10.756	1585	1586	1589	rBV2	238	193	0.02%	0.003%
53	11.091	1638	1641	1642	rBV2	673	564	0.05%	0.009%
54	11.189	1652	1657	1667	rVB	268529	334388	32.44%	5.440%
55	11.311	1674	1677	1681	rVB3	968	1268	0.12%	0.021%
56	11.384	1687	1689	1691	rBV2	191	161	0.02%	0.003%
57	11.469	1701	1703	1704	rVB2	264	157	0.02%	0.003%
58	11.494	1704	1707	1708	rBV2	149	181	0.02%	0.003%
59	11.567	1717	1719	1721	rVV	244	229	0.02%	0.004%
60	11.695	1739	1740	1743	rVB2	205	184	0.02%	0.003%
61	11.750	1743	1749	1751	rBV2	214	413	0.04%	0.007%
62	11.859	1765	1767	1768	rBV2	246	184	0.02%	0.003%
63	11.939	1778	1780	1783	rBV	142	153	0.01%	0.002%
64	12.018	1788	1793	1802	rBV	346222	453507	43.99%	7.379%
65	12.225	1824	1827	1829	rBV2	222	213	0.02%	0.003%
66	12.317	1837	1842	1854	rBV	350198	459573	44.58%	7.477%
67	12.457	1862	1865	1866	rBV	154	160	0.02%	0.003%
68	12.524	1875	1876	1879	rBV2	209	171	0.02%	0.003%
69	12.628	1891	1893	1895	rBV2	220	209	0.02%	0.003%
70	12.713	1905	1907	1910	rBV	167	174	0.02%	0.003%
71	12.756	1911	1914	1918	rVV2	347	482	0.05%	0.008%
72	12.993	1950	1953	1955	rVV2	270	309	0.03%	0.005%
73	13.408	2016	2021	2022	rBV2	121	169	0.02%	0.003%
74	13.499	2033	2036	2037	rBV2	186	206	0.02%	0.003%
75	13.579	2046	2049	2051	rBV2	136	159	0.02%	0.003%
76	13.603	2051	2053	2054	rVB	285	162	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
 Data File : VX040656.D
 Acq On : 15 Mar 2024 16:01
 Operator : JC/MD
 Sample : P1753-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YCKY6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
 Title : VOC Analysis

77	13.786	2078	2083	2084	rBV2	252	305	0.03%	0.005%
78	13.835	2089	2091	2093	rBV2	219	165	0.02%	0.003%
79	13.908	2101	2103	2105	rBV	349	377	0.04%	0.006%
80	14.042	2121	2125	2129	rBV2	162	278	0.03%	0.005%
81	14.103	2132	2135	2136	rBV2	155	205	0.02%	0.003%
82	14.121	2136	2138	2142	rVB2	395	436	0.04%	0.007%
83	14.152	2142	2143	2146	rBV2	176	159	0.02%	0.003%
84	14.231	2152	2156	2159	rBV2	197	282	0.03%	0.005%
85	14.432	2187	2189	2191	rVV2	170	160	0.02%	0.003%
86	14.475	2194	2196	2197	rBV	229	153	0.01%	0.002%
87	14.566	2208	2211	2217	rVB2	289	457	0.04%	0.007%
88	14.609	2217	2218	2219	rBV	243	152	0.01%	0.002%
89	14.688	2228	2231	2234	rVB2	208	278	0.03%	0.005%
90	14.713	2234	2235	2237	rBV2	282	213	0.02%	0.003%
91	14.774	2242	2245	2247	rBV3	251	351	0.03%	0.006%
92	14.835	2253	2255	2257	rVB2	317	230	0.02%	0.004%
93	14.896	2264	2265	2266	rBV	295	150	0.01%	0.002%
94	14.981	2276	2279	2281	rBV2	240	366	0.04%	0.006%
95	15.456	2355	2357	2359	rVB	278	209	0.02%	0.003%
96	15.639	2385	2387	2392	rVB	344	453	0.04%	0.007%
97	15.889	2427	2428	2430	rVB	438	216	0.02%	0.004%
98	15.999	2445	2446	2448	rBV2	236	182	0.02%	0.003%
99	16.121	2465	2466	2470	rBV3	250	259	0.03%	0.004%
100	16.609	2544	2546	2549	rBV2	244	195	0.02%	0.003%




Sum of corrected areas: 6146326

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
Data File : VX040656.D
Acq On : 15 Mar 2024 16:01
Operator : JC/MD
Sample : P1753-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YCKY6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

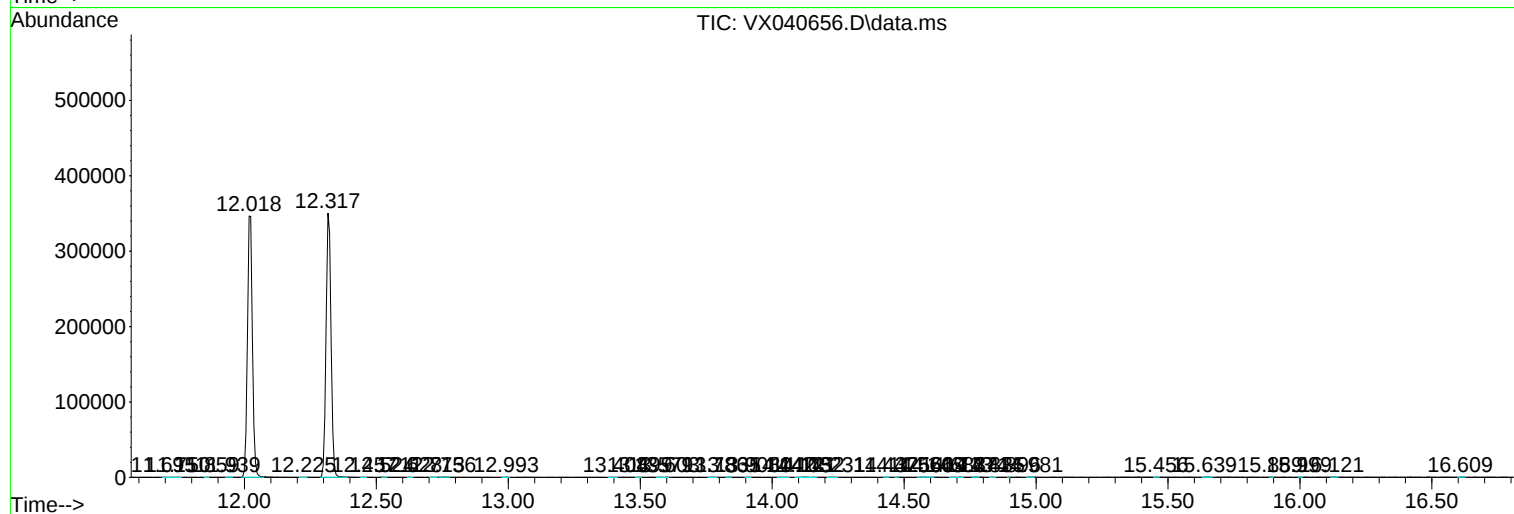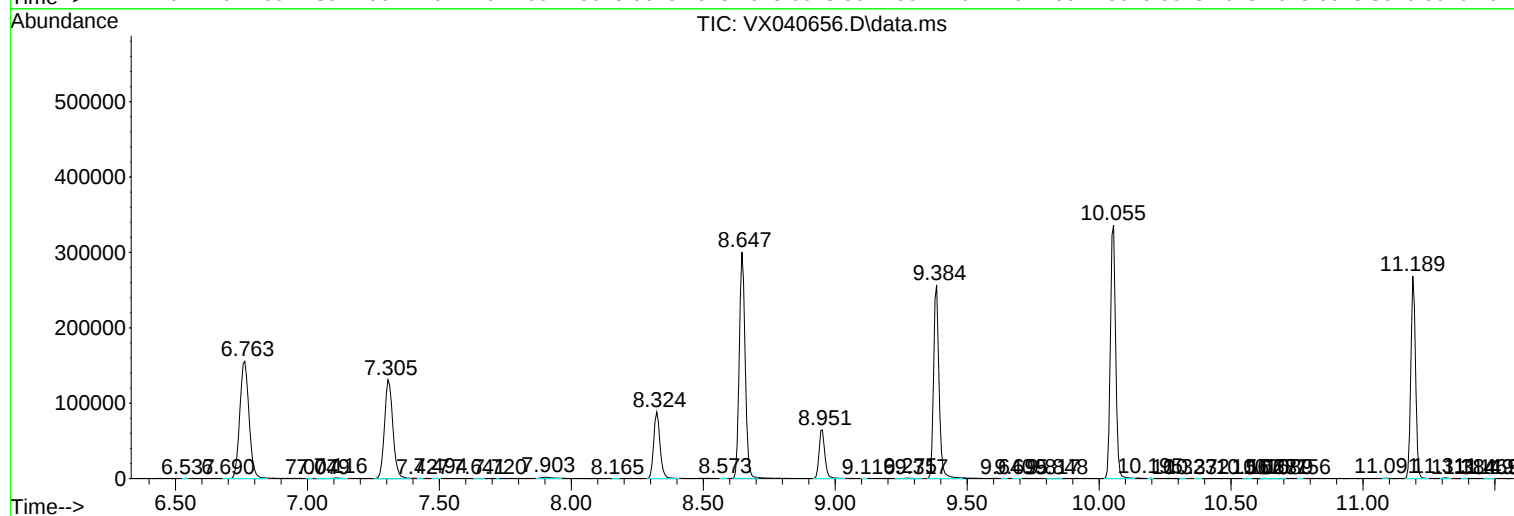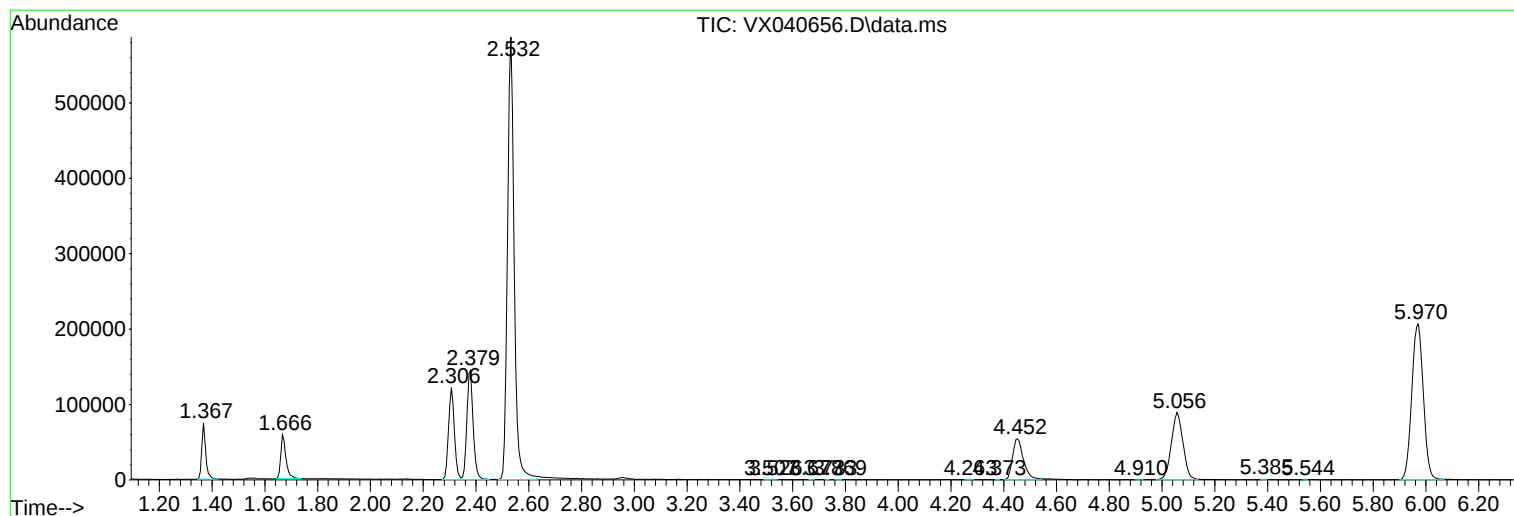

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
Data File : VX040656.D
Acq On : 15 Mar 2024 16:01
Operator : JC/MD
Sample : P1753-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YCKY6










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.532	137.44 ug/L	1030910	1,4-Difluorobenzene	6.763

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	83
2			Isopropyl Alcohol	60	C3H8O	000067-63-0	78
3			Isopropyl Alcohol	60	C3H8O	000067-63-0	64
4			Hydrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	9
5			Hydrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	9

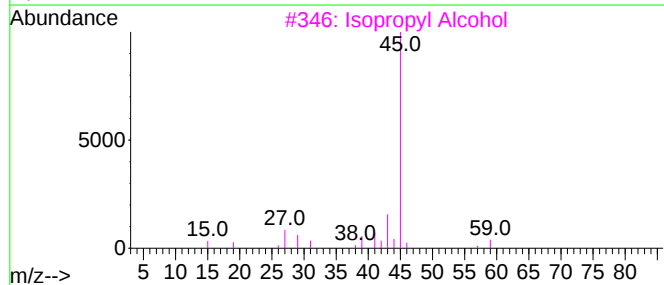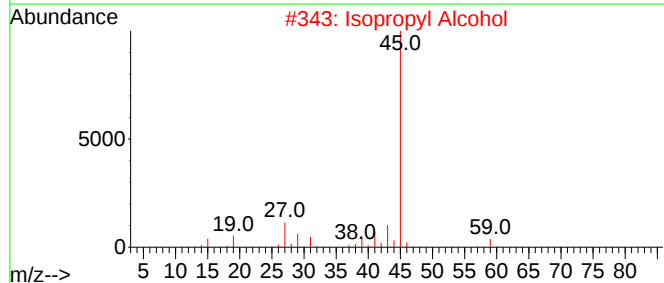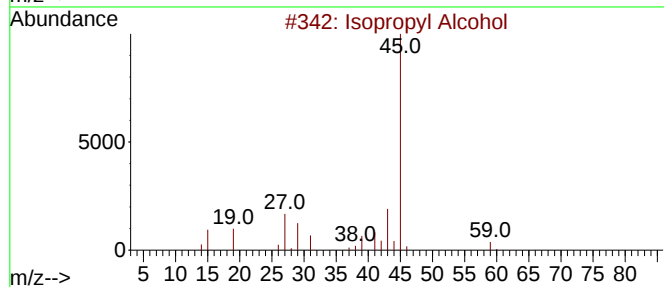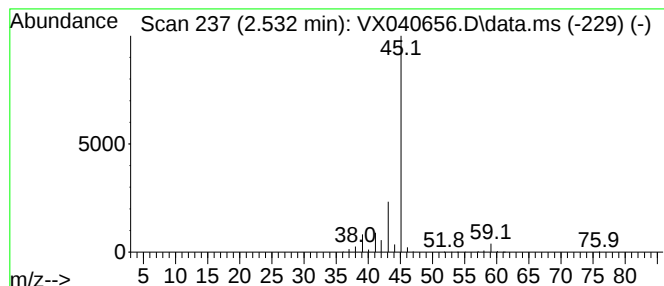

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
Data File : VX040656.D
Acq On : 15 Mar 2024 16:01
Operator : JC/MD
Sample : P1753-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YCKY6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.532	137.4	ug/L	1030910	1	6.763	375026	50.0