

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
 Data File : VX040660.D
 Acq On : 15 Mar 2024 17:33
 Operator : JC/MD
 Sample : P1753-22
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YCL38

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
 Title : VOC Analysis

Signal : TIC: VX040660.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.270	27	30	32	rBV2	783	762	0.12%	0.013%
2	1.368	42	46	58	rBV	74043	81754	13.35%	1.423%
3	1.666	91	95	108	rVB	53578	80814	13.20%	1.406%
4	1.837	122	123	125	rVB2	749	348	0.06%	0.006%
5	2.136	168	172	179	rVB2	3273	5148	0.84%	0.090%
6	2.313	193	201	207	rBV3	147427	279374	45.63%	4.861%
7	2.373	207	211	225	rVB	94422	160888	26.28%	2.800%
8	2.532	230	237	253	rBV	334901	599523	97.91%	10.432%
9	2.953	301	306	317	rVB4	3547	8563	1.40%	0.149%
10	3.117	325	333	339	rBV2	3542	7187	1.17%	0.125%
11	3.282	358	360	361	rBV	210	150	0.02%	0.003%
12	3.325	366	367	370	rBV	296	277	0.05%	0.005%
13	3.550	402	404	405	rVV	234	191	0.03%	0.003%
14	3.611	407	414	423	rVB2	8800	19951	3.26%	0.347%
15	3.770	438	440	443	rBV2	189	204	0.03%	0.004%
16	3.849	450	453	454	rBV	178	208	0.03%	0.004%
17	3.879	457	458	462	rVB	229	168	0.03%	0.003%
18	3.922	462	465	466	rBV	234	221	0.04%	0.004%
19	4.209	510	512	515	rVB	220	188	0.03%	0.003%
20	4.276	521	523	526	rVB2	175	151	0.02%	0.003%
21	4.452	543	552	566	rBV	54788	181347	29.62%	3.156%
22	5.056	636	651	666	rBV	86704	273240	44.63%	4.754%
23	5.269	683	686	687	rBV	145	171	0.03%	0.003%
24	5.379	698	704	713	rVB4	3419	9662	1.58%	0.168%
25	5.458	716	717	720	rBV	274	192	0.03%	0.003%
26	5.507	724	725	728	rVB2	313	168	0.03%	0.003%
27	5.678	751	753	755	rVB2	222	165	0.03%	0.003%
28	5.861	781	783	785	rBV	169	174	0.03%	0.003%
29	5.970	788	801	813	rVV2	202564	612301	100.00%	10.654%
30	6.086	813	820	834	rVB	31455	81120	13.25%	1.412%
31	6.428	874	876	879	rVB2	326	351	0.06%	0.006%
32	6.458	879	881	882	rBV2	235	198	0.03%	0.003%
33	6.763	922	931	948	rBV	152534	370247	60.47%	6.442%
34	6.964	961	964	965	rBV2	208	151	0.02%	0.003%
35	7.019	971	973	977	rVB3	232	202	0.03%	0.004%
36	7.117	984	989	994	rBV3	1405	2912	0.48%	0.051%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
 Data File : VX040660.D
 Acq On : 15 Mar 2024 17:33
 Operator : JC/MD
 Sample : P1753-22
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YCL38

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
 Title : VOC Analysis

37	7.306	1012	1020	1036	rBV	129061	280519	45.81%	4.881%
38	7.434	1036	1041	1047	rVB3	1407	2572	0.42%	0.045%
39	7.562	1060	1062	1065	rVB2	266	306	0.05%	0.005%
40	7.586	1065	1066	1070	rBV	220	288	0.05%	0.005%
41	7.714	1086	1087	1089	rBV	184	167	0.03%	0.003%
42	7.824	1103	1105	1108	rBV	135	158	0.03%	0.003%
43	7.854	1108	1110	1113	rVB2	204	207	0.03%	0.004%
44	7.903	1114	1118	1120	rVV2	625	832	0.14%	0.014%
45	7.933	1121	1123	1126	rVV2	566	574	0.09%	0.010%
46	7.958	1126	1127	1130	rVB2	449	258	0.04%	0.004%
47	8.324	1181	1187	1200	rVV	89072	143323	23.41%	2.494%
48	8.482	1212	1213	1214	rBV	363	201	0.03%	0.003%
49	8.647	1234	1240	1250	rBV	290544	454554	74.24%	7.909%
50	8.836	1270	1271	1273	rBV	223	203	0.03%	0.004%
51	8.952	1284	1290	1302	rBV	63227	96203	15.71%	1.674%
52	9.037	1302	1304	1305	rVB	379	221	0.04%	0.004%
53	9.104	1314	1315	1319	rBV2	172	172	0.03%	0.003%
54	9.269	1337	1342	1348	rBV3	578	1025	0.17%	0.018%
55	9.384	1355	1361	1380	rBV	248293	365357	59.67%	6.357%
56	9.622	1396	1400	1402	rBV2	187	251	0.04%	0.004%
57	9.689	1407	1411	1413	rBV2	252	318	0.05%	0.006%
58	9.738	1417	1419	1422	rVB	182	165	0.03%	0.003%
59	9.775	1422	1425	1427	rBV	218	279	0.05%	0.005%
60	9.854	1436	1438	1439	rVB2	349	186	0.03%	0.003%
61	9.872	1439	1441	1444	rVV2	166	188	0.03%	0.003%
62	10.055	1465	1471	1480	rBV	329912	461852	75.43%	8.036%
63	10.250	1500	1503	1505	rVB2	275	250	0.04%	0.004%
64	10.305	1509	1512	1515	rVB	280	307	0.05%	0.005%
65	10.500	1542	1544	1546	rBV2	228	292	0.05%	0.005%
66	11.030	1628	1631	1633	rBV2	629	659	0.11%	0.011%
67	11.085	1637	1640	1645	rBV4	626	919	0.15%	0.016%
68	11.189	1652	1657	1666	rBV	259568	326548	53.33%	5.682%
69	11.317	1675	1678	1682	rVB	797	970	0.16%	0.017%
70	11.445	1697	1699	1703	rVB	305	358	0.06%	0.006%
71	11.597	1721	1724	1726	rBV2	159	180	0.03%	0.003%
72	11.652	1731	1733	1735	rBV	218	159	0.03%	0.003%
73	11.786	1753	1755	1756	rBV	193	169	0.03%	0.003%
74	11.811	1756	1759	1761	rVV2	120	188	0.03%	0.003%
75	11.982	1784	1787	1788	rBV2	185	195	0.03%	0.003%
76	12.018	1788	1793	1801	rBV	307280	398144	65.02%	6.928%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
 Data File : VX040660.D
 Acq On : 15 Mar 2024 17:33
 Operator : JC/MD
 Sample : P1753-22
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YCL38

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
 Title : VOC Analysis

77	12.122	1809	1810	1811	rBV	348	217	0.04%	0.004%
78	12.195	1820	1822	1824	rVV	317	225	0.04%	0.004%
79	12.213	1824	1825	1827	rVV	214	164	0.03%	0.003%
80	12.317	1837	1842	1849	rBV	326113	422475	69.00%	7.351%
81	12.518	1873	1875	1880	rBV	178	338	0.06%	0.006%
82	12.683	1901	1902	1907	rBV	213	238	0.04%	0.004%
83	12.768	1912	1916	1918	rBV	384	506	0.08%	0.009%
84	13.073	1964	1966	1968	rBV	225	195	0.03%	0.003%
85	13.329	2007	2008	2010	rBV	198	152	0.02%	0.003%
86	13.439	2021	2026	2028	rVB2	570	765	0.12%	0.013%
87	13.597	2049	2052	2053	rBV	191	176	0.03%	0.003%
88	13.646	2057	2060	2061	rBV2	141	157	0.03%	0.003%
89	13.762	2077	2079	2081	rVB	262	160	0.03%	0.003%
90	13.804	2082	2086	2087	rBV2	131	165	0.03%	0.003%
91	13.932	2104	2107	2109	rBV2	182	224	0.04%	0.004%
92	14.134	2136	2140	2142	rBV	224	284	0.05%	0.005%
93	14.347	2173	2175	2176	rBV	211	150	0.02%	0.003%
94	14.890	2263	2264	2267	rBV	170	199	0.03%	0.003%
95	15.066	2291	2293	2296	rBV2	255	278	0.05%	0.005%
96	15.249	2320	2323	2325	rBV	289	427	0.07%	0.007%
97	15.444	2353	2355	2357	rVB	331	225	0.04%	0.004%
98	15.487	2360	2362	2364	rBV	300	306	0.05%	0.005%
99	15.676	2391	2393	2397	rBV2	314	333	0.05%	0.006%
100	16.322	2495	2499	2500	rBV3	202	249	0.04%	0.004%




Sum of corrected areas: 5746996

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
Data File : VX040660.D
Acq On : 15 Mar 2024 17:33
Operator : JC/MD
Sample : P1753-22
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YCL38

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

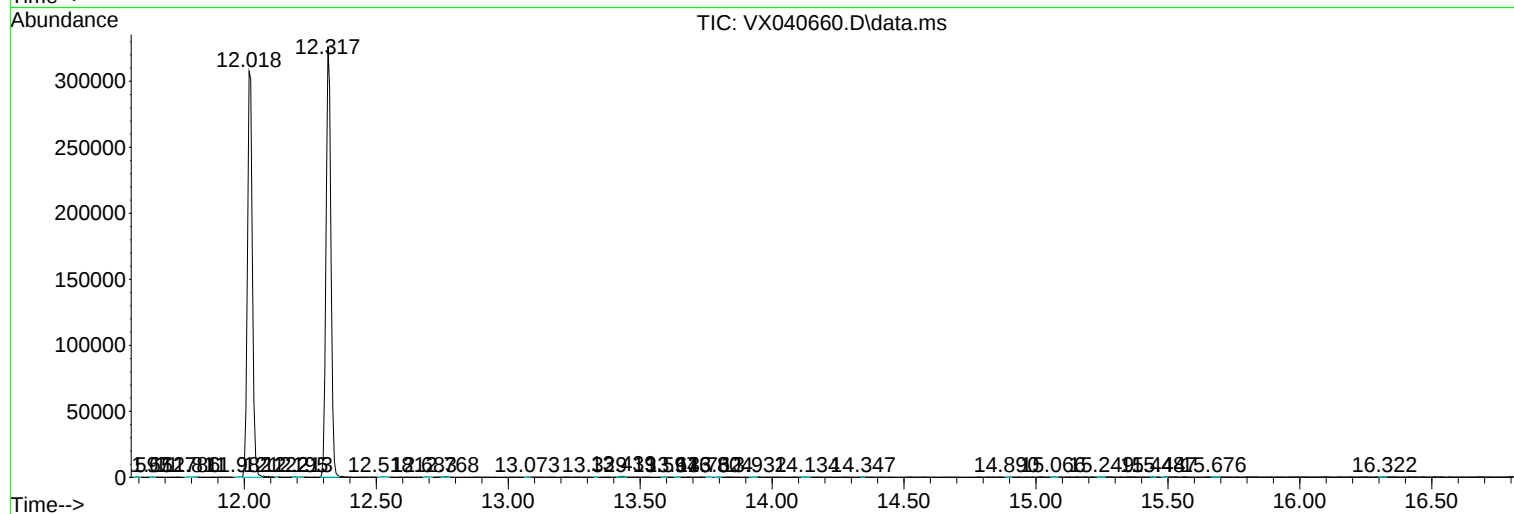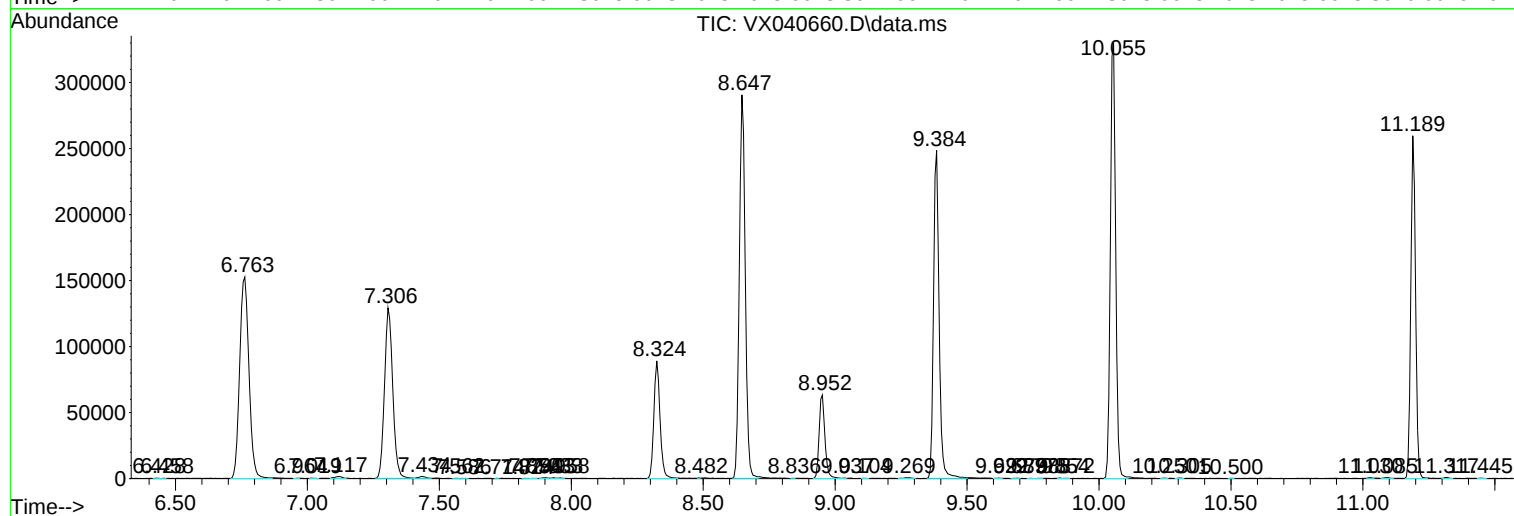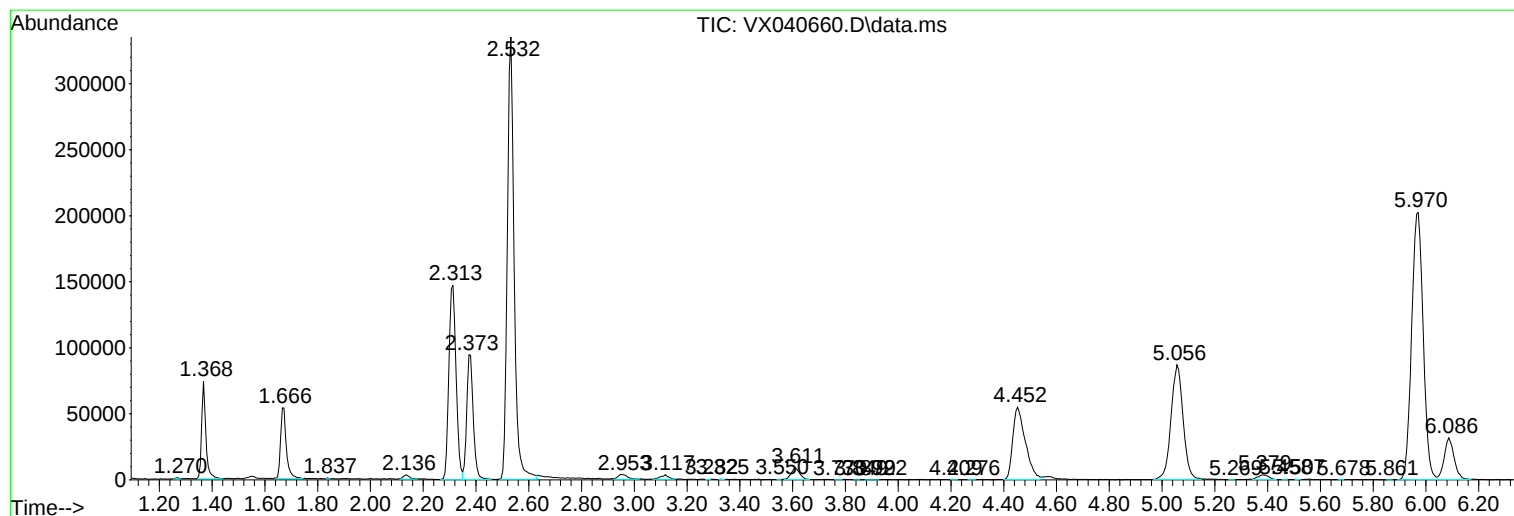

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
Data File : VX040660.D
Acq On : 15 Mar 2024 17:33
Operator : JC/MD
Sample : P1753-22
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YCL38










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.532	80.96 ug/L	599523	1,4-Difluorobenzene	6.763

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	78
2			Isopropyl Alcohol	60	C3H8O	000067-63-0	78
3			Isopropyl Alcohol	60	C3H8O	000067-63-0	56
4			Hydrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	9
5			Hydrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	9

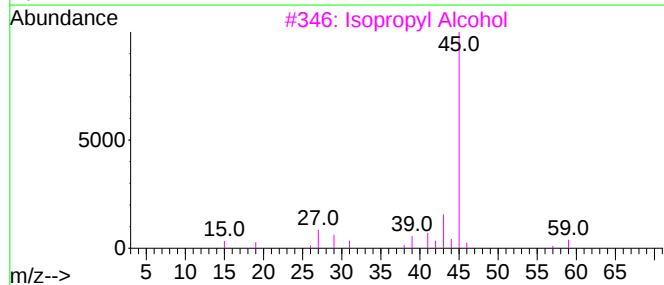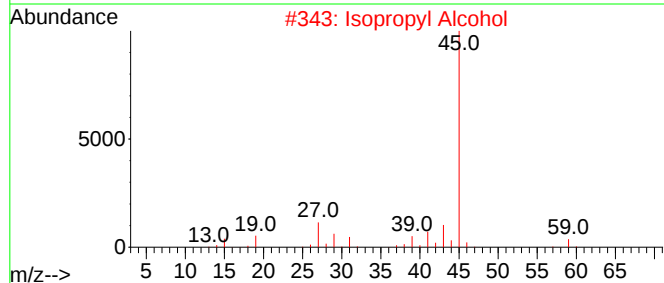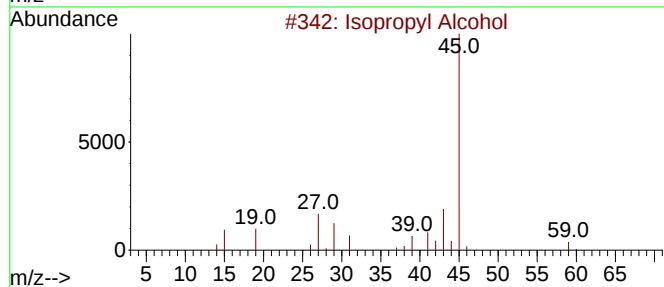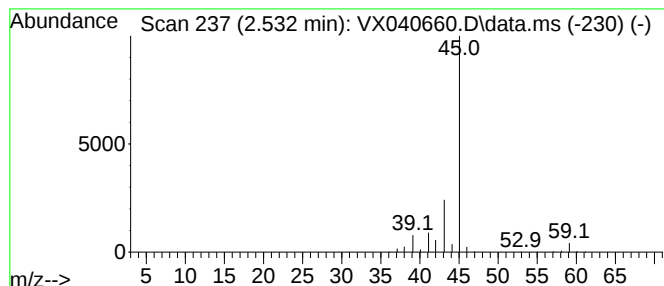

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
Data File : VX040660.D
Acq On : 15 Mar 2024 17:33
Operator : JC/MD
Sample : P1753-22
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YCL38

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.532	81.0	ug/L	599523	1	6.763	370247	50.0