

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
 Data File : VX040665.D
 Acq On : 15 Mar 2024 20:13
 Operator : JC/MD
 Sample : VX0315WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK665

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
 Title : VOC Analysis

Signal : TIC: VX040665.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	54	rBV	86016	89308	13.10%	1.753%
2	1.551	72	76	77	rBV4	1456	2149	0.32%	0.042%
3	1.666	91	95	108	rVB	67325	92947	13.64%	1.824%
4	2.307	193	200	209	rBV	137036	212828	31.23%	4.178%
5	2.508	230	233	240	rVB2	951	1460	0.21%	0.029%
6	2.648	255	256	259	rVV2	235	234	0.03%	0.005%
7	2.733	268	270	274	rBV	209	269	0.04%	0.005%
8	2.788	277	279	283	rVB3	768	927	0.14%	0.018%
9	2.843	286	288	292	rBV2	168	320	0.05%	0.006%
10	3.081	324	327	328	rBV2	318	313	0.05%	0.006%
11	3.447	384	387	389	rVB2	311	269	0.04%	0.005%
12	3.465	389	390	393	rBV2	179	192	0.03%	0.004%
13	3.697	426	428	432	rBV2	198	249	0.04%	0.005%
14	3.745	432	436	438	rBV	201	226	0.03%	0.004%
15	3.818	447	448	451	rVV	240	192	0.03%	0.004%
16	4.343	531	534	535	rBV	206	222	0.03%	0.004%
17	4.452	543	552	566	rBV	61143	169675	24.90%	3.331%
18	4.745	599	600	603	rVB	321	188	0.03%	0.004%
19	4.806	608	610	613	rVB2	326	350	0.05%	0.007%
20	4.940	629	632	633	rVB2	273	221	0.03%	0.004%
21	5.056	640	651	667	rVV	93521	290651	42.65%	5.705%
22	5.373	698	703	704	rBV2	304	334	0.05%	0.007%
23	5.483	719	721	724	rVB2	178	201	0.03%	0.004%
24	5.641	745	747	750	rBV	206	241	0.04%	0.005%
25	5.964	789	800	818	rBV2	226953	681549	100.00%	13.378%
26	6.288	850	853	856	rBV2	171	237	0.03%	0.005%
27	6.422	872	875	878	rBV2	222	286	0.04%	0.006%
28	6.623	904	908	909	rBV2	166	206	0.03%	0.004%
29	6.653	911	913	916	rBV2	195	243	0.04%	0.005%
30	6.763	922	931	945	rBV	153284	371502	54.51%	7.292%
31	6.922	956	957	960	rVB2	269	219	0.03%	0.004%
32	7.117	983	989	997	rVB5	2087	4627	0.68%	0.091%
33	7.306	1010	1020	1038	rVV	140547	313504	46.00%	6.154%
34	7.470	1045	1047	1048	rBV	477	399	0.06%	0.008%
35	7.574	1063	1064	1067	rBV	196	209	0.03%	0.004%
36	7.635	1072	1074	1077	rBV2	172	222	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
 Data File : VX040665.D
 Acq On : 15 Mar 2024 20:13
 Operator : JC/MD
 Sample : VX0315WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK665

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
 Title : VOC Analysis

37	7.885	1114	1115	1118	rBV2	187	227	0.03%	0.004%
38	7.940	1120	1124	1126	rBV2	649	800	0.12%	0.016%
39	8.007	1133	1135	1140	rVB2	289	404	0.06%	0.008%
40	8.177	1157	1163	1164	rBV	229	272	0.04%	0.005%
41	8.208	1167	1168	1170	rBV	269	212	0.03%	0.004%
42	8.324	1180	1187	1201	rBV	95233	157341	23.09%	3.088%
43	8.488	1210	1214	1218	rBV4	557	840	0.12%	0.016%
44	8.647	1234	1240	1251	rBV	329426	513907	75.40%	10.087%
45	8.860	1273	1275	1280	rVB3	240	330	0.05%	0.006%
46	8.946	1284	1289	1302	rVV	69413	108670	15.94%	2.133%
47	9.098	1311	1314	1321	rBV2	259	636	0.09%	0.012%
48	9.275	1340	1343	1347	rVB2	530	586	0.09%	0.012%
49	9.385	1355	1361	1372	rBV	273447	403299	59.17%	7.916%
50	9.574	1390	1392	1395	rVB2	400	300	0.04%	0.006%
51	9.616	1395	1399	1402	rBV2	176	278	0.04%	0.005%
52	9.750	1418	1421	1425	rVB2	228	294	0.04%	0.006%
53	9.836	1433	1435	1436	rBV	227	196	0.03%	0.004%
54	10.055	1465	1471	1485	rBV	327244	459328	67.39%	9.016%
55	10.195	1491	1494	1497	rBV	645	616	0.09%	0.012%
56	10.311	1509	1513	1516	rBV3	737	919	0.13%	0.018%
57	10.659	1566	1570	1571	rBV3	374	399	0.06%	0.008%
58	10.835	1595	1599	1602	rBV	188	257	0.04%	0.005%
59	10.927	1612	1614	1617	rBV	185	222	0.03%	0.004%
60	10.957	1617	1619	1620	rBV	372	291	0.04%	0.006%
61	11.006	1625	1627	1633	rVB2	140	274	0.04%	0.005%
62	11.189	1652	1657	1668	rBV	265779	329815	48.39%	6.474%
63	11.457	1695	1701	1704	rBV3	458	817	0.12%	0.016%
64	11.616	1725	1727	1730	rBV2	180	192	0.03%	0.004%
65	11.756	1746	1750	1755	rVB3	555	847	0.12%	0.017%
66	11.976	1782	1786	1788	rBV4	922	1288	0.19%	0.025%
67	12.018	1788	1793	1803	rVV	301661	401005	58.84%	7.871%
68	12.256	1828	1832	1833	rBV	168	224	0.03%	0.004%
69	12.317	1837	1842	1854	rVV	362475	458299	67.24%	8.996%
70	12.475	1865	1868	1870	rVB	238	271	0.04%	0.005%
71	12.652	1894	1897	1900	rBV2	214	333	0.05%	0.007%
72	12.762	1912	1915	1919	rVB3	193	332	0.05%	0.007%
73	12.920	1937	1941	1944	rVV2	142	203	0.03%	0.004%
74	13.116	1970	1973	1977	rVB3	997	1414	0.21%	0.028%
75	13.366	2011	2014	2016	rBV	229	310	0.05%	0.006%
76	13.494	2033	2035	2037	rBV	188	226	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
 Data File : VX040665.D
 Acq On : 15 Mar 2024 20:13
 Operator : JC/MD
 Sample : VX0315WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK665

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
 Title : VOC Analysis

77	13.591	2048	2051	2056	rVV3	1295	1841	0.27%	0.036%
78	13.780	2078	2082	2086	rVV2	1165	1500	0.22%	0.029%
79	13.847	2091	2093	2096	rVB	236	218	0.03%	0.004%
80	13.932	2105	2107	2109	rBV	222	208	0.03%	0.004%
81	13.963	2109	2112	2115	rBV3	1015	1151	0.17%	0.023%
82	14.054	2124	2127	2130	rBV	269	332	0.05%	0.007%
83	14.085	2130	2132	2135	rBV2	235	220	0.03%	0.004%
84	14.128	2135	2139	2146	rVB3	569	856	0.13%	0.017%
85	14.195	2146	2150	2151	rBV2	233	300	0.04%	0.006%
86	14.341	2172	2174	2176	rBV2	225	277	0.04%	0.005%
87	14.487	2195	2198	2200	rBV	209	268	0.04%	0.005%
88	14.524	2203	2204	2207	rVB2	223	193	0.03%	0.004%
89	14.554	2207	2209	2211	rBV	193	248	0.04%	0.005%
90	14.682	2228	2230	2232	rBV2	203	202	0.03%	0.004%
91	14.749	2239	2241	2245	rBV2	195	255	0.04%	0.005%
92	15.194	2311	2314	2316	rBV2	281	316	0.05%	0.006%
93	15.633	2385	2386	2389	rBV2	260	274	0.04%	0.005%
94	15.761	2405	2407	2412	rVB2	330	467	0.07%	0.009%
95	15.804	2412	2414	2417	rBV3	226	282	0.04%	0.006%
96	16.060	2451	2456	2457	rBV2	216	329	0.05%	0.006%
97	16.109	2461	2464	2465	rVB	285	237	0.03%	0.005%
98	16.188	2473	2477	2479	rBV	319	370	0.05%	0.007%
99	16.463	2521	2522	2525	rBV2	314	364	0.05%	0.007%
100	16.761	2569	2571	2572	rBV2	193	191	0.03%	0.004%




Sum of corrected areas: 5094542

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
Data File : VX040665.D
Acq On : 15 Mar 2024 20:13
Operator : JC/MD
Sample : VX0315WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK665

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

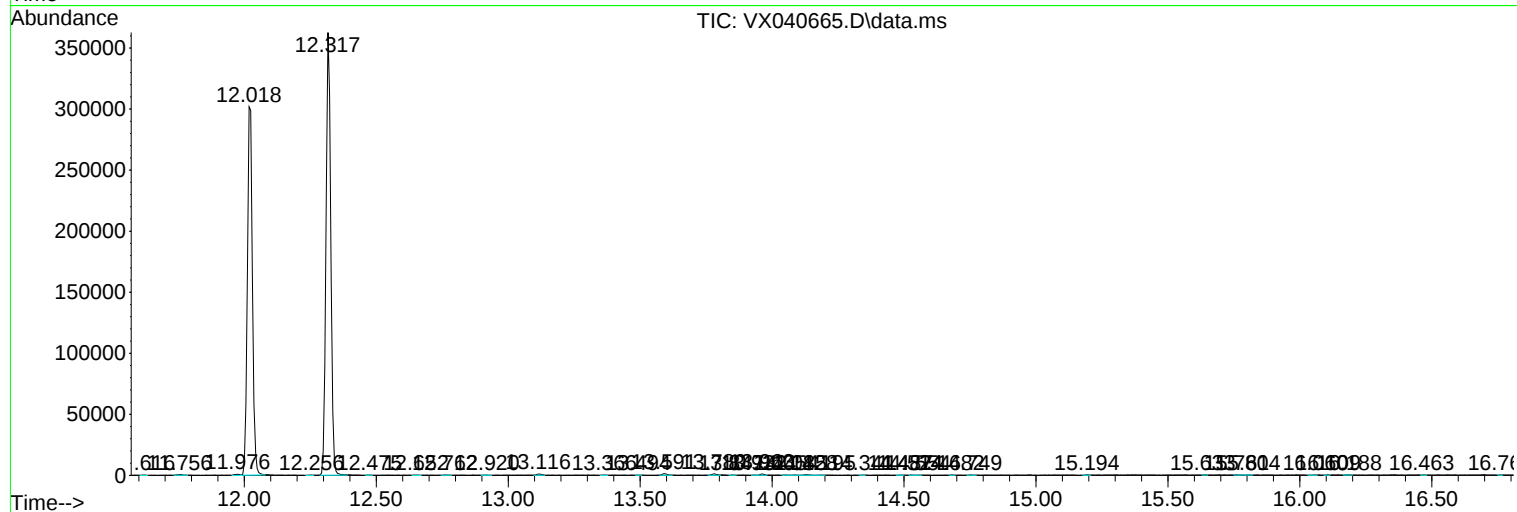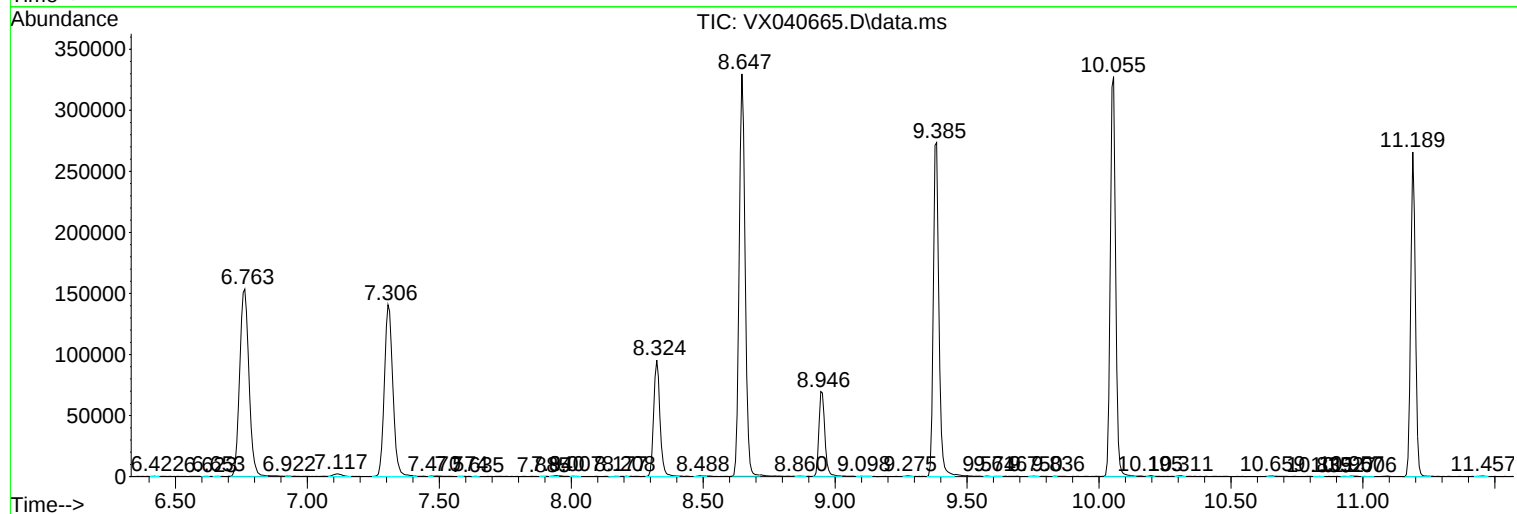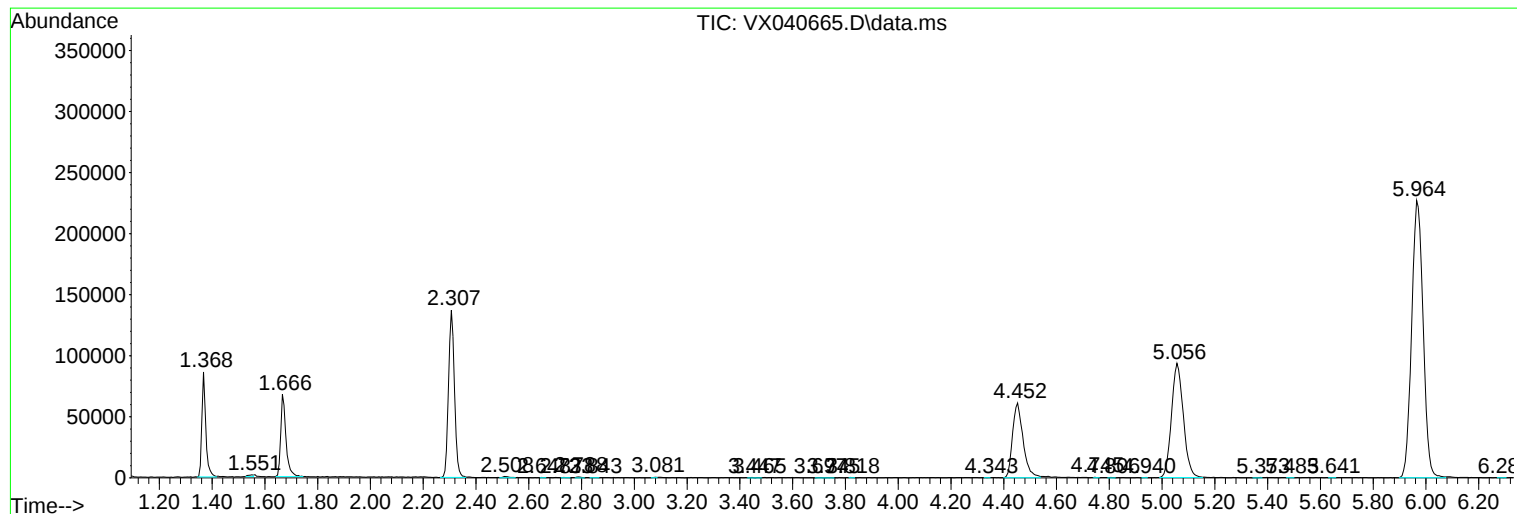

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
Data File : VX040665.D
Acq On : 15 Mar 2024 20:13
Operator : JC/MD
Sample : VX0315WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK665

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM030724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
Data File : VX040665.D
Acq On : 15 Mar 2024 20:13
Operator : JC/MD
Sample : VX0315WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK665

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc