

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
 Data File : VX040667.D
 Acq On : 15 Mar 2024 20:58
 Operator : JC/MD
 Sample : P1754-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YCKT7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
 Title : VOC Analysis

Signal : TIC: VX040667.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.270	27	30	32	rBV2	1050	965	0.11%	0.016%
2	1.368	42	46	63	rVB	75285	82403	9.26%	1.388%
3	1.666	91	95	109	rVB	57574	84243	9.47%	1.419%
4	2.136	169	172	176	rVB4	2473	3491	0.39%	0.059%
5	2.306	194	200	207	rBV	124850	195192	21.94%	3.289%
6	2.374	207	211	222	rVB	44948	74708	8.40%	1.259%
7	2.532	229	237	254	rBV	487202	889727	100.00%	14.990%
8	3.111	328	332	339	rVB4	1327	2831	0.32%	0.048%
9	3.617	407	415	425	rVV3	5138	11832	1.33%	0.199%
10	3.751	435	437	439	rBV	193	192	0.02%	0.003%
11	3.898	458	461	462	rBV	184	180	0.02%	0.003%
12	3.959	469	471	472	rBV	233	173	0.02%	0.003%
13	4.062	487	488	490	rBV	221	178	0.02%	0.003%
14	4.227	511	515	520	rBV2	210	399	0.04%	0.007%
15	4.276	520	523	524	rVV2	182	197	0.02%	0.003%
16	4.300	525	527	529	rVB	212	188	0.02%	0.003%
17	4.446	542	551	570	rBV	55129	164326	18.47%	2.769%
18	4.818	610	612	615	rVV2	204	250	0.03%	0.004%
19	4.885	621	623	626	rBV2	151	204	0.02%	0.003%
20	5.056	638	651	671	rVB2	89098	281507	31.64%	4.743%
21	5.215	676	677	679	rBV2	269	250	0.03%	0.004%
22	5.343	696	698	700	rBV2	205	177	0.02%	0.003%
23	5.367	700	702	703	rBV	222	199	0.02%	0.003%
24	5.440	712	714	717	rBV2	174	202	0.02%	0.003%
25	5.550	730	732	735	rBV2	266	322	0.04%	0.005%
26	5.830	775	778	779	rBV	220	225	0.03%	0.004%
27	5.970	789	801	817	rBV2	208257	636365	71.52%	10.721%
28	6.440	876	878	881	rBV2	238	275	0.03%	0.005%
29	6.483	881	885	888	rVV2	171	243	0.03%	0.004%
30	6.757	921	930	944	rBV	163614	391065	43.95%	6.589%
31	6.928	956	958	962	rVB3	259	247	0.03%	0.004%
32	7.123	985	990	994	rVB4	1120	1747	0.20%	0.029%
33	7.232	1005	1008	1009	rBV2	168	174	0.02%	0.003%
34	7.306	1012	1020	1037	rVV	137443	296473	33.32%	4.995%
35	7.476	1046	1048	1051	rBV2	256	295	0.03%	0.005%
36	7.525	1054	1056	1059	rVV	262	202	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
 Data File : VX040667.D
 Acq On : 15 Mar 2024 20:58
 Operator : JC/MD
 Sample : P1754-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YCKT7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
 Title : VOC Analysis

37	7.763	1088	1095	1098	rBV2	215	422	0.05%	0.007%
38	7.891	1111	1116	1118	rBV2	703	880	0.10%	0.015%
39	7.958	1125	1127	1131	rVB2	323	349	0.04%	0.006%
40	8.031	1135	1139	1141	rBV2	195	289	0.03%	0.005%
41	8.196	1163	1166	1167	rBV	218	219	0.02%	0.004%
42	8.324	1181	1187	1199	rVV	93526	149983	16.86%	2.527%
43	8.446	1205	1207	1210	rVB	331	265	0.03%	0.004%
44	8.494	1210	1215	1218	rVV3	502	844	0.09%	0.014%
45	8.519	1218	1219	1222	rVB2	394	399	0.04%	0.007%
46	8.647	1233	1240	1249	rBV	295518	466030	52.38%	7.852%
47	8.811	1264	1267	1270	rVB	369	459	0.05%	0.008%
48	8.946	1284	1289	1297	rBV	65463	100195	11.26%	1.688%
49	9.275	1337	1343	1348	rVB2	1848	2708	0.30%	0.046%
50	9.384	1355	1361	1374	rBV	262759	380468	42.76%	6.410%
51	9.775	1422	1425	1427	rBV	277	240	0.03%	0.004%
52	9.854	1435	1438	1441	rBV2	231	238	0.03%	0.004%
53	10.055	1465	1471	1483	rBV	346435	485274	54.54%	8.176%
54	10.183	1491	1492	1493	rBV	448	219	0.02%	0.004%
55	10.262	1503	1505	1506	rBV	230	227	0.03%	0.004%
56	10.305	1509	1512	1521	rVB2	497	969	0.11%	0.016%
57	10.384	1521	1525	1526	rBV	212	243	0.03%	0.004%
58	10.604	1559	1561	1563	rBV	222	217	0.02%	0.004%
59	10.653	1566	1569	1572	rBV	449	782	0.09%	0.013%
60	10.963	1617	1620	1623	rBV	543	506	0.06%	0.009%
61	11.061	1634	1636	1638	rBV2	239	278	0.03%	0.005%
62	11.092	1638	1641	1643	rBV	434	451	0.05%	0.008%
63	11.152	1647	1651	1652	rBV2	218	239	0.03%	0.004%
64	11.189	1652	1657	1664	rBV	248030	312082	35.08%	5.258%
65	11.311	1673	1677	1681	rVB3	1667	2196	0.25%	0.037%
66	11.457	1698	1701	1705	rVB2	391	471	0.05%	0.008%
67	11.512	1705	1710	1712	rBV2	162	224	0.03%	0.004%
68	11.567	1716	1719	1720	rBV	228	208	0.02%	0.004%
69	11.756	1747	1750	1757	rVB3	791	1047	0.12%	0.018%
70	11.817	1758	1760	1762	rBV	233	218	0.02%	0.004%
71	11.835	1762	1763	1769	rBV	189	299	0.03%	0.005%
72	11.975	1780	1786	1788	rBV2	684	892	0.10%	0.015%
73	12.018	1788	1793	1808	rVV	321619	427826	48.09%	7.208%
74	12.317	1837	1842	1851	rBV	380789	464812	52.24%	7.831%
75	12.701	1902	1905	1907	rBV2	218	258	0.03%	0.004%
76	12.756	1912	1914	1919	rVB3	608	876	0.10%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
 Data File : VX040667.D
 Acq On : 15 Mar 2024 20:58
 Operator : JC/MD
 Sample : P1754-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YCKT7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
 Title : VOC Analysis

77	12.866	1930	1932	1935	rBV3	520	431	0.05%	0.007%
78	12.951	1942	1946	1947	rBV	200	211	0.02%	0.004%
79	12.975	1948	1950	1951	rVV	288	232	0.03%	0.004%
80	13.116	1971	1973	1977	rVB2	832	686	0.08%	0.012%
81	13.280	1997	2000	2003	rBV2	229	311	0.03%	0.005%
82	13.591	2048	2051	2054	rBV3	756	889	0.10%	0.015%
83	13.695	2066	2068	2070	rBV	164	184	0.02%	0.003%
84	13.774	2079	2081	2087	rBV3	622	1122	0.13%	0.019%
85	13.963	2109	2112	2116	rBV	577	720	0.08%	0.012%
86	14.128	2136	2139	2145	rVV2	593	692	0.08%	0.012%
87	14.274	2161	2163	2165	rBV	176	187	0.02%	0.003%
88	14.310	2168	2169	2172	rVB2	267	208	0.02%	0.004%
89	14.512	2199	2202	2203	rBV	194	238	0.03%	0.004%
90	14.609	2216	2218	2222	rBV3	283	310	0.03%	0.005%
91	14.676	2227	2229	2230	rBV	280	239	0.03%	0.004%
92	14.768	2241	2244	2245	rBV2	232	249	0.03%	0.004%
93	14.920	2268	2269	2272	rBV	214	234	0.03%	0.004%
94	14.993	2279	2281	2284	rBV2	193	224	0.03%	0.004%
95	15.371	2341	2343	2344	rBV2	299	198	0.02%	0.003%
96	15.469	2354	2359	2363	rBV2	247	572	0.06%	0.010%
97	15.566	2373	2375	2377	rBV2	293	266	0.03%	0.004%
98	15.847	2420	2421	2424	rBV	241	175	0.02%	0.003%
99	16.219	2480	2482	2484	rBV2	294	281	0.03%	0.005%
100	16.578	2540	2541	2542	rBV	318	184	0.02%	0.003%




Sum of corrected areas: 5935492

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
Data File : VX040667.D
Acq On : 15 Mar 2024 20:58
Operator : JC/MD
Sample : P1754-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YCKT7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

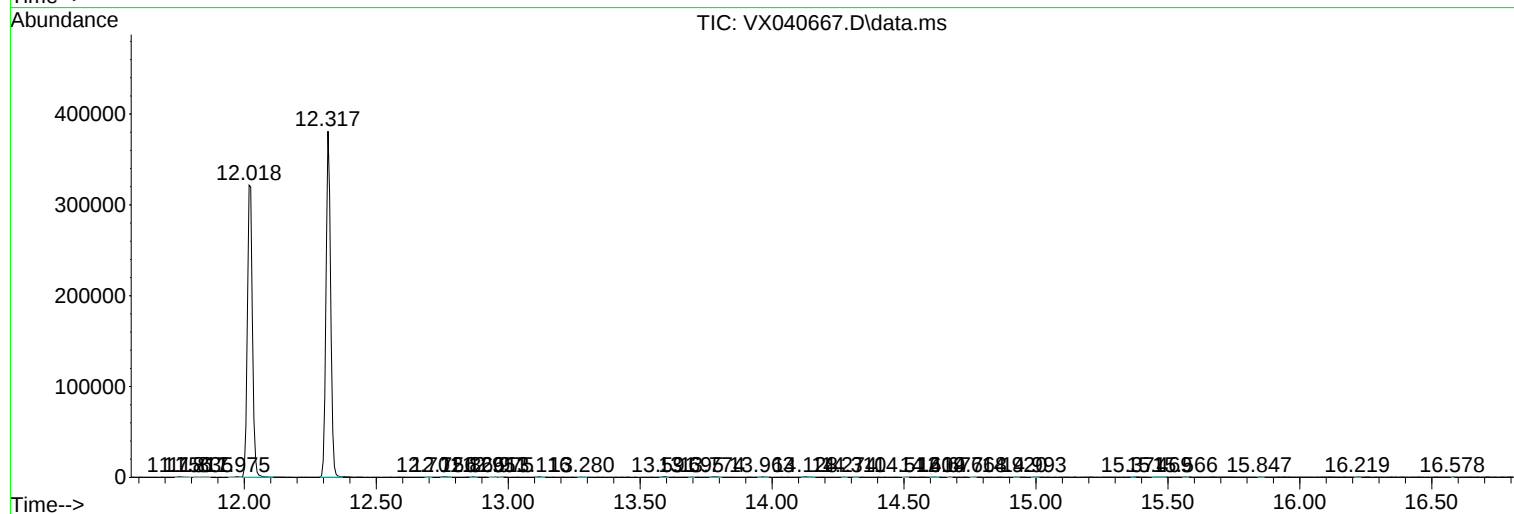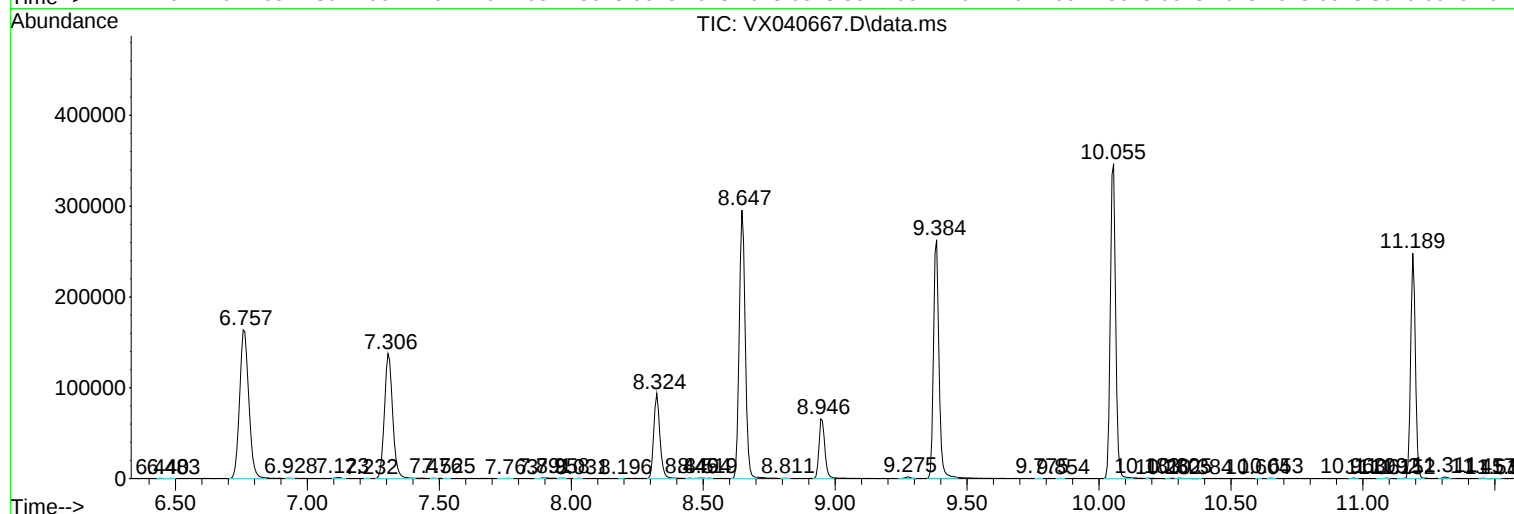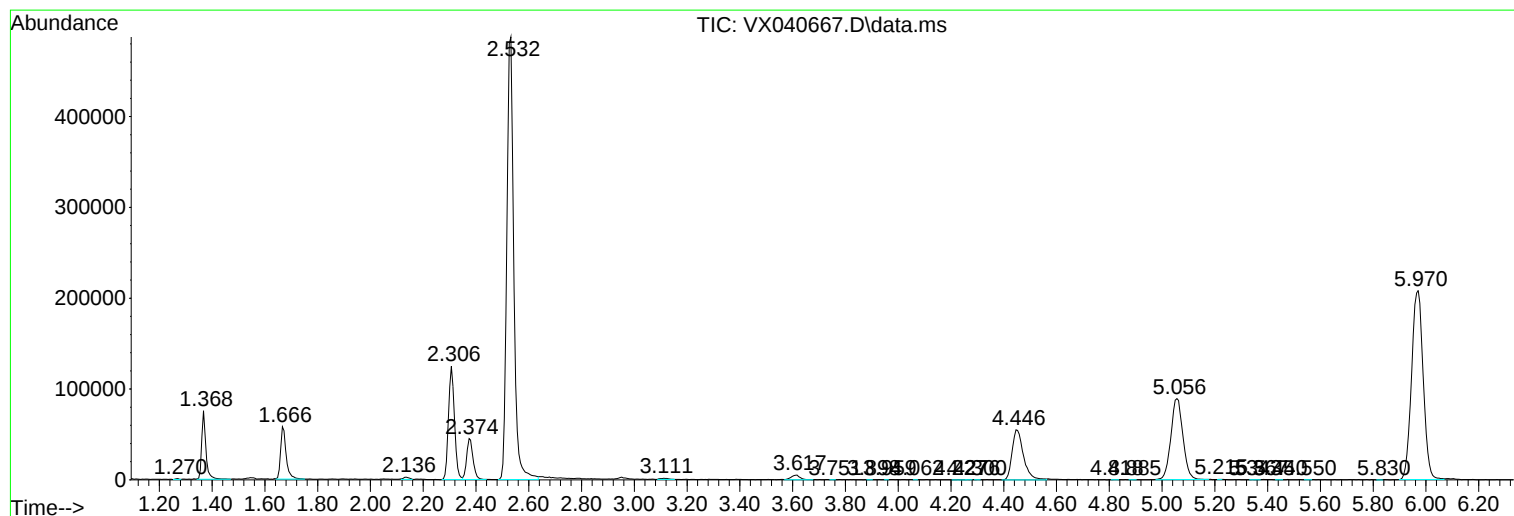

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
Data File : VX040667.D
Acq On : 15 Mar 2024 20:58
Operator : JC/MD
Sample : P1754-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YCKT7










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.532	113.76 ug/L	889727	1,4-Difluorobenzene	6.757

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	78
2			Isopropyl Alcohol	60	C3H8O	000067-63-0	78
3			Isopropyl Alcohol	60	C3H8O	000067-63-0	64
4			Isopropyl Alcohol	60	C3H8O	000067-63-0	9
5			Hydrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	9

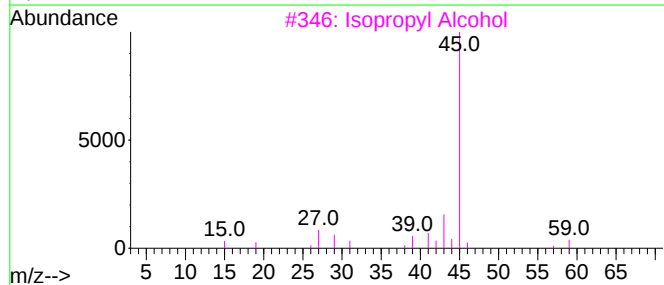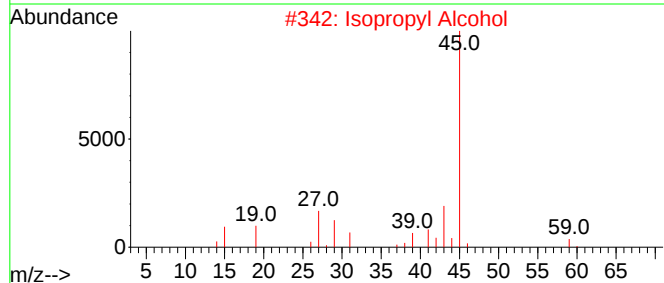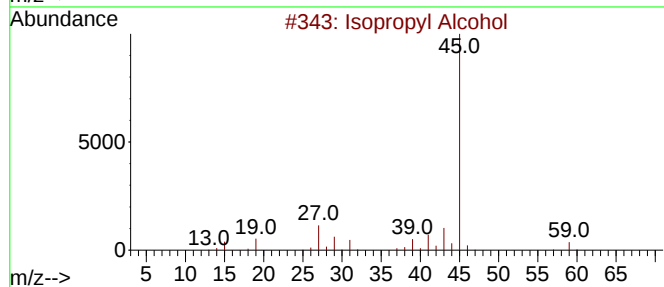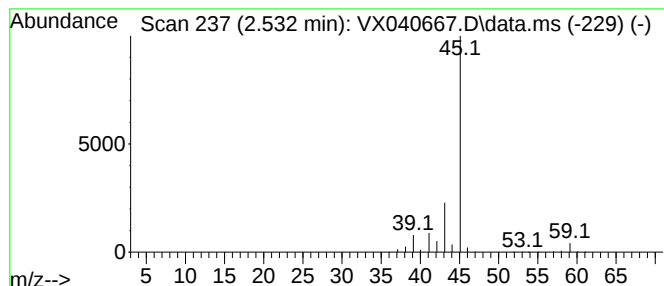

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
Data File : VX040667.D
Acq On : 15 Mar 2024 20:58
Operator : JC/MD
Sample : P1754-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YCKT7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.532	113.8	ug/L	889727	1	6.757	391065	50.0