

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
 Data File : VX040669.D
 Acq On : 15 Mar 2024 21:44
 Operator : JC/MD
 Sample : P1754-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YCL07

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
 Title : VOC Analysis

Signal : TIC: VX040669.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.270	26	30	33	rBV	4194	4201	0.67%	0.071%
2	1.368	42	46	56	rVB	78122	83353	13.31%	1.411%
3	1.666	91	95	108	rVB	54768	81249	12.98%	1.376%
4	2.136	168	172	179	rVB3	3749	5799	0.93%	0.098%
5	2.191	179	181	183	rVB	726	397	0.06%	0.007%
6	2.215	183	185	189	rVB3	484	518	0.08%	0.009%
7	2.307	193	200	207	rBV2	140636	259101	41.38%	4.387%
8	2.380	207	212	223	rVB	112591	186181	29.74%	3.152%
9	2.532	230	237	255	rBV	219575	395280	63.13%	6.692%
10	2.947	301	305	315	rVB3	2795	6276	1.00%	0.106%
11	3.099	325	330	334	rVB2	1253	2314	0.37%	0.039%
12	3.306	361	364	366	rBV3	321	460	0.07%	0.008%
13	3.367	373	374	378	rVB2	164	156	0.02%	0.003%
14	3.489	392	394	397	rBV2	395	388	0.06%	0.007%
15	3.611	406	414	422	rBV	4238	9060	1.45%	0.153%
16	3.703	427	429	433	rVB	203	191	0.03%	0.003%
17	3.867	452	456	461	rBV5	705	1665	0.27%	0.028%
18	4.020	480	481	483	rBV2	252	183	0.03%	0.003%
19	4.056	485	487	489	rBV2	189	211	0.03%	0.004%
20	4.483	543	557	572	rBV2	86402	355468	56.77%	6.018%
21	4.702	591	593	595	rVB	284	157	0.03%	0.003%
22	4.788	606	607	610	rVB2	169	157	0.03%	0.003%
23	5.056	639	651	673	rVB2	88183	277088	44.25%	4.691%
24	5.385	698	705	715	rVB2	2644	7163	1.14%	0.121%
25	5.538	728	730	731	rBV	243	238	0.04%	0.004%
26	5.745	762	764	766	rBV	254	237	0.04%	0.004%
27	5.879	784	786	787	rBV	181	155	0.02%	0.003%
28	5.971	789	801	820	rBV2	209719	626134	100.00%	10.600%
29	6.367	864	866	870	rBV2	196	264	0.04%	0.004%
30	6.477	881	884	887	rBV	215	298	0.05%	0.005%
31	6.501	887	888	892	rVV2	185	172	0.03%	0.003%
32	6.580	898	901	907	rBV2	157	259	0.04%	0.004%
33	6.763	921	931	945	rBV	156415	378001	60.37%	6.400%
34	7.123	982	990	1005	rVV	94784	206375	32.96%	3.494%
35	7.306	1012	1020	1036	rBV	133187	290350	46.37%	4.916%
36	7.428	1037	1040	1047	rVB2	2494	4306	0.69%	0.073%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
 Data File : VX040669.D
 Acq On : 15 Mar 2024 21:44
 Operator : JC/MD
 Sample : P1754-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YCL07

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
 Title : VOC Analysis

37	7.684	1079	1082	1085	rBV2	162	265	0.04%	0.004%
38	7.739	1088	1091	1094	rBV2	158	180	0.03%	0.003%
39	7.848	1106	1109	1110	rVV	360	307	0.05%	0.005%
40	7.903	1114	1118	1123	rVV4	1036	1996	0.32%	0.034%
41	7.940	1123	1124	1127	rVV2	713	665	0.11%	0.011%
42	7.982	1129	1131	1132	rBV	211	168	0.03%	0.003%
43	8.324	1181	1187	1199	rBV	92271	147014	23.48%	2.489%
44	8.482	1211	1213	1217	rVB4	343	474	0.08%	0.008%
45	8.647	1234	1240	1251	rBV	292468	462028	73.79%	7.822%
46	8.763	1257	1259	1261	rBV2	331	230	0.04%	0.004%
47	8.805	1265	1266	1268	rBV	307	224	0.04%	0.004%
48	8.952	1284	1290	1304	rBV	64464	100820	16.10%	1.707%
49	9.086	1310	1312	1315	rBV2	172	205	0.03%	0.003%
50	9.275	1338	1343	1352	rBV4	5393	8348	1.33%	0.141%
51	9.385	1355	1361	1378	rBV	258734	380289	60.74%	6.438%
52	9.641	1402	1403	1410	rVV2	279	336	0.05%	0.006%
53	9.732	1416	1418	1420	rBV	266	206	0.03%	0.003%
54	10.055	1465	1471	1487	rBV	326274	466391	74.49%	7.896%
55	10.305	1508	1512	1518	rVB3	564	969	0.15%	0.016%
56	10.403	1527	1528	1531	rBV	216	215	0.03%	0.004%
57	10.573	1553	1556	1560	rBV	200	280	0.04%	0.005%
58	10.866	1600	1604	1607	rBV2	247	371	0.06%	0.006%
59	11.000	1623	1626	1628	rBV2	188	198	0.03%	0.003%
60	11.092	1638	1641	1644	rVB	630	668	0.11%	0.011%
61	11.189	1652	1657	1664	rBV	254023	317755	50.75%	5.380%
62	11.287	1671	1673	1674	rBV	330	189	0.03%	0.003%
63	11.311	1674	1677	1682	rVV3	912	1286	0.21%	0.022%
64	11.451	1697	1700	1701	rVV	283	321	0.05%	0.005%
65	11.677	1735	1737	1740	rVB2	200	230	0.04%	0.004%
66	11.732	1740	1746	1748	rBV2	184	250	0.04%	0.004%
67	11.756	1748	1750	1754	rBV2	307	349	0.06%	0.006%
68	11.969	1781	1785	1788	rBV2	498	652	0.10%	0.011%
69	12.018	1788	1793	1804	rVV	309380	408131	65.18%	6.910%
70	12.122	1807	1810	1813	rVB3	310	481	0.08%	0.008%
71	12.244	1825	1830	1831	rBV2	221	349	0.06%	0.006%
72	12.317	1837	1842	1853	rBV	324479	411042	65.65%	6.959%
73	12.396	1853	1855	1858	rVV4	420	556	0.09%	0.009%
74	12.445	1861	1863	1865	rVB	208	173	0.03%	0.003%
75	12.506	1871	1873	1876	rVB2	186	155	0.02%	0.003%
76	12.530	1876	1877	1879	rBV	157	167	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
 Data File : VX040669.D
 Acq On : 15 Mar 2024 21:44
 Operator : JC/MD
 Sample : P1754-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YCL07

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
 Title : VOC Analysis

77	12.756	1911	1914	1915	rBV	456	473	0.08%	0.008%
78	12.841	1925	1928	1929	rBV	232	230	0.04%	0.004%
79	12.866	1929	1932	1935	rVB2	206	207	0.03%	0.004%
80	12.963	1946	1948	1950	rBV	270	191	0.03%	0.003%
81	12.994	1950	1953	1955	rVB2	647	623	0.10%	0.011%
82	13.073	1963	1966	1967	rBV2	194	181	0.03%	0.003%
83	13.116	1971	1973	1977	rVB	464	374	0.06%	0.006%
84	13.353	2010	2012	2014	rBV2	227	188	0.03%	0.003%
85	13.439	2022	2026	2028	rBV2	335	375	0.06%	0.006%
86	13.597	2049	2052	2054	rVB2	401	503	0.08%	0.009%
87	13.658	2059	2062	2063	rBV2	309	264	0.04%	0.004%
88	13.780	2079	2082	2085	rBV3	387	573	0.09%	0.010%
89	13.969	2110	2113	2118	rVB4	363	619	0.10%	0.010%
90	14.036	2120	2124	2126	rBV	167	216	0.03%	0.004%
91	14.548	2205	2208	2209	rBV	282	379	0.06%	0.006%
92	14.652	2223	2225	2227	rVB2	207	187	0.03%	0.003%
93	14.719	2234	2236	2238	rBV	215	199	0.03%	0.003%
94	14.853	2254	2258	2259	rBV2	299	321	0.05%	0.005%
95	14.908	2265	2267	2270	rVB3	254	278	0.04%	0.005%
96	15.396	2341	2347	2349	rVB2	368	694	0.11%	0.012%
97	15.505	2363	2365	2367	rBV2	225	157	0.03%	0.003%
98	15.548	2371	2372	2376	rVB2	251	215	0.03%	0.004%
99	15.792	2411	2412	2415	rBV2	205	230	0.04%	0.004%
100	16.432	2515	2517	2520	rBV2	195	241	0.04%	0.004%




Sum of corrected areas: 5906656

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
Data File : VX040669.D
Acq On : 15 Mar 2024 21:44
Operator : JC/MD
Sample : P1754-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YCL07

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

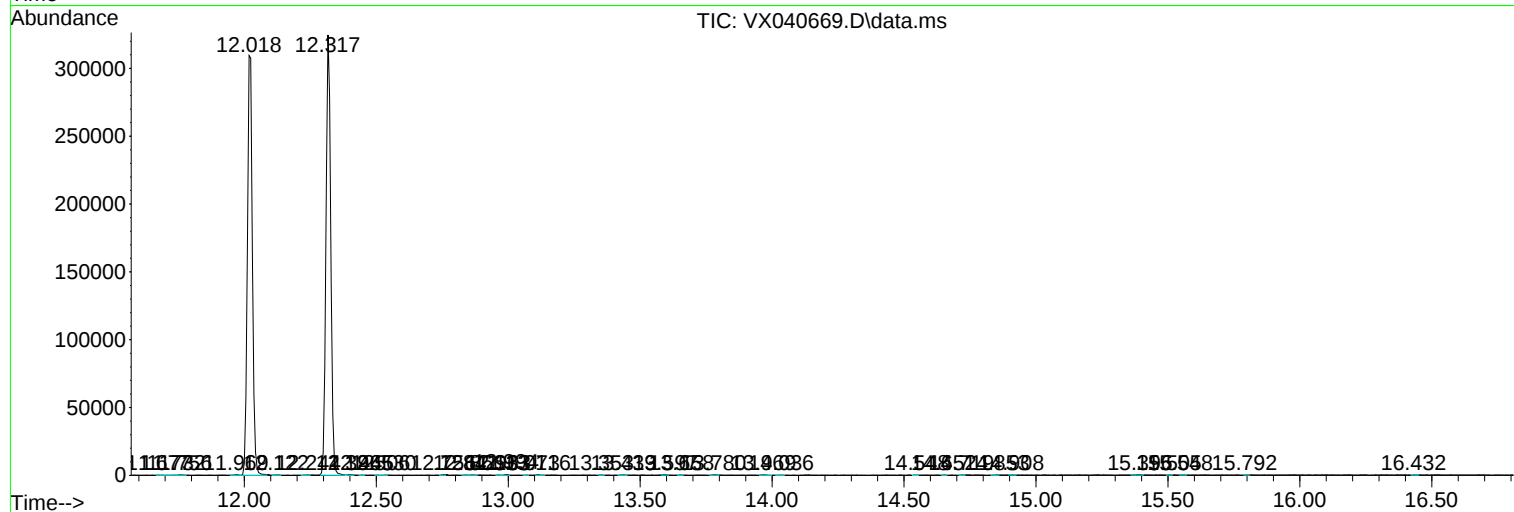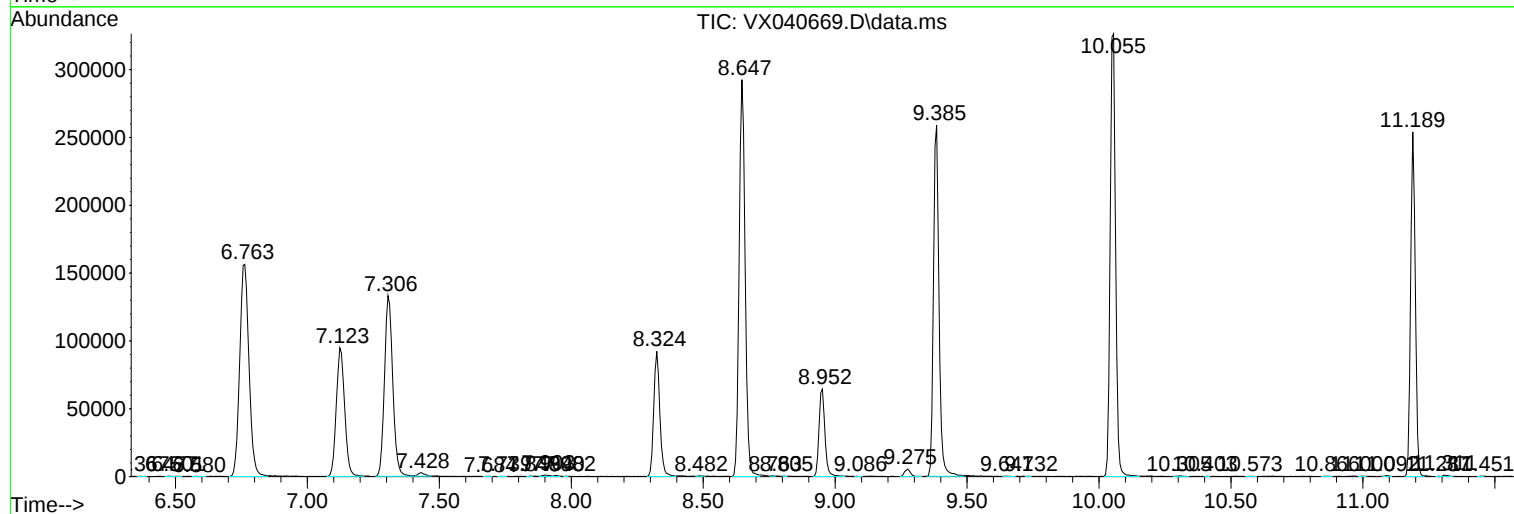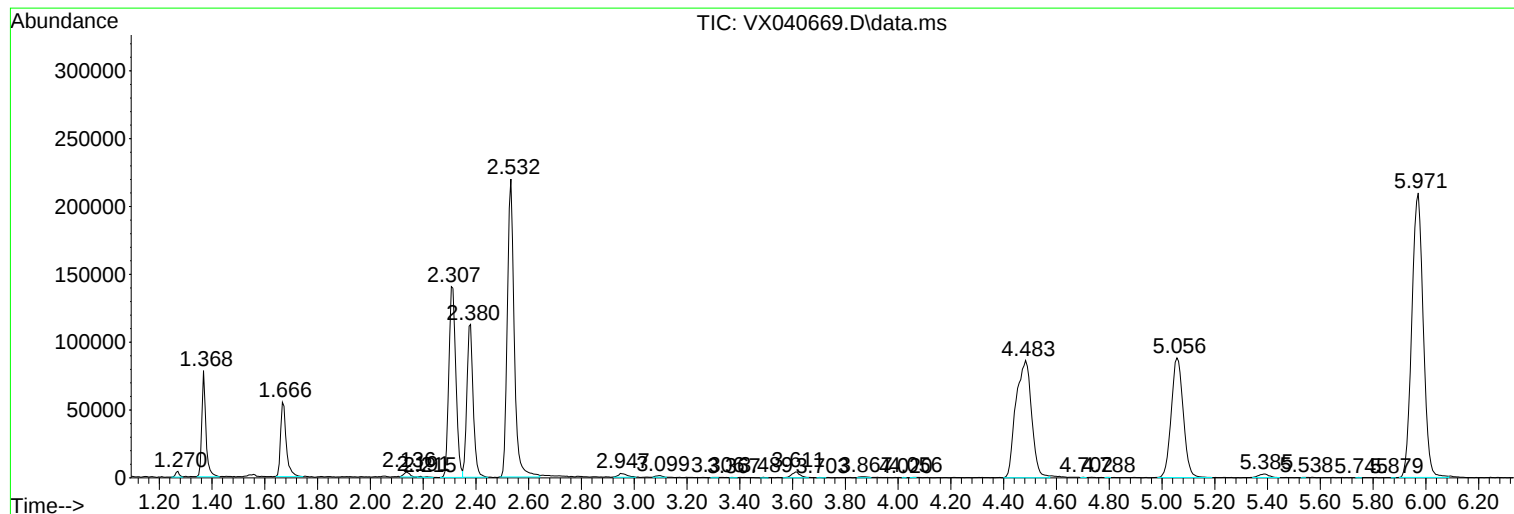

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
Data File : VX040669.D
Acq On : 15 Mar 2024 21:44
Operator : JC/MD
Sample : P1754-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YCL07










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM030724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.532	52.29 ug/L	395280	1,4-Difluorobenzene	6.763

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	78
2			Isopropyl Alcohol	60	C3H8O	000067-63-0	78
3			Isopropyl Alcohol	60	C3H8O	000067-63-0	56
4			Hydrazine, ethyl-	60	C2H8N2	000624-80-6	9
5			Isopropyl Alcohol	60	C3H8O	000067-63-0	9

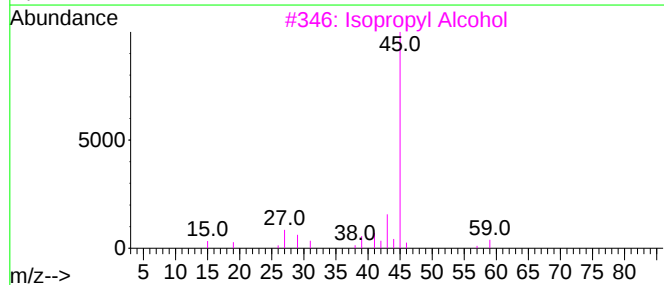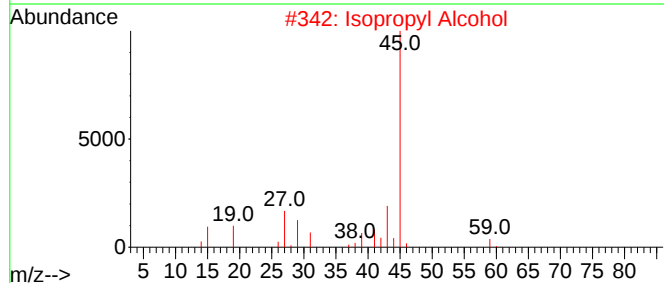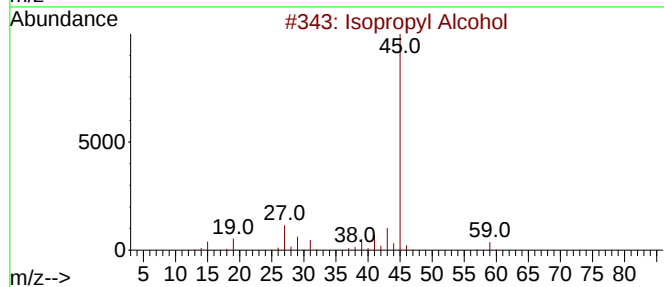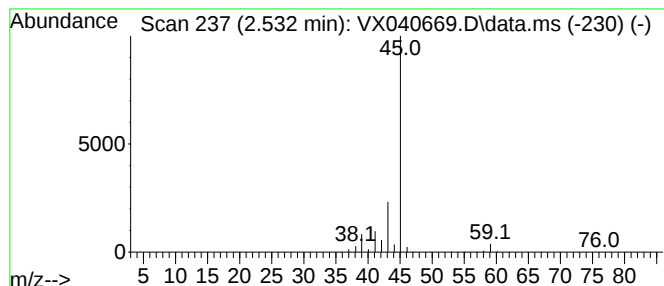

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
Data File : VX040669.D
Acq On : 15 Mar 2024 21:44
Operator : JC/MD
Sample : P1754-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YCL07

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.532	52.3	ug/L	395280	1	6.763	378001	50.0