

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
 Data File : VX040670.D
 Acq On : 15 Mar 2024 22:07
 Operator : JC/MD
 Sample : P1754-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YCL08

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
 Title : VOC Analysis

Signal : TIC: VX040670.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	7	9	12	rVB2	823	604	0.07%	0.009%
2	1.270	27	30	33	rVB	1513	1167	0.13%	0.018%
3	1.368	41	46	63	rVB2	102800	121966	13.47%	1.832%
4	1.666	90	95	104	rBV	57588	79115	8.74%	1.188%
5	2.087	162	164	165	rBV2	488	292	0.03%	0.004%
6	2.136	168	172	178	rVB	7233	11011	1.22%	0.165%
7	2.319	194	202	208	rBV2	522212	905368	100.00%	13.598%
8	2.380	208	212	228	rVB	63695	106997	11.82%	1.607%
9	2.532	229	237	249	rBV	443315	781425	86.31%	11.736%
10	2.959	302	307	314	rVB4	3122	6428	0.71%	0.097%
11	3.410	375	381	382	rBV2	261	496	0.05%	0.007%
12	3.611	406	414	424	rVB2	12775	30387	3.36%	0.456%
13	3.764	431	439	446	rBV4	1165	3132	0.35%	0.047%
14	4.032	481	483	487	rBV2	218	286	0.03%	0.004%
15	4.123	495	498	500	rBV2	193	240	0.03%	0.004%
16	4.245	515	518	519	rBV	174	173	0.02%	0.003%
17	4.324	530	531	534	rBV	206	218	0.02%	0.003%
18	4.459	542	553	567	rBV3	55737	216457	23.91%	3.251%
19	5.056	632	651	668	rBV2	90537	328191	36.25%	4.929%
20	5.379	696	704	722	rVB3	19290	61660	6.81%	0.926%
21	5.501	722	724	725	rBV	291	248	0.03%	0.004%
22	5.702	756	757	760	rBV2	268	239	0.03%	0.004%
23	5.727	760	761	764	rVB2	274	214	0.02%	0.003%
24	5.800	771	773	775	rBV	193	207	0.02%	0.003%
25	5.867	783	784	787	rVB2	215	194	0.02%	0.003%
26	5.970	788	801	818	rBV2	202863	618738	68.34%	9.293%
27	6.147	828	830	831	rBV2	232	217	0.02%	0.003%
28	6.476	881	884	887	rBV2	157	222	0.02%	0.003%
29	6.763	922	931	945	rBV	151817	363235	40.12%	5.455%
30	7.123	983	990	1001	rBV2	22863	52338	5.78%	0.786%
31	7.306	1011	1020	1036	rBV	128870	284591	31.43%	4.274%
32	7.434	1038	1041	1047	rVB4	2270	3744	0.41%	0.056%
33	7.617	1069	1071	1073	rBV	191	217	0.02%	0.003%
34	7.781	1097	1098	1102	rBV	273	256	0.03%	0.004%
35	8.244	1172	1174	1177	rVB	218	186	0.02%	0.003%
36	8.275	1177	1179	1181	rBV	166	206	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
 Data File : VX040670.D
 Acq On : 15 Mar 2024 22:07
 Operator : JC/MD
 Sample : P1754-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YCL08

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
 Title : VOC Analysis

37	8.324	1181	1187	1200	rVV	87520	141708	15.65%	2.128%
38	8.494	1211	1215	1218	rBV3	324	473	0.05%	0.007%
39	8.574	1226	1228	1230	rVB2	252	219	0.02%	0.003%
40	8.647	1234	1240	1251	rBV	285711	448555	49.54%	6.737%
41	8.848	1271	1273	1275	rVB	229	174	0.02%	0.003%
42	8.952	1284	1290	1301	rVV	63253	97061	10.72%	1.458%
43	9.055	1305	1307	1311	rVV2	285	418	0.05%	0.006%
44	9.177	1324	1327	1328	rBV	218	221	0.02%	0.003%
45	9.275	1339	1343	1349	rVB4	1604	2265	0.25%	0.034%
46	9.385	1355	1361	1378	rBV	251347	367963	40.64%	5.526%
47	9.580	1390	1393	1395	rBV	172	210	0.02%	0.003%
48	9.616	1395	1399	1403	rBV3	2570	3905	0.43%	0.059%
49	9.750	1419	1421	1424	rBV2	224	278	0.03%	0.004%
50	9.842	1433	1436	1439	rVB2	341	352	0.04%	0.005%
51	9.884	1441	1443	1446	rVB	379	343	0.04%	0.005%
52	9.921	1446	1449	1451	rBV	373	498	0.06%	0.007%
53	9.970	1454	1457	1458	rBV2	168	215	0.02%	0.003%
54	10.055	1465	1471	1482	rBV	326076	452803	50.01%	6.801%
55	10.305	1510	1512	1515	rBV3	429	557	0.06%	0.008%
56	10.439	1532	1534	1537	rBV	181	239	0.03%	0.004%
57	10.494	1540	1543	1545	rVB	205	180	0.02%	0.003%
58	10.689	1573	1575	1577	rBV	199	163	0.02%	0.002%
59	10.726	1579	1581	1584	rBV2	157	179	0.02%	0.003%
60	10.774	1587	1589	1591	rVB	257	222	0.02%	0.003%
61	10.963	1618	1620	1623	rBV2	319	321	0.04%	0.005%
62	11.031	1629	1631	1634	rBV2	353	403	0.04%	0.006%
63	11.092	1639	1641	1645	rVB3	466	507	0.06%	0.008%
64	11.140	1645	1649	1652	rBV2	121	182	0.02%	0.003%
65	11.189	1652	1657	1664	rVV	251819	332245	36.70%	4.990%
66	11.317	1675	1678	1684	rVB3	957	1386	0.15%	0.021%
67	11.421	1692	1695	1697	rBV2	190	266	0.03%	0.004%
68	11.494	1706	1707	1708	rBV2	275	177	0.02%	0.003%
69	11.756	1748	1750	1754	rVB2	470	409	0.05%	0.006%
70	11.811	1756	1759	1762	rVB	164	201	0.02%	0.003%
71	11.847	1762	1765	1766	rBV	170	184	0.02%	0.003%
72	11.933	1776	1779	1782	rBV2	161	249	0.03%	0.004%
73	11.969	1782	1785	1788	rBV2	256	234	0.03%	0.004%
74	12.024	1788	1794	1803	rBV	322083	408946	45.17%	6.142%
75	12.317	1837	1842	1849	rBV	316665	403692	44.59%	6.063%
76	12.494	1869	1871	1874	rVV	197	185	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
 Data File : VX040670.D
 Acq On : 15 Mar 2024 22:07
 Operator : JC/MD
 Sample : P1754-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YCL08

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
 Title : VOC Analysis

77	12.707	1904	1906	1908	rBV	185	198	0.02%	0.003%
78	12.762	1908	1915	1921	rVV4	606	1232	0.14%	0.019%
79	12.823	1921	1925	1930	rBV2	273	524	0.06%	0.008%
80	13.116	1972	1973	1975	rVB2	326	222	0.02%	0.003%
81	13.146	1975	1978	1981	rBV	271	415	0.05%	0.006%
82	13.250	1992	1995	1997	rBV	139	169	0.02%	0.003%
83	13.433	2020	2025	2027	rBV2	454	548	0.06%	0.008%
84	13.701	2068	2069	2072	rVV	202	183	0.02%	0.003%
85	13.786	2079	2083	2086	rVB2	527	607	0.07%	0.009%
86	13.969	2110	2113	2116	rBV2	348	494	0.05%	0.007%
87	14.128	2137	2139	2141	rBV2	292	287	0.03%	0.004%
88	14.310	2164	2169	2170	rBV2	235	309	0.03%	0.005%
89	14.445	2189	2191	2193	rVB2	257	194	0.02%	0.003%
90	14.993	2279	2281	2282	rBV	248	189	0.02%	0.003%
91	15.042	2287	2289	2290	rBV2	264	247	0.03%	0.004%
92	15.158	2307	2308	2310	rBV	386	357	0.04%	0.005%
93	15.316	2332	2334	2338	rBV2	282	320	0.04%	0.005%
94	15.365	2340	2342	2344	rVB	398	255	0.03%	0.004%
95	15.390	2344	2346	2351	rBV4	397	671	0.07%	0.010%
96	15.700	2396	2397	2400	rBV	310	213	0.02%	0.003%
97	15.731	2400	2402	2404	rBV2	177	157	0.02%	0.002%
98	15.798	2410	2413	2416	rBV3	256	414	0.05%	0.006%
99	16.237	2484	2485	2488	rBV2	231	197	0.02%	0.003%
100	16.334	2499	2501	2505	rBV2	328	389	0.04%	0.006%




Sum of corrected areas: 6658244

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
Data File : VX040670.D
Acq On : 15 Mar 2024 22:07
Operator : JC/MD
Sample : P1754-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YCL08

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM030724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

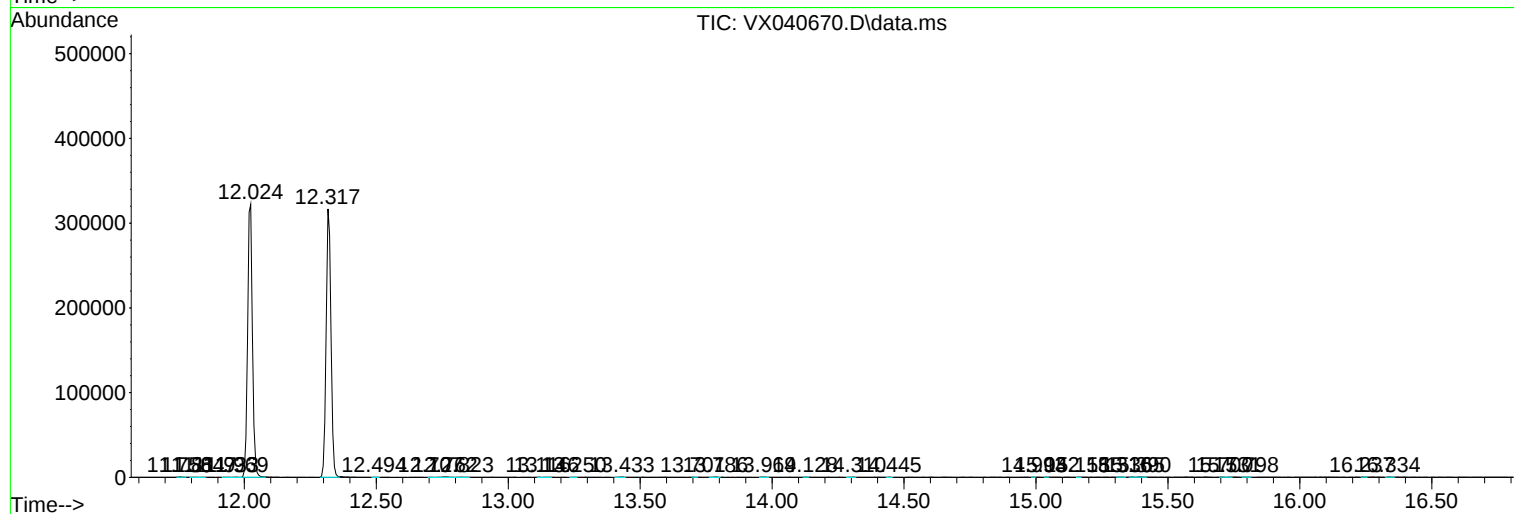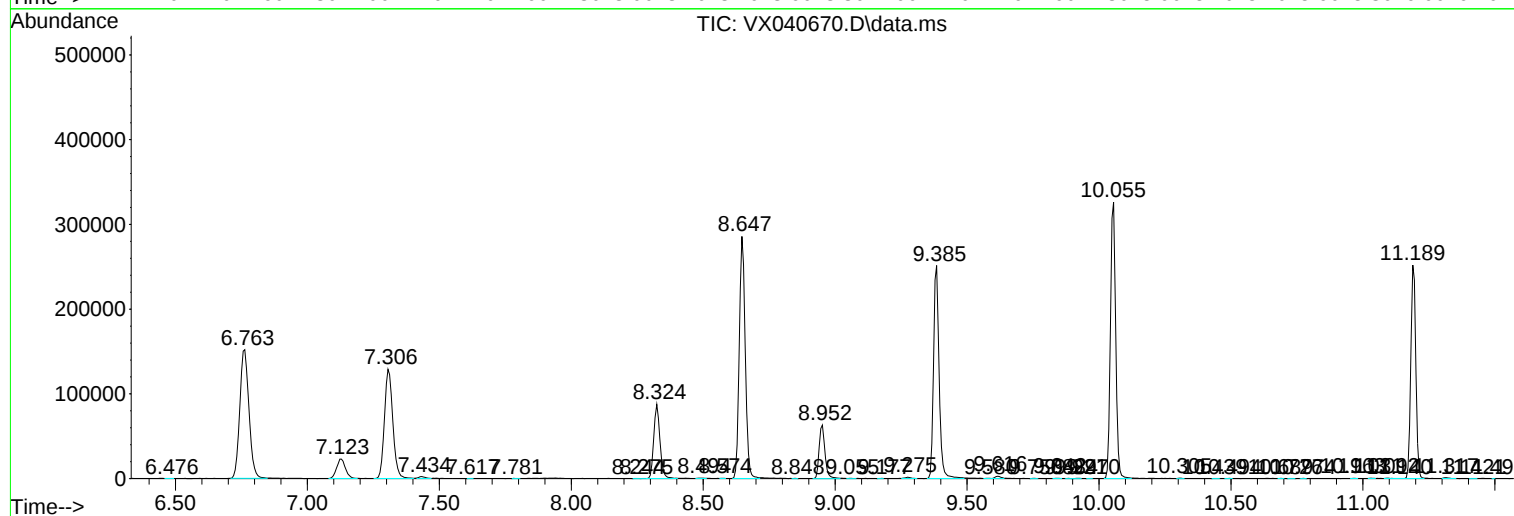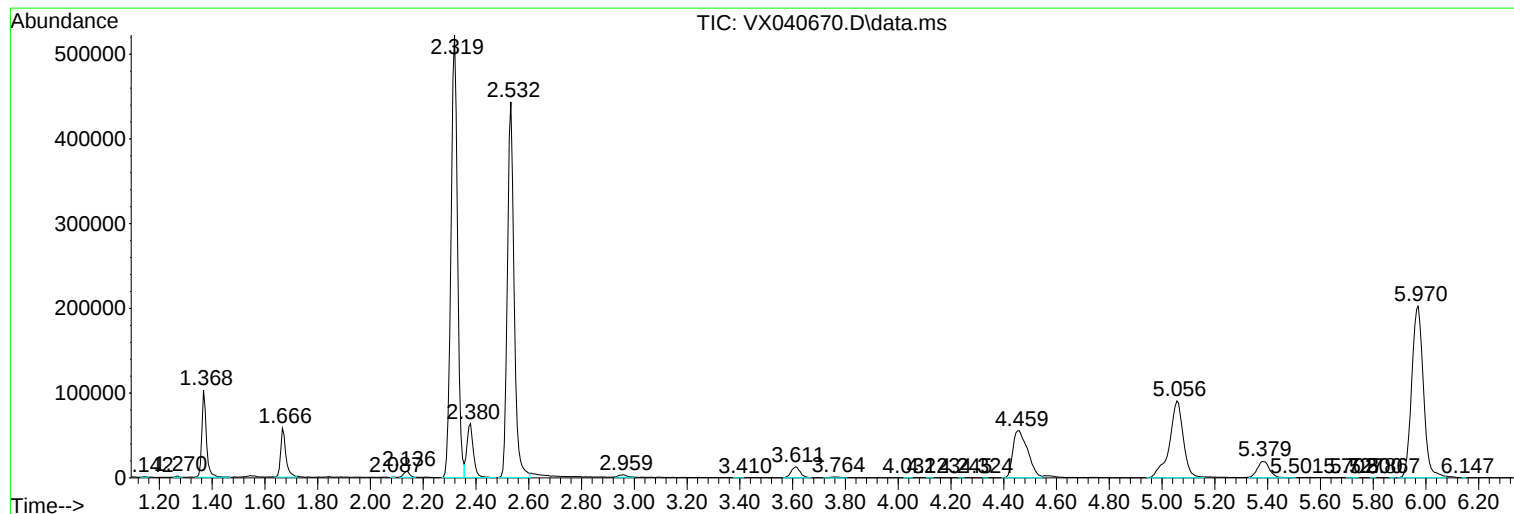

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
Data File : VX040670.D
Acq On : 15 Mar 2024 22:07
Operator : JC/MD
Sample : P1754-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YCL08










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.532	107.57 ug/L	781425	1,4-Difluorobenzene	6.763

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	78
2			Isopropyl Alcohol	60	C3H8O	000067-63-0	78
3			Isopropyl Alcohol	60	C3H8O	000067-63-0	56
4			Hydrazine, ethyl-	60	C2H8N2	000624-80-6	9
5			Isopropyl Alcohol	60	C3H8O	000067-63-0	9

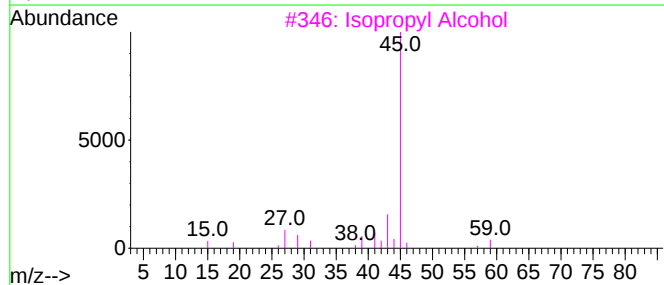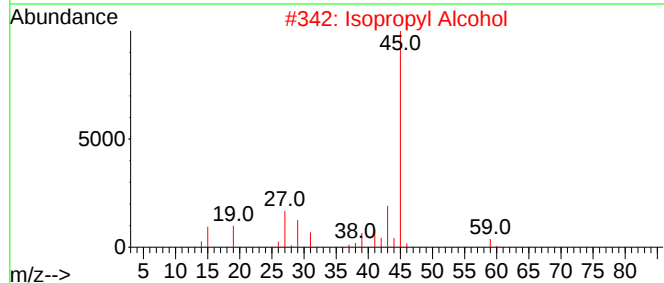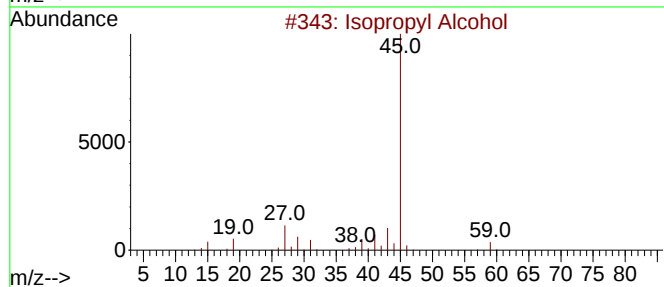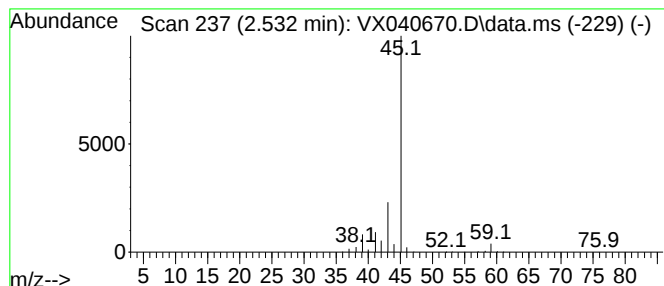

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
Data File : VX040670.D
Acq On : 15 Mar 2024 22:07
Operator : JC/MD
Sample : P1754-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YCL08

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.532	107.6	ug/L	781425	1	6.763	363235	50.0