
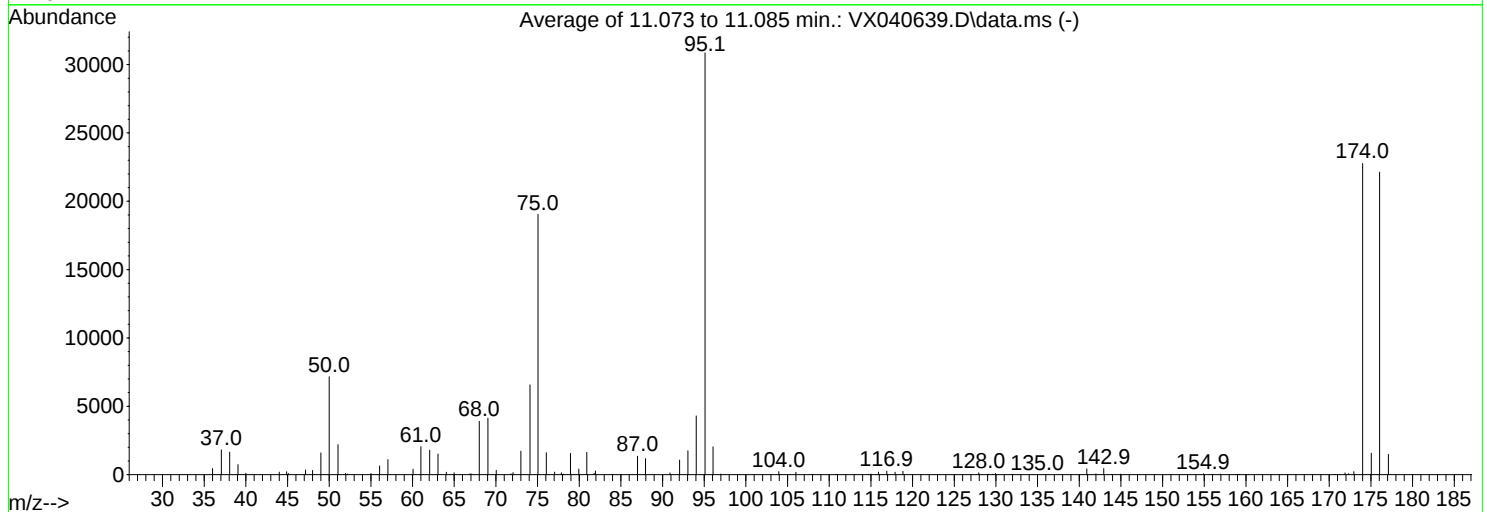


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031524\
Data File : VX040639.D
Acq On : 15 Mar 2024 09:10
Operator : JC/MD
Sample : BFB667
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB667

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM030724WMA.M
Title : VOC Analysis
Last Update : Tue Mar 19 01:22:22 2024

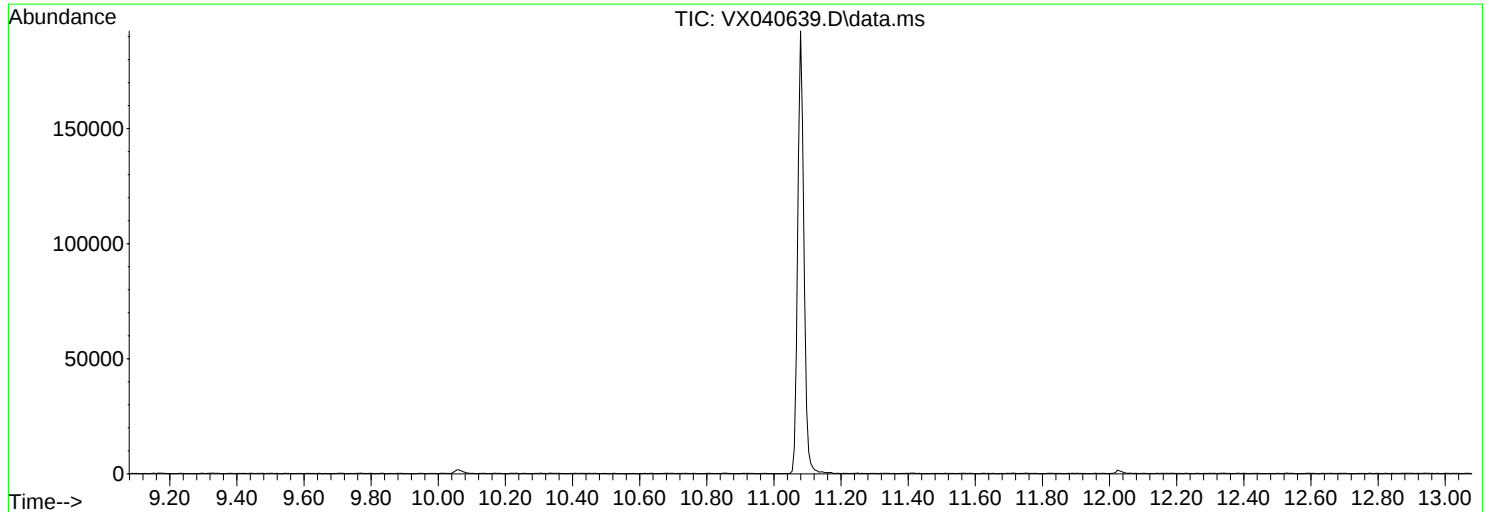

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.2	7170	PASS
75	95	30	80	61.7	19045	PASS
95	95	100	100	100.0	30859	PASS
96	95	5	9	6.6	2042	PASS
173	174	0.00	2	1.0	220	PASS
174	95	50	120	73.8	22771	PASS
175	174	5	9	6.9	1574	PASS
176	174	95	101	97.2	22133	PASS
177	176	5	9	6.7	1487	PASS

m/z	Abundance
39.90	82.0
44.00	91.0

Instrument :
MSVOA_X
ClientSampleId :
BFB667

m/z	Abundance
36.00	480.0
37.00	1888.0
38.00	1630.0
39.00	735.0
40.10	174.0
44.10	273.0
44.90	276.0
47.10	226.0
48.00	329.0
49.00	1589.0
50.00	6842.0
51.10	2173.0
51.90	76.0
55.00	66.0
56.10	610.0
57.00	1022.0
60.10	453.0
61.00	1988.0
62.00	1500.0
63.00	1409.0
64.10	110.0
65.00	132.0
66.90	82.0
68.00	3606.0
69.00	3791.0
70.00	286.0
72.10	174.0
73.00	1444.0
74.10	5922.0
75.00	16904.0
76.00	1330.0
77.80	245.0
78.90	1265.0
79.90	346.0
80.90	1475.0
81.80	268.0
87.10	1084.0
87.90	1056.0
90.90	103.0
92.10	1047.0
93.00	1536.0
94.00	4094.0
95.10	26880.0
96.10	1716.0
103.90	133.0
106.10	175.0
115.00	125.0
116.00	120.0
116.90	228.0
117.90	147.0
118.80	200.0
128.00	81.0
130.00	98.0
140.90	281.0
142.00	72.0
143.00	300.0
146.10	57.0
154.90	69.0
158.80	56.0
172.00	104.0
173.00	194.0
174.00	17728.0
175.00	1429.0
176.10	16256.0
177.10	1318.0

Instrument :
MSVOA_X
ClientSampleId :
BFB667

m/z	Abundance
36.00	487.0
37.10	2102.0
38.00	1990.0
39.10	850.0
40.00	186.0
44.00	362.0
44.90	351.0
47.10	415.0
48.00	380.0
49.10	1782.0
50.00	8516.0
51.00	2626.0
52.00	159.0
55.00	116.0
56.00	692.0
57.10	1363.0
60.00	459.0
61.00	2396.0
62.00	2156.0
63.10	1703.0
64.00	273.0
65.00	178.0
66.90	141.0
68.00	4763.0
69.00	4953.0
70.10	420.0
71.80	176.0
73.00	2028.0
74.10	7765.0
75.00	22800.0
76.10	2136.0
77.00	399.0
77.90	163.0
79.00	1861.0
80.00	461.0
80.90	2085.0
82.00	450.0
87.00	1608.0
88.00	1441.0
90.90	174.0
92.10	1111.0
93.00	2014.0
94.10	5152.0
95.10	37744.0
96.00	2565.0
97.00	74.0
104.00	355.0
106.00	242.0
110.80	59.0
113.10	63.0
114.70	65.0
115.90	243.0
117.00	332.0
117.80	146.0
118.80	242.0
127.90	141.0
129.10	55.0
129.90	157.0
135.00	54.0
137.00	60.0
140.90	468.0
142.00	108.0
142.90	499.0
145.00	63.0
154.90	66.0
156.90	55.0
159.20	74.0
170.70	55.0
171.80	128.0
172.30	199.0
172.80	198.0
174.00	26240.0
175.10	1714.0
176.00	26576.0
177.10	1736.0

Instrument :
MSVOA_X
ClientSampleId :
BFB667

m/z	Abundance
36.00	380.0
37.00	1455.0
38.10	1339.0
39.00	636.0
40.00	189.0
44.00	208.0
45.10	258.0
47.20	361.0
48.00	190.0
48.90	1421.0
50.00	6151.0
51.00	1817.0
52.20	158.0
55.00	76.0
56.00	598.0
57.00	911.0
60.00	297.0
61.00	1760.0
62.10	1707.0
63.10	1411.0
64.00	133.0
65.10	94.0
67.10	129.0
68.00	3328.0
69.10	3641.0
70.00	237.0
72.00	282.0
73.00	1679.0
74.10	6020.0
75.10	17432.0
76.00	1358.0
77.10	161.0
78.10	122.0
78.90	1540.0
80.00	436.0
80.90	1306.0
81.90	351.0
86.90	1339.0
88.00	1021.0
90.90	122.0
92.00	1036.0
93.10	1681.0
94.00	3631.0
95.10	27952.0
96.10	1844.0
97.00	55.0
104.00	188.0
105.90	109.0
107.00	55.0
110.00	52.0
115.80	198.0
116.80	222.0
118.00	222.0
118.90	305.0
127.90	189.0
129.60	66.0
140.90	502.0
143.00	551.0
143.90	60.0
144.90	56.0
150.00	54.0
154.90	64.0
157.00	75.0
171.90	168.0
173.00	267.0
174.00	24344.0
175.10	1580.0
176.00	23568.0
177.10	1407.0

Instrument :
MSVOA_X
ClientSampleId :
BFB667