

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX031620\
 Data File : VX015293.D
 Acq On : 16 Mar 2020 14:50
 Operator : JC/SP
 Sample : L1903-18DL 50X
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TT101D2-20200310DL

Quant Time: Mar 17 08:22:09 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X030420W.M
 Quant Title : SW846 8260
 QLast Update : Wed Mar 04 14:19:10 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.65	168	308169	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.85	114	508422	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	486138	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.07	152	249224	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.06	65	178807	48.91	ug/l	0.00
Spiked Amount 50.000			Recovery	=	97.82%	
35) Dibromofluoromethane	5.49	113	151967	47.38	ug/l	0.00
Spiked Amount 50.000			Recovery	=	94.76%	
50) Toluene-d8	8.71	98	621192	50.91	ug/l	0.00
Spiked Amount 50.000			Recovery	=	101.82%	
62) 4-Bromofluorobenzene	11.13	95	228822	52.58	ug/l	0.00
Spiked Amount 50.000			Recovery	=	105.16%	
Target Compounds						
44) Trichloroethene	7.21	130	87134	22.437	ug/l	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX031620\
Data File : VX015293.D
Acq On : 16 Mar 2020 14:50
Operator : JC/SP
Sample : L1903-18DL 50X
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TT101D2-20200310DL

Quant Time: Mar 17 08:22:09 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X030420W.M
Quant Title : SW846 8260
QLast Update : Wed Mar 04 14:19:10 2020
Response via : Initial Calibration

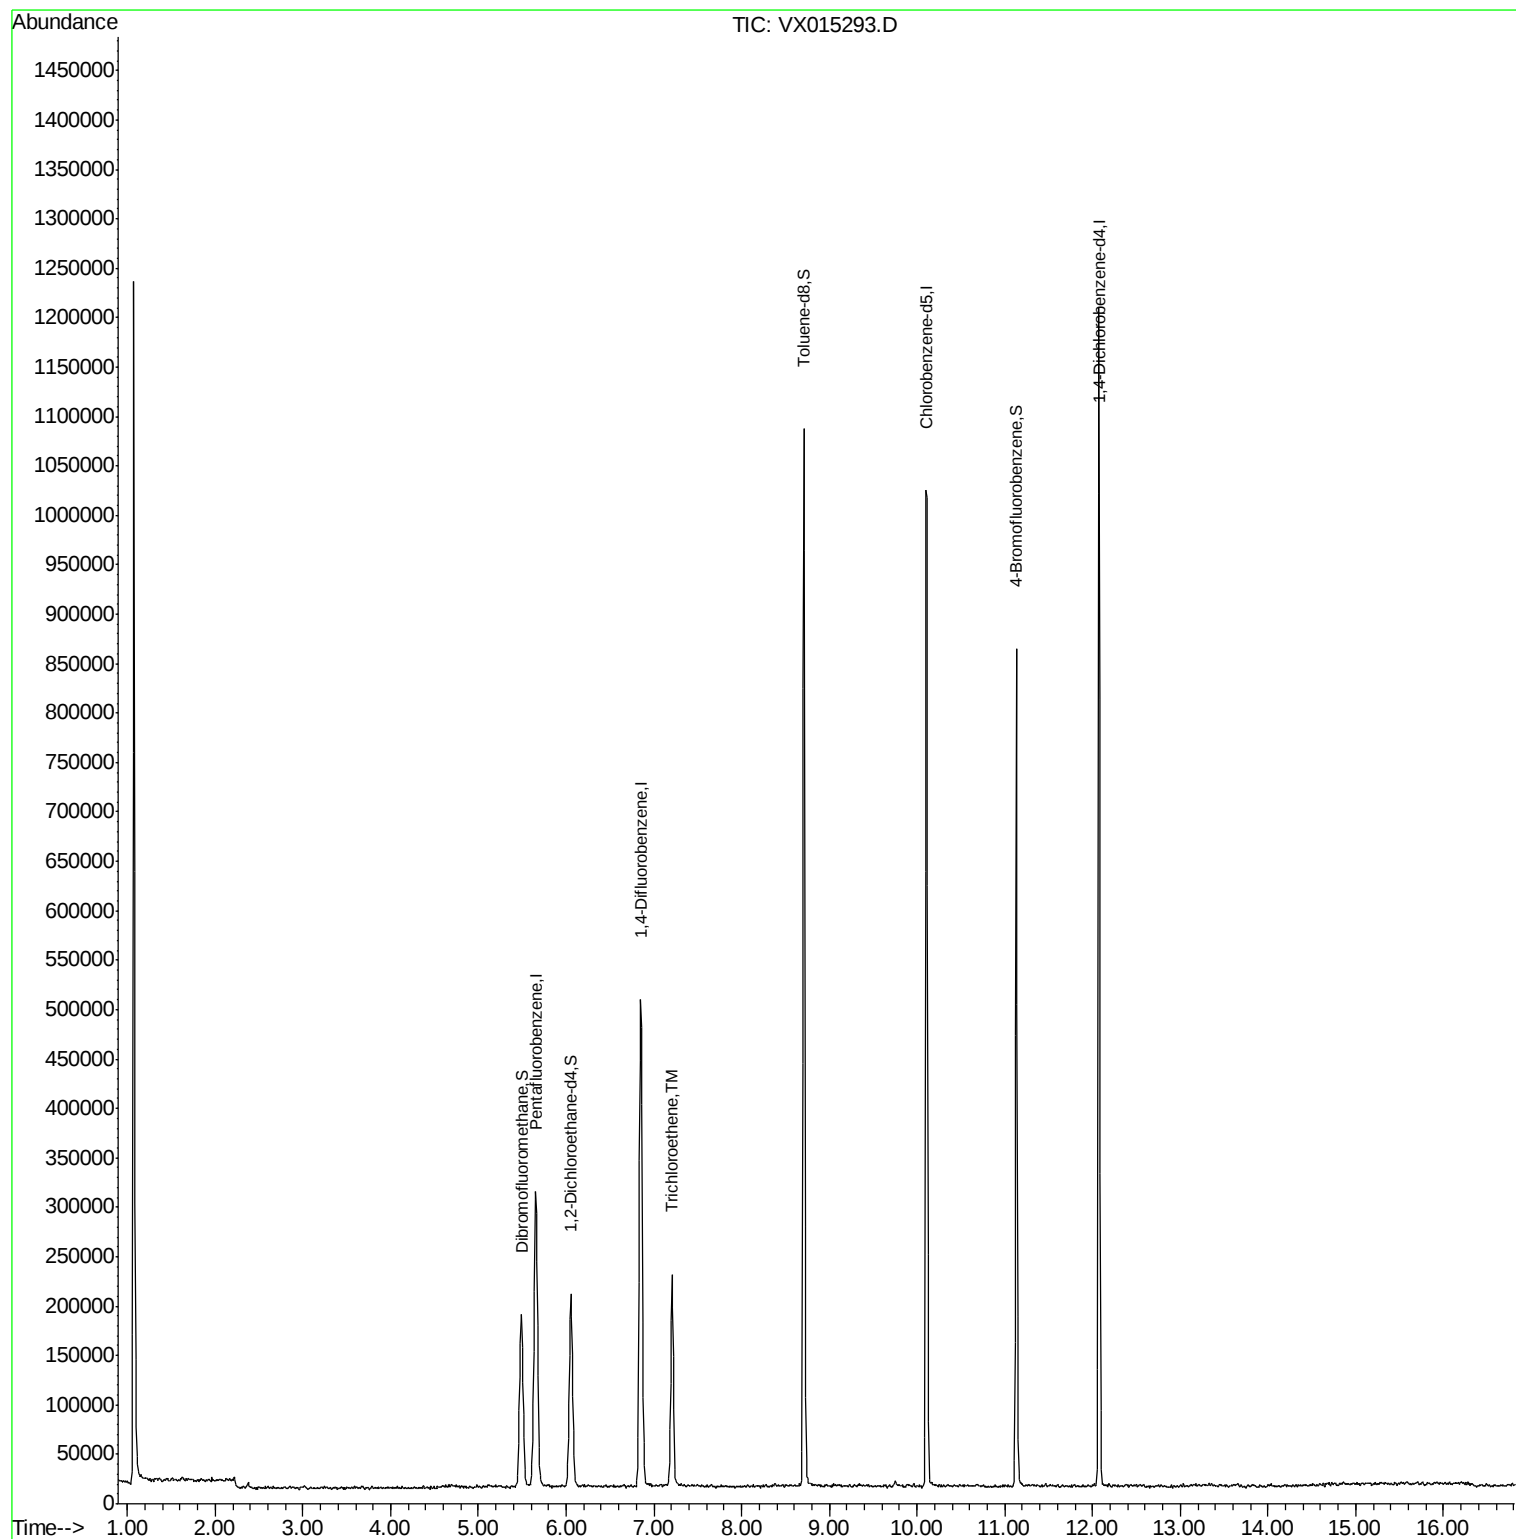

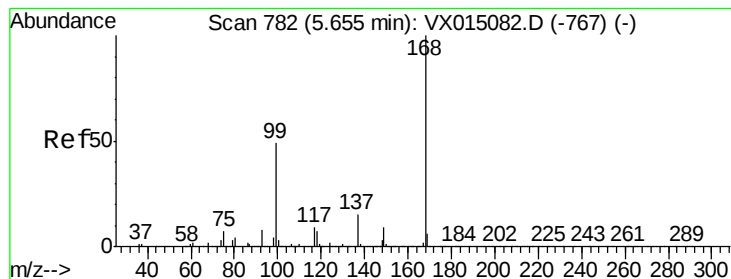

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.65 min Scan# 782

Delta R.T. -0.00 min

Lab File: VX015293.D

Acq: 16 Mar 2020 14:50

Instrument :

MSVOA_X

ClientSampleId :


TT101D2-20200310DL

Tot Ion:168 Resp: 308169

Ion Ratio Lower Upper




168 100

99 48.8 39.4 59.2

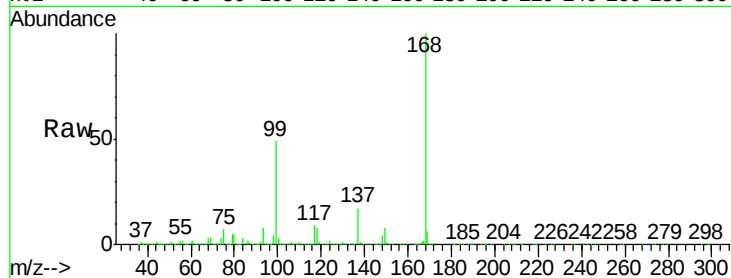

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

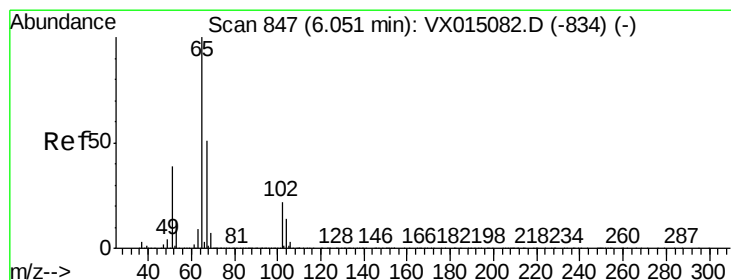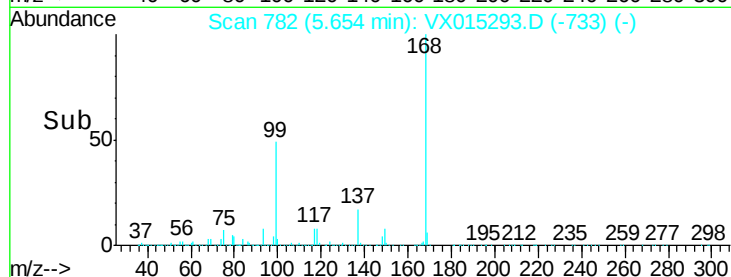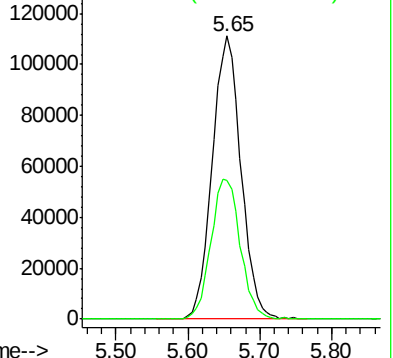

#33

1,2-Dichloroethane-d4

Concen: 48.907 ug/l

RT: 6.06 min Scan# 848

Delta R.T. 0.01 min

Lab File: VX015293.D


Acq: 16 Mar 2020 14:50

Tgt Ion: 65 Resp: 178807

Ion Ratio Lower Upper



65 100


67 53.6 0.0 105.6

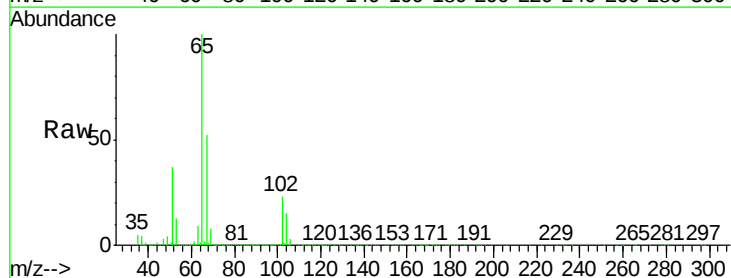

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

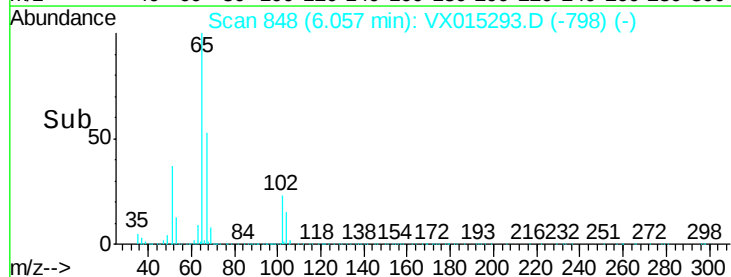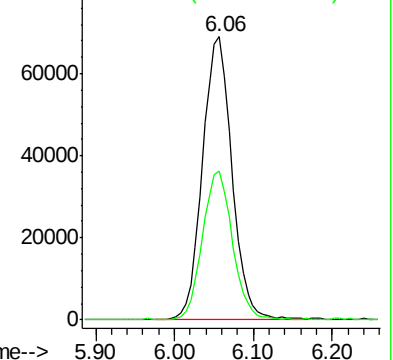

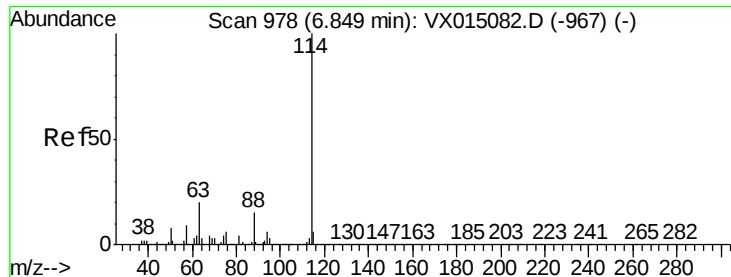

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.85 min Scan# 978

Delta R.T. -0.00 min

Lab File: VX015293.D

Acq: 16 Mar 2020 14:50

Instrument :

MSVOA_X

ClientSampleId :

TT101D2-20200310DL


Tot Ion:114 Resp: 508422

Ion Ratio Lower Upper

114 100

63 21.0 0.0 40.0




88 15.8 0.0 30.6

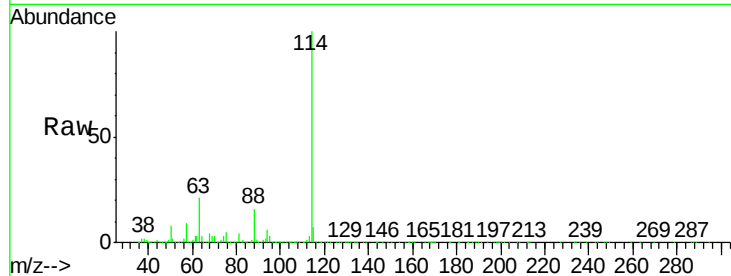

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

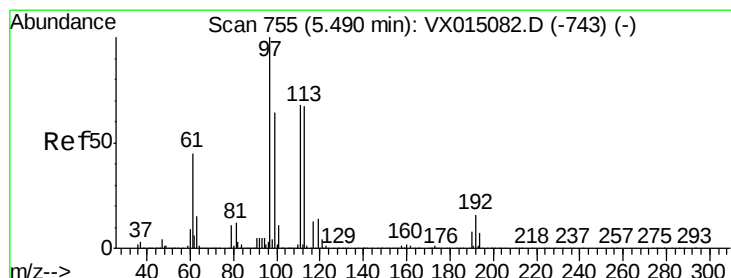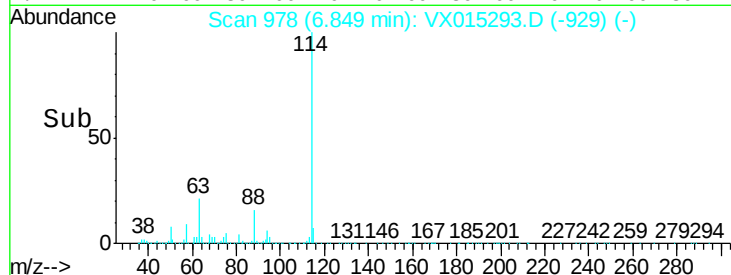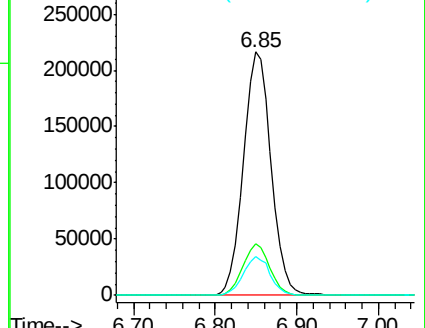

#35

Dibromofluoromethane

Concen: 47.379 ug/l

RT: 5.49 min Scan# 755

Delta R.T. -0.00 min

Lab File: VX015293.D

Acq: 16 Mar 2020 14:50


Tgt Ion:113 Resp: 151967

Ion Ratio Lower Upper

113 100

111 104.2 82.6 123.8



192 23.8 18.6 28.0

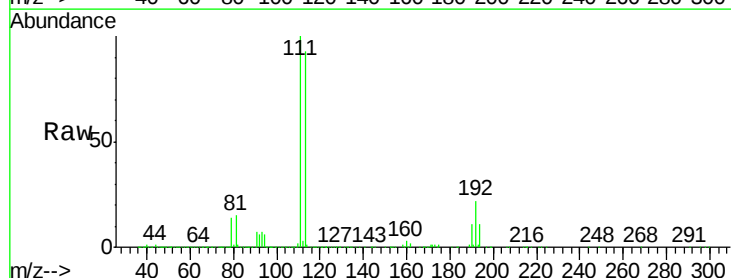


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

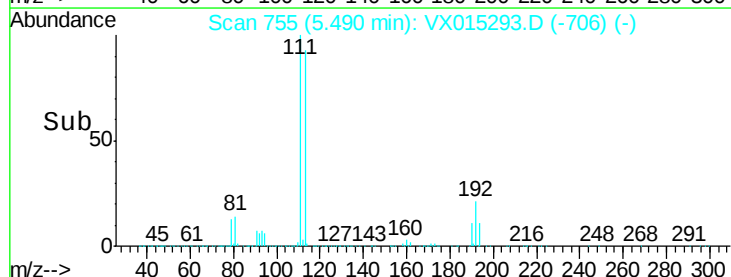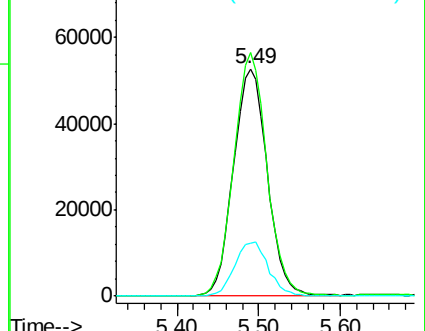

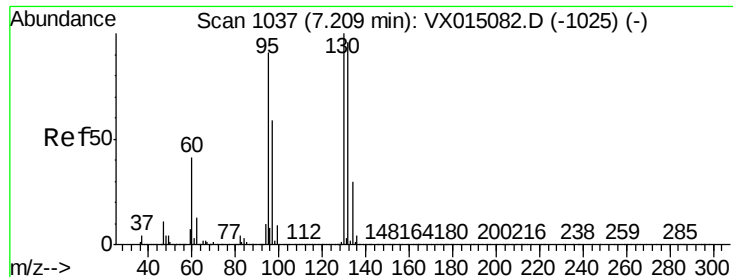

#44

Trichloroethene

Concen: 22.437 ug/l

RT: 7.21 min Scan# 1037

Delta R.T. -0.00 min

Lab File: VX015293.D

Acq: 16 Mar 2020 14:50

Instrument :

MSVOA_X

ClientSampleId :


TT101D2-20200310DL

Tot Ion:130 Resp: 87134

Ion Ratio Lower Upper




130 100

95 96.2 0.0 181.2

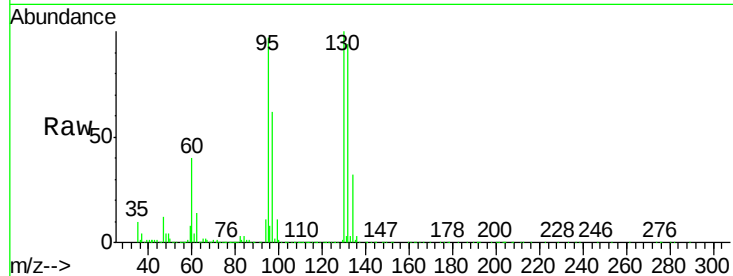

Abundance Ion 129.80 (129.50 to 130.50): V

Ion 94.90 (94.60 to 95.60): VX0

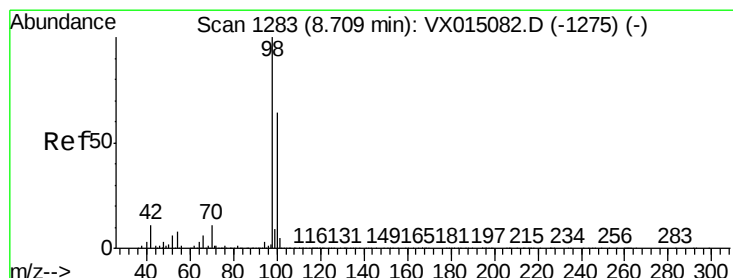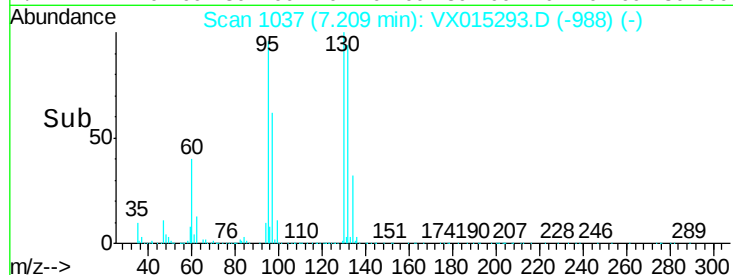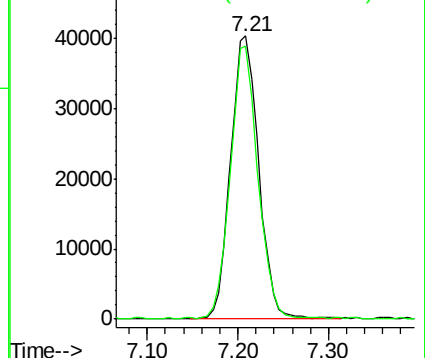

#50

Toluene-d8

Concen: 50.914 ug/l

RT: 8.71 min Scan# 1283

Delta R.T. -0.00 min

Lab File: VX015293.D


Acq: 16 Mar 2020 14:50

Tgt Ion: 98 Resp: 621192

Ion Ratio Lower Upper



98 100


100 65.7 52.4 78.6

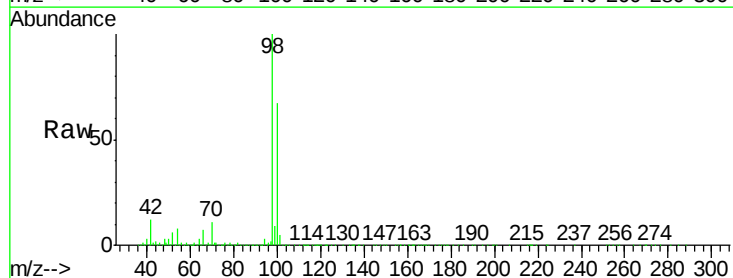

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): VX0

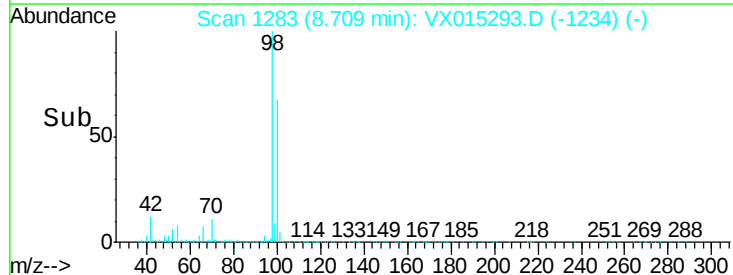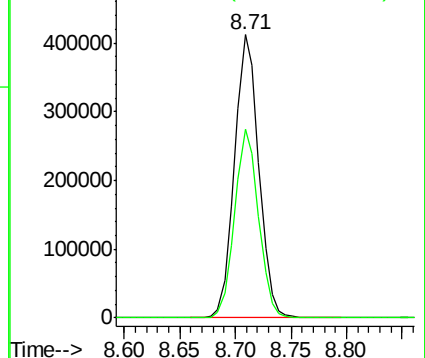

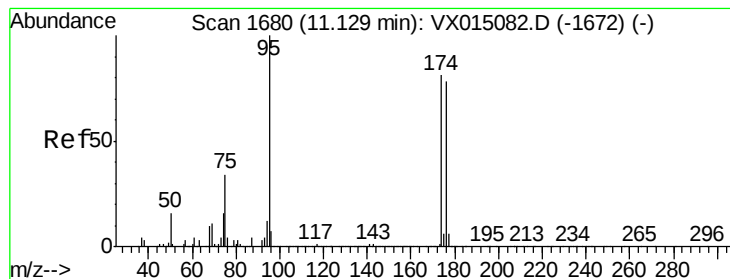

#62

4-Bromofluorobenzene

Concen: 52.580 ug/l

RT: 11.13 min Scan# 1680

Delta R.T. -0.00 min

Lab File: VX015293.D

Acq: 16 Mar 2020 14:50

Instrument :

MSVOA_X

ClientSampleId :

TT101D2-20200310DL


Tot Ion: 95 Resp: 228822

Ion Ratio Lower Upper

95 100

174 87.6 0.0 177.6

176 84.8 0.0 170.2

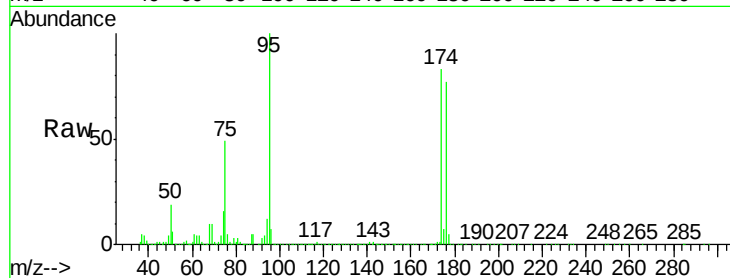


Abundance Ion 94.90 (94.60 to 95.60): VX015082.D (-1672) (-)

Ion 173.80 (173.50 to 174.50): VX015082.D (-1672) (-)

Ion 175.80 (175.50 to 176.50): VX015082.D (-1672) (-)

Time-->

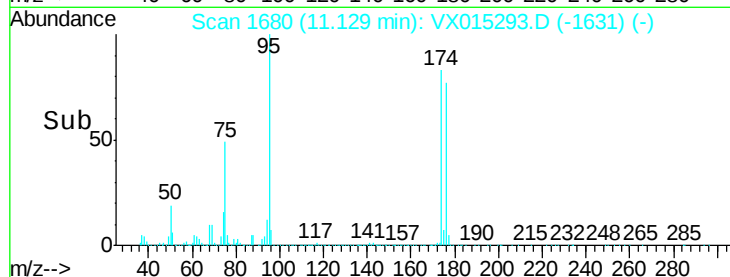


Abundance Ion 94.90 (94.60 to 95.60): VX015293.D (-1631) (-)

Ion 173.80 (173.50 to 174.50): VX015293.D (-1631) (-)

Ion 175.80 (175.50 to 176.50): VX015293.D (-1631) (-)

Time-->

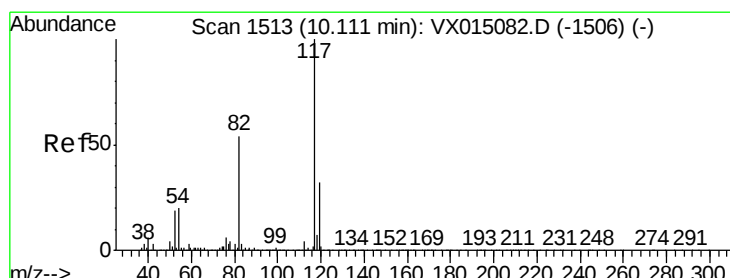

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.11 min Scan# 1513

Delta R.T. -0.00 min

Lab File: VX015293.D

Acq: 16 Mar 2020 14:50


Tgt Ion: 117 Resp: 486138

Ion Ratio Lower Upper

117 100

82 53.1 43.3 64.9

119 33.1 25.8 38.8

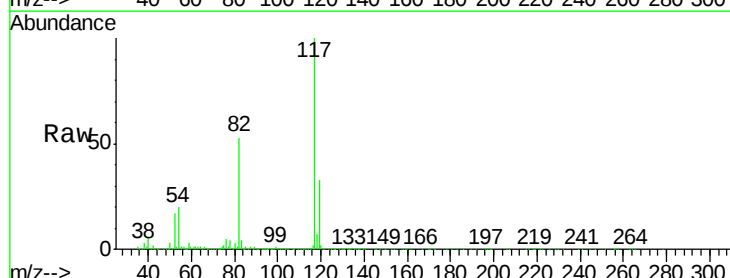


Abundance Ion 116.90 (116.60 to 117.60): VX015082.D (-1506) (-)

Ion 82.00 (81.70 to 82.70): VX015082.D (-1506) (-)

Ion 118.90 (118.60 to 119.60): VX015082.D (-1506) (-)

Time-->

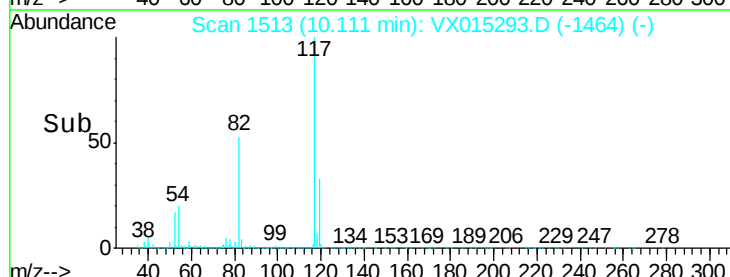


Abundance Ion 116.90 (116.60 to 117.60): VX015293.D (-1464) (-)

Ion 82.00 (81.70 to 82.70): VX015293.D (-1464) (-)

Ion 118.90 (118.60 to 119.60): VX015293.D (-1464) (-)

Time-->

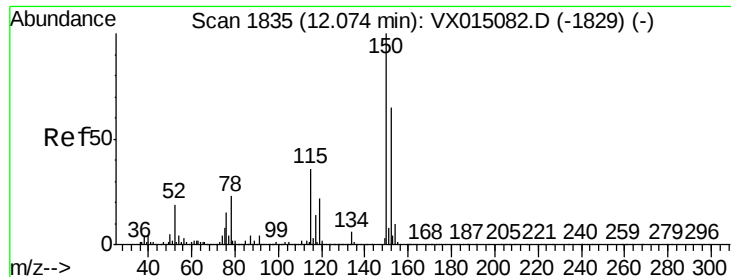

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.07 min Scan# 1835

Delta R.T. -0.00 min

Lab File: VX015293.D

Acq: 16 Mar 2020 14:50

Instrument :

MSVOA_X

ClientSampleId :

TT101D2-20200310DL

Tot Ion:152 Resp: 249224

Ion Ratio Lower Upper

152 100

115 56.4 38.2 114.6

150 157.7 0.0 343.8

