

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031621\
 Data File : VX021249.D
 Acq On : 16 Mar 2021 17:12
 Operator : JC/MD
 Sample : M1648-07DL 4X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMP1-41727:28DL

Quant Time: Mar 17 02:40:58 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
 Quant Title : SW846 8260
 QLast Update : Tue Mar 16 14:00:21 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.623	168	74629	50.00	ug/l	-0.01
34) 1,4-Difluorobenzene	6.829	114	119782	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.094	117	98574	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.059	152	41969	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.029	65	55002	44.93	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	89.86%		
35) Dibromofluoromethane	5.464	113	39855	48.90	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	97.80%		
50) Toluene-d8	8.694	98	144965	49.02	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	98.04%		
62) 4-Bromofluorobenzene	11.118	95	50912	44.33	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	88.66%		
Target Compounds						Qvalue
3) Chloromethane	1.316	50	2558	Below Cal		100
5) Bromomethane	1.628	94	189	0.48	ug/l	89
10) Methyl Iodide	2.499	142	340	0.50	ug/l #	86
11) Tert butyl alcohol	3.017	59	803	3.90	ug/l #	86
13) Acrolein	2.275	56	245	5.09	ug/l #	28
15) Acrylonitrile	3.123	53	107	0.22	ug/l #	55
16) Acetone	2.422	43	16521	36.68	ug/l	92
17) Carbon Disulfide	2.552	76	854	0.92	ug/l #	75
18) Methyl Acetate	2.752	43	971	0.79	ug/l #	87
20) Methylene Chloride	2.834	84	464	0.50	ug/l #	88
25) 2-Butanone	4.635	43	8524	12.31	ug/l #	89
31) Cyclohexane	5.541	56	687	0.46	ug/l #	74
36) 1,1-Dichloropropene	5.629	75	6832	5.66	ug/l #	48
37) Ethyl Acetate	4.635	43	8524	6.09	ug/l #	64
38) Carbon Tetrachloride	5.629	117	8251	6.58	ug/l #	17
40) Benzene	6.117	78	1014	0.30	ug/l #	79
49) 1,4-Dioxane	7.723	88	175	Below Cal	#	1
51) 4-Methyl-2-Pentanone	8.617	43	586	0.44	ug/l #	73
52) Toluene	8.765	92	92937	45.19	ug/l	96
59) 2-Hexanone	9.476	43	568	0.57	ug/l #	53
67) Ethyl Benzene	10.235	91	1158	0.31	ug/l	93
68) m/p-Xylenes	10.341	106	1911	1.43	ug/l	86
69) o-Xylene	10.682	106	845	0.65	ug/l	96
76) 1,2,3-Trichloropropane	11.118	75	28187	28.95	ug/l #	38
78) n-propylbenzene	11.341	91	1162	0.32	ug/l	95
79) 2-Chlorotoluene	11.418	91	570	0.26	ug/l #	48
80) 1,3,5-Trimethylbenzene	11.488	105	1045	0.40	ug/l	99
81) trans-1,4-Dichloro-2-b...	11.118	75	28187	78.61	ug/l #	12
84) 1,2,4-Trimethylbenzene	11.788	105	3878	1.45	ug/l	95
89) n-Butylbenzene	12.371	91	768	0.31	ug/l	87
93) 1,2,4-Trichlorobenzene	13.624	180	215	0.25	ug/l #	90
94) Hexachlorobutadiene	13.765	225	157	0.43	ug/l	86
95) Naphthalene	13.818	128	3481	1.17	ug/l	97
96) 1,2,3-Trichlorobenzene	14.000	180	237	0.28	ug/l #	78

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031621\
Data File : VX021249.D
Acq On : 16 Mar 2021 17:12
Operator : JC/MD
Sample : M1648-07DL 4X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1


Instrument :
MSVOA_X
ClientSampleId :
COMP1-41727:28DL


Quant Time: Mar 17 02:40:58 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
Quant Title : SW846 8260
QLast Update : Tue Mar 16 14:00:21 2021
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

(#)=qualifier out of range (m)=manual integration (+)=signals summed						

Quant Time: Mar 17 02:40:58 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
Quant Title : SW846 8260
QLast Update : Tue Mar 16 14:00:21 2021
Response via : Initial Calibration




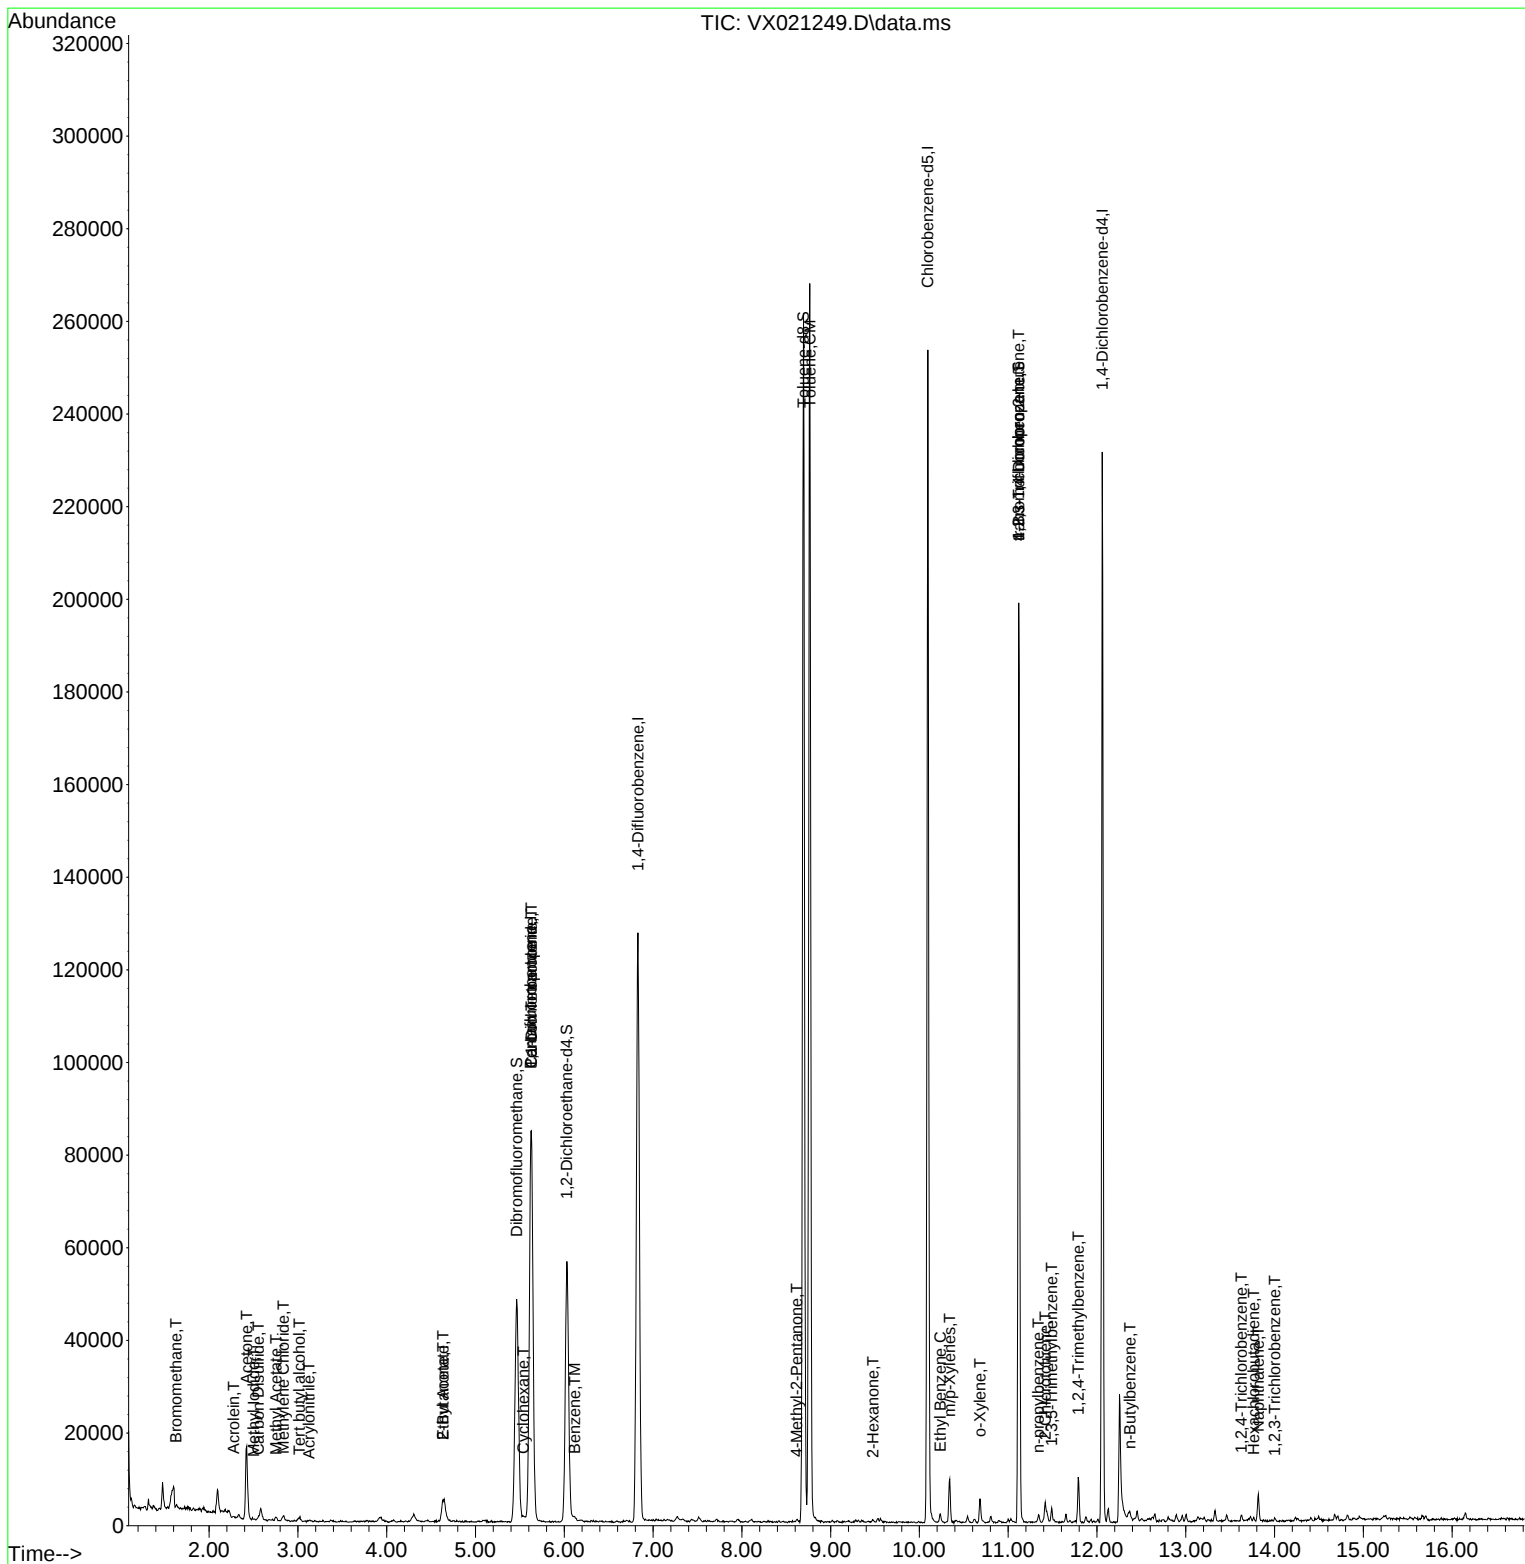




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.623 min Scan# 771
Delta R.T. -0.012 min
Lab File: VX021249.D
Acq: 16 Mar 2021 17:12




Instrument :
MSVOA_X
ClientSampleId :
COMP1-41727:28DL


Tgt Ion:168 Resp: 74629
Ion Ratio Lower Upper
168 100
99 64.8 45.8 68.6

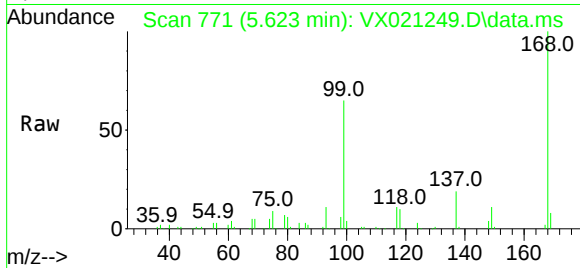

#5
Bromomethane
Concen: 0.48 ug/l
RT: 1.628 min Scan# 92
Delta R.T. 0.005 min
Lab File: VX021249.D
Acq: 16 Mar 2021 17:12


Tgt Ion: 94 Resp: 189
Ion Ratio Lower Upper
94 100
96 85.0 76.4 114.6

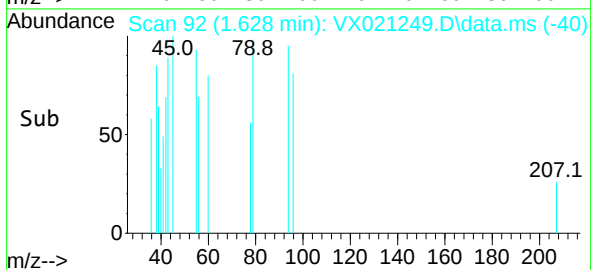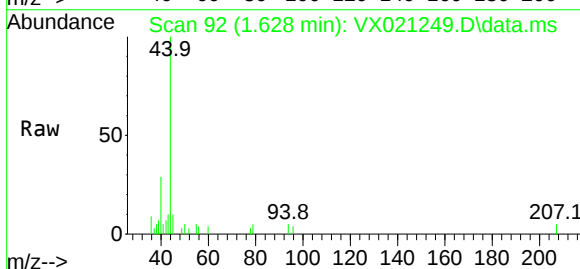






#10
Methyl Iodide
Concen: 0.50 ug/l
RT: 2.499 min Scan# 240
Delta R.T. 0.012 min
Lab File: VX021249.D
Acq: 16 Mar 2021 17:12

Instrument :
MSVOA_X
ClientSampleId :
COMP1-41727:28DL







Tgt Ion:142 Resp: 340
Ion Ratio Lower Upper
142 100
127 37.6 33.3 49.9
141 0.0 11.4 17.0#



#11
Tert butyl alcohol
Concen: 3.90 ug/l
RT: 3.017 min Scan# 328
Delta R.T. -0.000 min
Lab File: VX021249.D
Acq: 16 Mar 2021 17:12


Tgt Ion: 59 Resp: 803
Ion Ratio Lower Upper
59 100
57 4.6 7.8 11.8#

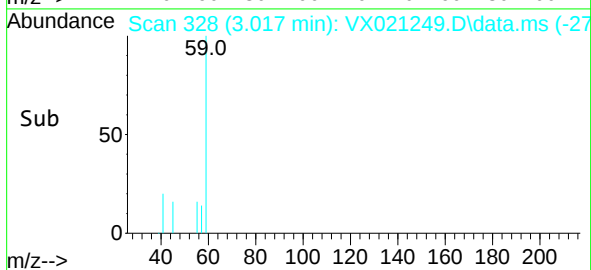



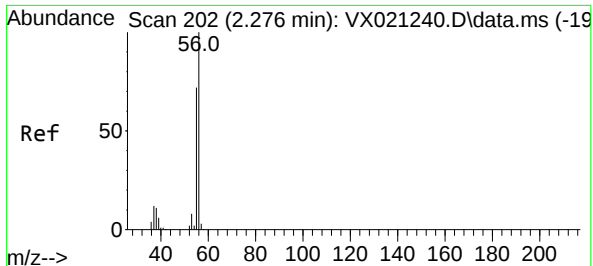


#13
Acrolein
Concen: 5.09 ug/l
RT: 2.275 min Scan# 202
Delta R.T. -0.001 min
Lab File: VX021249.D
Acq: 16 Mar 2021 17:12


Instrument :
MSVOA_X
ClientSampleId :
COMP1-41727:28DL

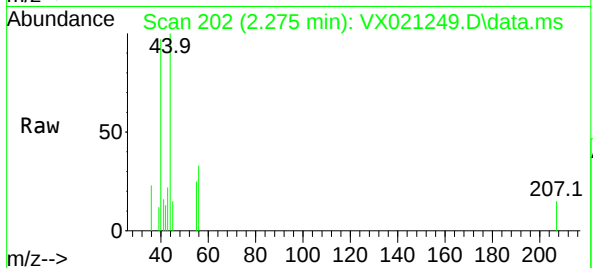



Tgt Ion: 56 Resp: 245
Ion Ratio Lower Upper
56 100
55 130.2 56.4 84.6#

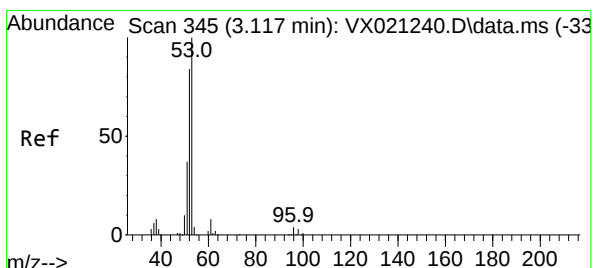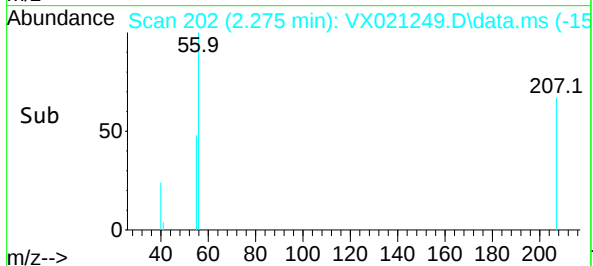


#15
Acrylonitrile
Concen: 0.22 ug/l
RT: 3.123 min Scan# 346
Delta R.T. 0.006 min
Lab File: VX021249.D
Acq: 16 Mar 2021 17:12

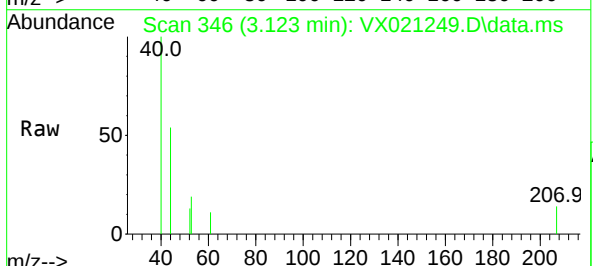

Tgt Ion: 53 Resp: 107
Ion Ratio Lower Upper
53 100
52 115.9 65.3 97.9#
51 0.0 28.2 42.2#




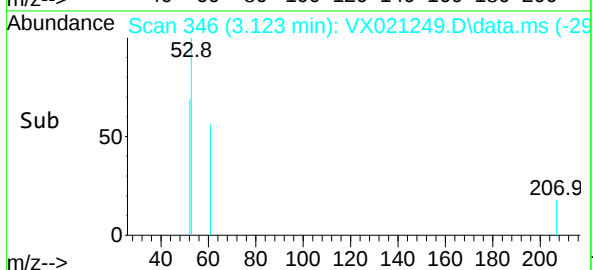




#16
Acetone
Concen: 36.68 ug/l
RT: 2.422 min Scan# 227
Delta R.T. -0.001 min
Lab File: VX021249.D
Acq: 16 Mar 2021 17:12




Instrument :
MSVOA_X
ClientSampleId :
COMP1-41727:28DL


Tgt Ion: 43 Resp: 16521
Ion Ratio Lower Upper
43 100
58 30.2 27.8 41.8



#17
Carbon Disulfide
Concen: 0.92 ug/l
RT: 2.552 min Scan# 249
Delta R.T. -0.000 min
Lab File: VX021249.D
Acq: 16 Mar 2021 17:12

Tgt Ion: 76 Resp: 854
Ion Ratio Lower Upper
76 100
78 0.0 7.2 10.8#


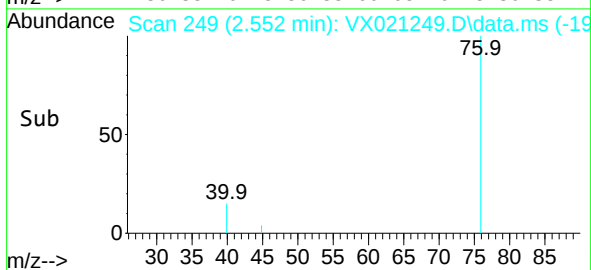






#18
Methyl Acetate
Concen: 0.79 ug/l
RT: 2.752 min Scan# 283
Delta R.T. -0.000 min
Lab File: VX021249.D
Acq: 16 Mar 2021 17:12




Instrument :
MSVOA_X
ClientSampleId :
COMP1-41727:28DL


Tgt Ion: 43 Resp: 971
Ion Ratio Lower Upper
43 100
74 20.4 21.9 32.9#



#20
Methylene Chloride
Concen: 0.50 ug/l
RT: 2.834 min Scan# 297
Delta R.T. -0.001 min
Lab File: VX021249.D
Acq: 16 Mar 2021 17:12

Tgt Ion: 84 Resp: 464
Ion Ratio Lower Upper
84 100
49 98.9 88.6 132.8
51 50.6 27.0 40.6#
86 65.7 50.3 75.5



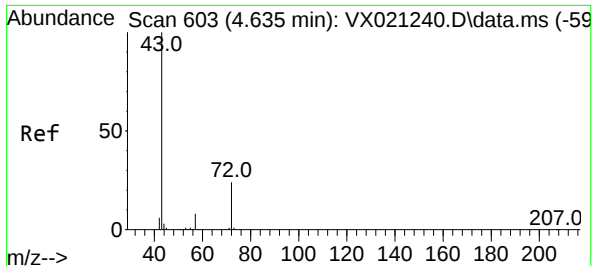

#25

2-Butanone

Concen: 12.31 ug/l

RT: 4.635 min Scan# 603

Delta R.T. -0.000 min

Lab File: VX021249.D

Acq: 16 Mar 2021 17:12

Instrument :

MSVOA_X

ClientSampleId :





COMP1-41727:28DL

Tgt Ion: 43 Resp: 8524

Ion Ratio Lower Upper

43 100

72 23.7 23.7 35.5#

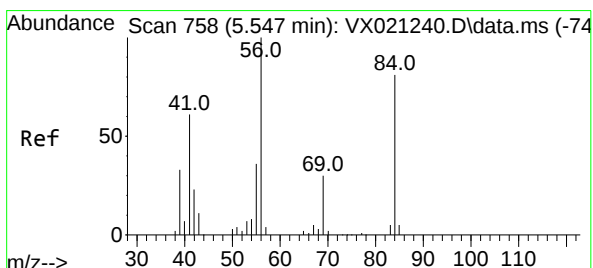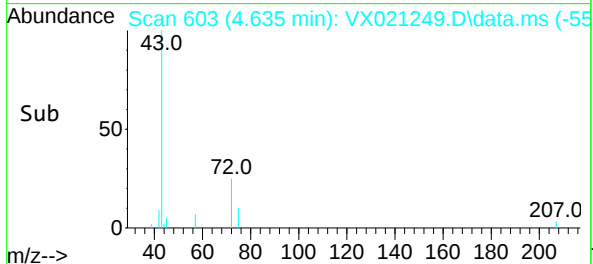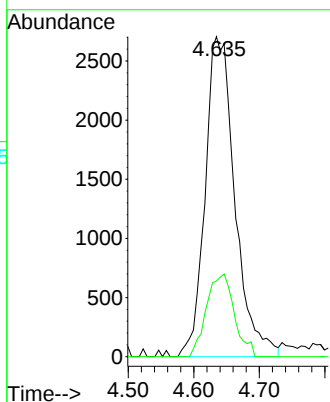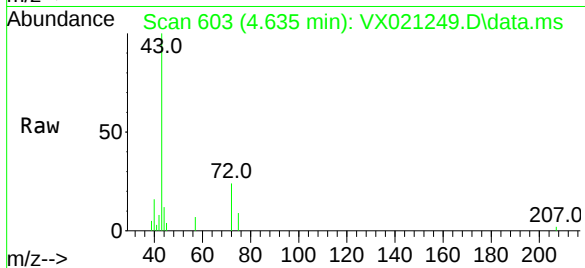

#31

Cyclohexane

Concen: 0.46 ug/l

RT: 5.541 min Scan# 757

Delta R.T. -0.006 min

Lab File: VX021249.D

Acq: 16 Mar 2021 17:12




Tgt Ion: 56 Resp: 687


Ion Ratio Lower Upper

56 100

69 0.0 25.3 37.9#

84 74.8 71.4 107.0


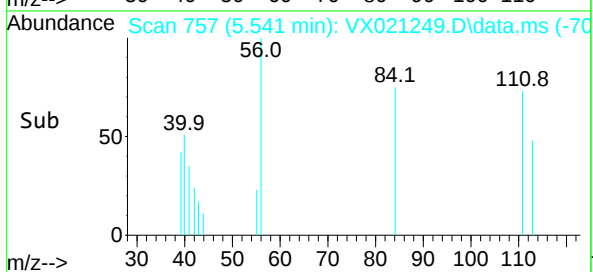
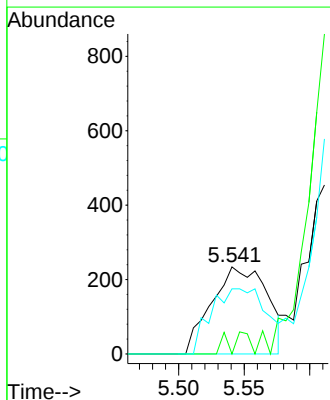
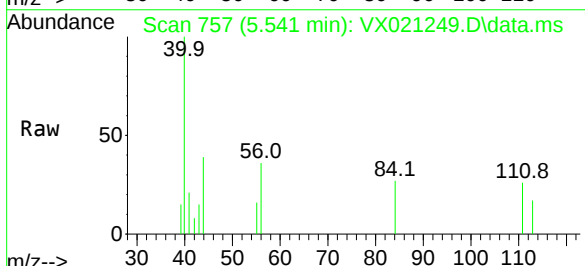




#33
 1,2-Dichloroethane-d4
 Concen: 44.93 ug/l
 RT: 6.029 min Scan# 840
 Delta R.T. -0.000 min
 Lab File: VX021249.D
 Acq: 16 Mar 2021 17:12




Instrument :
 MSVOA_X
 ClientSampleId :
 COMP1-41727:28DL


Tgt Ion: 65 Resp: 55002
 Ion Ratio Lower Upper
 65 100
 67 50.1 0.0 105.4

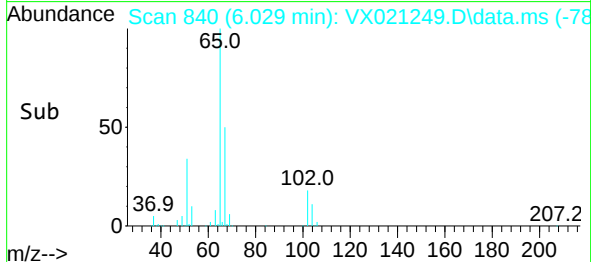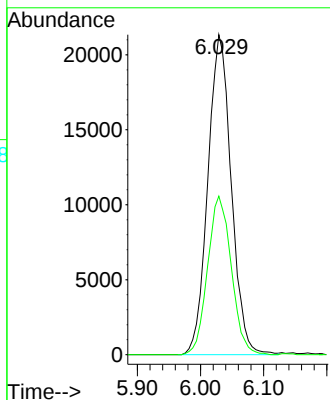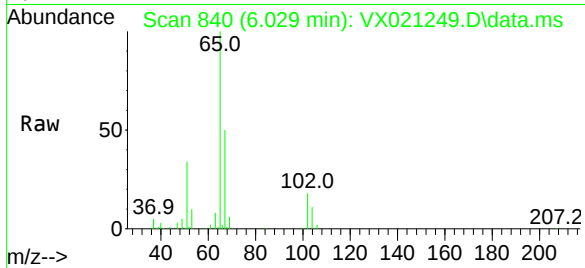

#34
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 6.829 min Scan# 976
 Delta R.T. -0.000 min
 Lab File: VX021249.D
 Acq: 16 Mar 2021 17:12

Tgt Ion: 114 Resp: 119782
 Ion Ratio Lower Upper
 114 100
 63 23.6 0.0 40.8
 88 17.0 0.0 32.8



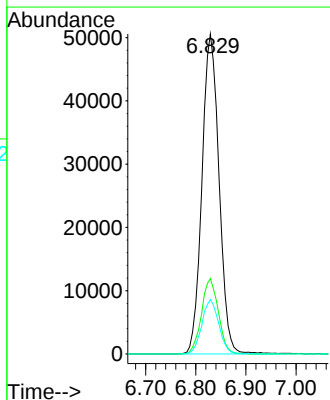
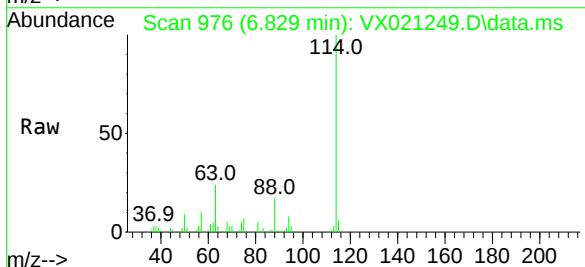




#35
Dibromofluoromethane
Concen: 48.90 ug/l
RT: 5.464 min Scan# 744
Delta R.T. 0.000 min
Lab File: VX021249.D
Acq: 16 Mar 2021 17:12




Instrument :
MSVOA_X
ClientSampleId :
COMP1-41727:28DL


Tgt Ion:113 Resp: 39855
Ion Ratio Lower Upper
113 100
111 103.7 81.9 122.9
192 18.3 16.7 25.1

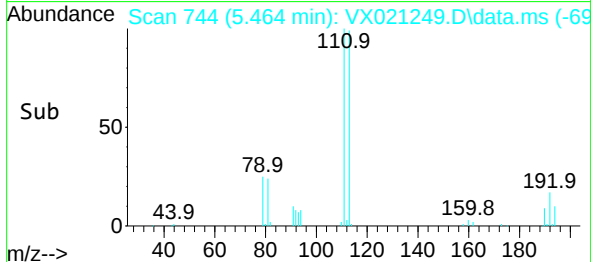

#36
1,1-Dichloropropene
Concen: 5.66 ug/l
RT: 5.629 min Scan# 772
Delta R.T. -0.141 min
Lab File: VX021249.D
Acq: 16 Mar 2021 17:12

Tgt Ion: 75 Resp: 6832
Ion Ratio Lower Upper
75 100
110 8.4 18.1 54.4#
77 0.0 25.3 37.9#


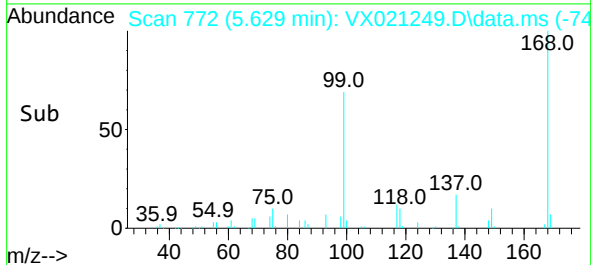






#37
Ethyl Acetate
Concen: 6.09 ug/l
RT: 4.635 min Scan# 603
Delta R.T. -0.159 min
Lab File: VX021249.D
Acq: 16 Mar 2021 17:12




Instrument :
MSVOA_X
ClientSampleId :
COMP1-41727:28DL


Tgt Ion: 43 Resp: 8524
Ion Ratio Lower Upper
43 100
61 0.0 12.8 19.2#
70 0.0 10.5 15.7#

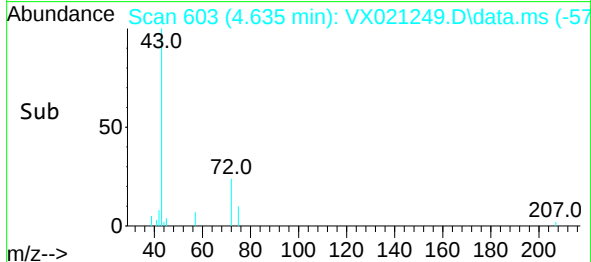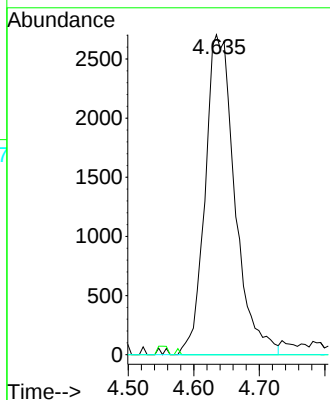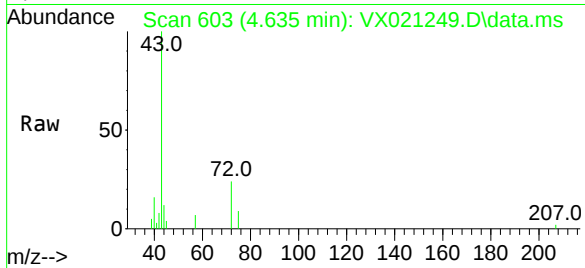

#38
Carbon Tetrachloride
Concen: 6.58 ug/l
RT: 5.629 min Scan# 772
Delta R.T. -0.129 min
Lab File: VX021249.D
Acq: 16 Mar 2021 17:12

Tgt Ion: 117 Resp: 8251
Ion Ratio Lower Upper
117 100
119 6.1 76.2 114.2#
121 0.0 24.8 37.2#



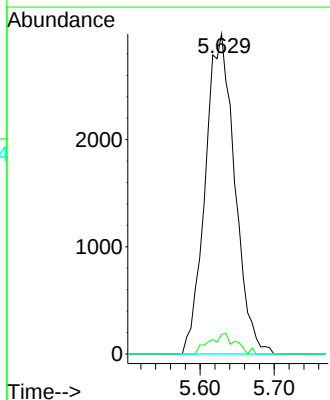
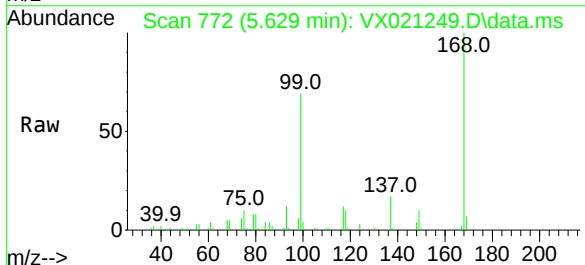




#40
Benzene
Concen: 0.30 ug/l
RT: 6.117 min Scan# 855
Delta R.T. 0.006 min
Lab File: VX021249.D
Acq: 16 Mar 2021 17:12




Instrument :
MSVOA_X
ClientSampleId :
COMP1-41727:28DL


Tgt Ion: 78 Resp: 1014
Ion Ratio Lower Upper
78 100
77 33.8 18.9 28.3#



#49
1,4-Dioxane
Concen: Below Cal
RT: 7.723 min Scan# 1128
Delta R.T. 0.011 min
Lab File: VX021249.D
Acq: 16 Mar 2021 17:12

Tgt Ion: 88 Resp: 175
Ion Ratio Lower Upper
88 100
43 242.9 23.2 34.8#
58 90.9 55.0 82.4#


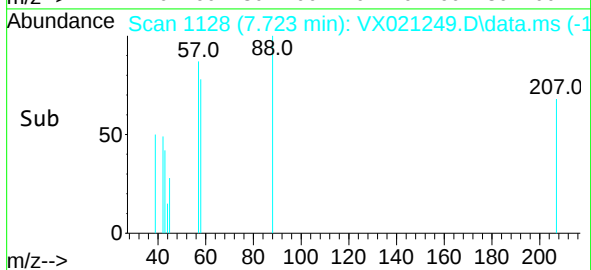






#50
Toluene-d8
Concen: 49.02 ug/l
RT: 8.694 min Scan# 1293
Delta R.T. -0.000 min
Lab File: VX021249.D
Acq: 16 Mar 2021 17:12




Instrument :
MSVOA_X
ClientSampleId :
COMP1-41727:28DL


Tgt Ion: 98 Resp: 144965
Ion Ratio Lower Upper
98 100
100 64.0 51.9 77.9



#51
4-Methyl-2-Pentanone
Concen: 0.44 ug/l
RT: 8.617 min Scan# 1280
Delta R.T. -0.001 min
Lab File: VX021249.D
Acq: 16 Mar 2021 17:12

Tgt Ion: 43 Resp: 586
Ion Ratio Lower Upper
43 100
58 26.5 35.4 53.0#


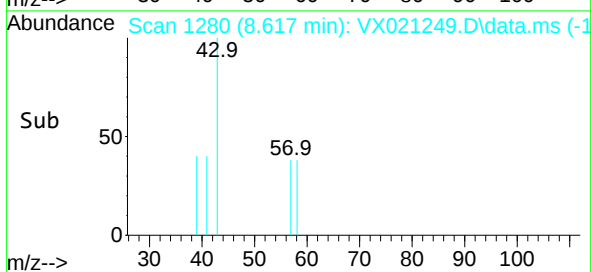

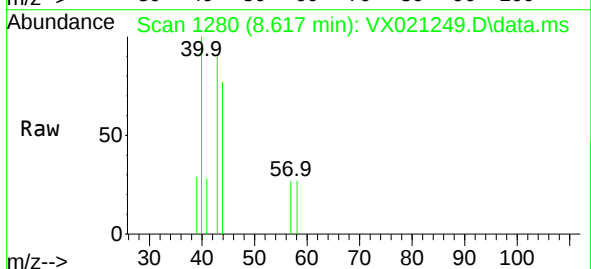




#52
Toluene
Concen: 45.19 ug/l
RT: 8.765 min Scan# 1305
Delta R.T. -0.000 min
Lab File: VX021249.D
Acq: 16 Mar 2021 17:12




Instrument :
MSVOA_X
ClientSampleId :
COMP1-41727:28DL


Tgt Ion: 92 Resp: 92937
Ion Ratio Lower Upper
92 100
91 177.0 137.1 205.7

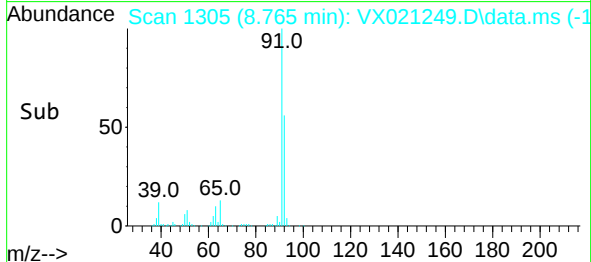

#59
2-Hexanone
Concen: 0.57 ug/l
RT: 9.476 min Scan# 1426
Delta R.T. 0.005 min
Lab File: VX021249.D
Acq: 16 Mar 2021 17:12

Tgt Ion: 43 Resp: 568
Ion Ratio Lower Upper
43 100
58 25.9 30.9 92.8#




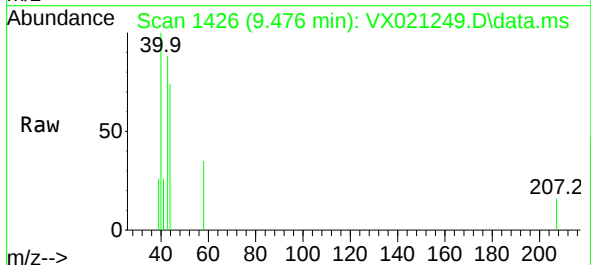




#62
4-Bromofluorobenzene
Concen: 44.33 ug/l
RT: 11.118 min Scan# 1705
Delta R.T. -0.000 min
Lab File: VX021249.D
Acq: 16 Mar 2021 17:12




Instrument :
MSVOA_X
ClientSampleId :
COMP1-41727:28DL


Tgt Ion: 95 Resp: 50912
Ion Ratio Lower Upper
95 100
174 71.6 0.0 154.6
176 67.6 0.0 155.8



#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.094 min Scan# 1531
Delta R.T. 0.000 min
Lab File: VX021249.D
Acq: 16 Mar 2021 17:12

Tgt Ion: 117 Resp: 98574
Ion Ratio Lower Upper
117 100
82 59.9 47.4 71.2
119 32.3 26.6 39.8


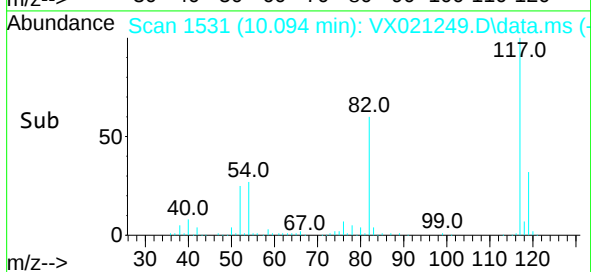






#67
Ethyl Benzene
Concen: 0.31 ug/l
RT: 10.235 min Scan# 1555
Delta R.T. -0.001 min
Lab File: VX021249.D
Acq: 16 Mar 2021 17:12




Instrument :
MSVOA_X
ClientSampleId :
COMP1-41727:28DL


Tgt Ion: 91 Resp: 1158
Ion Ratio Lower Upper
91 100
106 27.1 24.6 37.0

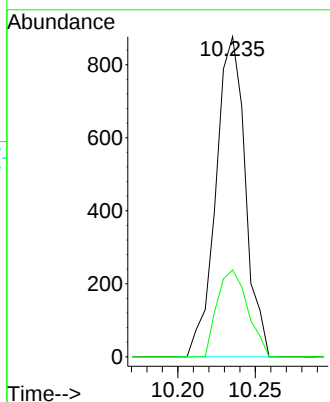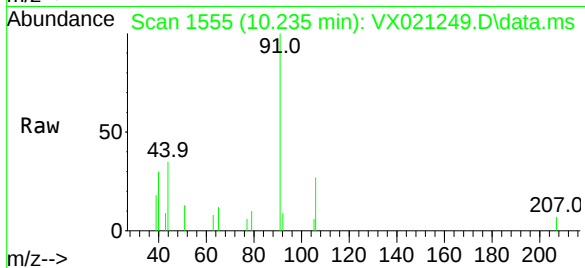

#68
m/p-Xylenes
Concen: 1.43 ug/l
RT: 10.341 min Scan# 1573
Delta R.T. 0.000 min
Lab File: VX021249.D
Acq: 16 Mar 2021 17:12

Tgt Ion: 106 Resp: 1911
Ion Ratio Lower Upper
106 100
91 224.6 162.8 244.2



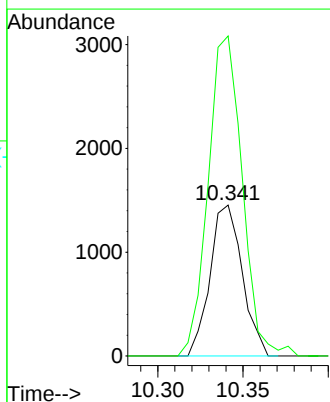
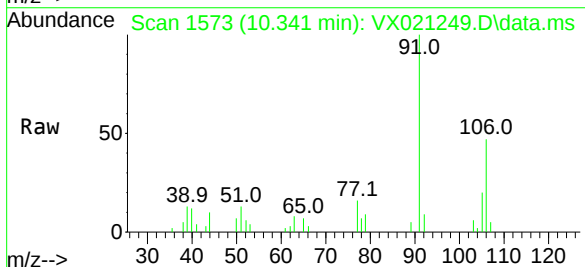




#69
o-Xylene
Concen: 0.65 ug/l
RT: 10.682 min Scan# 1631
Delta R.T. -0.001 min
Lab File: VX021249.D
Acq: 16 Mar 2021 17:12




Instrument :
MSVOA_X
ClientSampleId :
COMP1-41727:28DL


Tgt Ion:106 Resp: 845
Ion Ratio Lower Upper
106 100
91 223.1 108.1 324.2

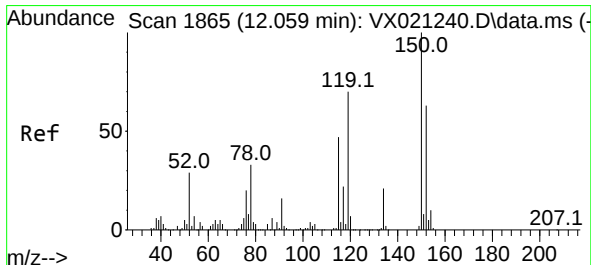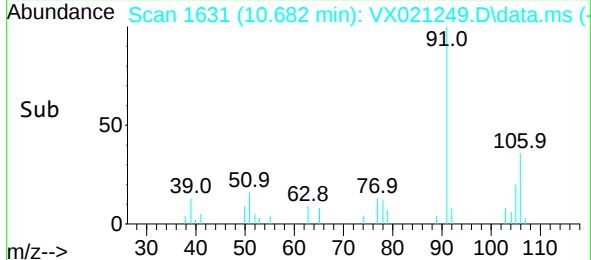

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.059 min Scan# 1865
Delta R.T. 0.000 min
Lab File: VX021249.D
Acq: 16 Mar 2021 17:12

Tgt Ion:152 Resp: 41969
Ion Ratio Lower Upper
152 100
115 61.0 41.1 123.3
150 158.7 0.0 349.0




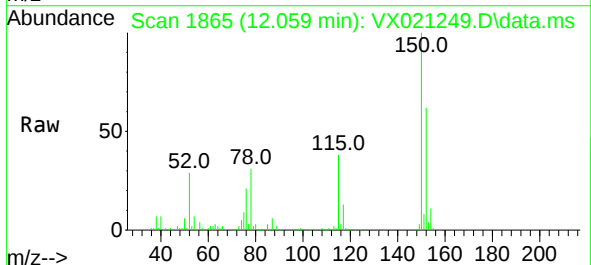


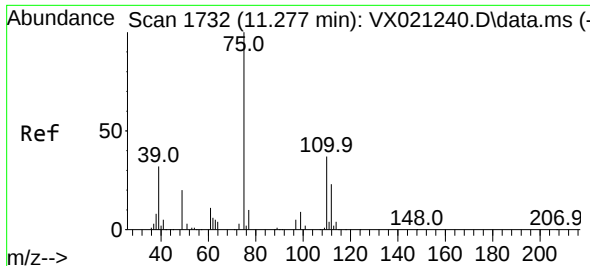

#76
1,2,3-Trichloropropane
Concen: 28.95 ug/l
RT: 11.118 min Scan# 1705
Delta R.T. -0.159 min
Lab File: VX021249.D
Acq: 16 Mar 2021 17:12




Instrument :
MSVOA_X
ClientSampleId :
COMP1-41727:28DL


Tgt Ion: 75 Resp: 28187
Ion Ratio Lower Upper
75 100
77 1.1 19.1 57.5#

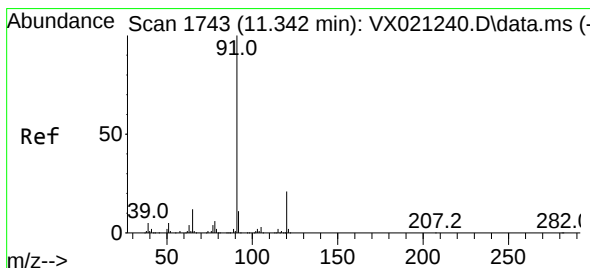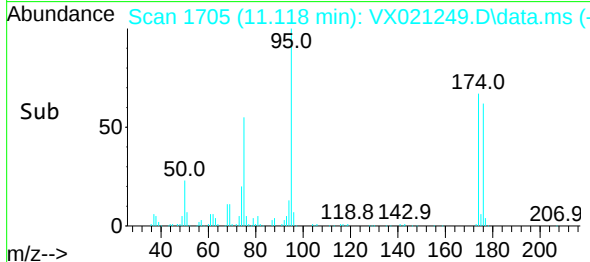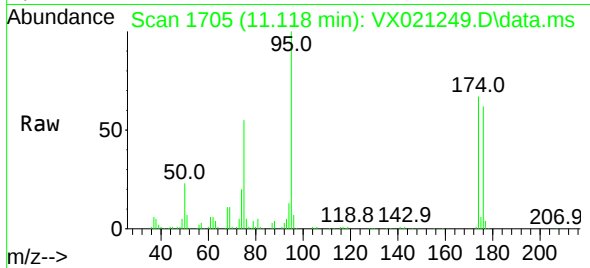

#78
n-propylbenzene
Concen: 0.32 ug/l
RT: 11.341 min Scan# 1743
Delta R.T. -0.001 min
Lab File: VX021249.D
Acq: 16 Mar 2021 17:12

Tgt Ion: 91 Resp: 1162
Ion Ratio Lower Upper
91 100
120 20.5 11.5 34.5


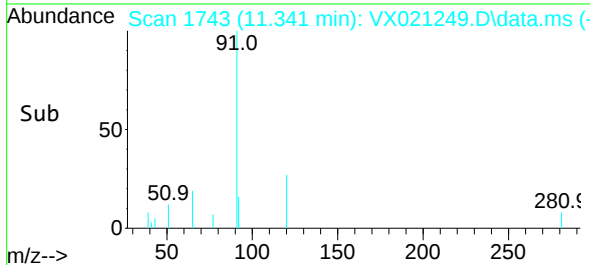

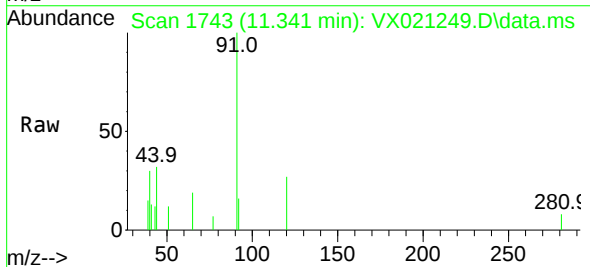


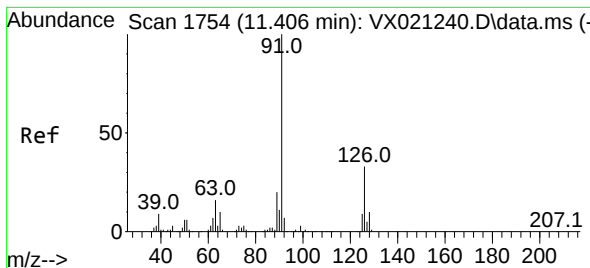

#79
2-Chlorotoluene
Concen: 0.26 ug/l
RT: 11.418 min Scan# 1756
Delta R.T. 0.012 min
Lab File: VX021249.D
Acq: 16 Mar 2021 17:12




Instrument :
MSVOA_X
ClientSampleId :
COMP1-41727:28DL


Tgt Ion: 91 Resp: 570
Ion Ratio Lower Upper
91 100
126 3.9 16.6 49.8#

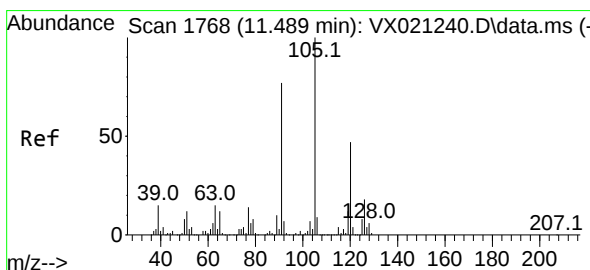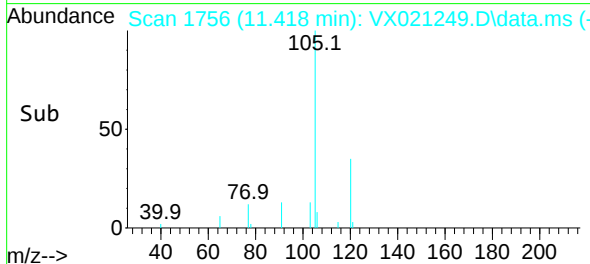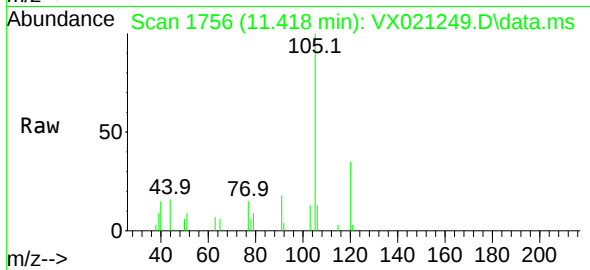

#80
1,3,5-Trimethylbenzene
Concen: 0.40 ug/l
RT: 11.488 min Scan# 1768
Delta R.T. -0.001 min
Lab File: VX021249.D
Acq: 16 Mar 2021 17:12


Tgt Ion: 105 Resp: 1045
Ion Ratio Lower Upper
105 100
120 47.0 23.8 71.5

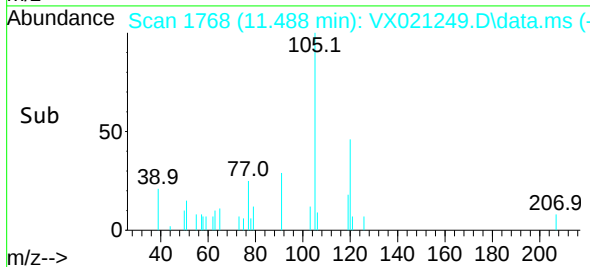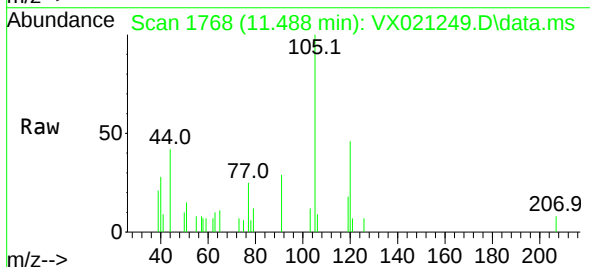



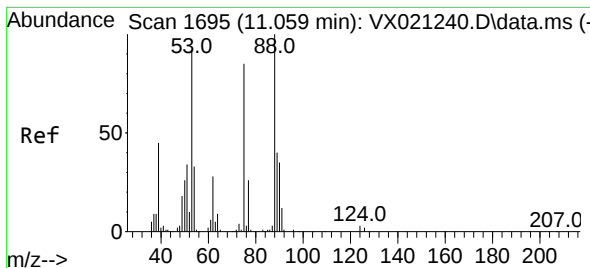


#81
trans-1,4-Dichloro-2-butene
Concen: 78.61 ug/l
RT: 11.118 min Scan# 1705
Delta R.T. 0.059 min
Lab File: VX021249.D
Acq: 16 Mar 2021 17:12


Instrument :
MSVOA_X
ClientSampleId :
COMP1-41727:28DL

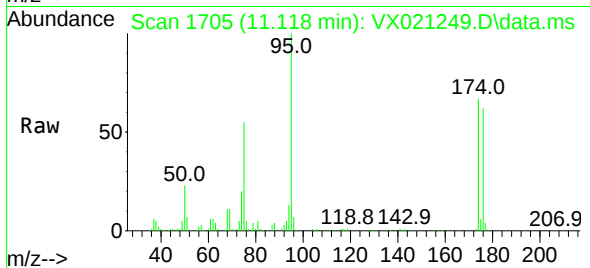



Tgt Ion: 75 Resp: 28187
Ion Ratio Lower Upper
75 100
53 0.0 74.5 111.7#
89 0.0 37.9 56.9#

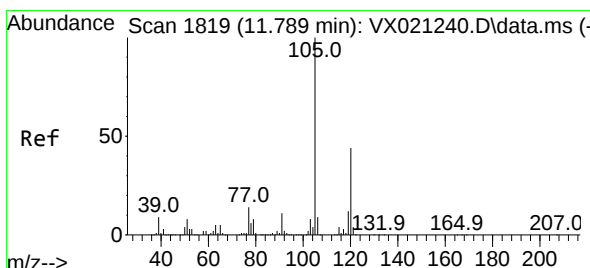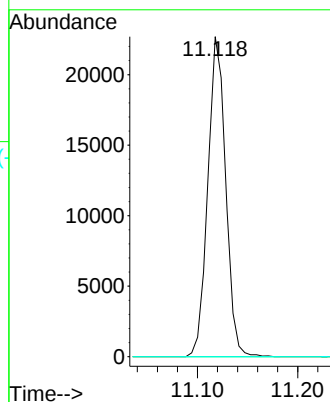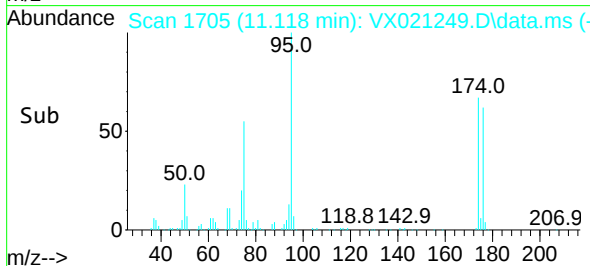


#84
1,2,4-Trimethylbenzene
Concen: 1.45 ug/l
RT: 11.788 min Scan# 1819
Delta R.T. -0.001 min
Lab File: VX021249.D
Acq: 16 Mar 2021 17:12

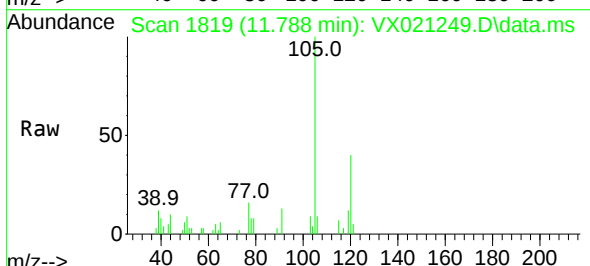

Tgt Ion: 105 Resp: 3878
Ion Ratio Lower Upper
105 100
120 42.0 22.4 67.3



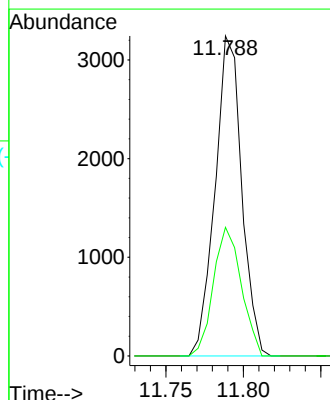
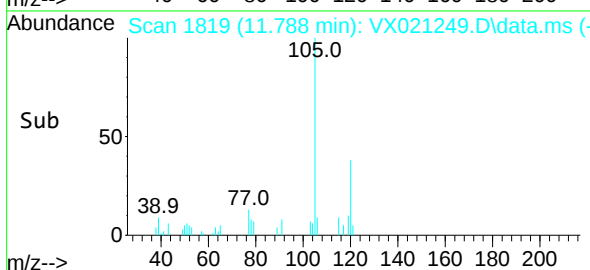




#89
n-Butylbenzene
Concen: 0.31 ug/l
RT: 12.371 min Scan# 1918
Delta R.T. -0.000 min
Lab File: VX021249.D
Acq: 16 Mar 2021 17:12




Instrument :
MSVOA_X
ClientSampleId :
COMP1-41727:28DL


Tgt Ion: 91	Resp:	768	
Ion	Ratio	Lower	Upper
91	100		
92	44.3	27.4	82.0
134	30.7	13.2	39.5

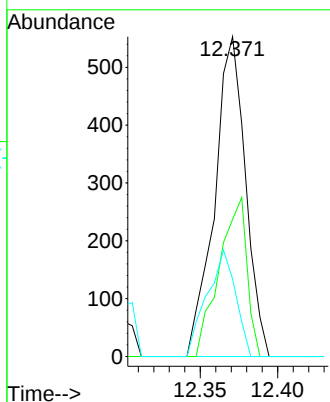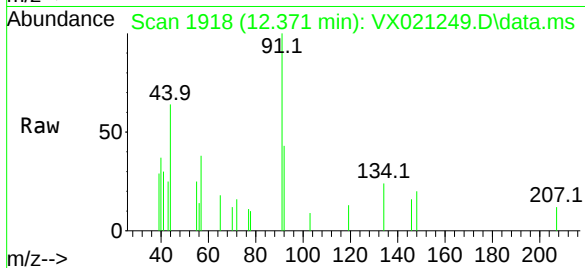

#93
1,2,4-Trichlorobenzene
Concen: 0.25 ug/l
RT: 13.624 min Scan# 2131
Delta R.T. -0.006 min
Lab File: VX021249.D
Acq: 16 Mar 2021 17:12

Tgt Ion:180	Resp:	215	
Ion	Ratio	Lower	Upper
180	100		
182	92.1	47.7	143.1
145	47.9	15.0	45.0#



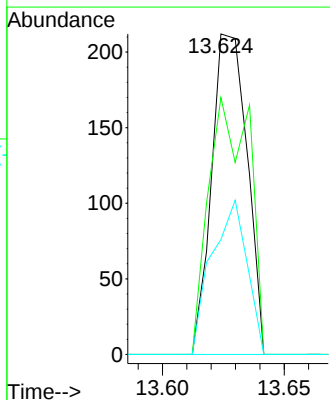
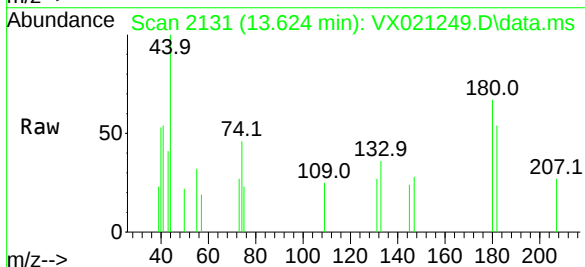




#94
Hexachlorobutadiene
Concen: 0.43 ug/l
RT: 13.765 min Scan# 2155
Delta R.T. 0.000 min
Lab File: VX021249.D
Acq: 16 Mar 2021 17:12




Instrument :
MSVOA_X
ClientSampleId :
COMP1-41727:28DL


Tgt Ion:	225	Resp:	157
Ion	Ratio	Lower	Upper
225	100		
223	61.8	31.1	93.2
227	42.7	31.6	95.0

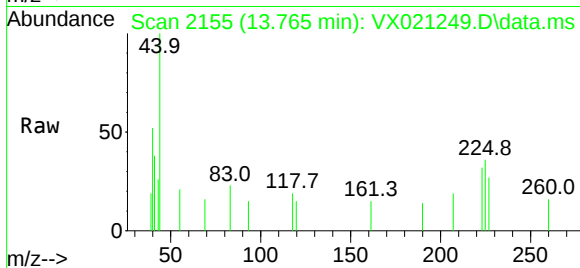

#95
Naphthalene
Concen: 1.17 ug/l
RT: 13.818 min Scan# 2164
Delta R.T. 0.000 min
Lab File: VX021249.D
Acq: 16 Mar 2021 17:12


Tgt Ion:	128	Resp:	3481
Ion	Ratio	Lower	Upper
128	100		
127	11.2	10.3	15.5
129	10.7	8.8	13.2

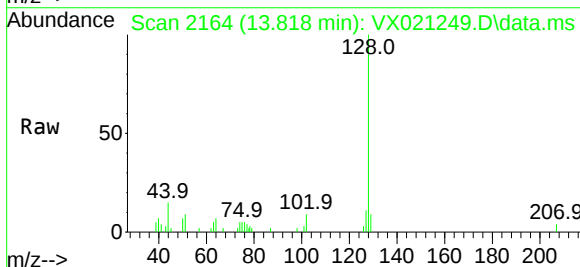

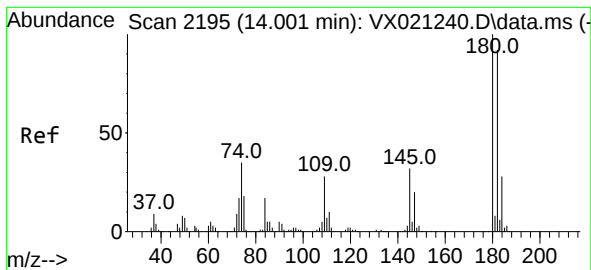

#96
 1,2,3-Trichlorobenzene
 Concen: 0.28 ug/l
 RT: 14.000 min Scan# 2195
 Delta R.T. -0.001 min
 Lab File: VX021249.D
 Acq: 16 Mar 2021 17:12

Instrument :
 MSVOA_X
 ClientSampleId :
 COMP1-41727:28DL

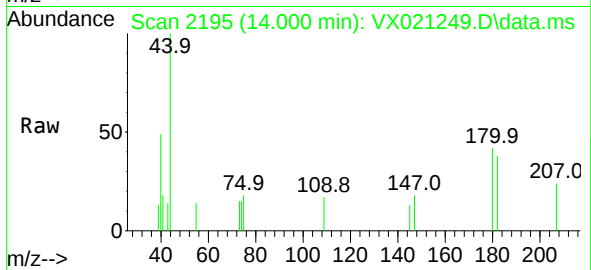

Tgt Ion:180 Resp: 237
 Ion Ratio Lower Upper
 180 100
 182 76.4 47.6 142.9
 145 16.0 16.1 48.3#

