


Chloromethane


Response Ratio

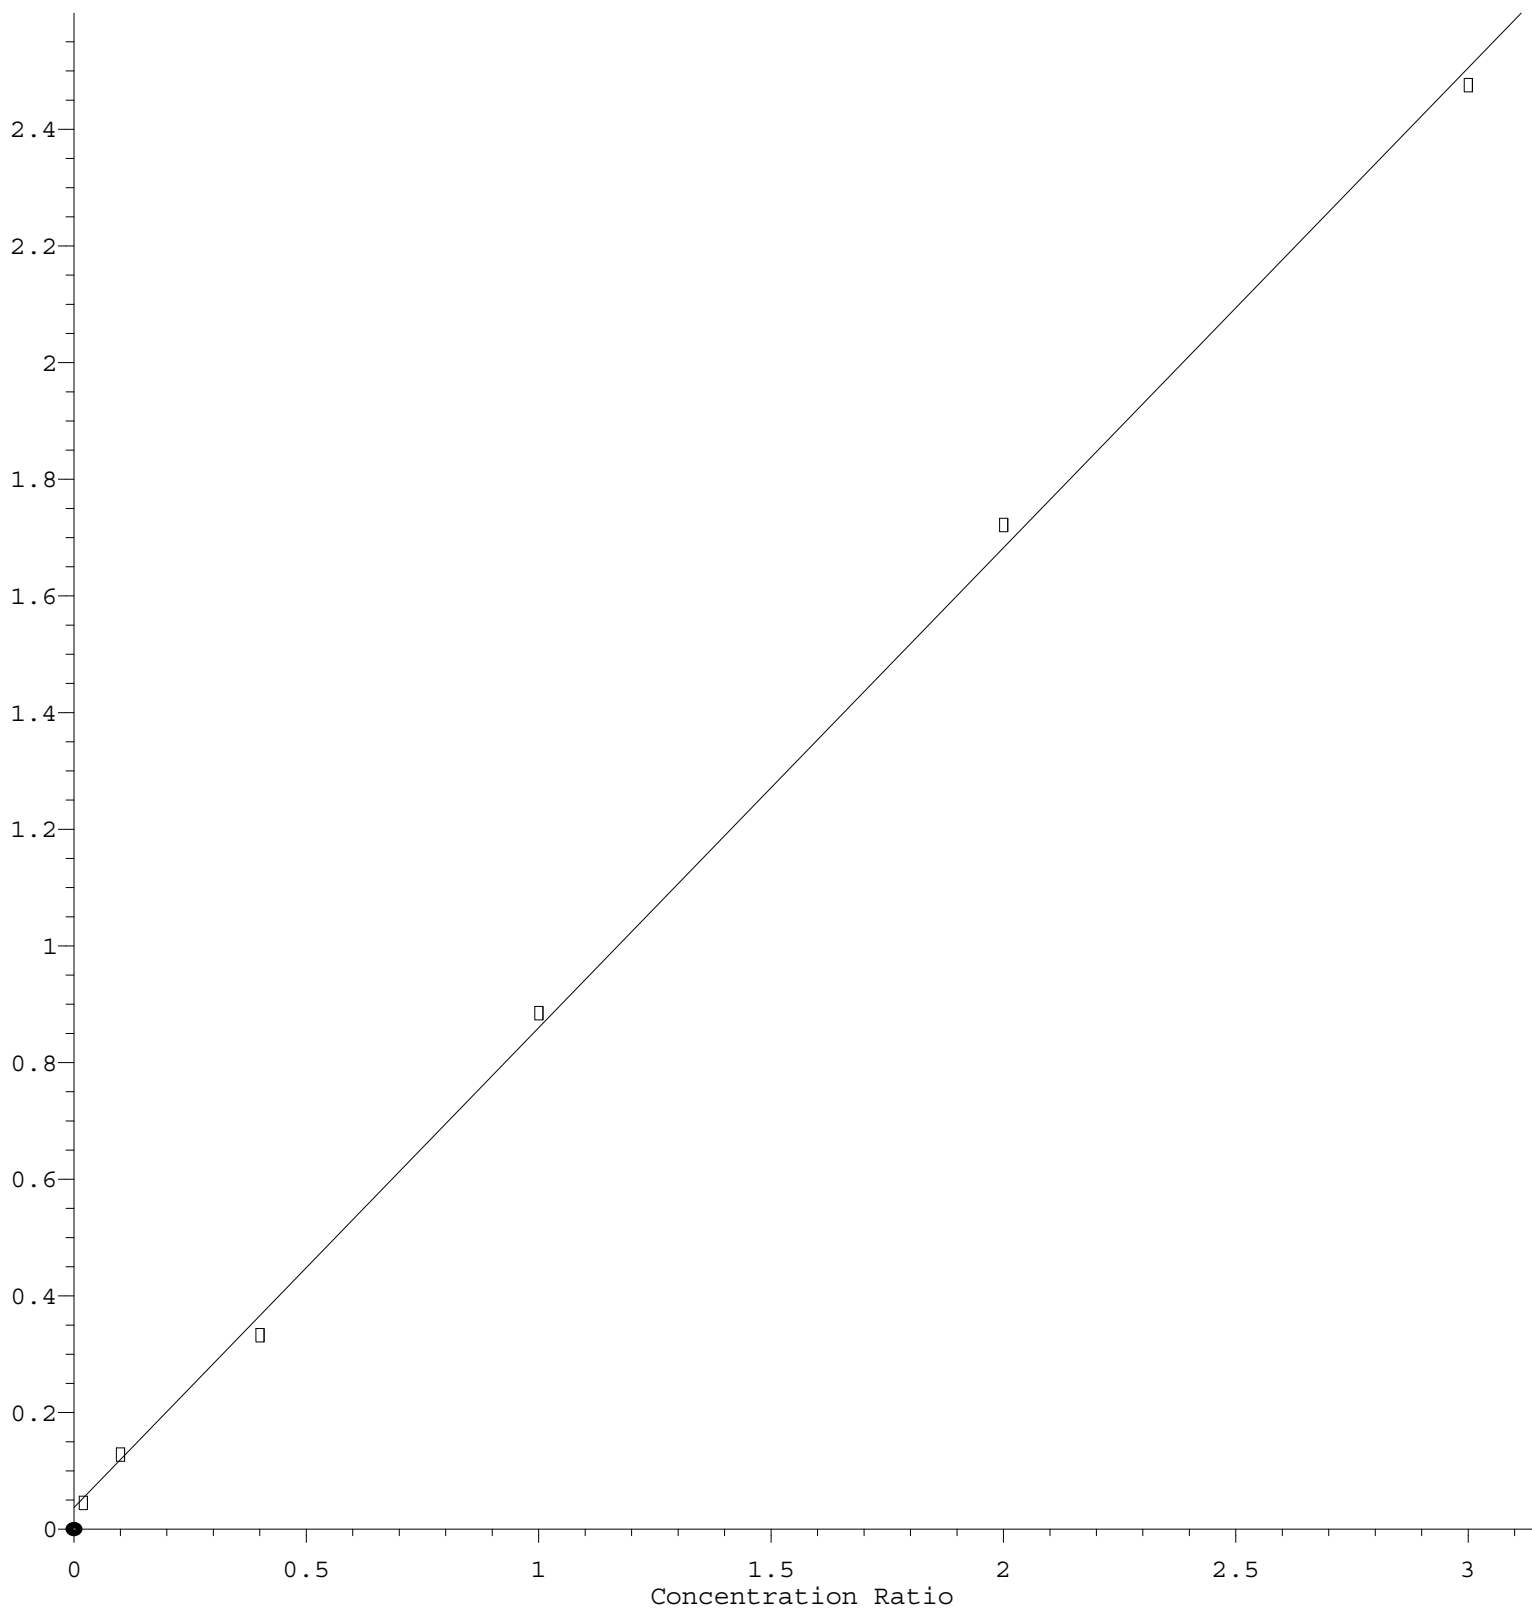

Response = $8.228 \times 10^{-1} \times \text{Amt} + 3.709 \times 10^{-2}$
Coef of Det (r^2) = 0.999105 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X031621W.M
Calibration Table Last Updated: Tue Mar 16 14:00:21 2021

Acrolein

Response Ratio

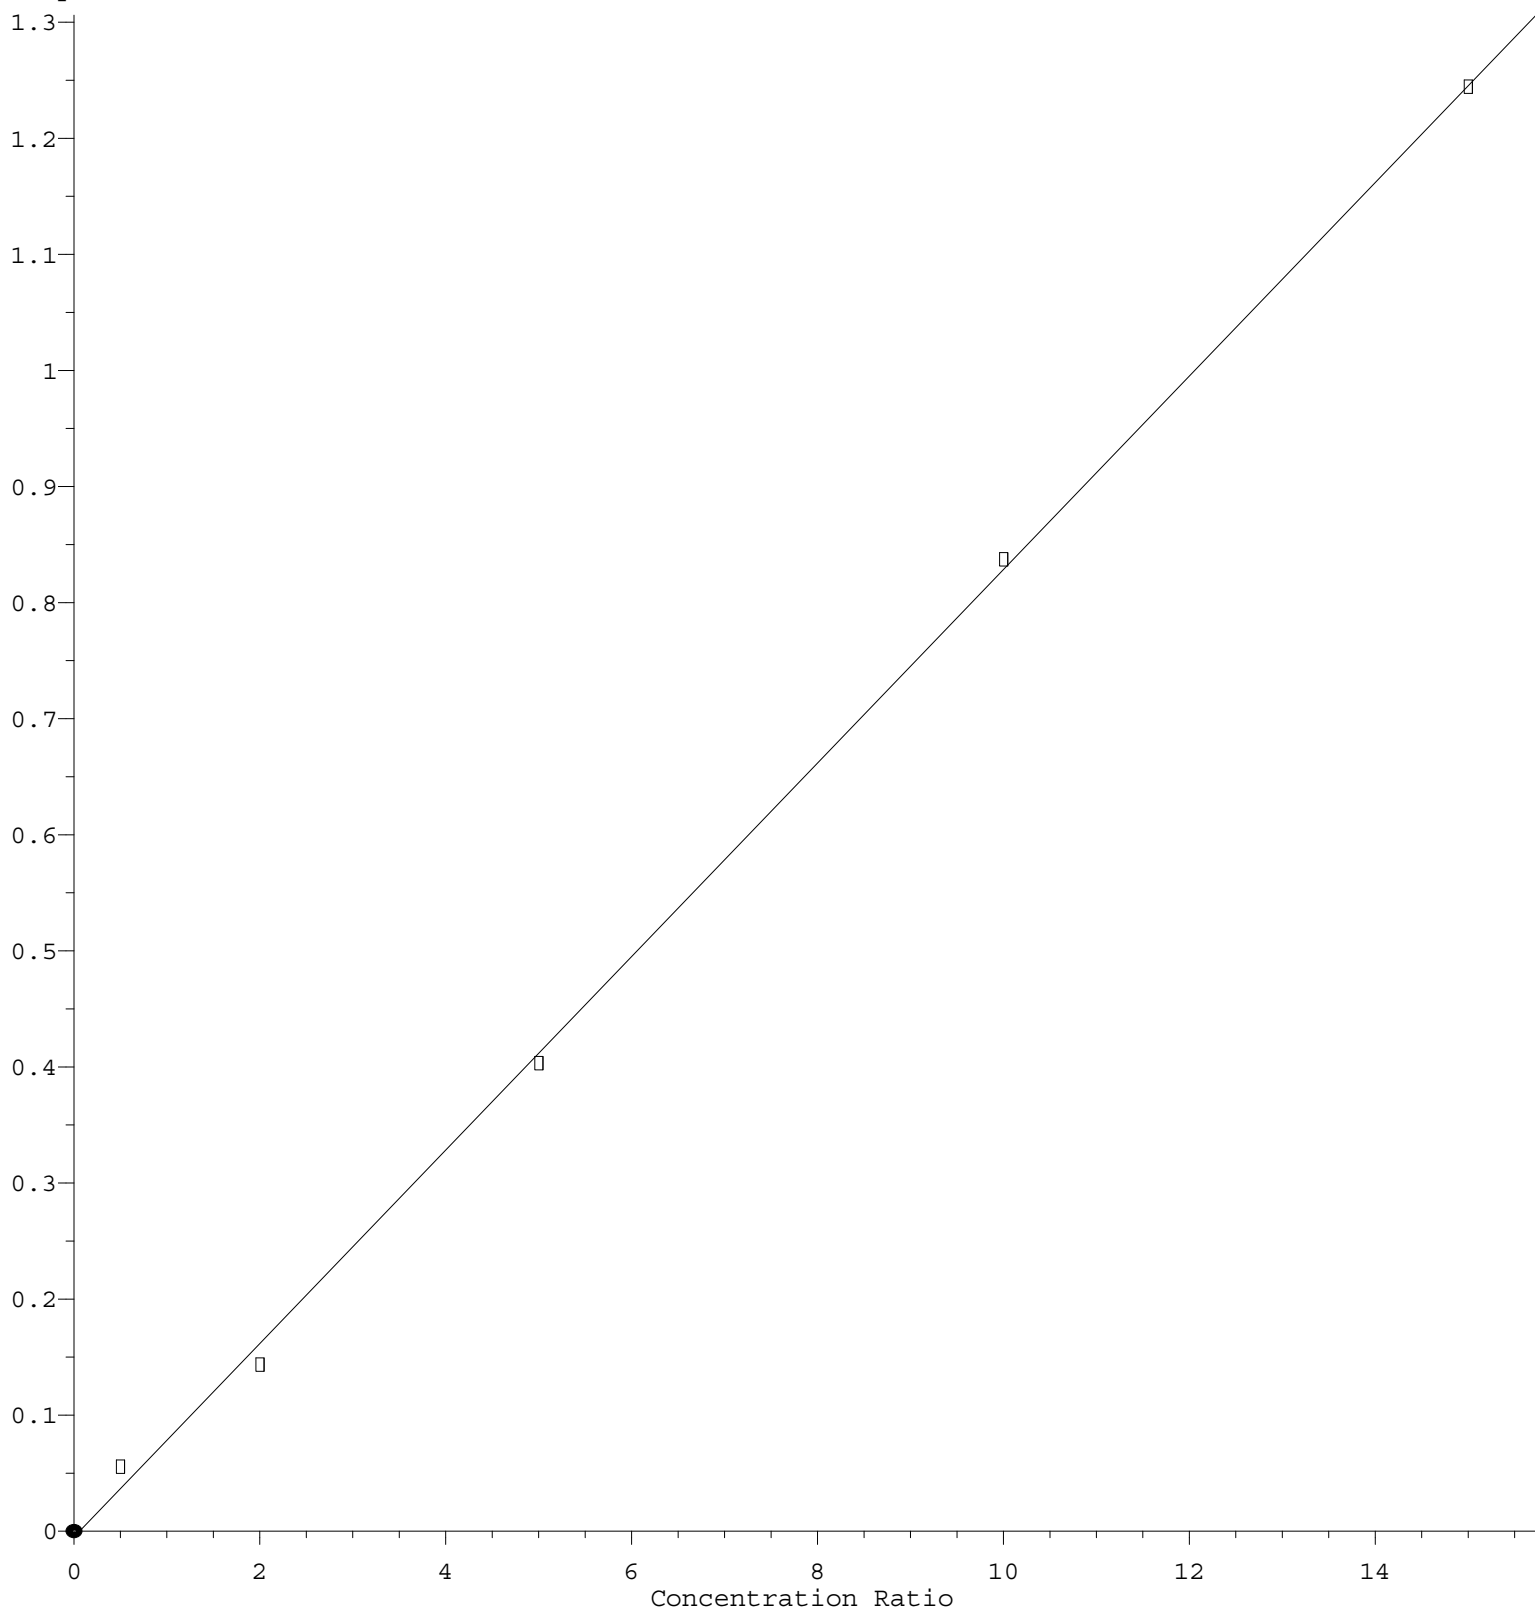

$$\text{Response} = 8.338\text{e-}002 * \text{Amt} - 5.209\text{e-}003$$


Coef of Det (r^2) = 0.999160 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X031621W.M

Calibration Table Last Updated: Tue Mar 16 14:00:21 2021

Carbon Disulfide

Response Ratio

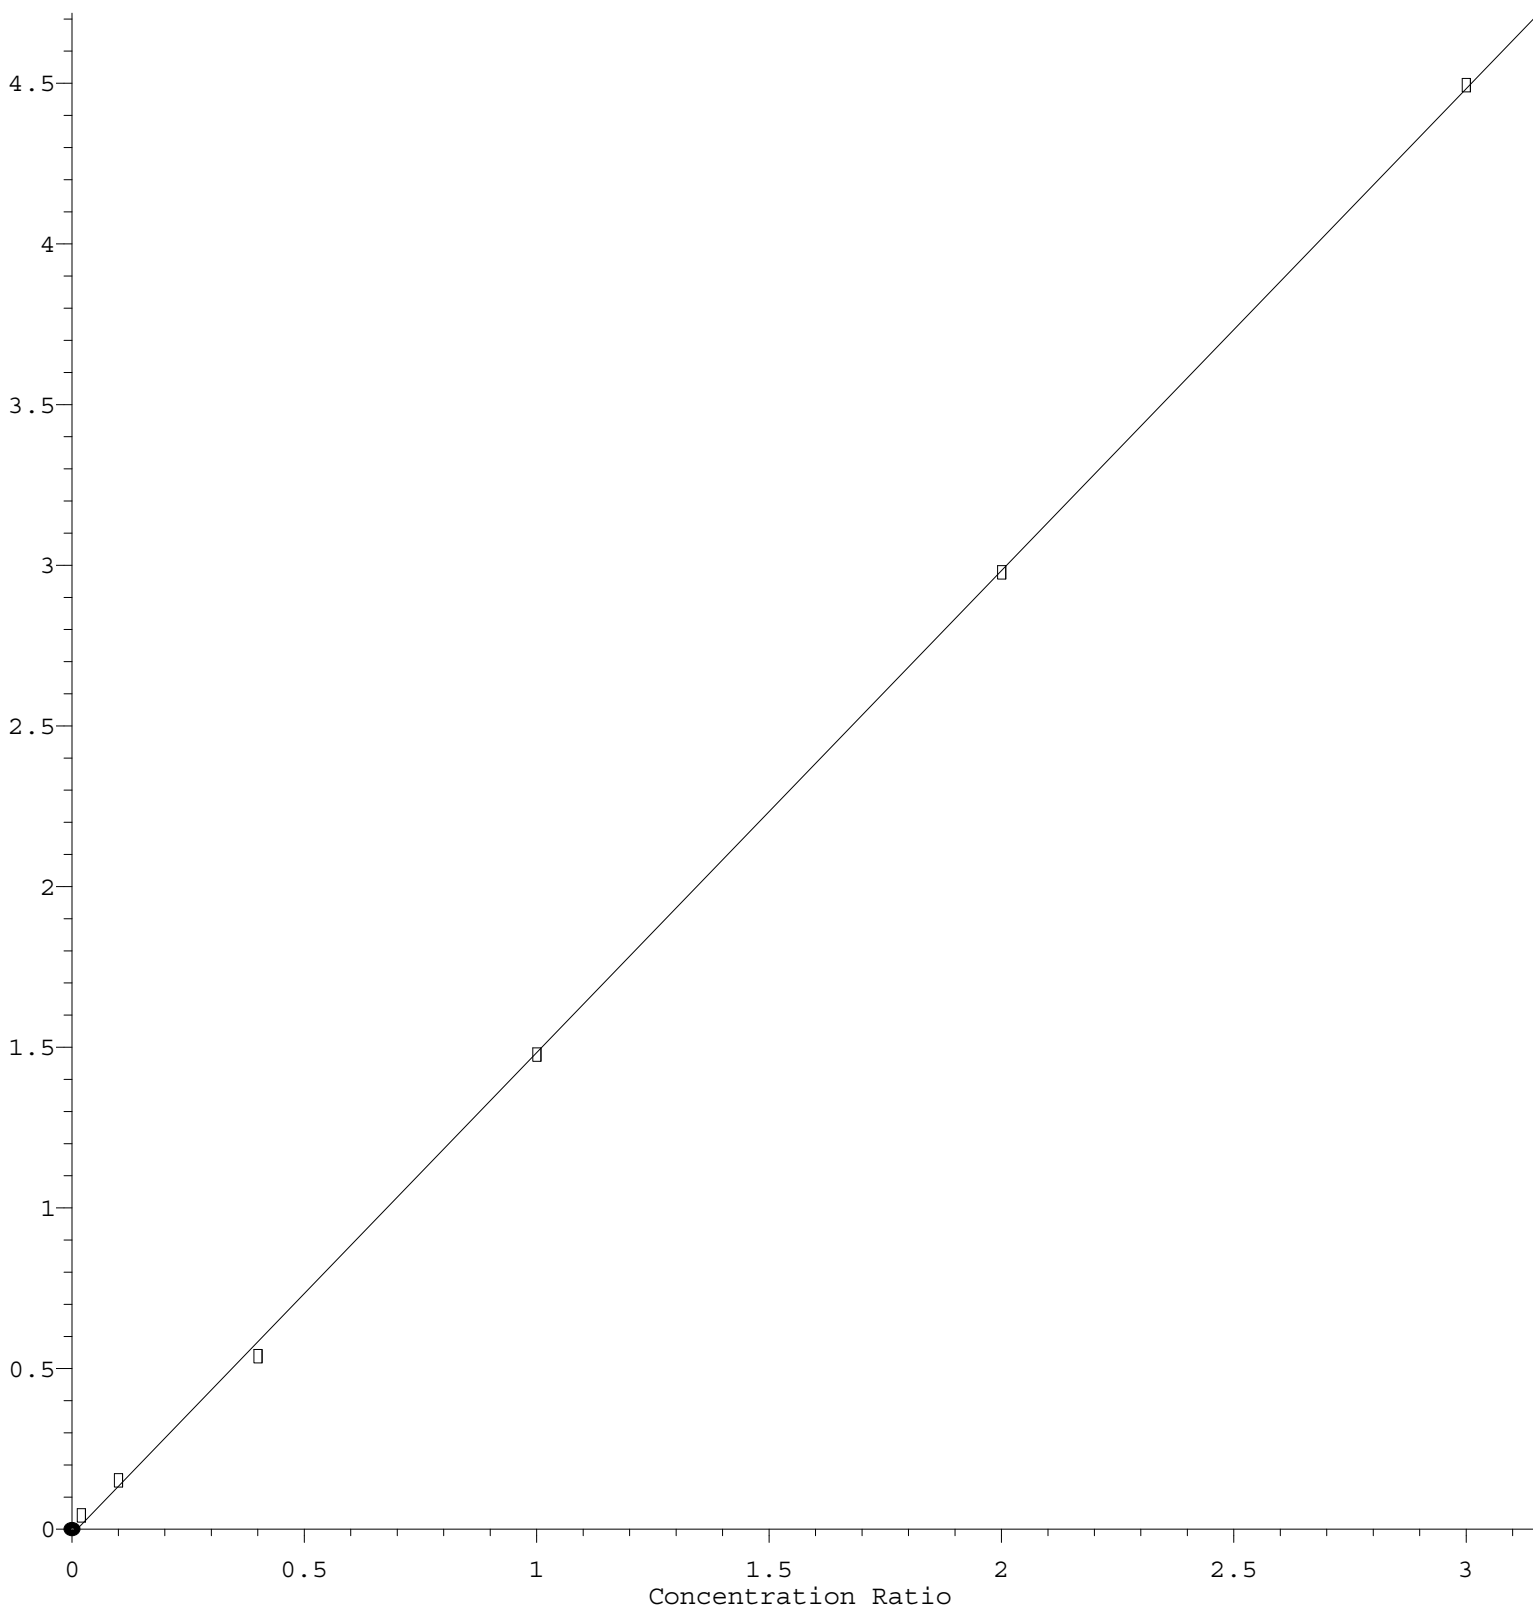


$$\text{Response} = 1.500\text{e}+000 * \text{Amt} - 1.608\text{e}-002$$

Coef of Det (r^2) = 0.999785 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X031621W.M

Calibration Table Last Updated: Tue Mar 16 14:00:21 2021

1,4-Dioxane

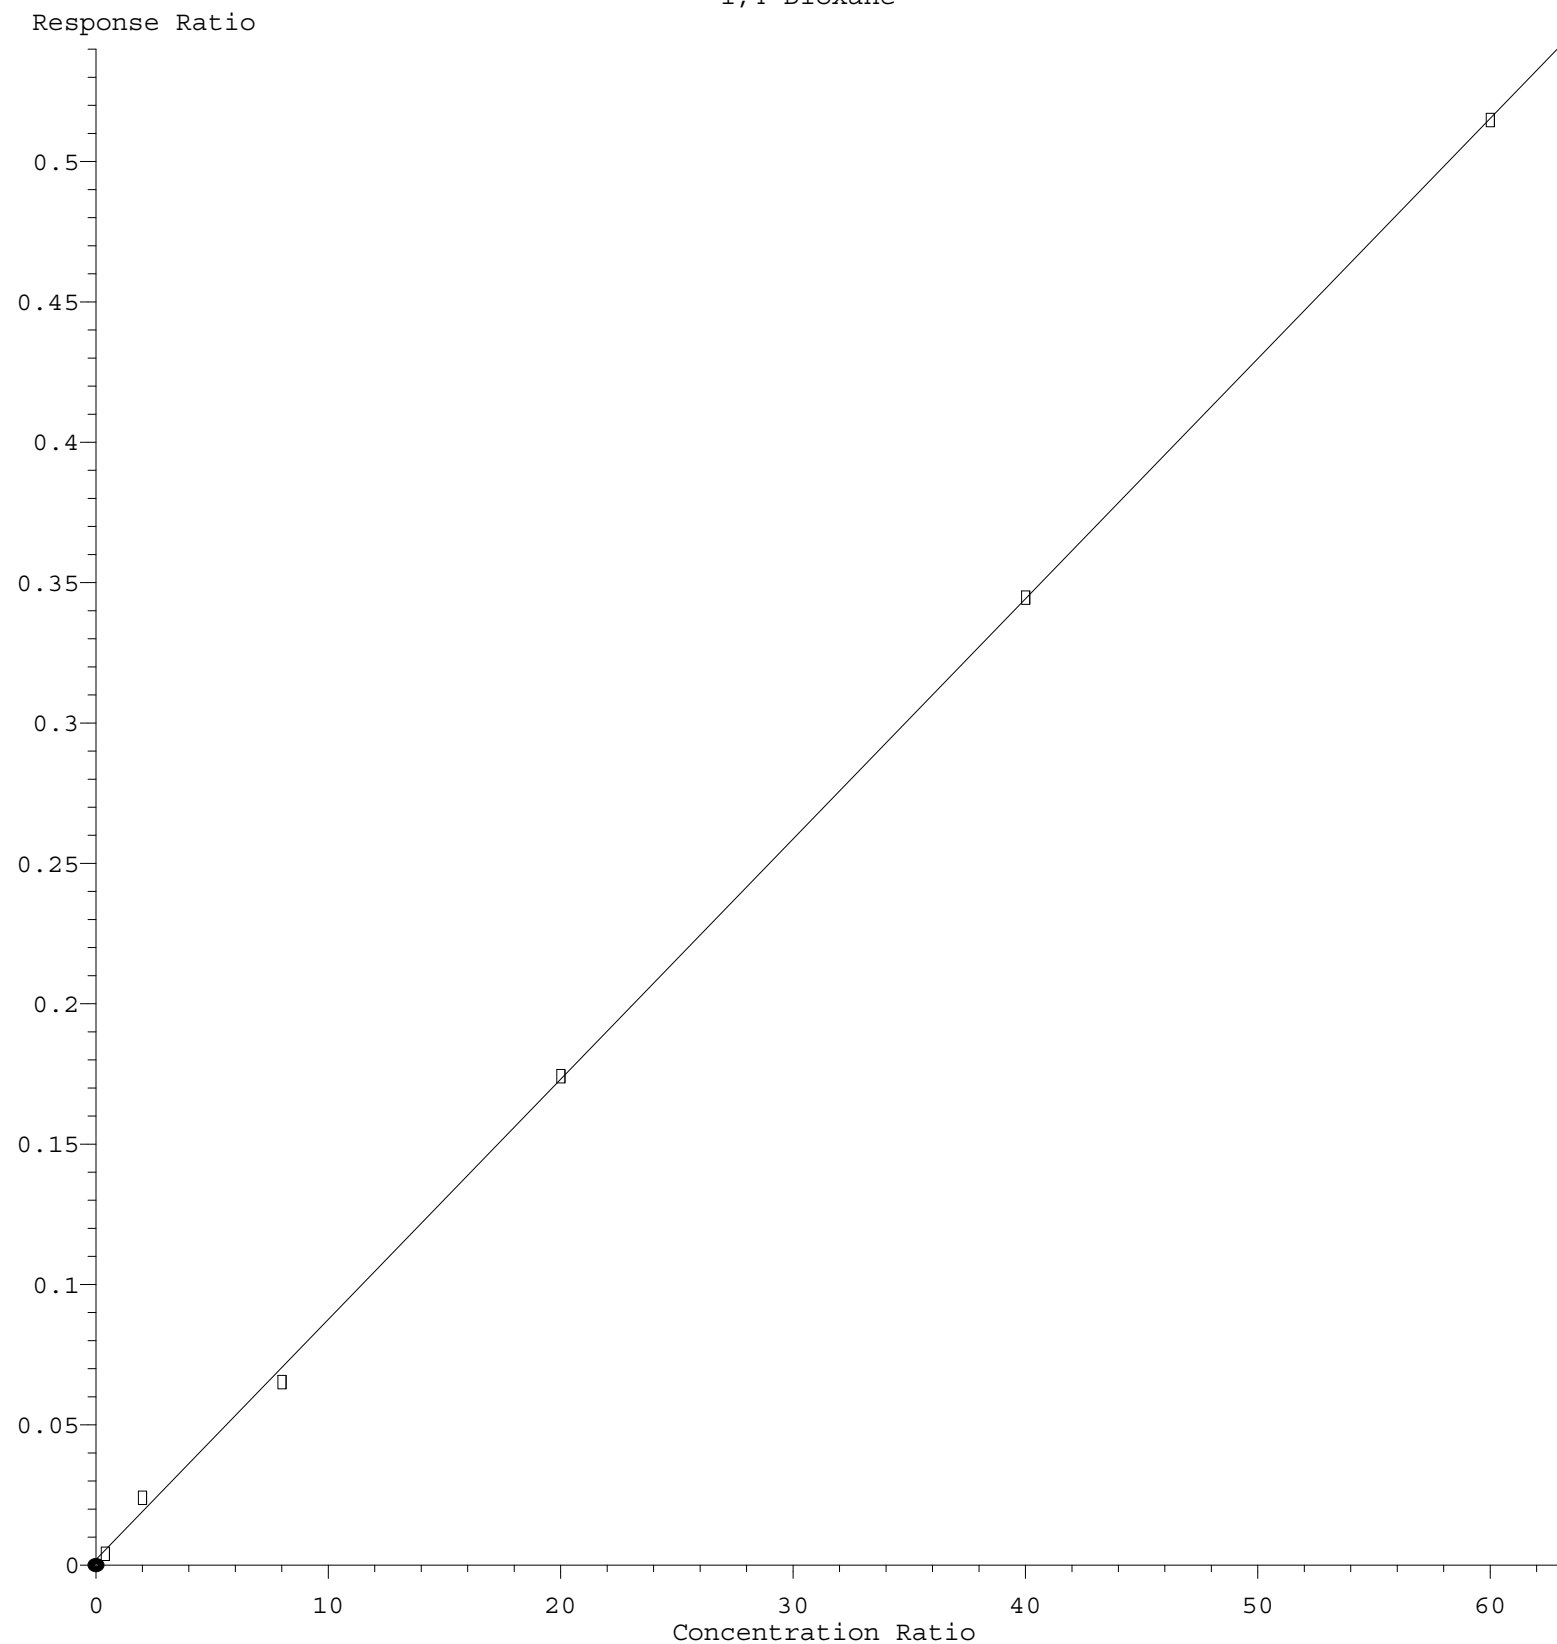

Response = $8.552 \times 10^{-3} \times \text{Amt} + 1.936 \times 10^{-3}$
 Coef of Det (r^2) = 0.999737 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X031621W.M
 Calibration Table Last Updated: Tue Mar 16 14:00:21 2021