
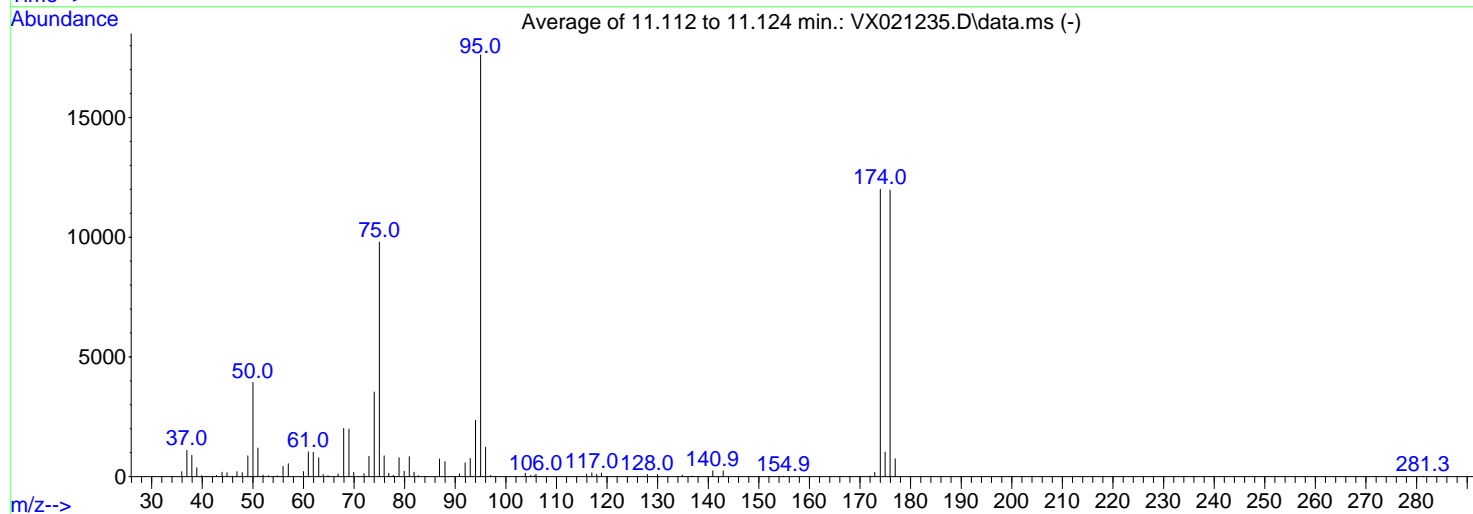


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX031621\  
 Data File : VX021235.D  
 Acq On : 16 Mar 2021 09:02  
 Operator : JC/MD  
 Sample : BFB  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X031621W.M  
 Title : SW846 8260  
 Last Update : Tue Mar 16 14:00:21 2021

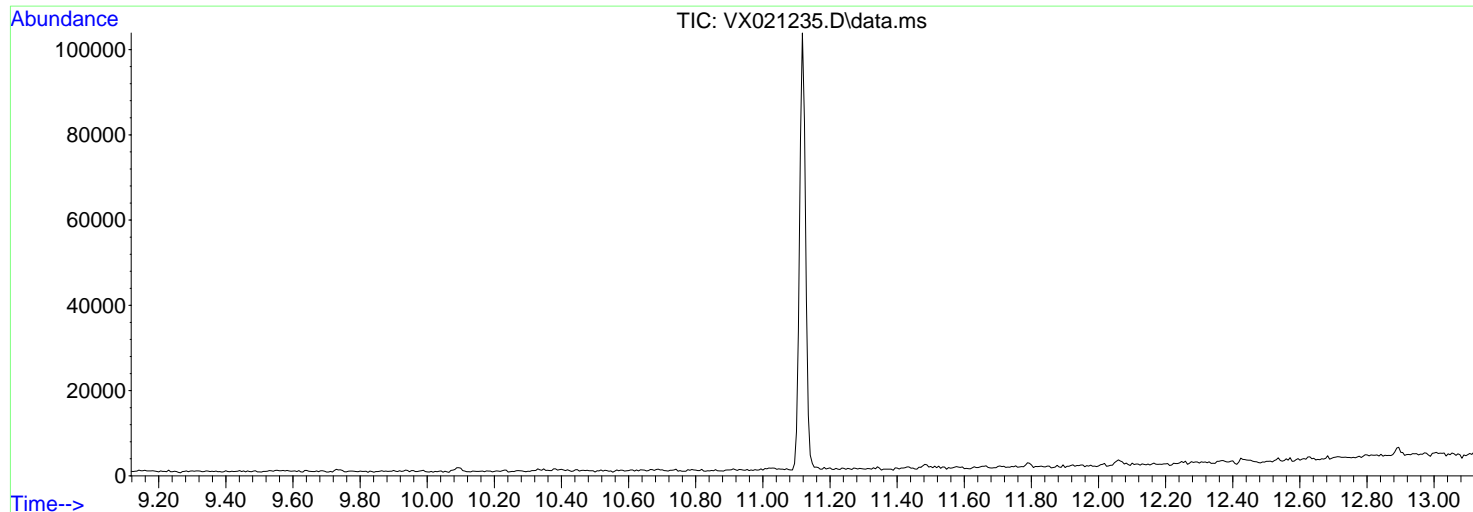

AutoFind: Scans 1704, 1705, 1706; Background Corrected with Scan 1698

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result
50	95	15	40	22.3	3936	PASS
75	95	30	60	55.6	9801	PASS
95	95	100	100	100.0	17618	PASS
96	95	5	9	7.0	1233	PASS
173	174	0.00	2	1.4	172	PASS
174	95	50	100	68.1	12006	PASS
175	174	5	9	8.6	1028	PASS
176	174	95	101	99.6	11962	PASS
177	176	5	9	6.2	747	PASS