

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031622\
 Data File : VX027475.D
 Acq On : 16 Mar 2022 16:50
 Operator : JC/MD
 Sample : N1977-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EB-20220315

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X030822W.M
 Title : SW846 8260

Signal : TIC: VX027475.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	31	36	39	rBV6	10657	23938	1.37%	0.237%
2	1.557	71	77	88	rVB10	11453	27947	1.60%	0.277%
3	2.538	229	238	247	rBV	17751	33036	1.89%	0.327%
4	5.391	692	706	722	rBV2	214580	623678	35.68%	6.182%
5	5.556	722	733	750	rVB	362168	1031971	59.04%	10.228%
6	5.958	789	799	815	rBV	213331	575455	32.92%	5.704%
7	6.763	921	931	949	rBV	538307	1302909	74.54%	12.914%
8	8.653	1234	1241	1250	rBV	1109732	1747907	100.00%	17.324%
9	10.055	1465	1471	1485	rBV	1175838	1554821	88.95%	15.411%
10	11.085	1634	1640	1653	rBV	945449	1225911	70.14%	12.151%
11	12.024	1789	1794	1804	rBV	1224629	1466034	83.87%	14.531%
12	13.701	2059	2069	2070	rBV8	8772	21533	1.23%	0.213%
13	14.329	2168	2172	2175	rBV	13081	17836	1.02%	0.177%
14	14.438	2183	2190	2200	rVB	10969	28658	1.64%	0.284%
15	14.530	2201	2205	2208	rBV	22384	30671	1.75%	0.304%
16	14.566	2208	2211	2218	rVB	32573	45470	2.60%	0.451%
17	14.829	2250	2254	2260	rVB	25221	37242	2.13%	0.369%
18	14.908	2260	2267	2271	rBV3	17765	32579	1.86%	0.323%
19	14.957	2271	2275	2279	rVV	27390	37196	2.13%	0.369%
20	15.146	2300	2306	2316	rVB2	48567	102731	5.88%	1.018%
21	15.292	2323	2330	2335	rBV3	22127	51509	2.95%	0.511%
22	15.505	2362	2365	2372	rVB7	10687	19940	1.14%	0.198%
23	15.639	2383	2387	2394	rVB5	9789	18852	1.08%	0.187%
24	15.810	2410	2415	2423	rVB4	12242	31526	1.80%	0.312%




Sum of corrected areas: 10089350

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031622\
Data File : VX027475.D
Acq On : 16 Mar 2022 16:50
Operator : JC/MD
Sample : N1977-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB-20220315

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X030822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

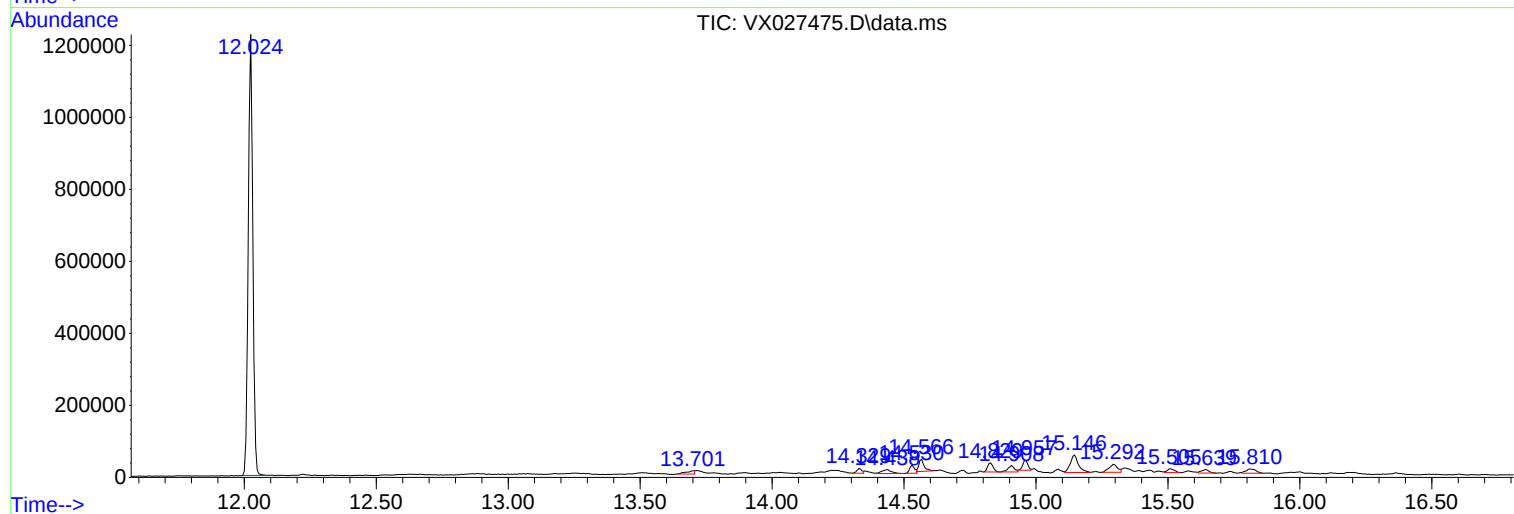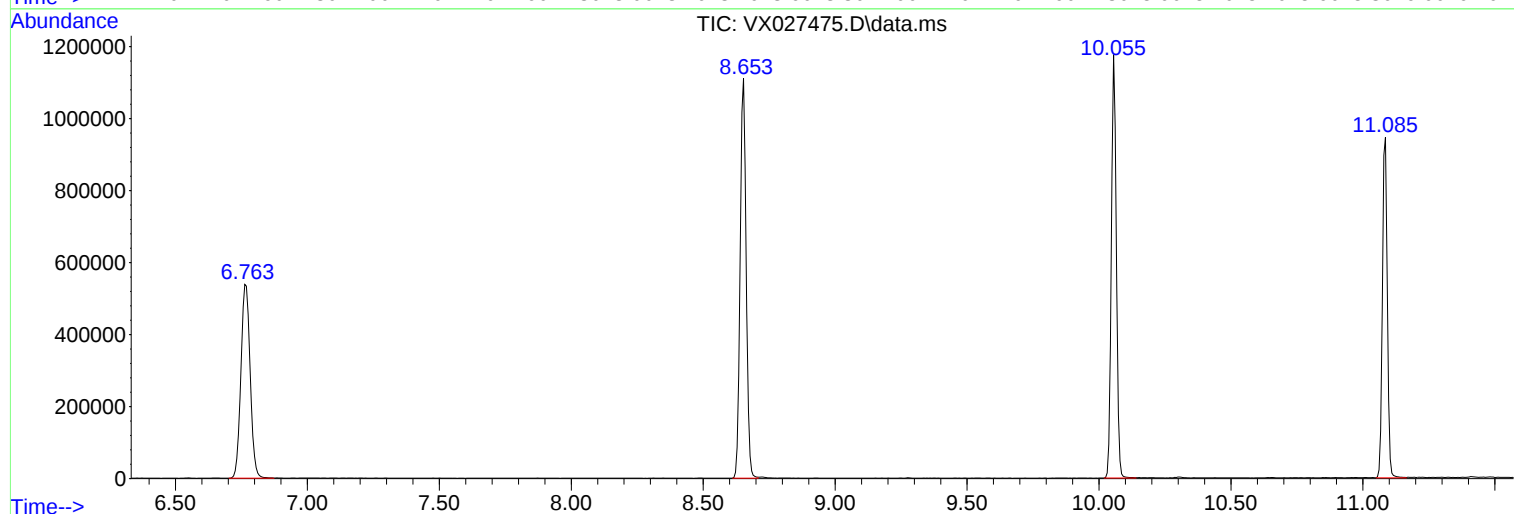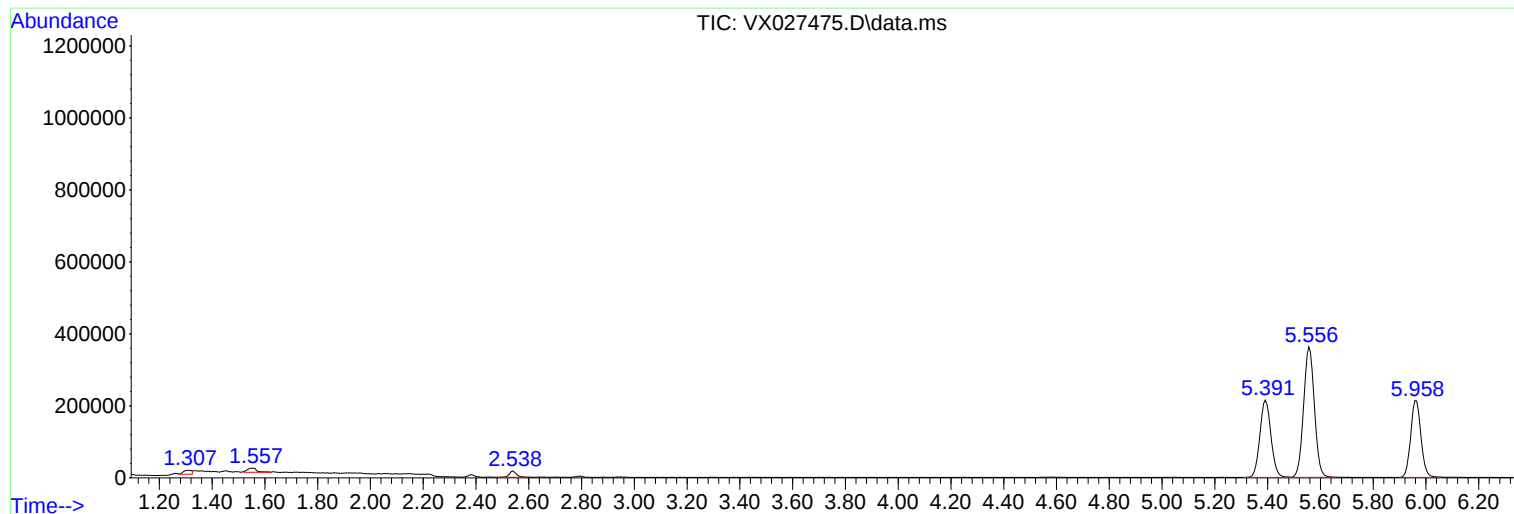

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031622\
Data File : VX027475.D
Acq On : 16 Mar 2022 16:50
Operator : JC/MD
Sample : N1977-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB-20220315

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X030822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031622\
Data File : VX027475.D
Acq On : 16 Mar 2022 16:50
Operator : JC/MD
Sample : N1977-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB-20220315

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X030822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc