

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031622\
 Data File : VX027477.D
 Acq On : 16 Mar 2022 17:47
 Operator : JC/MD
 Sample : N1977-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TB-20220315

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X030822W.M

Title : SW846 8260

Signal : TIC: VX027477.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.538	229	238	251	rBV	31006	58613	3.23%	0.595%
2	2.940	297	304	317	rBV2	14733	35085	1.93%	0.356%
3	4.574	560	572	588	rBV2	8150	28903	1.59%	0.293%
4	5.385	694	705	721	rBV2	220865	652332	35.93%	6.622%
5	5.556	721	733	748	rVV	357018	1024742	56.45%	10.403%
6	5.958	788	799	814	rBV	226591	601134	33.11%	6.103%
7	6.763	921	931	945	rBV	545339	1290801	71.10%	13.104%
8	8.647	1232	1240	1255	rBV	1126883	1815461	100.00%	18.430%
9	10.055	1465	1471	1485	rBV	1208628	1618914	89.17%	16.435%
10	11.085	1634	1640	1654	rBV	1002918	1290147	71.06%	13.097%
11	12.024	1788	1794	1808	rBV	1192879	1434274	79.00%	14.561%




Sum of corrected areas: 9850406

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031622\
Data File : VX027477.D
Acq On : 16 Mar 2022 17:47
Operator : JC/MD
Sample : N1977-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-20220315

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X030822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

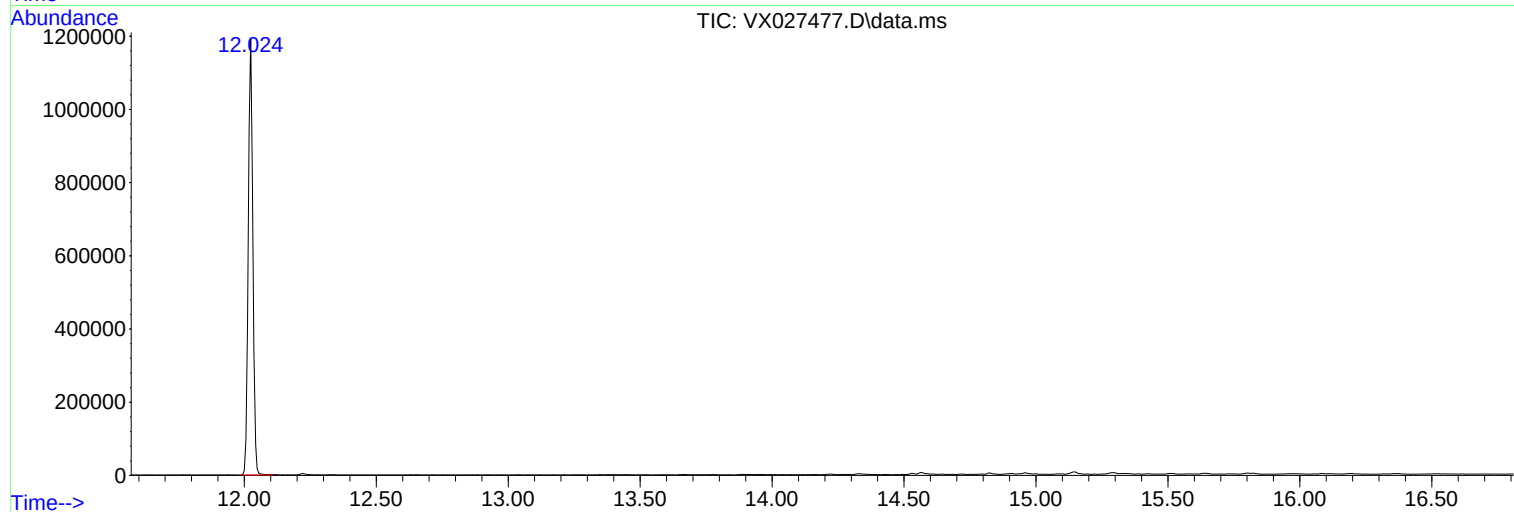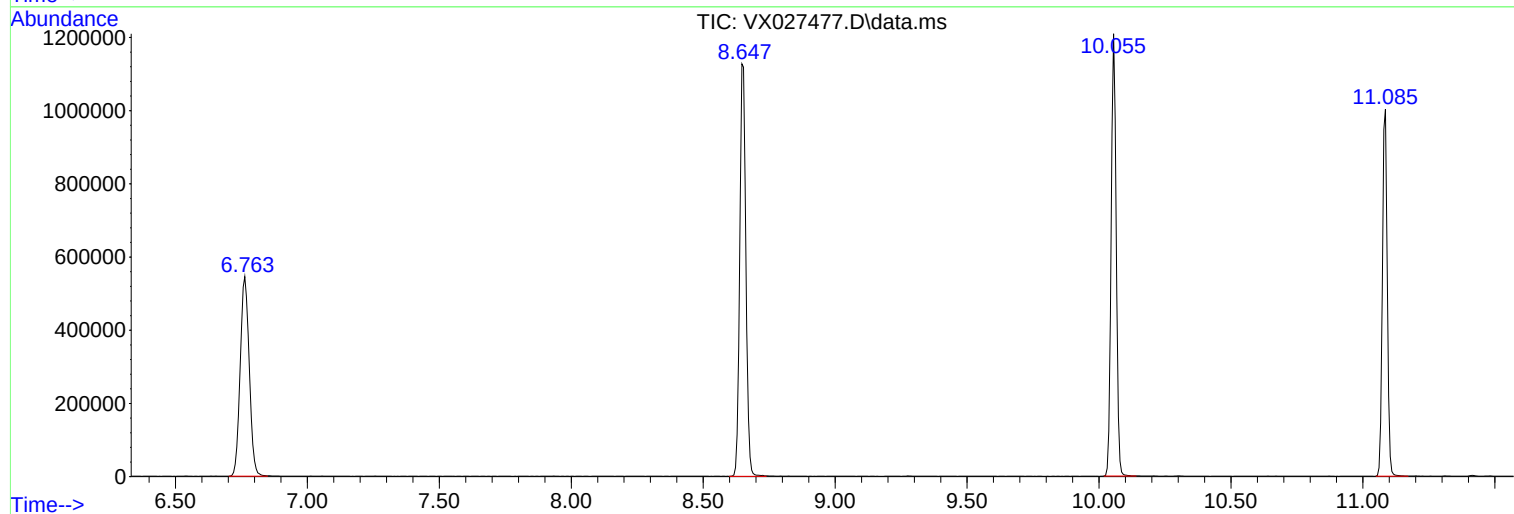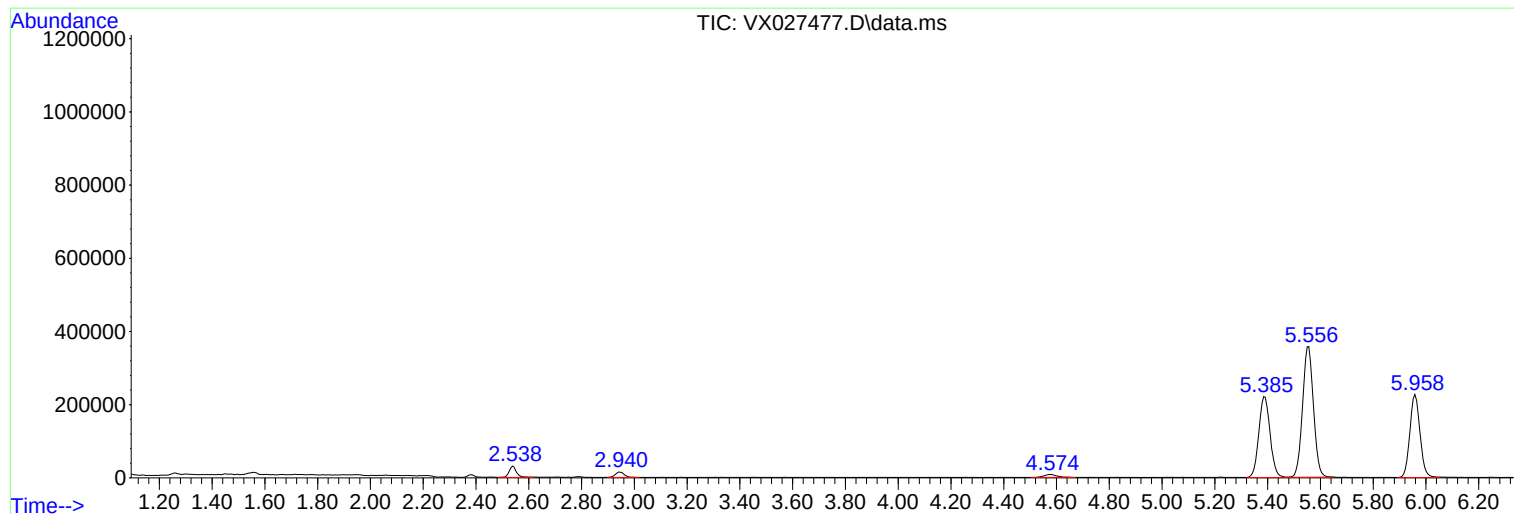

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031622\
Data File : VX027477.D
Acq On : 16 Mar 2022 17:47
Operator : JC/MD
Sample : N1977-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-20220315

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X030822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031622\
Data File : VX027477.D
Acq On : 16 Mar 2022 17:47
Operator : JC/MD
Sample : N1977-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-20220315

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X030822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc