

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031623\
 Data File : VX034571.D
 Acq On : 17 Mar 2023 07:59
 Operator : JC/MD
 Sample : 01907-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 33959

Quant Time: Mar 17 08:34:48 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
 Quant Title : SW846 8260
 QLast Update : Mon Mar 13 10:29:32 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	261696	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	521941	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	418382	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	198901	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	229335	60.238	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 120.480%#	
35) Dibromofluoromethane	5.385	113	143318	41.588	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 83.180%	
50) Toluene-d8	8.647	98	633647	49.255	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 98.520%	
62) 4-Bromofluorobenzene	11.079	95	225337	43.365	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 86.740%	


Target Compounds			Qvalue			
3) Chloromethane	1.294	50	418	Below Cal	#	42
11) Tert butyl alcohol	2.953	59	13296	16.771	ug/l #	93
13) Acrolein	2.233	56	2409	3.841	ug/l	99
16) Acetone	2.374	43	135292	75.441	ug/l	99
17) Carbon Disulfide	2.514	76	18359	2.277	ug/l	98
18) Methyl Acetate	2.709	43	7822	1.335	ug/l	99
20) Methylene Chloride	2.788	84	13081	3.758	ug/l	98
25) 2-Butanone	4.562	43	21968	8.561	ug/l	100
29) Tetrahydrofuran	5.038	42	1506	0.951	ug/l #	53
36) 1,1-Dichloropropene	5.550	75	22037	4.163	ug/l #	50
37) Ethyl Acetate	4.715	43	61360	10.611	ug/l	97
38) Carbon Tetrachloride	5.550	117	27491	5.221	ug/l #	15
40) Benzene	6.038	78	47095	3.042	ug/l	99
43) Isopropyl Acetate	6.336	43	284413	29.034	ug/l	99
48) Methyl methacrylate	7.586	41	9747	2.069	ug/l #	15
49) 1,4-Dioxane	7.641	88	75	0.758	ug/l #	1
51) 4-Methyl-2-Pentanone	8.574	43	540581	95.128	ug/l #	79
52) Toluene	8.720	92	31897	3.327	ug/l	99
53) t-1,3-Dichloropropene	8.952	75	1562	0.261	ug/l #	43
54) cis-1,3-Dichloropropene	8.549	75	89106	13.743	ug/l #	63
57) 1,3-Dichloropropane	9.482	76	9260	1.370	ug/l #	43
59) 2-Hexanone	9.482	43	146853	33.430	ug/l #	53
67) Ethyl Benzene	10.195	91	10292	0.626	ug/l	100
68) m/p-Xylenes	10.299	106	21332	3.379	ug/l	97
69) o-Xylene	10.640	106	30371	4.794	ug/l	99
70) Styrene	10.659	104	6824	0.668	ug/l #	29
74) N-amyl acetate	10.768	43	4228	0.574	ug/l #	53
76) 1,2,3-Trichloropropane	11.079	75	123879	27.125	ug/l #	34
81) trans-1,4-Dichloro-2-b...	11.079	75	123879	73.381	ug/l #	8
84) 1,2,4-Trimethylbenzene	11.750	105	825656	62.655	ug/l #	32
85) sec-Butylbenzene	11.750	105	825656	51.949	ug/l #	56
95) Naphthalene	13.774	128	249756	17.054	ug/l	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031623\
Data File : VX034571.D
Acq On : 17 Mar 2023 07:59
Operator : JC/MD
Sample : 01907-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
33959

Quant Time: Mar 17 08:34:48 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260
QLast Update : Mon Mar 13 10:29:32 2023
Response via : Initial Calibration



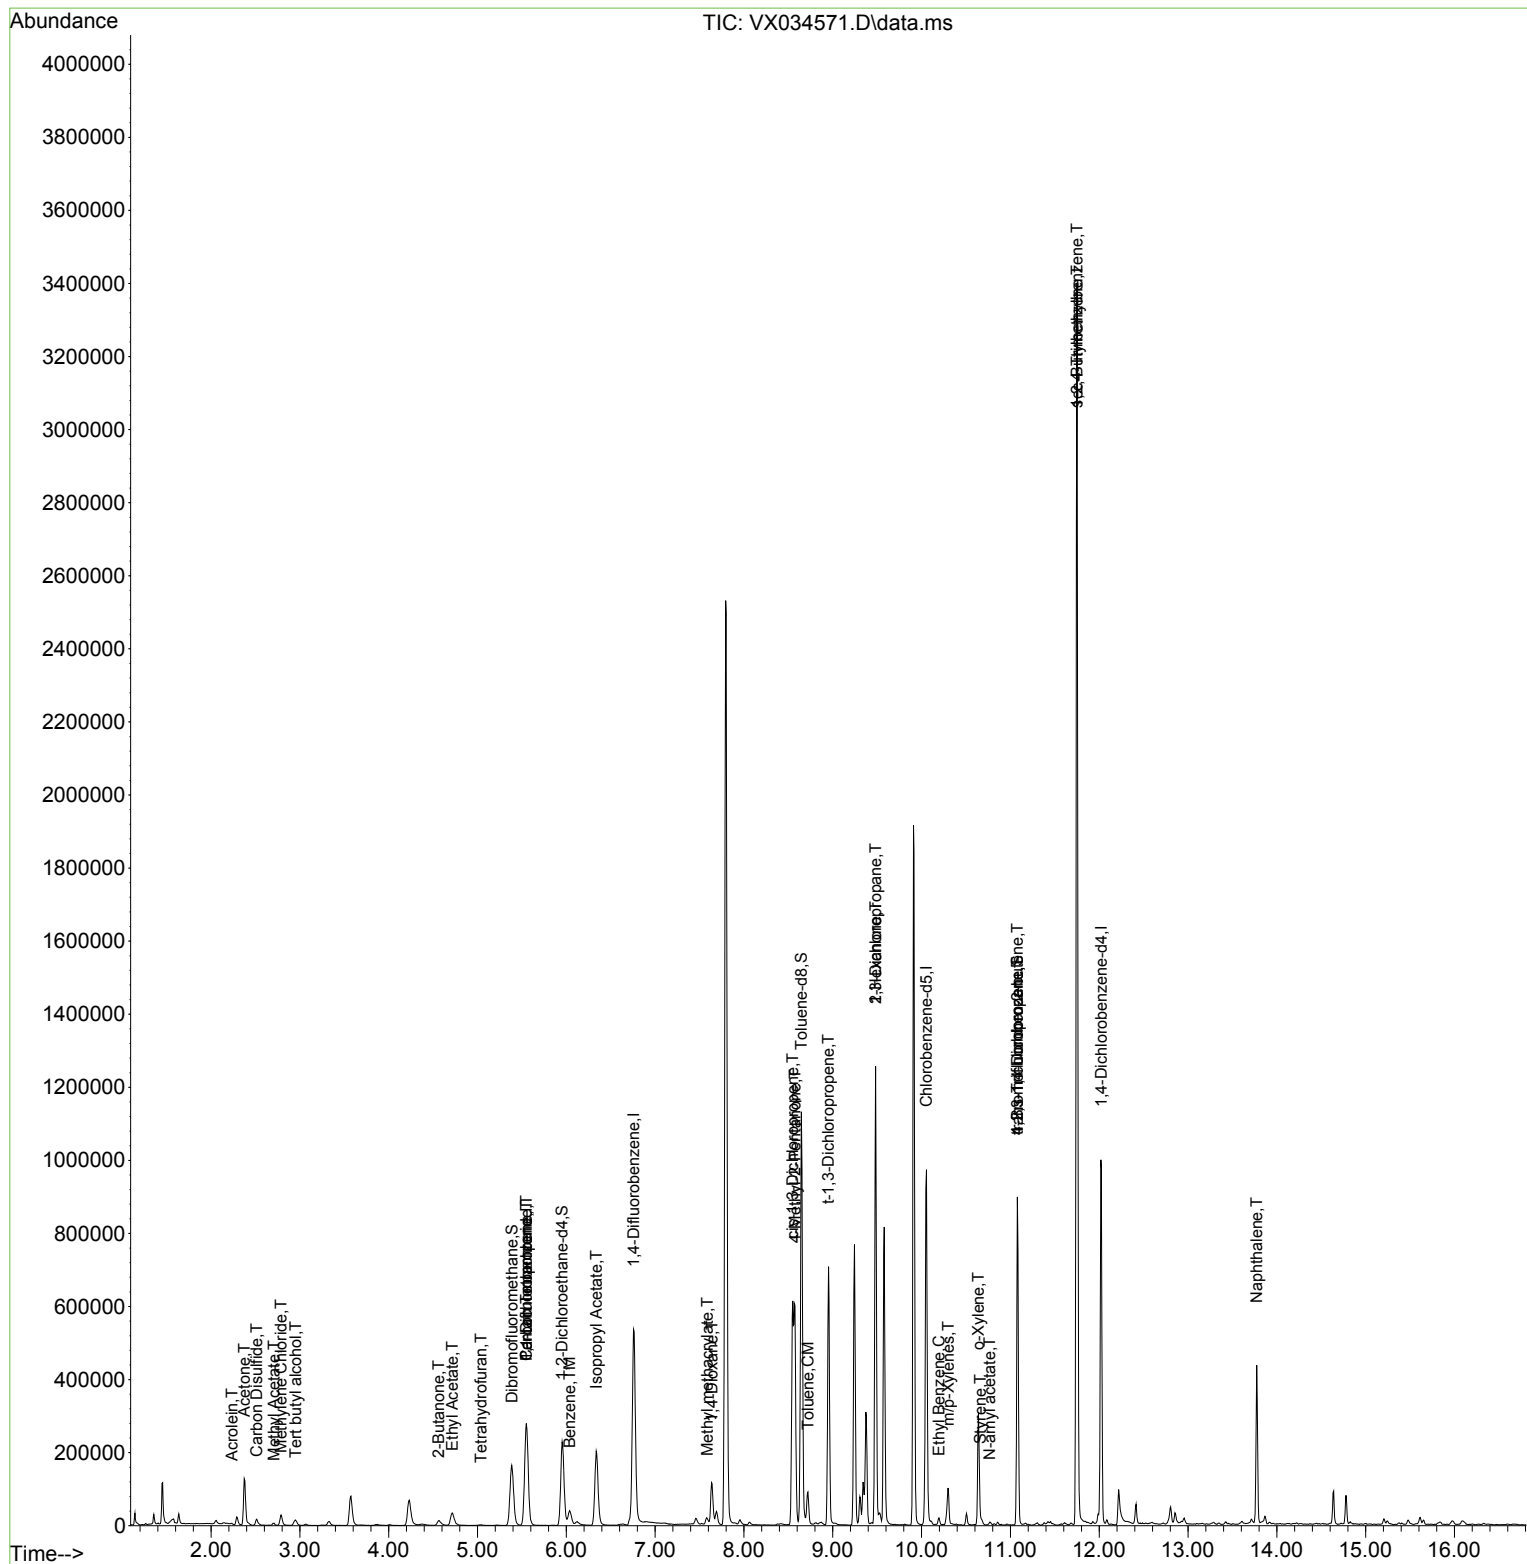




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX034571.D
Acq: 17 Mar 2023 07:59




Instrument :
MSVOA_X
ClientSampleId :
33959


Tgt Ion:168 Resp: 261696
Ion Ratio Lower Upper
168 100
99 61.3 45.7 68.5

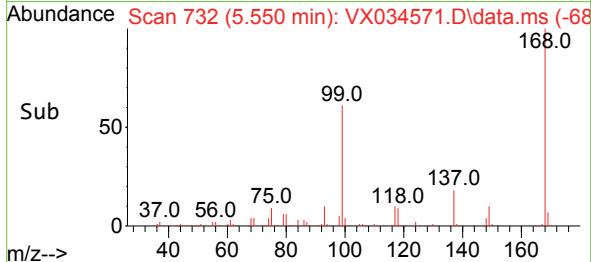

#3
Chloromethane
Concen: Below Cal
RT: 1.294 min Scan# 34
Delta R.T. -0.007 min
Lab File: VX034571.D
Acq: 17 Mar 2023 07:59

Tgt Ion: 50 Resp: 418
Ion Ratio Lower Upper
50 100
52 0.0 25.9 38.9#









#11
Tert butyl alcohol
Concen: 16.771 ug/l
RT: 2.953 min Scan# 306
Delta R.T. 0.000 min
Lab File: VX034571.D
Acq: 17 Mar 2023 07:59




Instrument :
MSVOA_X
ClientSampleId :
33959


Tgt Ion: 59 Resp: 13296
Ion Ratio Lower Upper
59 100
57 7.7 8.1 12.1#

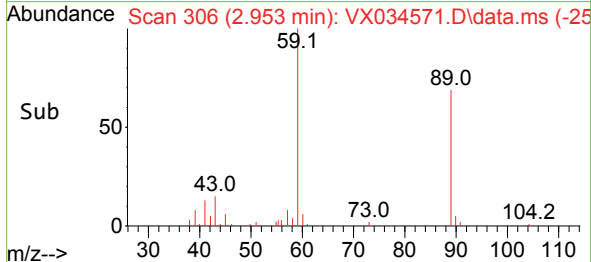

#13
Acrolein
Concen: 3.841 ug/l
RT: 2.233 min Scan# 188
Delta R.T. 0.000 min
Lab File: VX034571.D
Acq: 17 Mar 2023 07:59

Tgt Ion: 56 Resp: 2409
Ion Ratio Lower Upper
56 100
55 69.8 56.6 85.0









#16
Acetone
Concen: 75.441 ug/l
RT: 2.374 min Scan# 211
Delta R.T. 0.000 min
Lab File: VX034571.D
Acq: 17 Mar 2023 07:59




Instrument :
MSVOA_X
ClientSampleId :
33959


Tgt Ion: 43 Resp: 135292
Ion Ratio Lower Upper
43 100
58 30.2 24.7 37.1

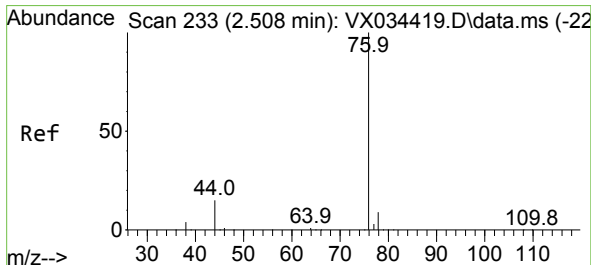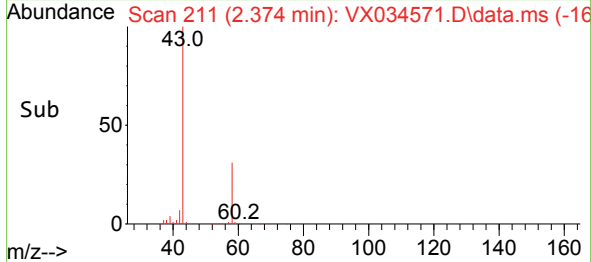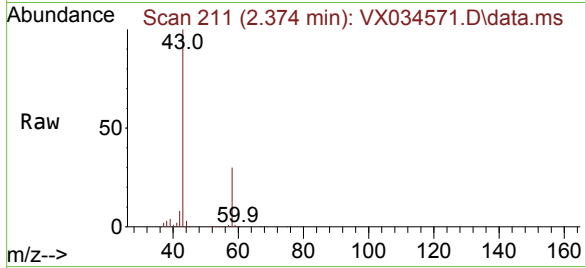

#17
Carbon Disulfide
Concen: 2.277 ug/l
RT: 2.514 min Scan# 234
Delta R.T. 0.006 min
Lab File: VX034571.D
Acq: 17 Mar 2023 07:59

Tgt Ion: 76 Resp: 18359
Ion Ratio Lower Upper
76 100
78 8.2 7.2 10.8




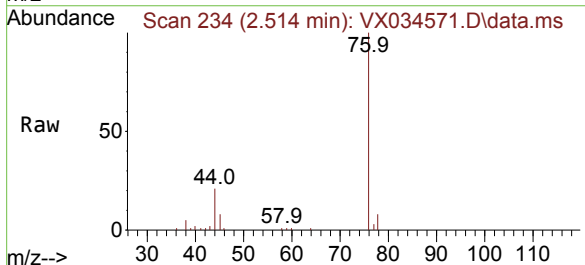


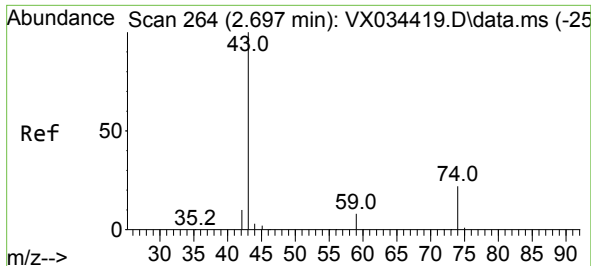

#18
Methyl Acetate
Concen: 1.335 ug/l
RT: 2.709 min Scan# 20
Delta R.T. 0.012 min
Lab File: VX034571.D
Acq: 17 Mar 2023 07:59




Instrument :
MSVOA_X
ClientSampleId :
33959


Tgt Ion: 43 Resp: 7822
Ion Ratio Lower Upper
43 100
74 22.5 18.3 27.5

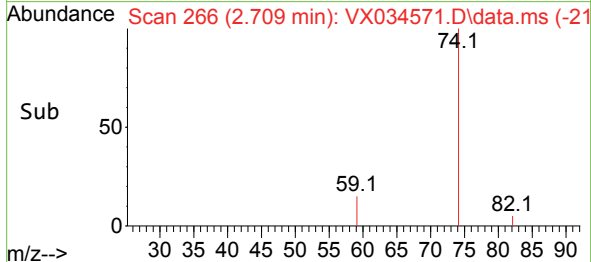

#20
Methylene Chloride
Concen: 3.758 ug/l
RT: 2.788 min Scan# 279
Delta R.T. 0.006 min
Lab File: VX034571.D
Acq: 17 Mar 2023 07:59

Tgt Ion: 84 Resp: 13081
Ion Ratio Lower Upper
84 100
49 126.8 103.8 155.8
51 40.7 31.8 47.8
86 62.4 51.4 77.2




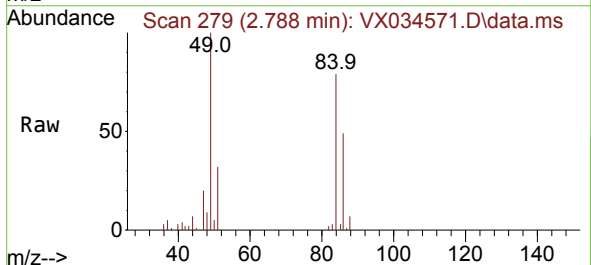


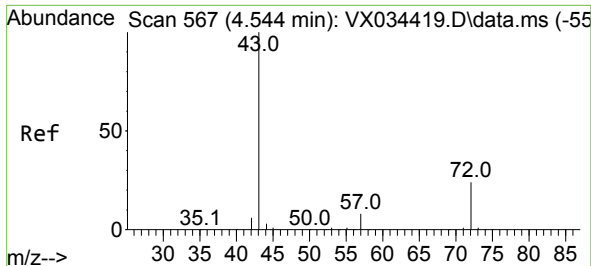

#25
2-Butanone
Concen: 8.561 ug/l
RT: 4.562 min Scan# 51
Delta R.T. 0.018 min
Lab File: VX034571.D
Acq: 17 Mar 2023 07:59




Instrument :
MSVOA_X
ClientSampleId :
33959


Tgt Ion: 43 Resp: 21968
Ion Ratio Lower Upper
43 100
72 24.1 19.3 28.9



#29
Tetrahydrofuran
Concen: 0.951 ug/l
RT: 5.038 min Scan# 648
Delta R.T. 0.043 min
Lab File: VX034571.D
Acq: 17 Mar 2023 07:59

Tgt Ion: 42 Resp: 1506
Ion Ratio Lower Upper
42 100
72 0.0 34.5 51.7#
71 24.0 32.1 48.1#







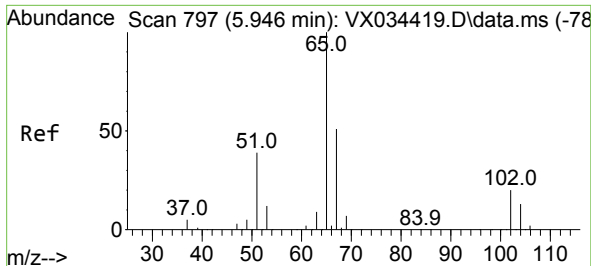

#33
1,2-Dichloroethane-d4
Concen: 60.238 ug/l
RT: 5.952 min Scan# 797
Delta R.T. 0.006 min
Lab File: VX034571.D
Acq: 17 Mar 2023 07:59




Instrument :
MSVOA_X
ClientSampleId :
33959


Tgt Ion: 65 Resp: 229335
Ion Ratio Lower Upper
65 100
67 49.1 0.0 104.0

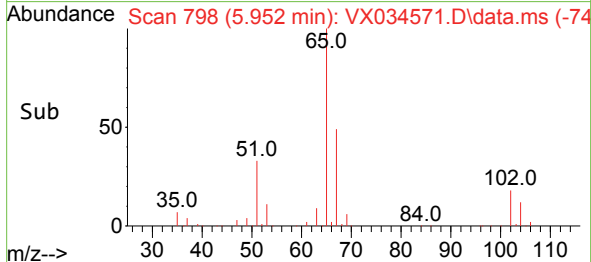

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 930
Delta R.T. 0.000 min
Lab File: VX034571.D
Acq: 17 Mar 2023 07:59

Tgt Ion: 114 Resp: 521941
Ion Ratio Lower Upper
114 100
63 22.4 0.0 42.2
88 17.7 0.0 33.2


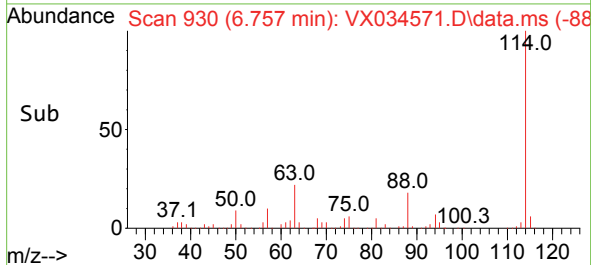




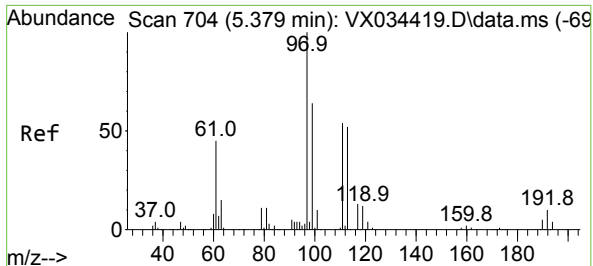

#35
Dibromofluoromethane
Concen: 41.588 ug/l
RT: 5.385 min Scan# 704
Delta R.T. 0.006 min
Lab File: VX034571.D
Acq: 17 Mar 2023 07:59




Instrument :
MSVOA_X
ClientSampleId :
33959


Tgt Ion:113 Resp: 143318
Ion Ratio Lower Upper
113 100
111 101.2 83.7 125.5
192 18.5 15.4 23.2

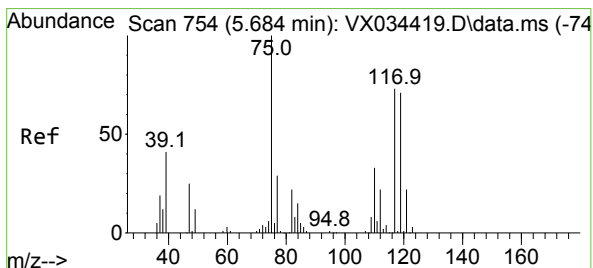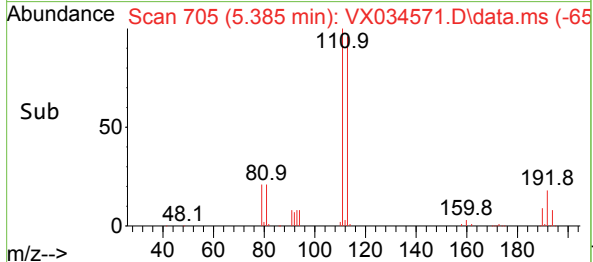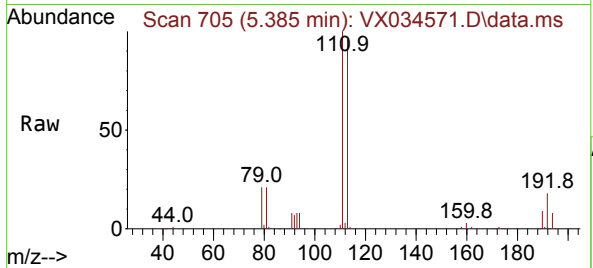

#36
1,1-Dichloropropene
Concen: 4.163 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.134 min
Lab File: VX034571.D
Acq: 17 Mar 2023 07:59

Tgt Ion: 75 Resp: 22037
Ion Ratio Lower Upper
75 100
110 8.4 17.5 52.5#
77 0.0 24.3 36.5#

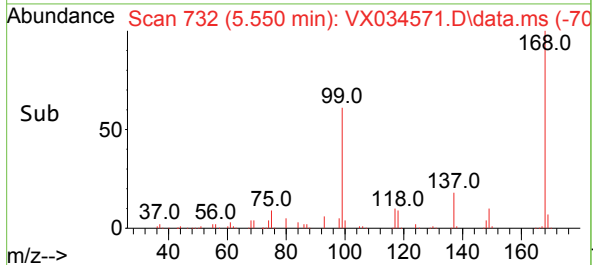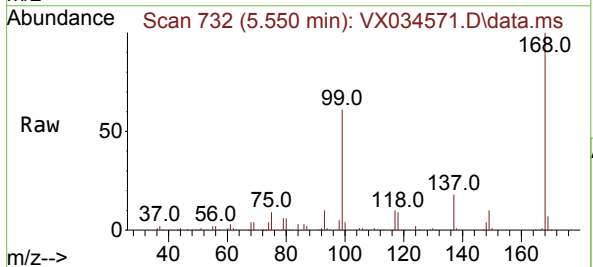



#37

Ethyl Acetate

Concen: 10.611 ug/l

RT: 4.715 min Scan# 593

Delta R.T. 0.012 min

Lab File: VX034571.D

Acq: 17 Mar 2023 07:59





Instrument :

MSVOA_X

ClientSampleId :

33959

Tgt Ion: 43	Resp: 61360
Ion Ratio	Lower Upper
43 100	
61 14.0	10.2 15.4
70 11.8	8.2 12.4



#38

Carbon Tetrachloride

Concen: 5.221 ug/l




RT: 5.550 min Scan# 732


Delta R.T. -0.122 min

Lab File: VX034571.D

Acq: 17 Mar 2023 07:59

Tgt Ion: 117	Resp: 27491
Ion Ratio	Lower Upper
117 100	
119 4.1	76.6 114.8#
121 0.0	23.8 35.6#


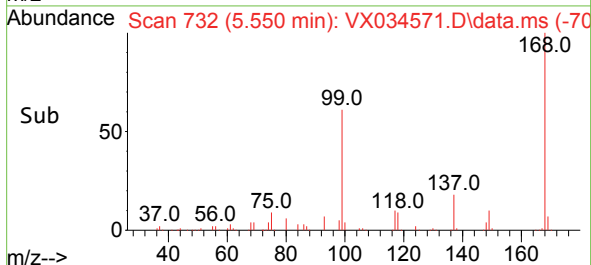
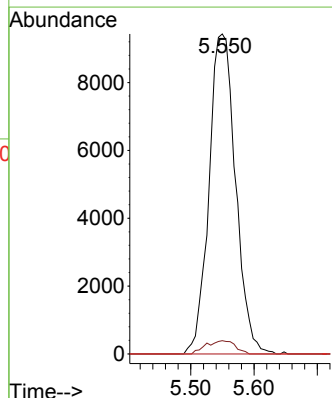



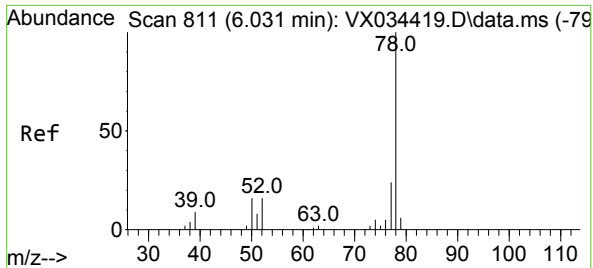

#40
Benzene
Concen: 3.042 ug/l
RT: 6.038 min Scan# 811
Delta R.T. 0.006 min
Lab File: VX034571.D
Acq: 17 Mar 2023 07:59




Instrument :
MSVOA_X
ClientSampleId :
33959


Tgt Ion: 78 Resp: 47095
Ion Ratio Lower Upper
78 100
77 24.3 19.0 28.4

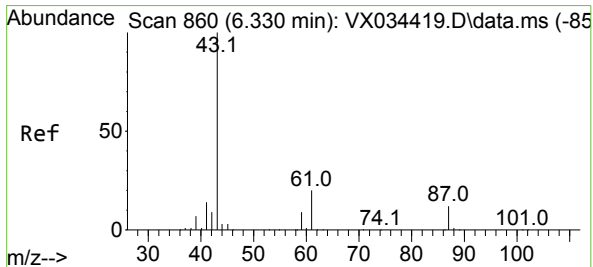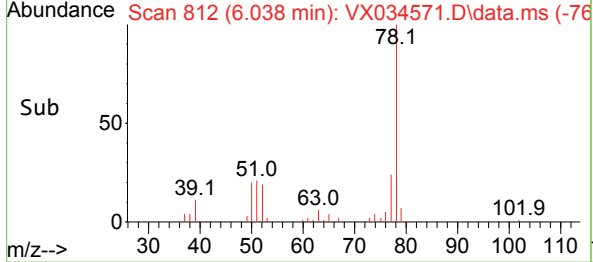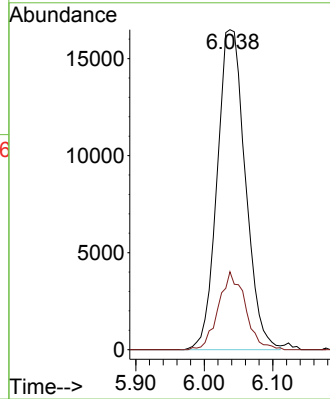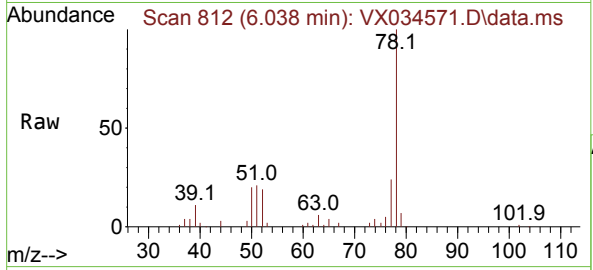

#43
Isopropyl Acetate
Concen: 29.034 ug/l
RT: 6.336 min Scan# 861
Delta R.T. 0.006 min
Lab File: VX034571.D
Acq: 17 Mar 2023 07:59

Tgt Ion: 43 Resp: 284413
Ion Ratio Lower Upper
43 100
61 18.3 15.2 22.8
87 12.2 9.8 14.8

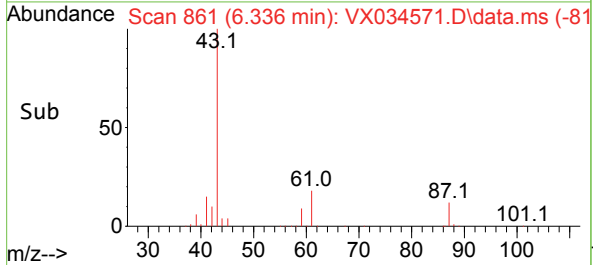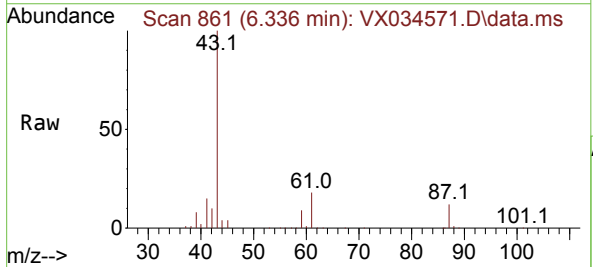



#48

Methyl methacrylate

Concen: 2.069 ug/l

RT: 7.586 min Scan# 1066

Delta R.T. -0.104 min

Lab File: VX034571.D

Acq: 17 Mar 2023 07:59

Instrument :

MSVOA_X

ClientSampleId :

33959





Tgt Ion: 41 Resp: 9747

Ion Ratio Lower Upper

41 100

69 0.0 62.2 93.4#

39 0.0 47.7 71.5#

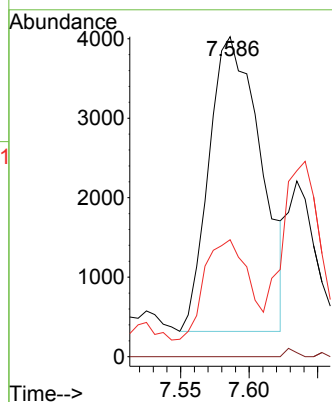

#49

1,4-Dioxane

Concen: 0.758 ug/l

RT: 7.641 min Scan# 1075

Delta R.T. -0.012 min

Lab File: VX034571.D

Acq: 17 Mar 2023 07:59




Tgt Ion: 88 Resp: 75


Ion Ratio Lower Upper

88 100

43 0.0 27.7 41.5#

58 6858.7 56.8 85.2#







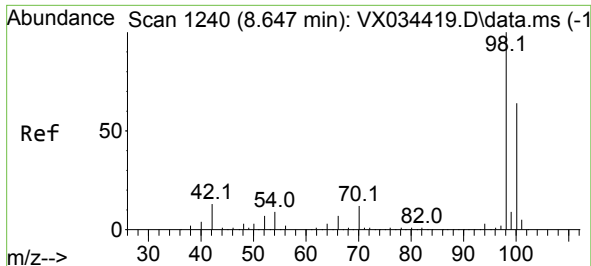

#50
Toluene-d8
Concen: 49.255 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX034571.D
Acq: 17 Mar 2023 07:59




Instrument :
MSVOA_X
ClientSampleId :
33959


Tgt Ion: 98 Resp: 633647
Ion Ratio Lower Upper
98 100
100 66.3 52.5 78.7

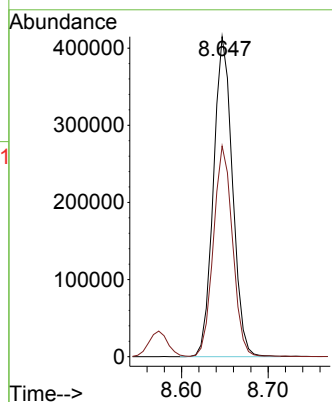

#51
4-Methyl-2-Pentanone
Concen: 95.128 ug/l
RT: 8.574 min Scan# 1228
Delta R.T. 0.006 min
Lab File: VX034571.D
Acq: 17 Mar 2023 07:59

Tgt Ion: 43 Resp: 540581
Ion Ratio Lower Upper
43 100
58 25.8 30.6 46.0#



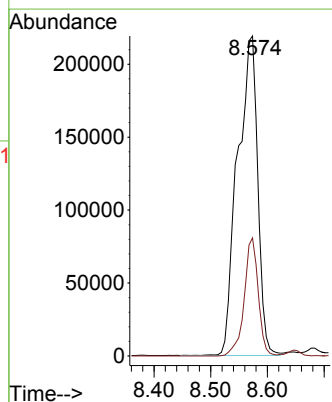





#52
Toluene
Concen: 3.327 ug/l
RT: 8.720 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX034571.D
Acq: 17 Mar 2023 07:59




Instrument :
MSVOA_X
ClientSampleId :
33959


Tgt Ion: 92 Resp: 31897
Ion Ratio Lower Upper
92 100
91 172.7 136.8 205.2

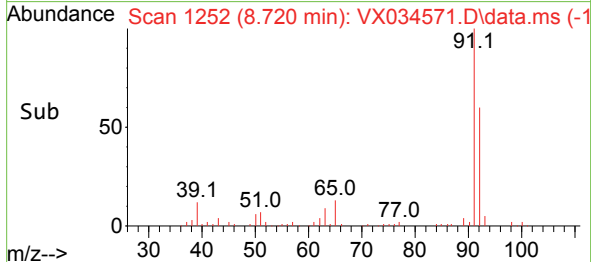

#53
t-1,3-Dichloropropene
Concen: 0.261 ug/l
RT: 8.952 min Scan# 1290
Delta R.T. -0.024 min
Lab File: VX034571.D
Acq: 17 Mar 2023 07:59

Tgt Ion: 75 Resp: 1562
Ion Ratio Lower Upper
75 100
77 0.0 25.4 38.2#









#54
 cis-1,3-Dichloropropene
 Concen: 13.743 ug/l
 RT: 8.549 min Scan# 1193
 Delta R.T. 0.189 min
 Lab File: VX034571.D
 Acq: 17 Mar 2023 07:59




Instrument :
 MSVOA_X
 ClientSampleId :
 33959


Tgt Ion: 75 Resp: 89106
 Ion Ratio Lower Upper
 75 100
 77 0.7 25.0 37.4#
 39 36.3 44.6 66.8#

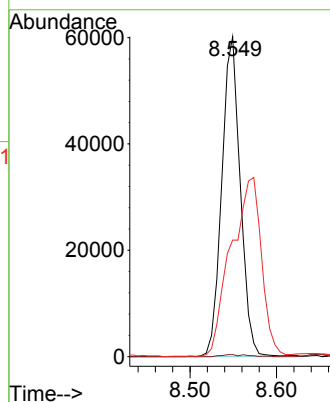

#57
 1,3-Dichloropropane
 Concen: 1.370 ug/l
 RT: 9.482 min Scan# 1377
 Delta R.T. 0.177 min
 Lab File: VX034571.D
 Acq: 17 Mar 2023 07:59

Tgt Ion: 76 Resp: 9260
 Ion Ratio Lower Upper
 76 100
 78 0.5 25.8 38.8#









#59
2-Hexanone
Concen: 33.430 ug/l
RT: 9.482 min Scan# 11
Delta R.T. 0.055 min
Lab File: VX034571.D
Acq: 17 Mar 2023 07:59




Instrument :
MSVOA_X
ClientSampleId :
33959


Tgt Ion: 43 Resp: 146853
Ion Ratio Lower Upper
43 100
58 19.6 26.3 78.9#



#62
4-Bromofluorobenzene
Concen: 43.365 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX034571.D
Acq: 17 Mar 2023 07:59

Tgt Ion: 95 Resp: 225337
Ion Ratio Lower Upper
95 100
174 74.2 0.0 147.4
176 72.5 0.0 140.6



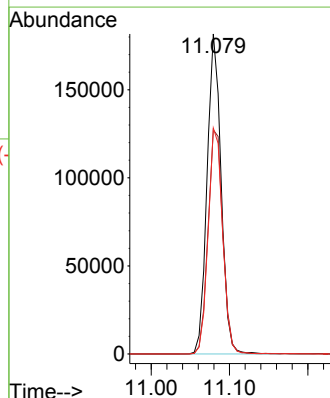



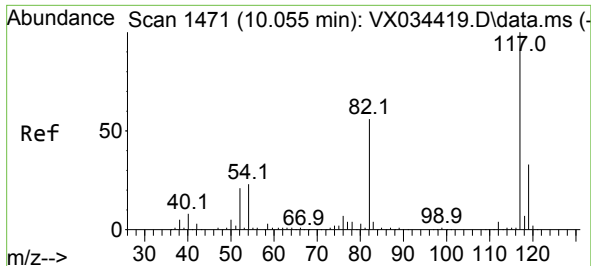

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX034571.D
Acq: 17 Mar 2023 07:59




Instrument :
MSVOA_X
ClientSampleId :
33959


Tgt Ion:117 Resp: 418382
Ion Ratio Lower Upper
117 100
82 57.6 45.0 67.4
119 31.8 26.0 39.0

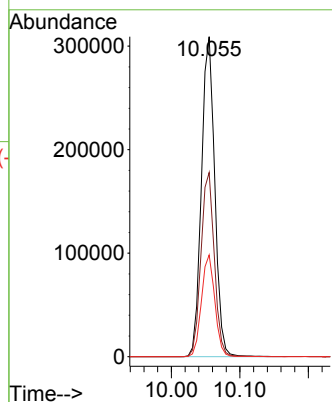

#67
Ethyl Benzene
Concen: 0.626 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX034571.D
Acq: 17 Mar 2023 07:59

Tgt Ion: 91 Resp: 10292
Ion Ratio Lower Upper
91 100
106 32.1 25.6 38.4



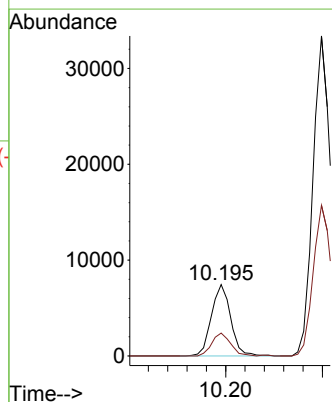



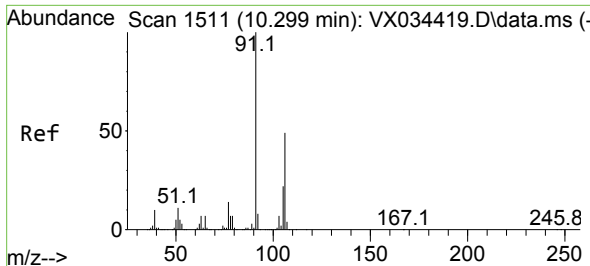

#68
m/p-Xylenes
Concen: 3.379 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. 0.000 min
Lab File: VX034571.D
Acq: 17 Mar 2023 07:59




Instrument :
MSVOA_X
ClientSampleId :
33959


Tgt Ion:106 Resp: 21332
Ion Ratio Lower Upper
106 100
91 209.2 164.0 246.0

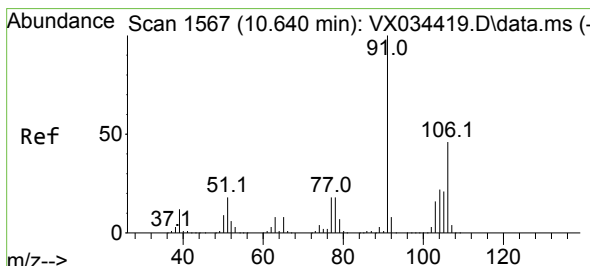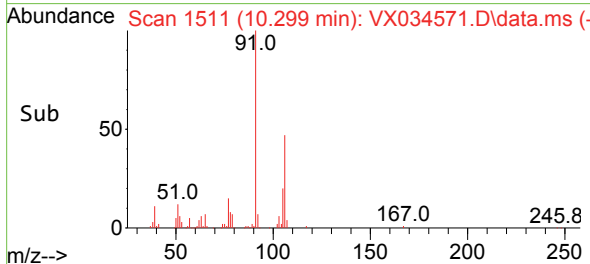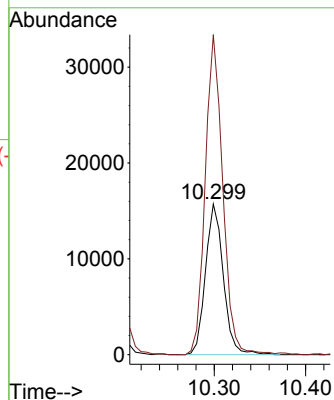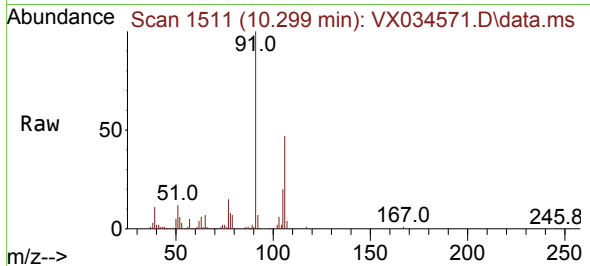

#69
o-Xylene
Concen: 4.794 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. 0.000 min
Lab File: VX034571.D
Acq: 17 Mar 2023 07:59

Tgt Ion:106 Resp: 30371
Ion Ratio Lower Upper
106 100
91 218.4 108.5 325.3

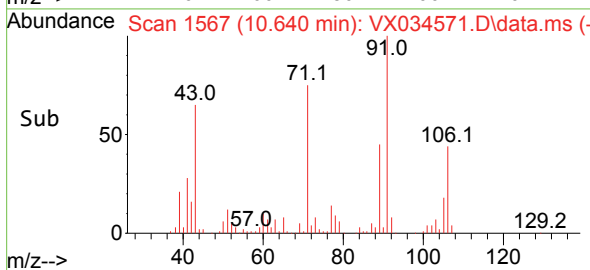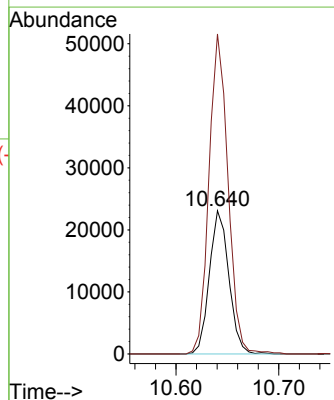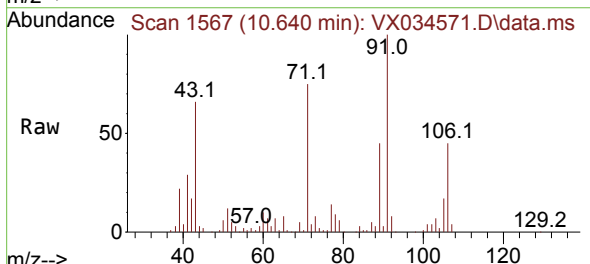



#70

Styrene

Concen: 0.668 ug/l

RT: 10.659 min Scan# 1569

Delta R.T. 0.006 min

Lab File: VX034571.D

Acq: 17 Mar 2023 07:59

Instrument :

MSVOA_X

ClientSampleId :

33959





Tgt Ion:104 Resp: 6824

Ion Ratio Lower Upper

104 100

78 110.8 43.4 65.2#

103 101.4 44.2 66.2#

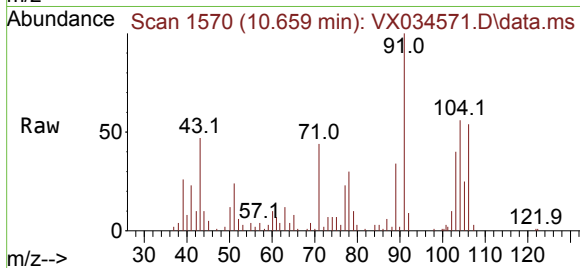

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1794

Delta R.T. 0.000 min

Lab File: VX034571.D

Acq: 17 Mar 2023 07:59




Tgt Ion:152 Resp: 198901


Ion Ratio Lower Upper

152 100

115 61.4 45.0 135.0

150 156.9 0.0 352.4

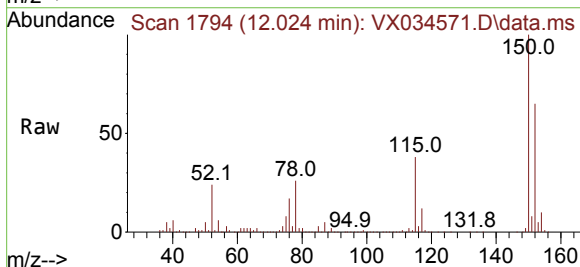



#74

N-amy1 acetate

Concen: 0.574 ug/l

RT: 10.768 min Scan# 1

Delta R.T. -0.073 min

Lab File: VX034571.D

Acq: 17 Mar 2023 07:59

Instrument :

MSVOA_X

ClientSampleId :

33959

Tgt Ion: 43 Resp: 4228





Ion Ratio Lower Upper

43 100

70 0.0 32.1 48.1#

55 30.5 18.3 27.5#

61 0.0 18.8 28.2#

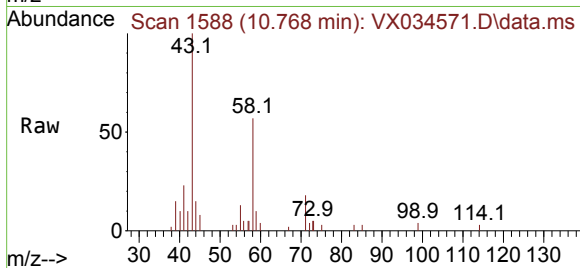

#76

1,2,3-Trichloropropane

Concen: 27.125 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.158 min

Lab File: VX034571.D




Acq: 17 Mar 2023 07:59


Tgt Ion: 75 Resp: 123879

Ion Ratio Lower Upper

75 100

77 1.1 21.6 64.8#




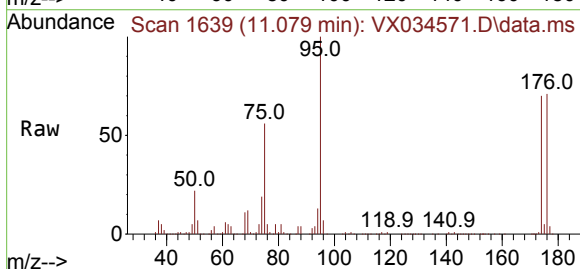


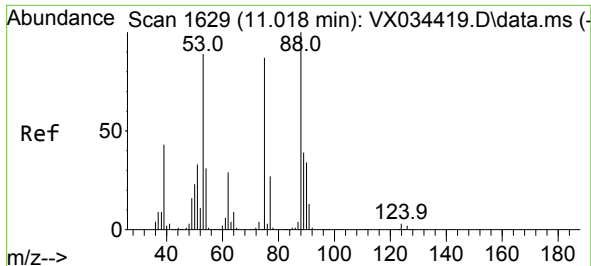

#81
trans-1,4-Dichloro-2-butene
Concen: 73.381 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX034571.D
Acq: 17 Mar 2023 07:59




Instrument :
MSVOA_X
ClientSampleId :
33959


Tgt Ion: 75 Resp: 123879
Ion Ratio Lower Upper
75 100
53 0.0 82.6 124.0#
89 0.0 36.9 55.3#

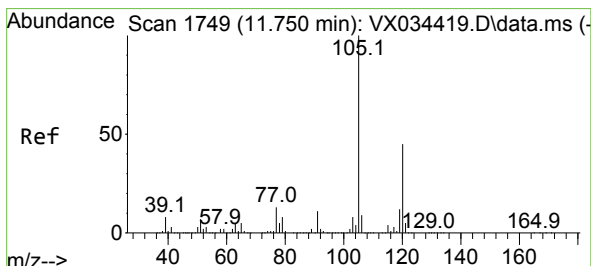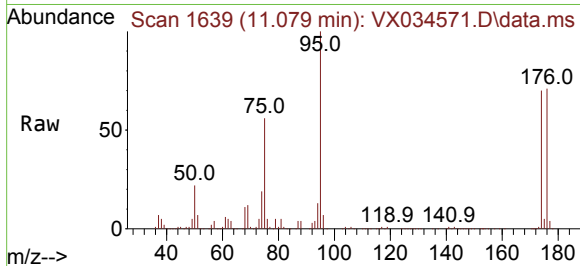

#84
1,2,4-Trimethylbenzene
Concen: 62.655 ug/l
RT: 11.750 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VX034571.D
Acq: 17 Mar 2023 07:59

Tgt Ion: 105 Resp: 825656
Ion Ratio Lower Upper
105 100
120 0.5 22.4 67.0#

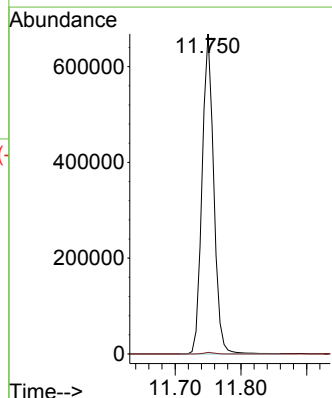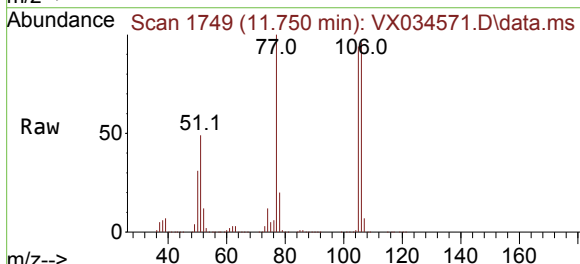



#85

sec-Butylbenzene

Concen: 51.949 ug/l

RT: 11.750 min Scan# 11

Delta R.T. -0.140 min

Lab File: VX034571.D

Acq: 17 Mar 2023 07:59

Instrument :

MSVOA_X

ClientSampleId :





33959

Tgt Ion:105 Resp: 825656

Ion Ratio Lower Upper

105 100

134 0.0 10.2 30.4#



#95

Naphthalene

Concen: 17.054 ug/l

RT: 13.774 min Scan# 2081

Delta R.T. 0.000 min

Lab File: VX034571.D

Acq: 17 Mar 2023 07:59

Tgt Ion:128 Resp: 249756

Ion Ratio Lower Upper

128 100

127 12.8 10.2 15.4

129 11.2 8.6 13.0

