

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031623\
 Data File : VX034533.D
 Acq On : 16 Mar 2023 10:16
 Operator : JC/MD
 Sample : VX0316MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0316MBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M

Title : SW846 8260

Signal : TIC: VX034533.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.569	70	79	82	rBV3	10870	23791	1.56%	0.290%
2	5.385	694	705	719	rBV	170335	495889	32.48%	6.041%
3	5.550	721	732	750	rVB	289657	827456	54.20%	10.080%
4	5.952	786	798	819	rBV	198961	536311	35.13%	6.534%
5	6.757	920	930	946	rBV	463402	1113053	72.91%	13.560%
6	8.647	1233	1240	1250	rBV	1001716	1526534	100.00%	18.597%
7	10.049	1465	1470	1483	rBV	1005908	1408336	92.26%	17.157%
8	11.079	1633	1639	1650	rBV	852842	1090392	71.43%	13.284%
9	12.018	1788	1793	1805	rBV	888234	1161930	76.12%	14.155%
10	13.725	2068	2073	2077	rBV2	19545	24922	1.63%	0.304%




Sum of corrected areas: 8208614

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031623\
Data File : VX034533.D
Acq On : 16 Mar 2023 10:16
Operator : JC/MD
Sample : VX0316MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0316MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

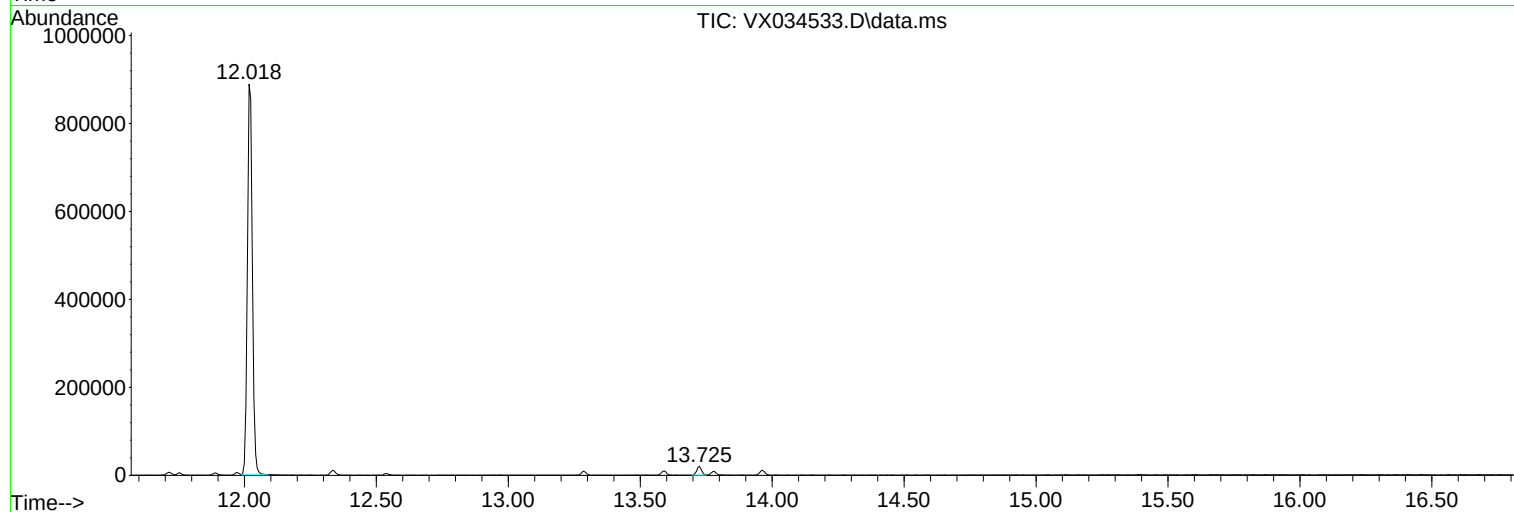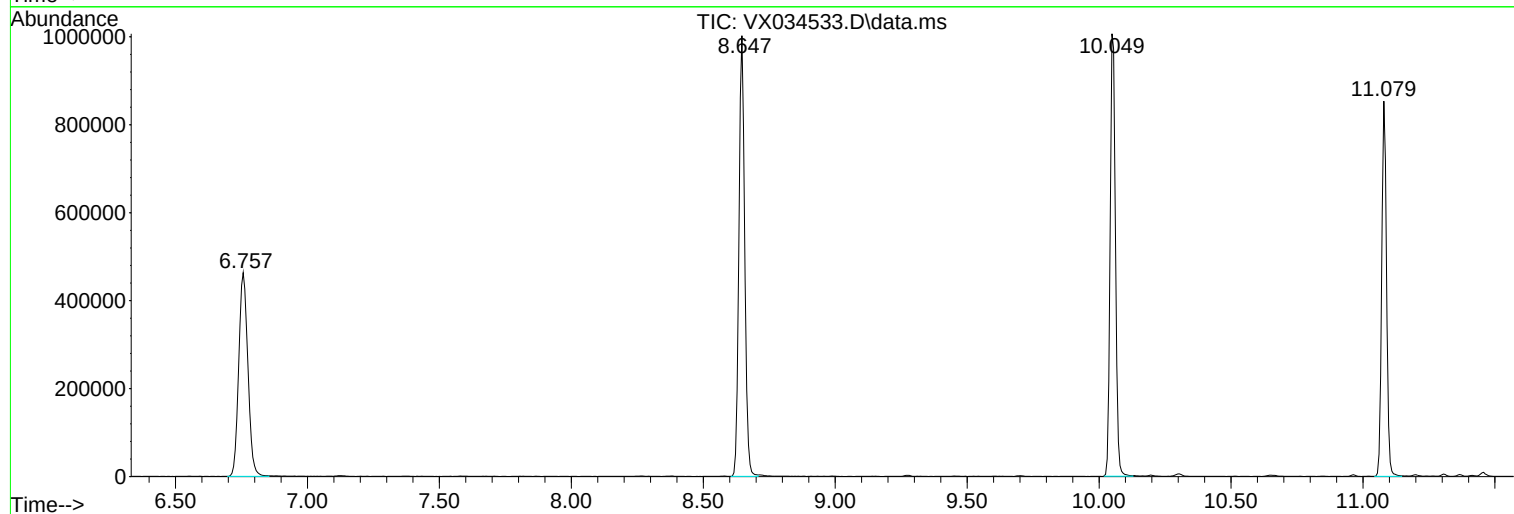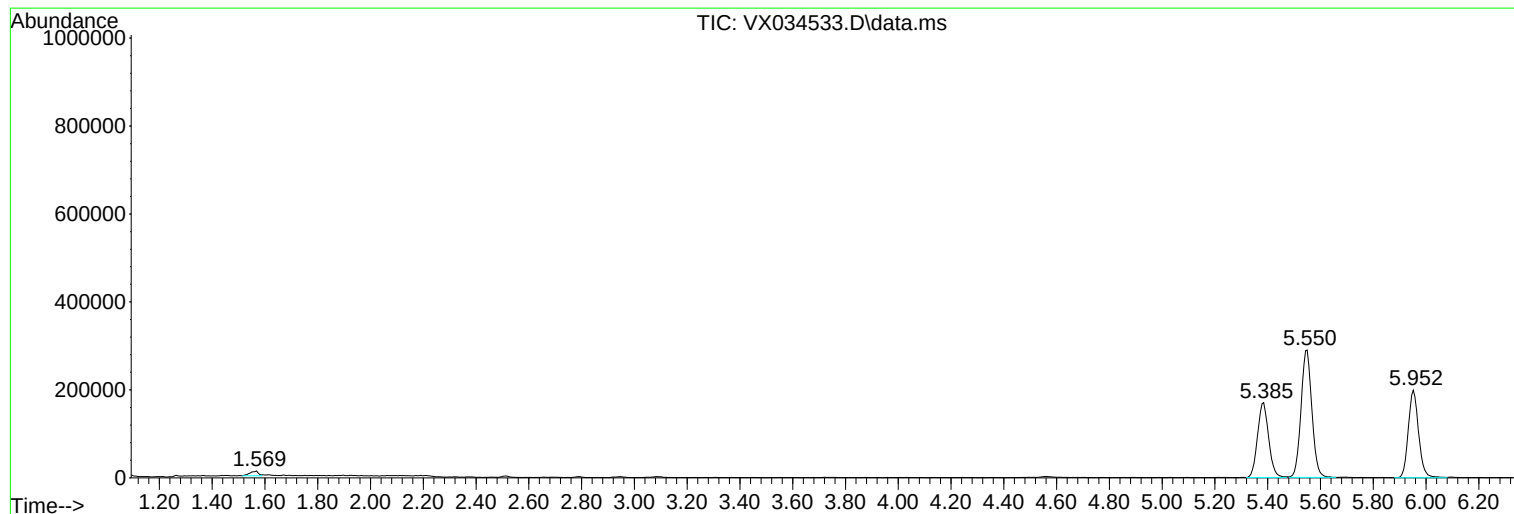

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031623\
Data File : VX034533.D
Acq On : 16 Mar 2023 10:16
Operator : JC/MD
Sample : VX0316MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0316MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031623\
Data File : VX034533.D
Acq On : 16 Mar 2023 10:16
Operator : JC/MD
Sample : VX0316MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0316MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc