

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX031720\
 Data File : VX015313.D
 Acq On : 17 Mar 2020 10:44
 Operator : JC/SP
 Sample : L1919-01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-SOIL-REF-6

Quant Time: Mar 18 01:18:07 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X030420W.M
 Quant Title : SW846 8260
 QLast Update : Wed Mar 04 14:19:10 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.65	168	314359	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	505526	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	483068	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.07	152	234057	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.05	65	181510	48.67	ug/l	0.00
Spiked Amount			Recovery	=	97.34%	
35) Dibromofluoromethane	5.50	113	157237	49.30	ug/l	0.00
Spiked Amount			Recovery	=	98.60%	
50) Toluene-d8	8.71	98	612674	50.50	ug/l	0.00
Spiked Amount			Recovery	=	101.00%	
62) 4-Bromofluorobenzene	11.13	95	218731	50.55	ug/l	0.00
Spiked Amount			Recovery	=	101.10%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Chloromethane	1.32	50	1142	0.293	ug/l	95
5) Bromomethane	1.65	94	989	0.407	ug/l	87
9) 1,1,2-Trichlorotrifluoroet	2.38	101	658	0.222	ug/l #	66
10) Methyl Iodide	2.51	142	1483	0.443	ug/l #	73
11) Tert butyl alcohol	3.05	59	144	0.223	ug/l #	1
13) Acrolein	2.26	56	268	0.441	ug/l #	15
15) Acrylonitrile	3.14	53	718	0.446	ug/l #	86
16) Acetone	2.44	43	2544	1.684	ug/l #	87
17) Carbon Disulfide	2.56	76	2703	0.319	ug/l #	77
20) Methylene Chloride	2.86	84	895	0.253	ug/l #	61
21) trans-1,2-Dichloroethene	3.16	96	910	0.279	ug/l #	20
28) Bromochloromethane	4.98	49	569	0.212	ug/l #	72
36) 1,1-Dichloropropene	5.80	75	953	0.204	ug/l #	57
38) Carbon Tetrachloride	5.65	117	28172	6.386	ug/l #	18
44) Trichloroethene	7.21	130	1049	0.272	ug/l	97
49) 1,4-Dioxane	7.75	88	86	1.025	ug/l #	1
76) 1,2,3-Trichloropropane	11.13	75	104839	22.456	ug/l #	34
81) trans-1,4-Dichloro-2-buten	11.13	75	104839	63.729	ug/l #	11
87) 1,3-Dichlorobenzene	12.02	146	1784	0.244	ug/l	94
88) 1,4-Dichlorobenzene	12.02	146	1784	0.236	ug/l	95
89) n-Butylbenzene	12.39	91	2637	0.222	ug/l	90
93) 1,2,4-Trichlorobenzene	13.64	180	1879	0.372	ug/l	89
94) Hexachlorobutadiene	13.78	225	928	0.358	ug/l	77
95) Naphthalene	13.83	128	3225	1.622	ug/l #	76
96) 1,2,3-Trichlorobenzene	14.01	180	1996	0.396	ug/l	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX031720\
Data File : VX015313.D
Acq On : 17 Mar 2020 10:44
Operator : JC/SP
Sample : L1919-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6

Quant Time: Mar 18 01:18:07 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X030420W.M
Quant Title : SW846 8260
QLast Update : Wed Mar 04 14:19:10 2020
Response via : Initial Calibration

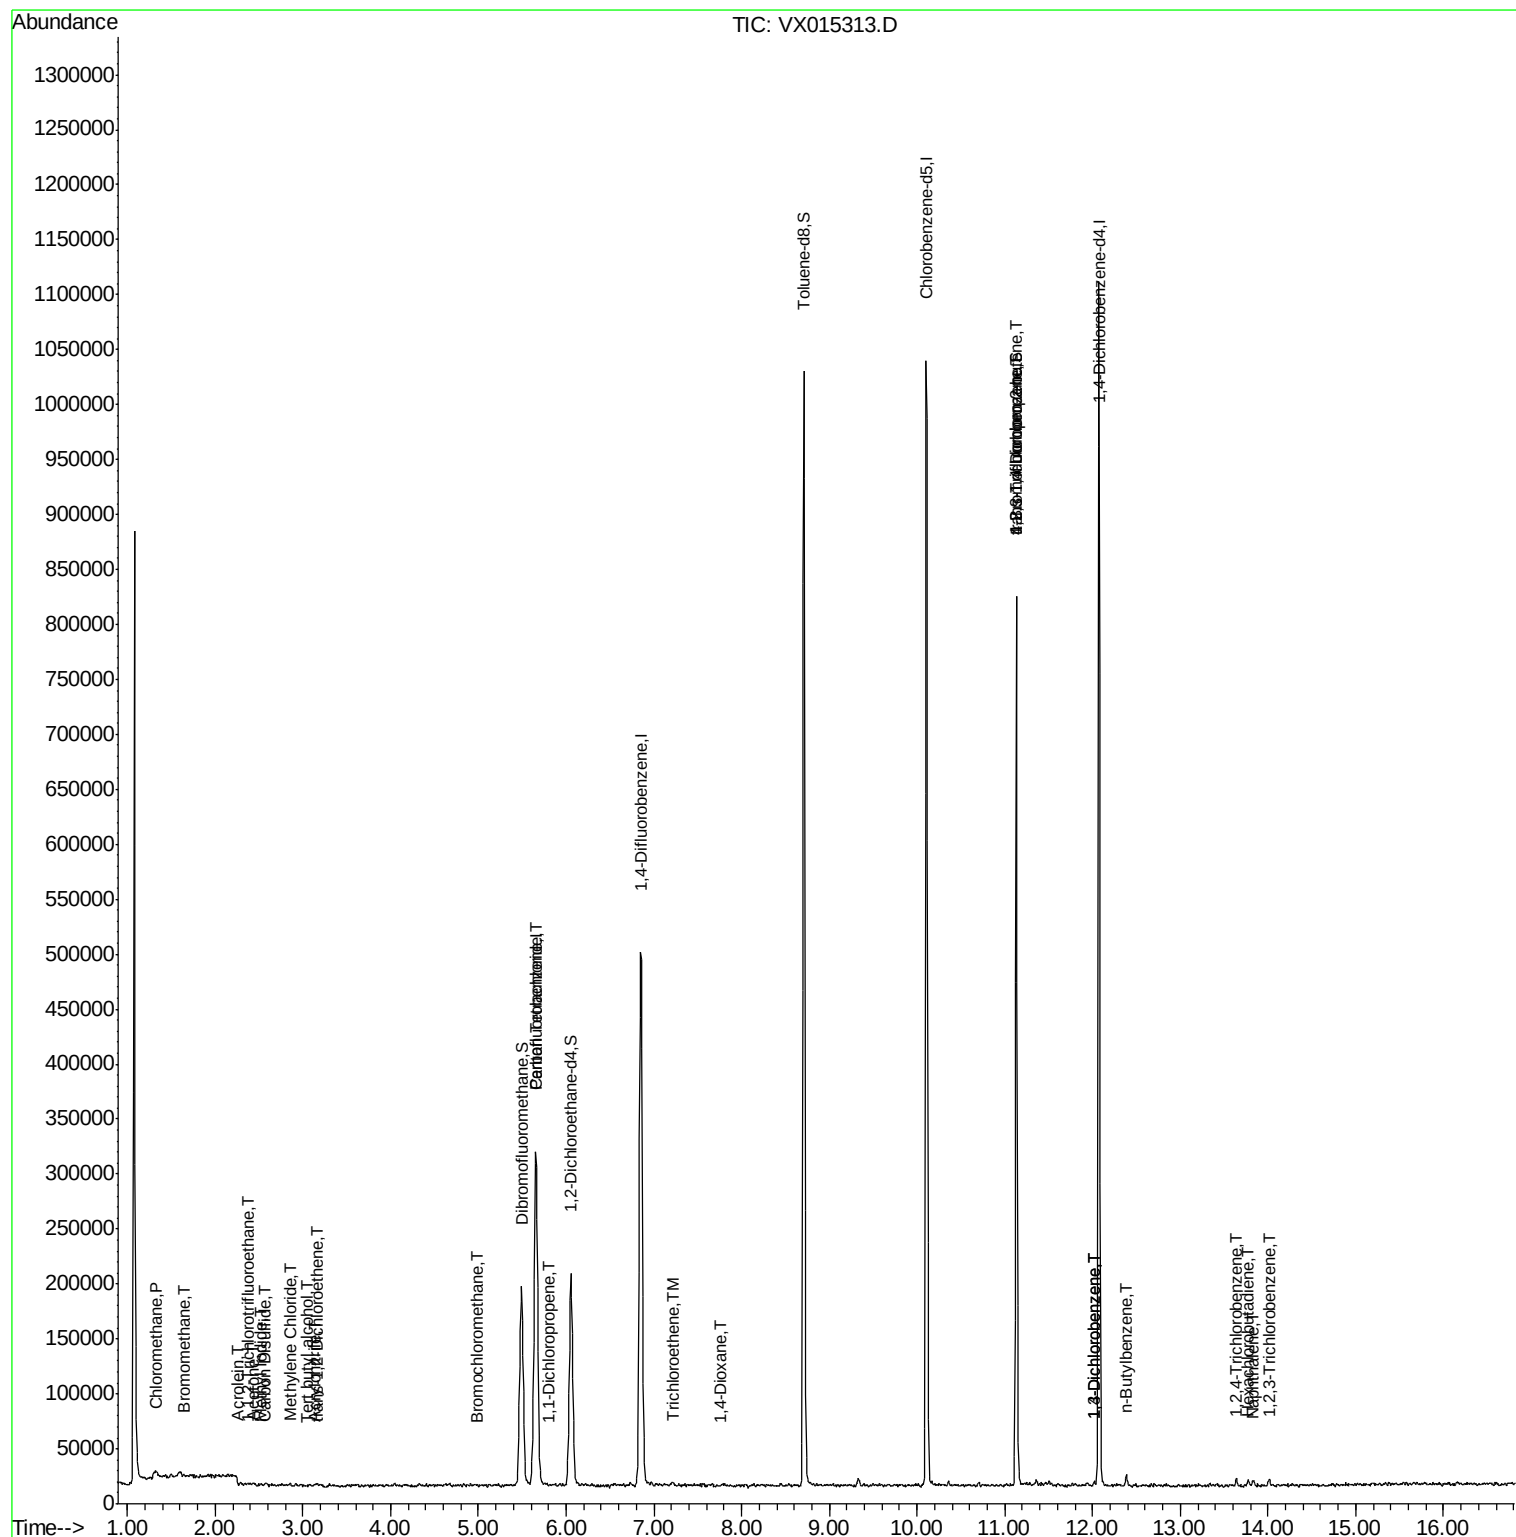

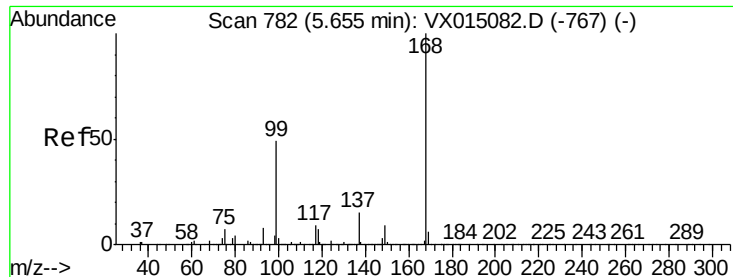


#1




Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.65 min Scan# 782
Delta R.T. 0.00 min
Lab File: VX015313.D
Acq: 17 Mar 2020 10:44

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6

Tot Ion:168 Resp: 314359
Ion Ratio Lower Upper
168 100
99 50.5 39.4 59.2

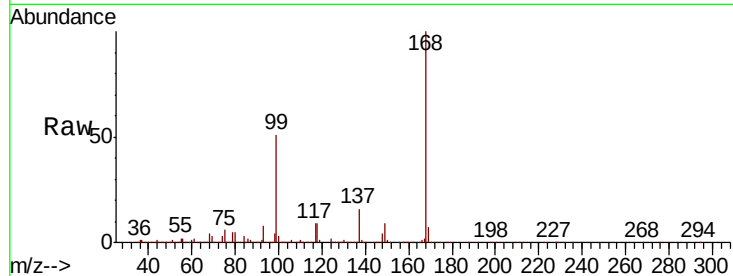


Abundance Ion 167.90 (167.60 to 168.60): V
Ion 98.90 (98.60 to 99.60): VX0

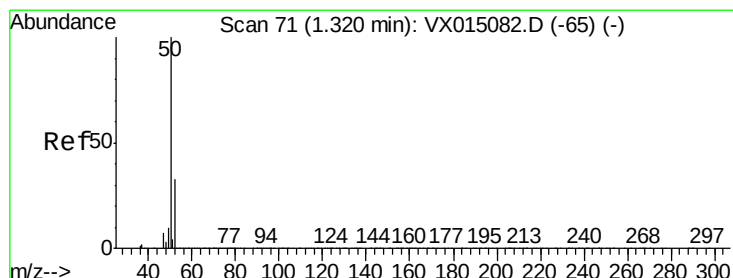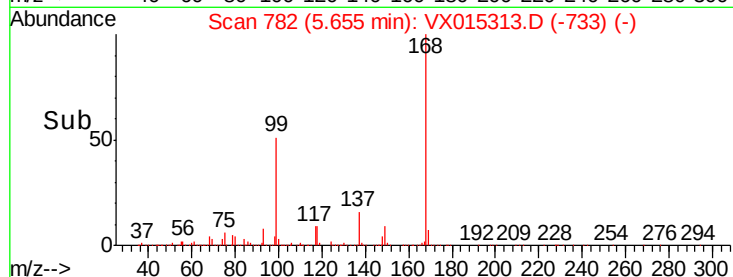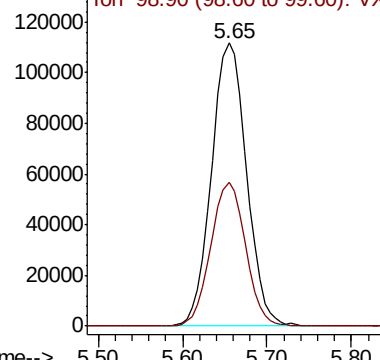



#3


Chloromethane
Concen: 0.293 ug/l
RT: 1.32 min Scan# 71
Delta R.T. 0.00 min
Lab File: VX015313.D
Acq: 17 Mar 2020 10:44

Tgt Ion: 50 Resp: 1142
Ion Ratio Lower Upper
50 100
52 29.7 26.2 39.2

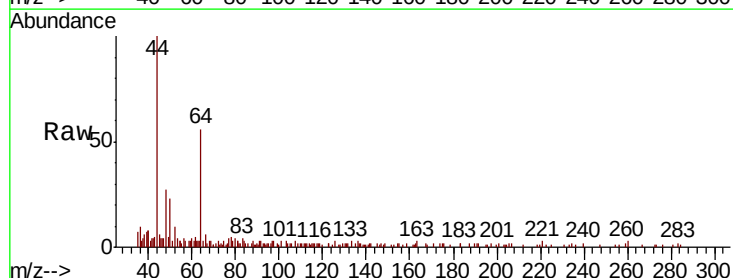

Abundance Ion 49.90 (49.60 to 50.60): VX0
Ion 51.90 (51.60 to 52.60): VX0

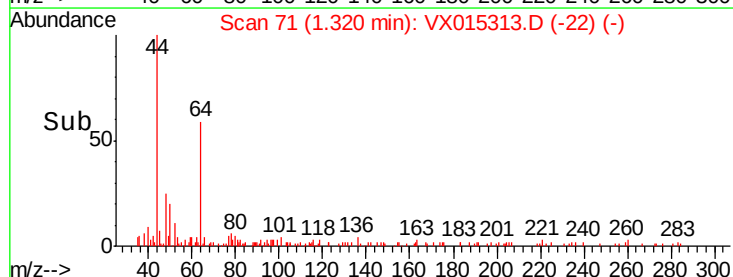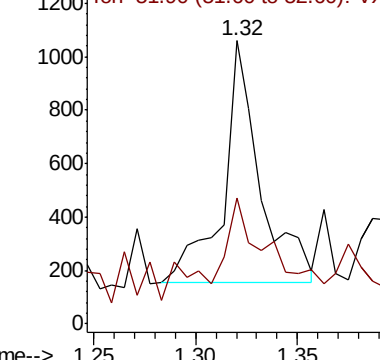



#5

Bromomethane

Concen: 0.407 ug/l

RT: 1.65 min Scan# 125

Delta R.T. 0.01 min

Lab File: VX015313.D

Acq: 17 Mar 2020 10:44

Instrument :

MSVOA_X

ClientSampleId :





STORAGE-BLANK-SOIL-REF-6

Tot Ion: 94 Resp: 989

Ion Ratio Lower Upper

94 100

96 81.2 74.6 111.8

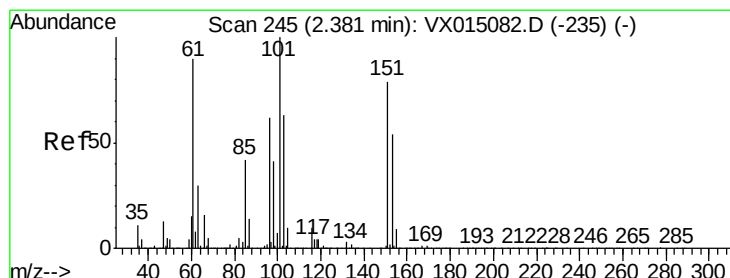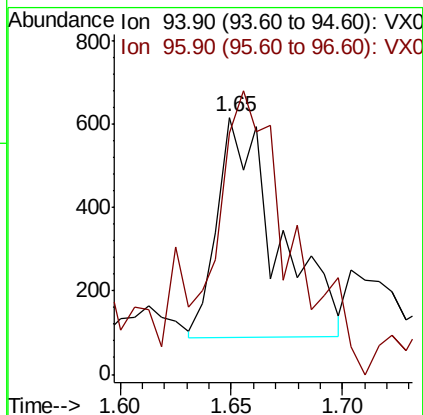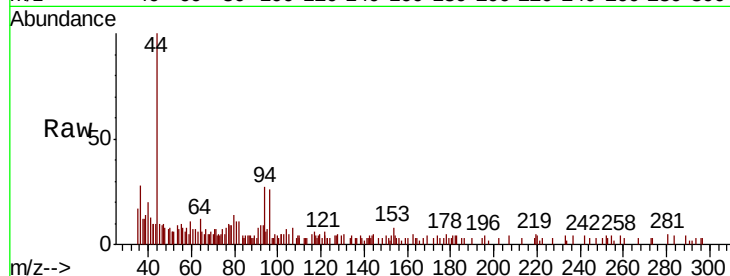

#9

1,1,2-Trichlorotrifluoroethane

Concen: 0.222 ug/l

RT: 2.38 min Scan# 245

Delta R.T. 0.00 min

Lab File: VX015313.D

Acq: 17 Mar 2020 10:44




Tgt Ion:101 Resp: 658


Ion Ratio Lower Upper

101 100

85 47.9 33.7 50.5

151 37.8 64.0 96.0#



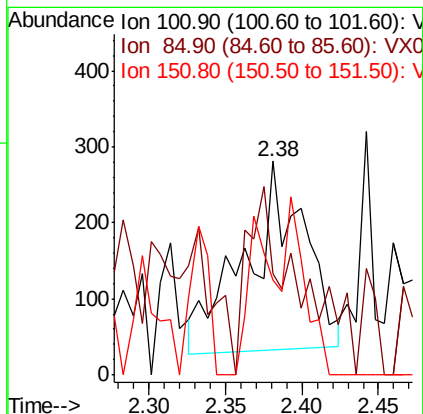
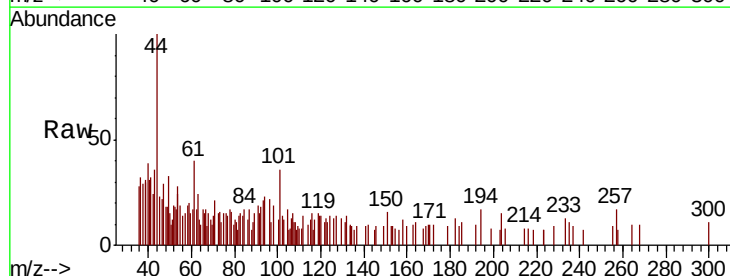




#10
Methvl Iodide
Concen: 0.443 ug/l
RT: 2.51 min Scan# 267
Delta R.T. 0.01 min
Lab File: VX015313.D
Acq: 17 Mar 2020 10:44




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6


Tot Ion:142 Resp: 1483
Ion Ratio Lower Upper
142 100
127 60.6 31.7 47.5#
141 16.3 11.3 16.9

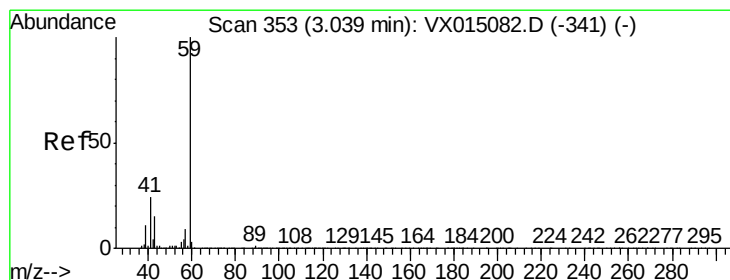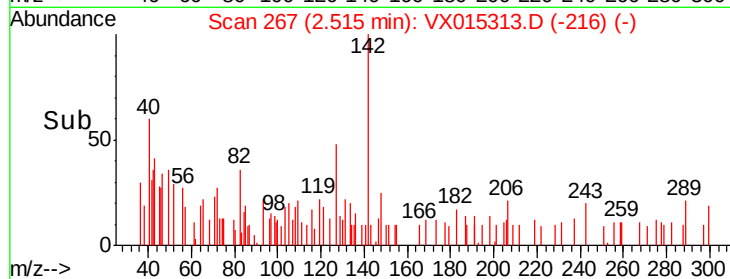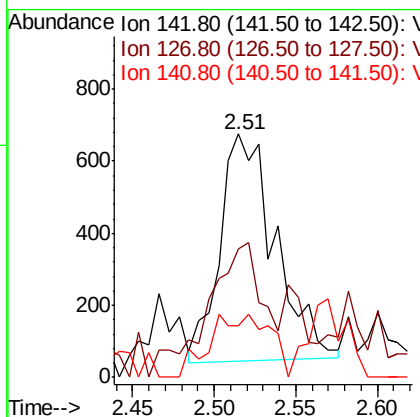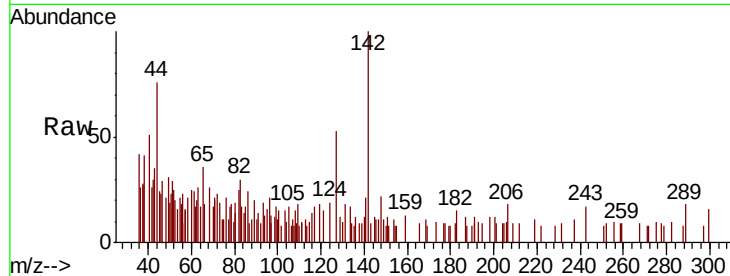

#11
Tert butyl alcohol
Concen: 0.223 ug/l
RT: 3.05 min Scan# 354
Delta R.T. 0.01 min
Lab File: VX015313.D
Acq: 17 Mar 2020 10:44

Tgt Ion: 59 Resp: 144
Ion Ratio Lower Upper
59 100
57 231.9 8.2 12.4#

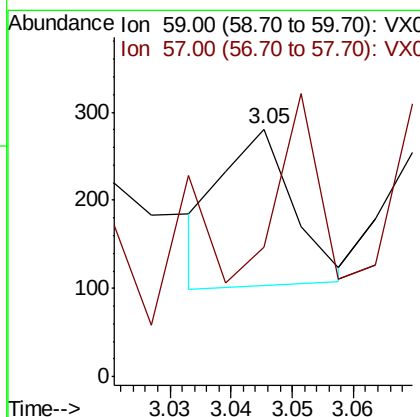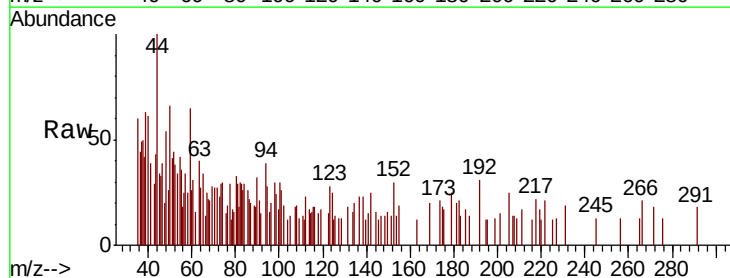



#13

Acrolein

Concen: 0.441 ug/l

RT: 2.26 min Scan# 225

Delta R.T. -0.02 min

Lab File: VX015313.D

Acq: 17 Mar 2020 10:44

Instrument :

MSVOA_X

ClientSampleId :





STORAGE-BLANK-SOIL-REF-6

Tot Ion: 56 Resp: 268

Ion Ratio Lower Upper

56 100

55 0.0 55.4 83.0#

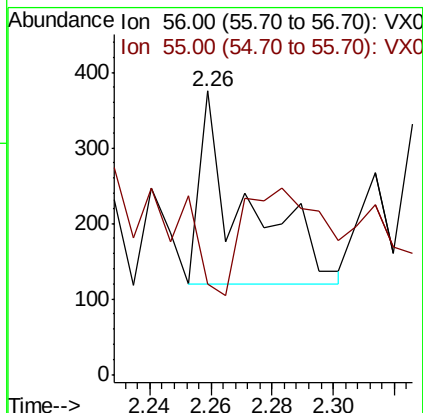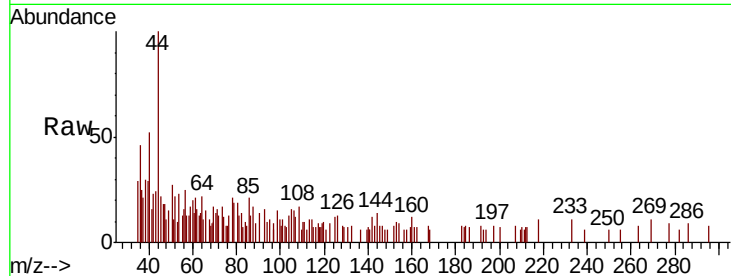

#15

Acrylonitrile

Concen: 0.446 ug/l

RT: 3.14 min Scan# 369

Delta R.T. 0.01 min

Lab File: VX015313.D

Acq: 17 Mar 2020 10:44




Tgt Ion: 53 Resp: 718


Ion Ratio Lower Upper

53 100

52 84.7 66.6 100.0

51 61.8 29.0 43.6#

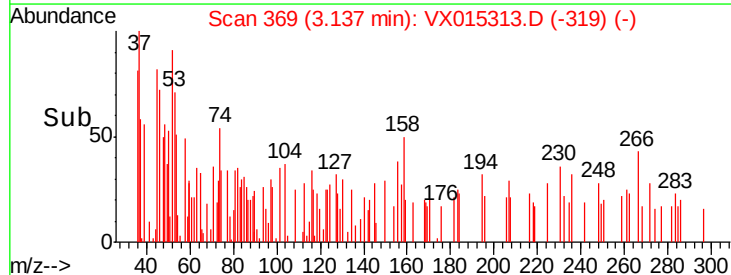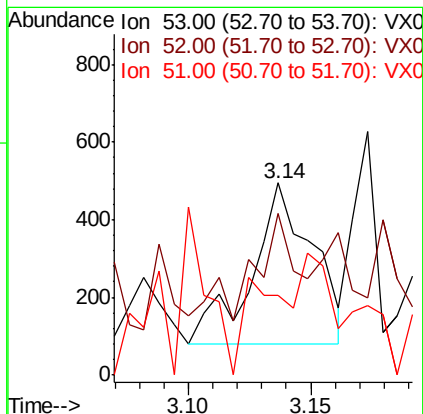

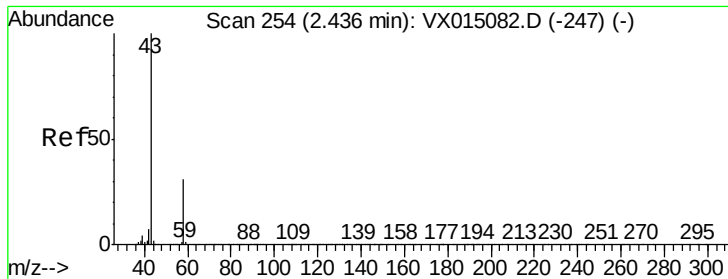

#16

Acetone

Concen: 1.684 ug/l

RT: 2.44 min Scan# 254

Delta R.T. 0.00 min

Lab File: VX015313.D

Acq: 17 Mar 2020 10:44

Instrument :

MSVOA_X

ClientSampleId :


STORAGE-BLANK-SOIL-REF-6

Tot Ion: 43 Resp: 2544

Ion Ratio Lower Upper




43 100

58 23.6 24.8 37.2#

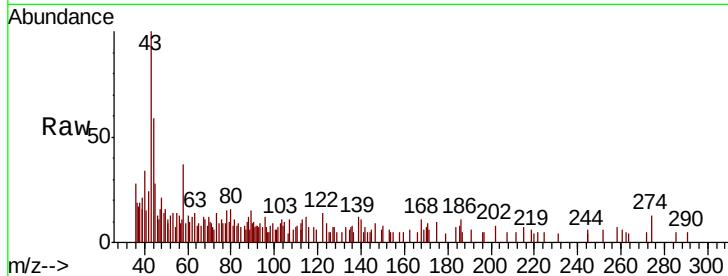

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

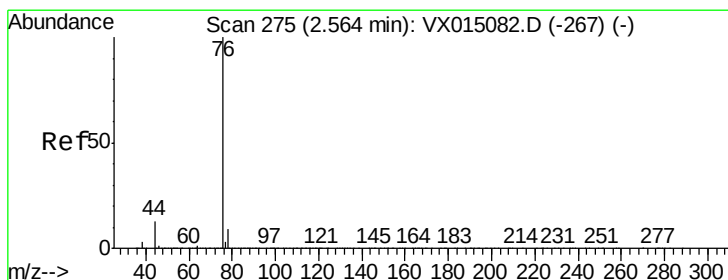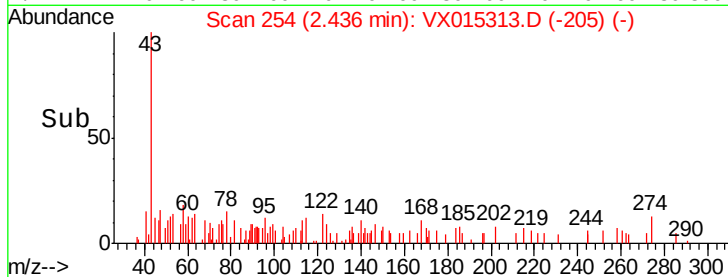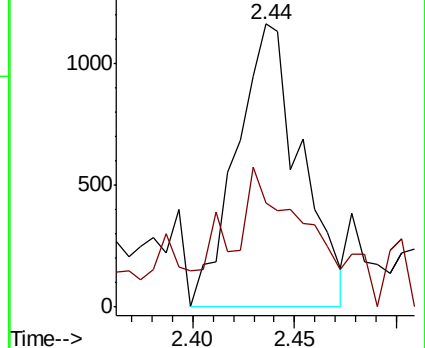

#17

Carbon Disulfide

Concen: 0.319 ug/l

RT: 2.56 min Scan# 275

Delta R.T. 0.00 min

Lab File: VX015313.D


Acq: 17 Mar 2020 10:44

Tgt Ion: 76 Resp: 2703

Ion Ratio Lower Upper



76 100


78 0.8 7.3 10.9#

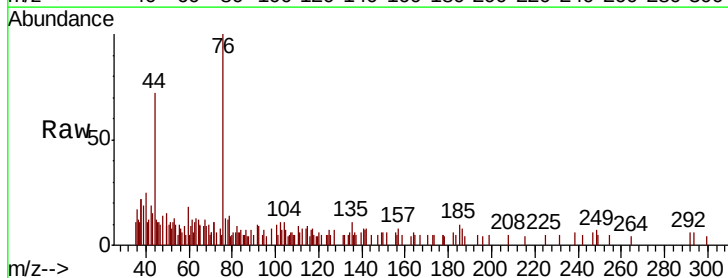

Abundance Ion 75.90 (75.60 to 76.60): VX0

Ion 77.90 (77.60 to 78.60): VX0

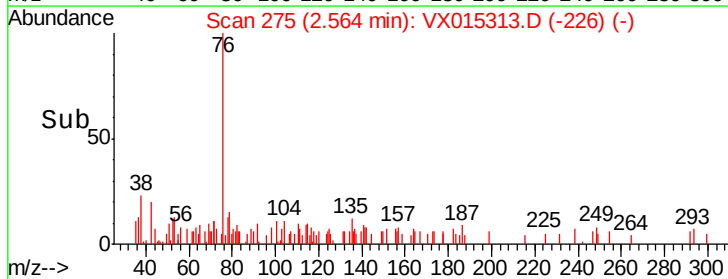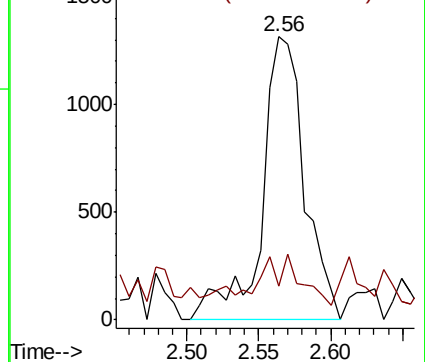

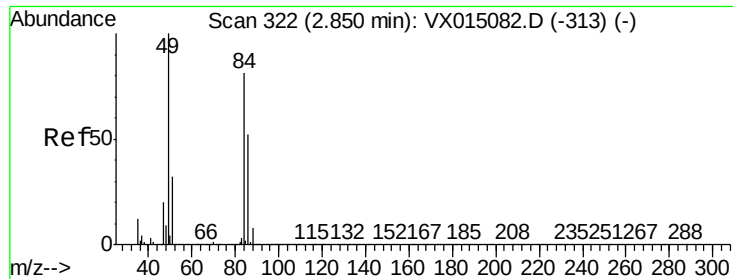

#20

Methylene Chloride

Concen: 0.253 ug/l

RT: 2.86 min Scan# 323





Delta R.T. 0.01 min

Lab File: VX015313.D

Acq: 17 Mar 2020 10:44

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6

Tot Ion:	84	Resp:	895
Ion	Ratio	Lower	Upper
84	100		
49	71.8	99.4	149.2#
51	22.1	31.5	47.3#
86	89.9	51.6	77.4#

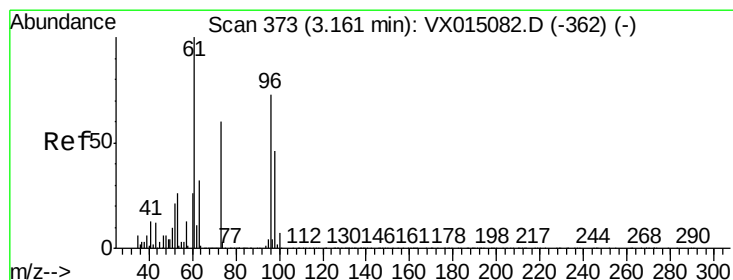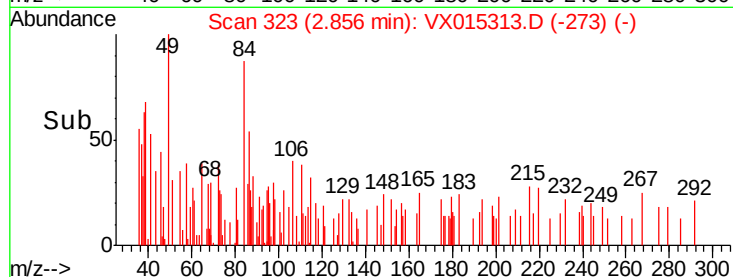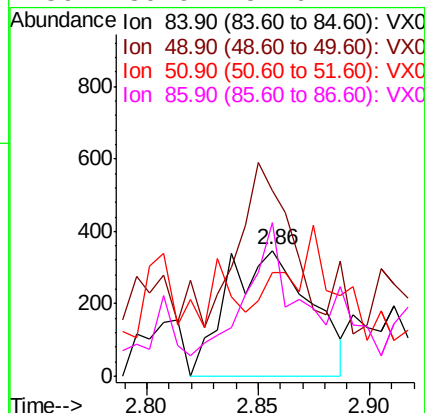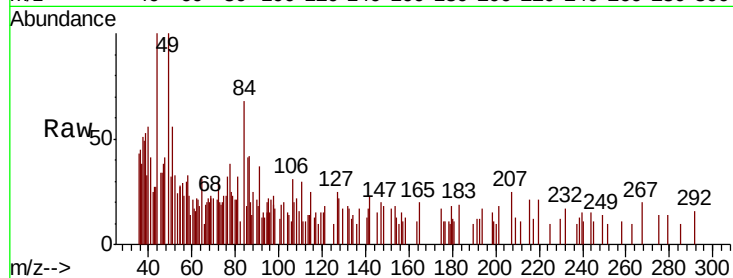

#21

trans-1,2-Dichloroethene

Concen: 0.279 ug/l




RT: 3.16 min Scan# 373


Delta R.T. 0.00 min

Lab File: VX015313.D

Acq: 17 Mar 2020 10:44

Tgt Ion:	96	Resp:	910
Ion	Ratio	Lower	Upper
96	100		
61	36.5	109.9	164.9#
98	118.4	50.2	75.2#


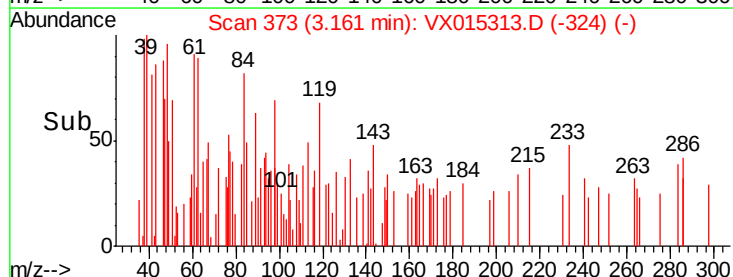
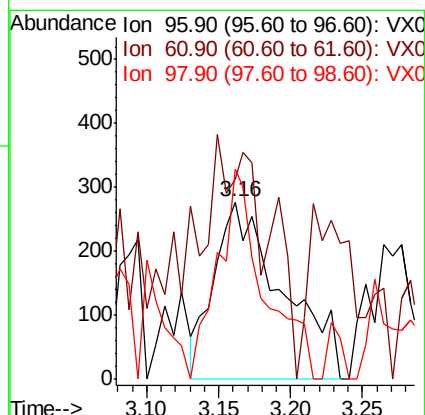
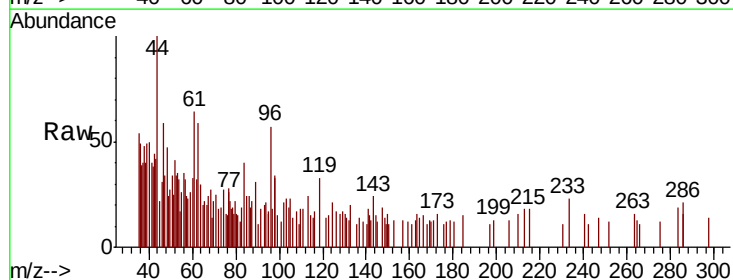


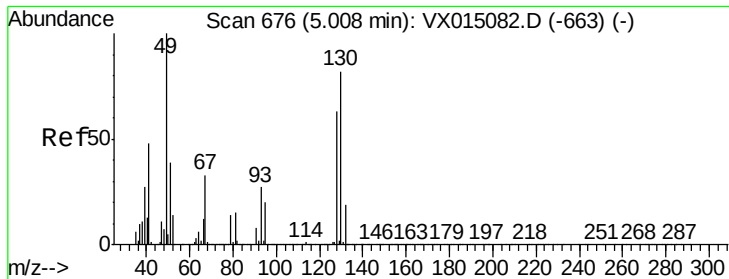

#28
Bromochloromethane
Concen: 0.212 ug/l
RT: 4.98 min Scan# 672
Delta R.T. -0.02 min
Lab File: VX015313.D
Acq: 17 Mar 2020 10:44




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6


Tot Ion: 49 Resp: 569
Ion Ratio Lower Upper
49 100
129 20.9 0.0 4.4#
130 56.9 65.0 97.6#

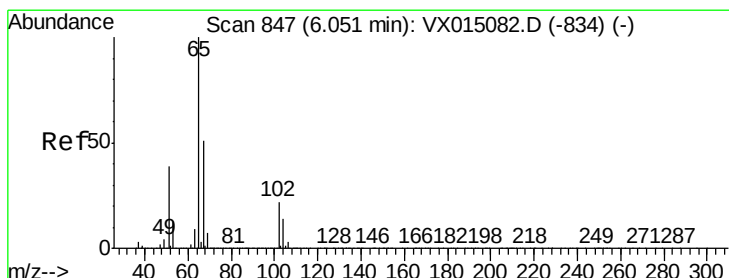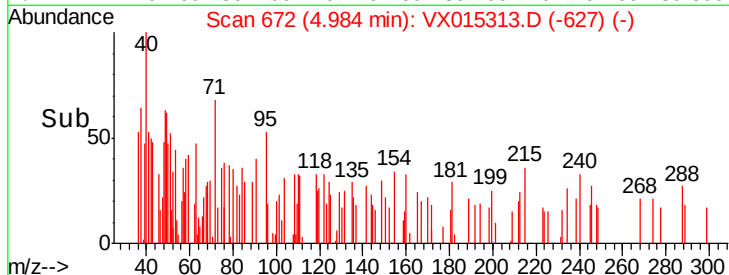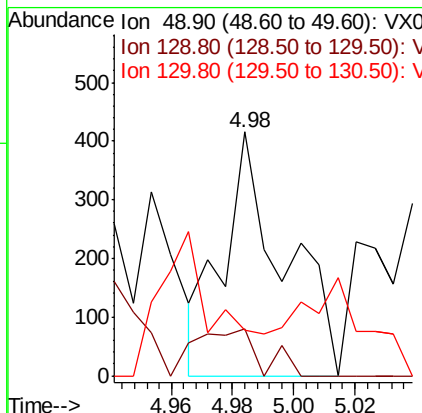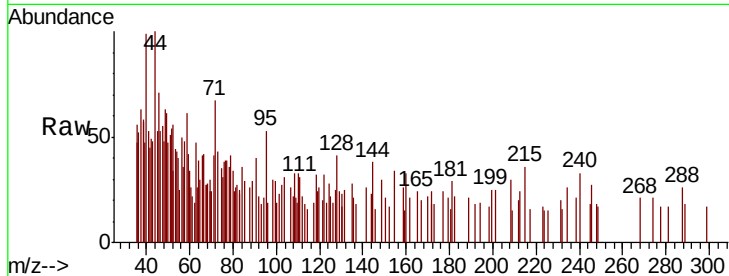

#33
1,2-Dichloroethane-d4
Concen: 48.669 ug/l
RT: 6.05 min Scan# 847
Delta R.T. 0.00 min
Lab File: VX015313.D
Acq: 17 Mar 2020 10:44

Tgt Ion: 65 Resp: 181510
Ion Ratio Lower Upper
65 100
67 53.8 0.0 105.6

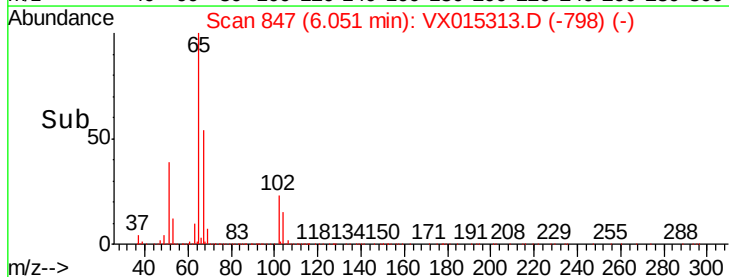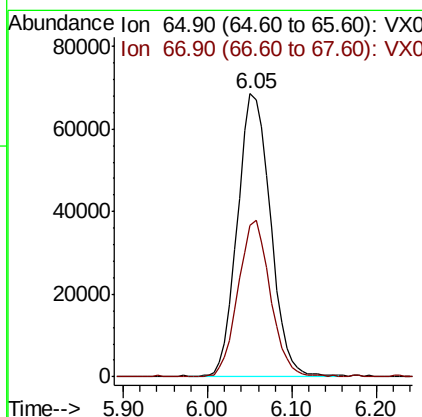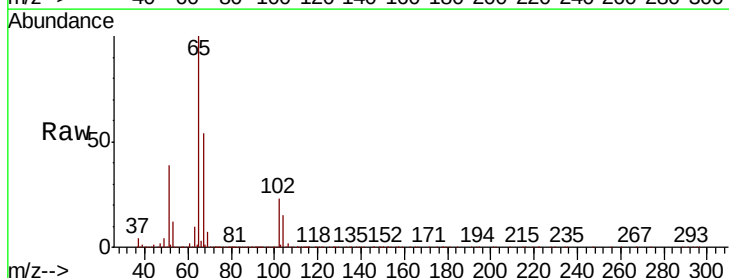



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.86 min Scan# 979

Delta R.T. 0.01 min

Lab File: VX015313.D

Acq: 17 Mar 2020 10:44

Instrument :

MSVOA_X

ClientSampleId :

STORAGE-BLANK-SOIL-REF-6


Tot Ion:114 Resp: 505526

Ion Ratio Lower Upper

114 100

63 20.1 0.0 40.0




88 15.4 0.0 30.6

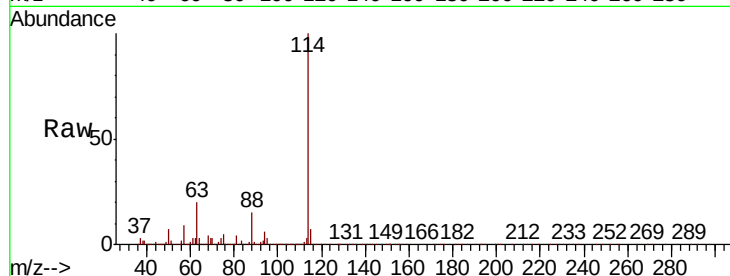

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

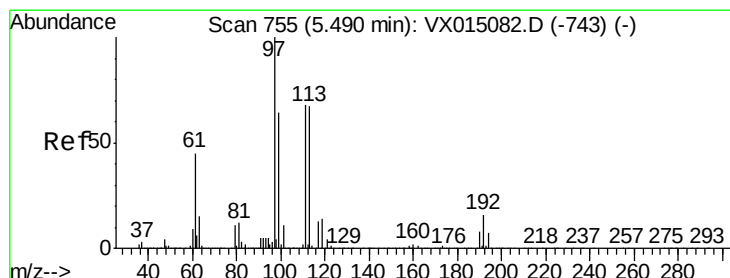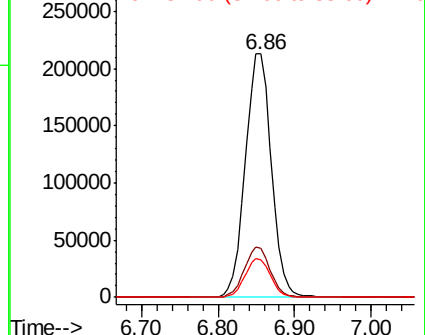

#35

Dibromofluoromethane

Concen: 49.303 ug/l

RT: 5.50 min Scan# 756

Delta R.T. 0.01 min

Lab File: VX015313.D

Acq: 17 Mar 2020 10:44


Tgt Ion:113 Resp: 157237

Ion Ratio Lower Upper

113 100

111 103.0 82.6 123.8



192 24.1 18.6 28.0

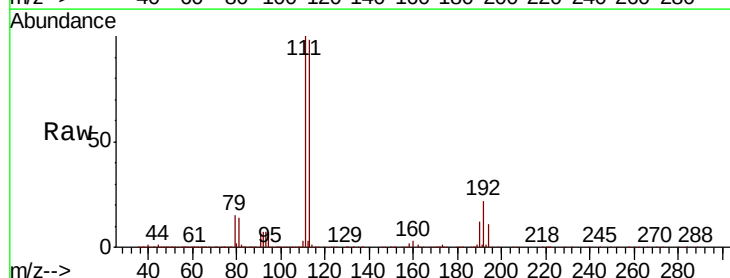


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V




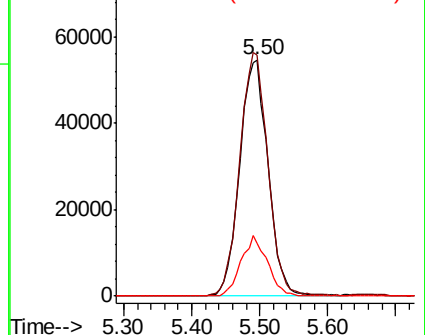




#36
 1,1-Dichloropropene
 Concen: 0.204 ug/l
 RT: 5.80 min Scan# 806
 Delta R.T. 0.01 min
 Lab File: VX015313.D
 Acq: 17 Mar 2020 10:44




Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-SOIL-REF-6


Tot Ion	Ratio	Lower	Upper
75	100		
110	0.0	17.9	53.8#
77	42.8	24.8	37.2#

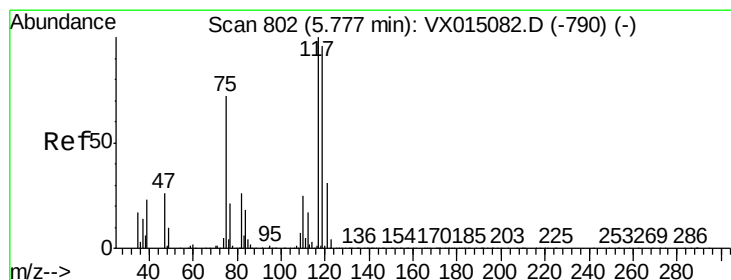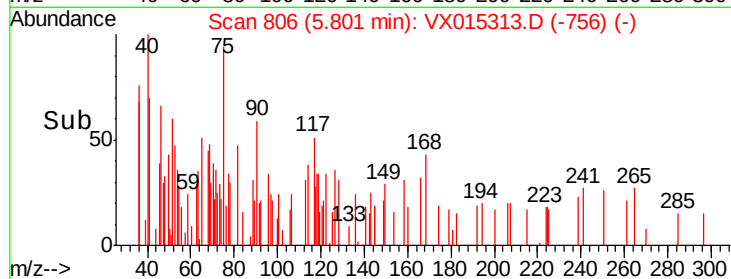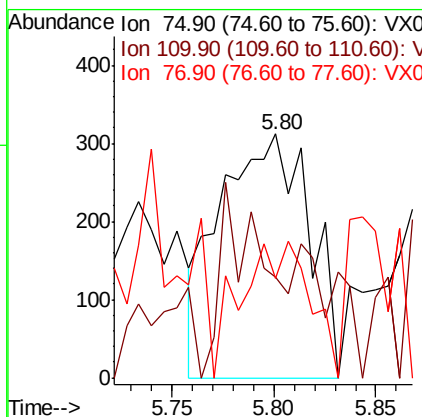

#38
 Carbon Tetrachloride
 Concen: 6.386 ug/l
 RT: 5.65 min Scan# 781
 Delta R.T. -0.13 min
 Lab File: VX015313.D
 Acq: 17 Mar 2020 10:44

Tgt Ion	Ratio	Lower	Upper
117	100		
119	7.8	76.9	115.3#
121	0.0	24.6	37.0#

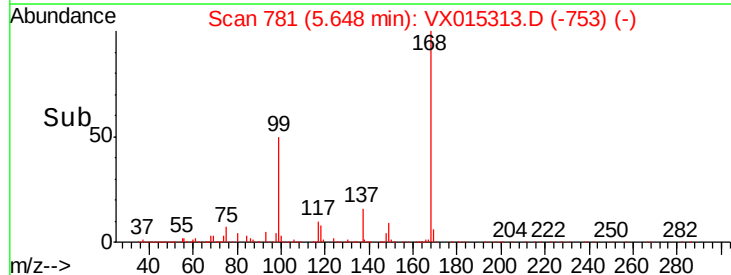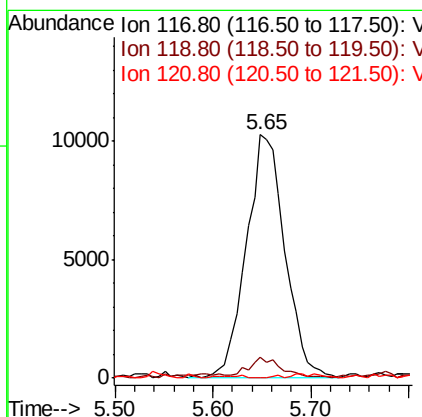

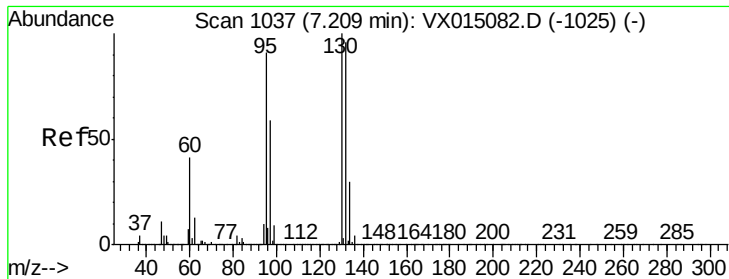

#44

Trichloroethene

Concen: 0.272 ug/l

RT: 7.21 min Scan# 1037

Delta R.T. 0.00 min

Lab File: VX015313.D

Acq: 17 Mar 2020 10:44

Instrument :

MSVOA_X

ClientSampleId :


STORAGE-BLANK-SOIL-REF-6

Tot Ion:130 Resp: 1049

Ion Ratio Lower Upper

130 100

95 87.5 0.0 181.2

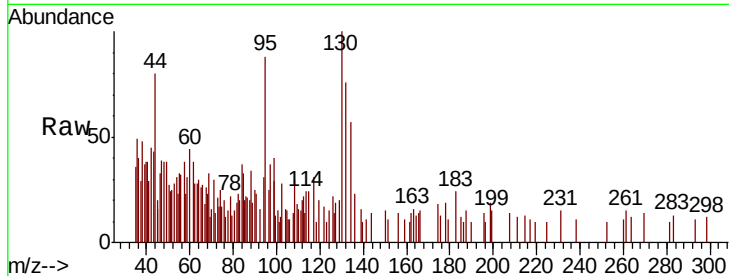

Abundance Ion 129.80 (129.50 to 130.50): V

Ion 94.90 (94.60 to 95.60): VX0

600

500

400

300


200

100


0

7.15 7.20 7.25

7.21

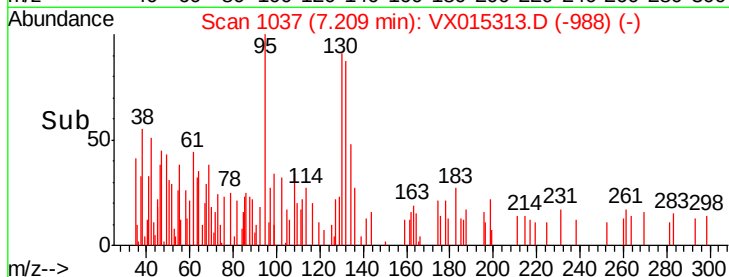

Time-->

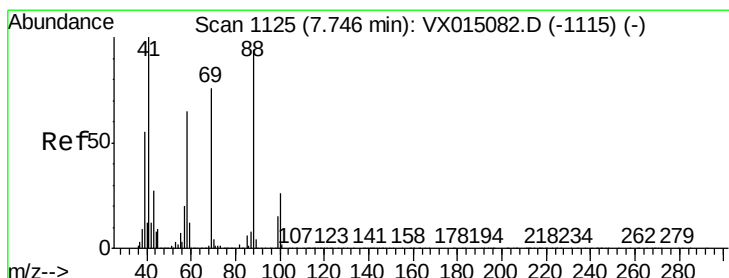

#49

1,4-Dioxane

Concen: 1.025 ug/l

RT: 7.75 min Scan# 1125

Delta R.T. 0.00 min

Lab File: VX015313.D

Acq: 17 Mar 2020 10:44


Tgt Ion: 88 Resp: 86

Ion Ratio Lower Upper

88 100

43 453.5 27.0 40.4#

58 383.7 55.6 83.4#

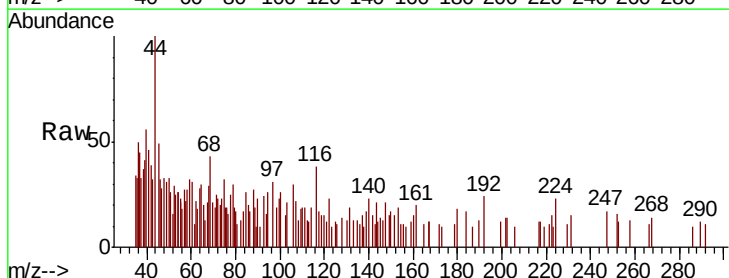

Abundance Ion 88.00 (87.70 to 88.70): VX0

Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

400

300


200

100


0

7.73 7.74 7.75

7.75

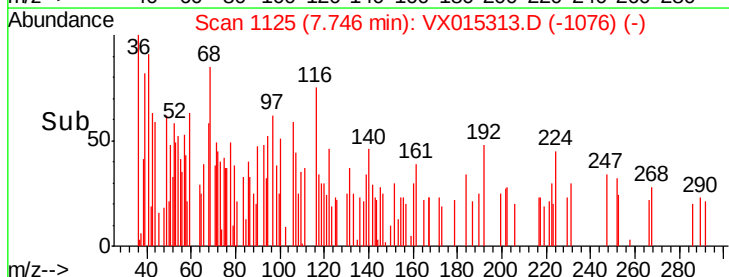

Time-->



#50

Toluene-d8

Concen: 50.504 ug/l

RT: 8.71 min Scan# 1283

Delta R.T. 0.00 min

Lab File: VX015313.D

Acq: 17 Mar 2020 10:44

Instrument :

MSVOA_X

ClientSampleId :





STORAGE-BLANK-SOIL-REF-6

Tot Ion: 98 Resp: 612674

Ion Ratio Lower Upper

98 100

100 66.1 52.4 78.6

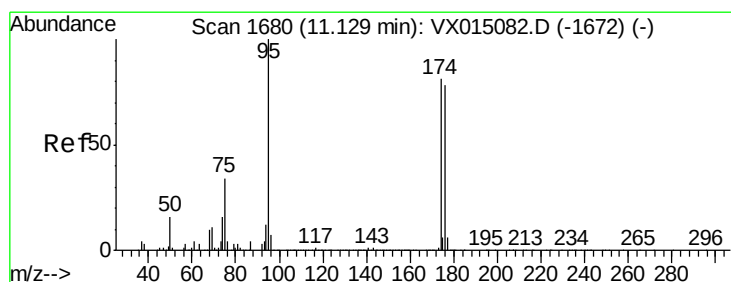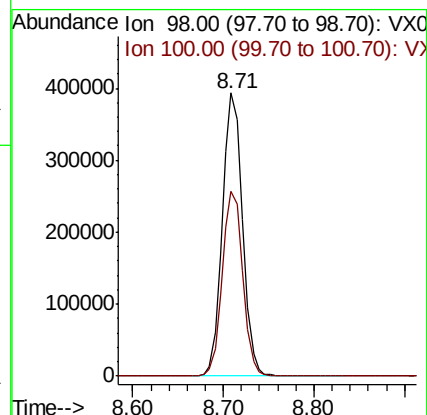

#62

4-Bromofluorobenzene

Concen: 50.549 ug/l

RT: 11.13 min Scan# 1680

Delta R.T. 0.00 min

Lab File: VX015313.D

Acq: 17 Mar 2020 10:44




Tgt Ion: 95 Resp: 218731


Ion Ratio Lower Upper

95 100

174 89.1 0.0 177.6

176 85.4 0.0 170.2


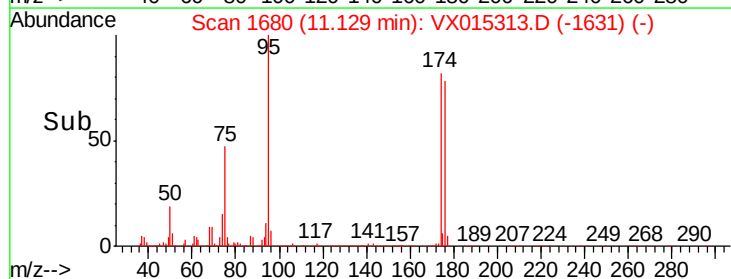
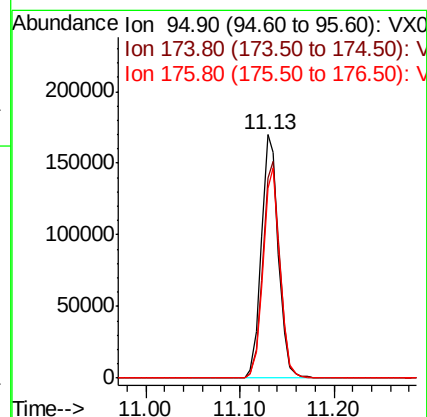





#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.11 min Scan# 1512
Delta R.T. -0.01 min
Lab File: VX015313.D
Acq: 17 Mar 2020 10:44




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6


Tot Ion	Ratio	Lower	Upper
117	100		
82	55.3	43.3	64.9
119	31.6	25.8	38.8

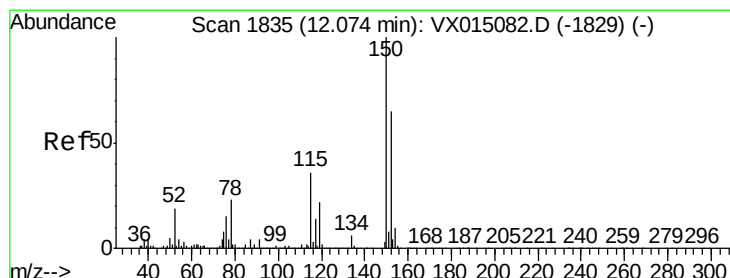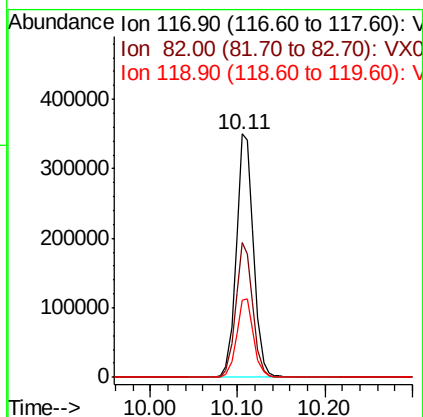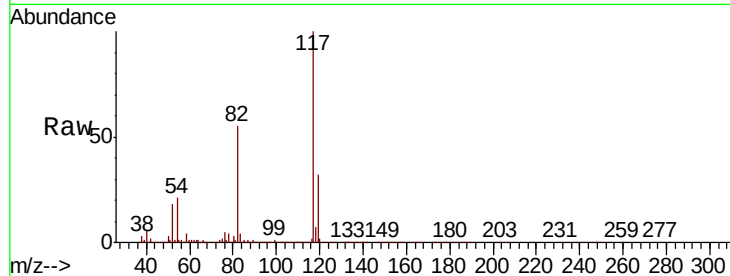

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.07 min Scan# 1835
Delta R.T. 0.00 min
Lab File: VX015313.D
Acq: 17 Mar 2020 10:44

Tgt Ion	Ratio	Lower	Upper
152	100		
115	55.4	38.2	114.6
150	155.3	0.0	343.8

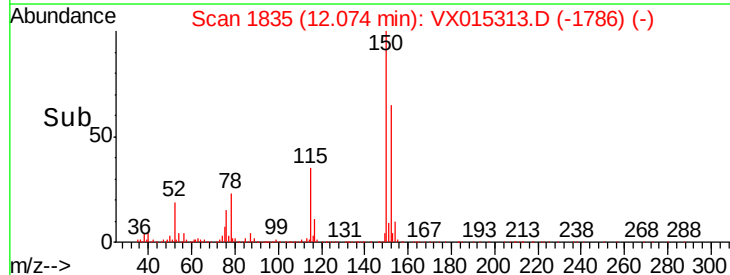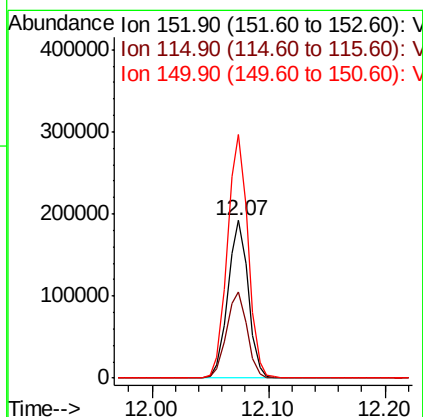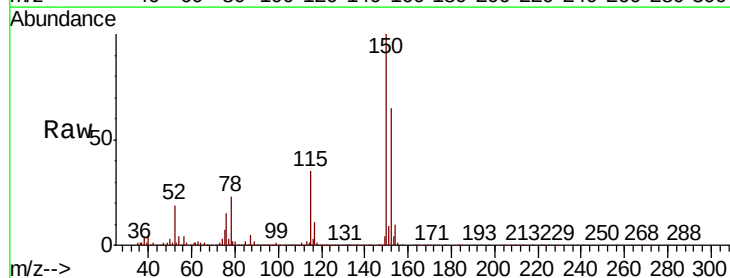



#76

1,2,3-Trichloropropane

Concen: 22.456 ug/l

RT: 11.13 min Scan# 1680

Delta R.T. -0.16 min

Lab File: VX015313.D

Acq: 17 Mar 2020 10:44

Instrument :

MSVOA_X

ClientSampleId :


STORAGE-BLANK-SOIL-REF-6

Tot Ion: 75 Resp: 104839

Ion Ratio Lower Upper




75 100

77 1.7 22.6 67.8#

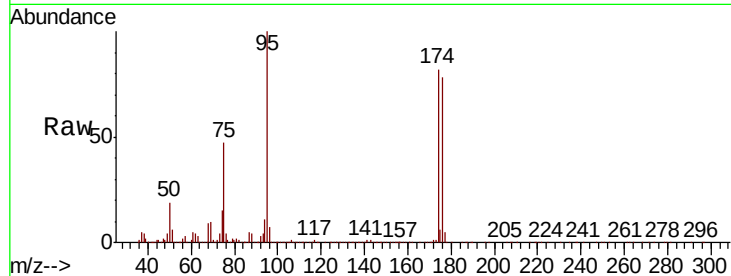

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0

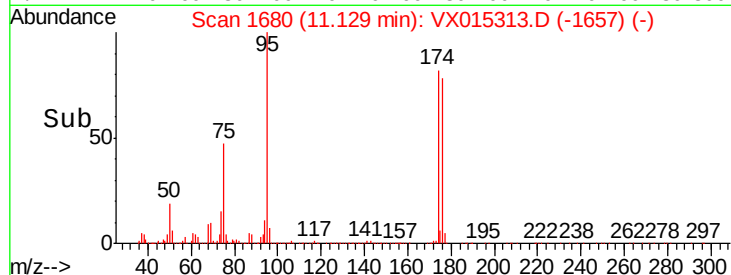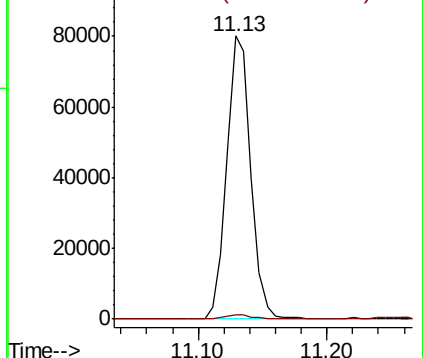

#81

trans-1,4-Dichloro-2-butene

Concen: 63.729 ug/l

RT: 11.13 min Scan# 1680

Delta R.T. 0.06 min

Lab File: VX015313.D

Acq: 17 Mar 2020 10:44


Tgt Ion: 75 Resp: 104839

Ion Ratio Lower Upper

75 100

53 0.2 77.9 116.9#



89 0.1 36.2 54.2#

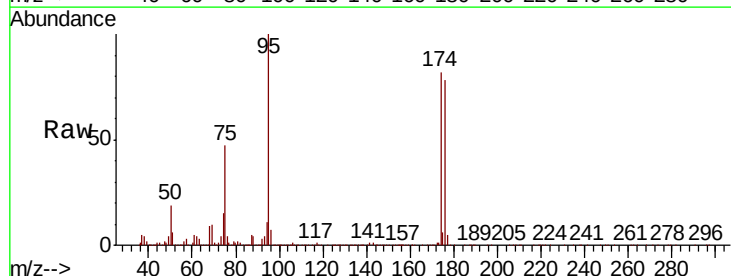


Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 53.00 (52.70 to 53.70): VX0

Ion 88.90 (88.60 to 89.60): VX0

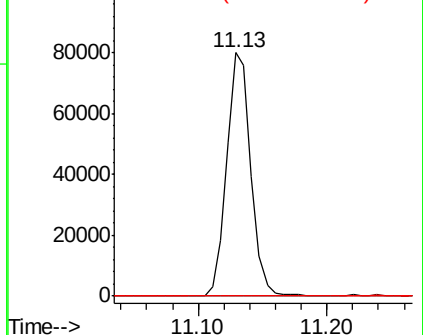

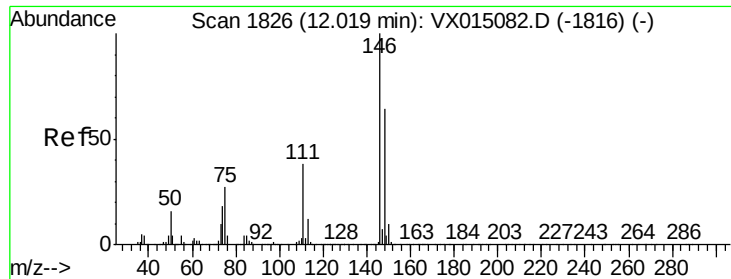

#87

1,3-Dichlorobenzene

Concen: 0.244 ug/l

RT: 12.02 min Scan# 1826

Delta R.T. 0.00 min

Lab File: VX015313.D

Acq: 17 Mar 2020 10:44

Instrument :

MSVOA_X

ClientSampleId :

STORAGE-BLANK-SOIL-REF-6


Tot Ion:146 Resp: 1784

Ion Ratio Lower Upper

146 100

111 42.7 19.1 57.1




148 67.4 31.9 95.5

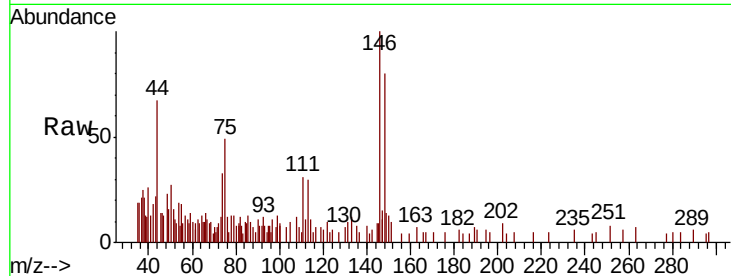

Abundance Ion 145.90 (145.60 to 146.60): V

Ion 110.90 (110.60 to 111.60): V

Ion 147.90 (147.60 to 148.60): V

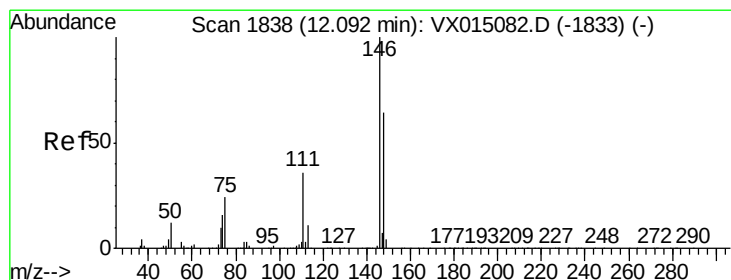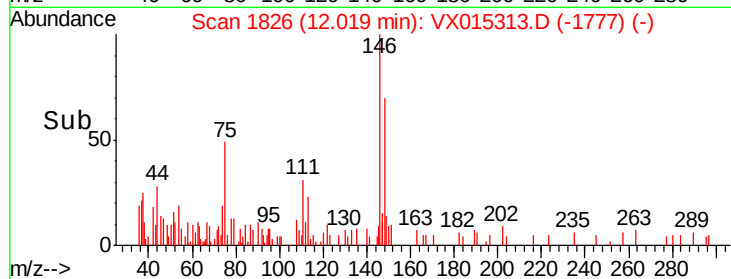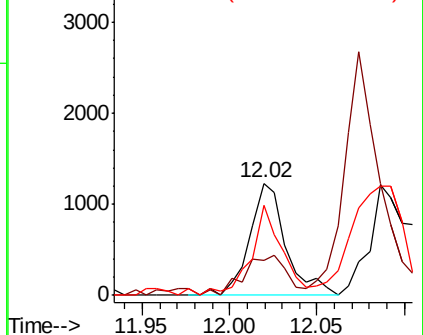

#88

1,4-Dichlorobenzene

Concen: 0.236 ug/l

RT: 12.02 min Scan# 1826

Delta R.T. -0.07 min

Lab File: VX015313.D

Acq: 17 Mar 2020 10:44


Tgt Ion:146 Resp: 1784

Ion Ratio Lower Upper

146 100

111 42.7 18.7 56.1



148 67.4 32.5 97.4




Abundance Ion 145.90 (145.60 to 146.60): V

Ion 110.90 (110.60 to 111.60): V

Ion 147.90 (147.60 to 148.60): V




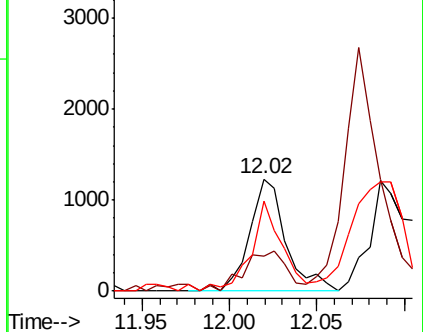




#89
n-Butylbenzene
Concen: 0.222 ug/l
RT: 12.39 min Scan# 1886
Delta R.T. 0.00 min
Lab File: VX015313.D
Acq: 17 Mar 2020 10:44




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6


Tot Ion: 91 Resp: 2637
Ion Ratio Lower Upper
91 100
92 51.0 27.2 81.6
134 37.0 13.5 40.5

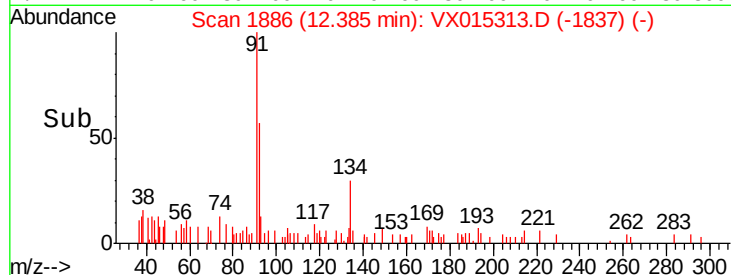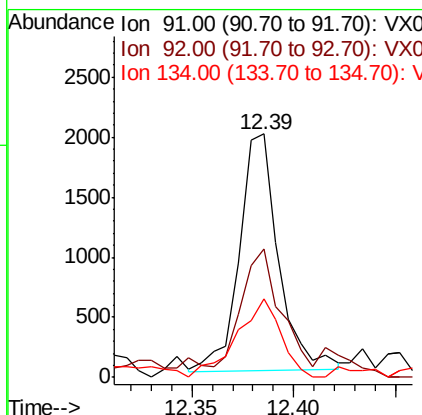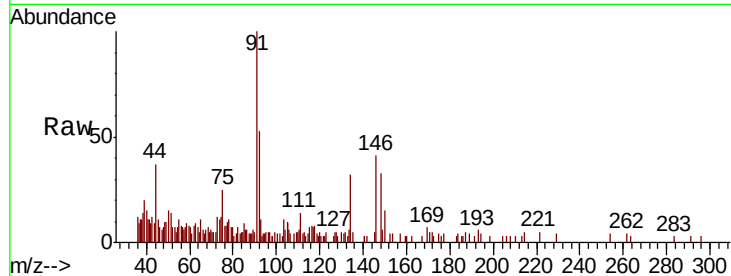

#93
1,2,4-Trichlorobenzene
Concen: 0.372 ug/l
RT: 13.64 min Scan# 2092
Delta R.T. 0.00 min
Lab File: VX015313.D
Acq: 17 Mar 2020 10:44

Tgt Ion: 180 Resp: 1879
Ion Ratio Lower Upper
180 100
182 103.2 47.6 142.8
145 38.2 14.1 42.2

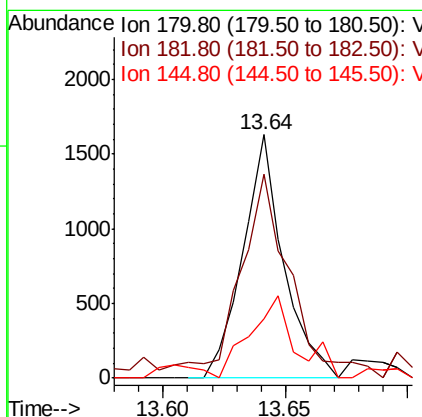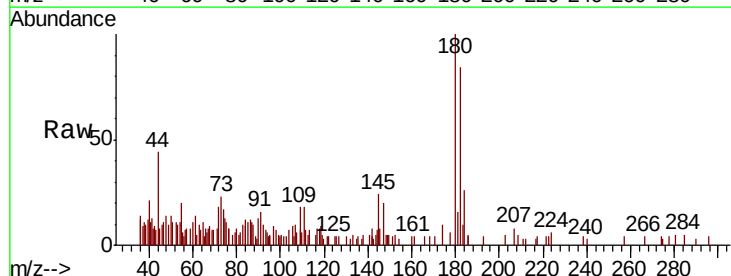







#94
Hexachlorobutadiene
Concen: 0.358 ug/l
RT: 13.78 min Scan# 2114
Delta R.T. 0.00 min
Lab File: VX015313.D
Acq: 17 Mar 2020 10:44

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6

Tot Ion:225 Resp: 928
Ion Ratio Lower Upper
225 100
223 74.5 31.3 93.9
227 86.4 31.1 93.2

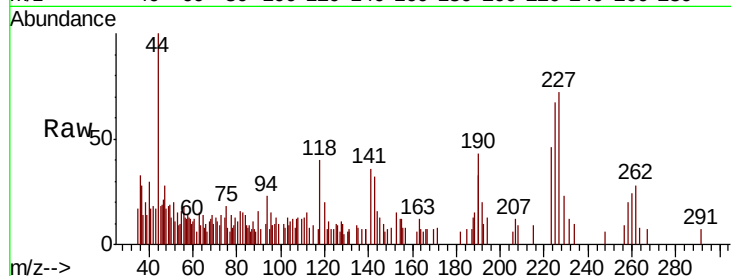


Abundance Ion 224.70 (224.40 to 225.40): V
Ion 222.70 (222.40 to 223.40): V
Ion 226.70 (226.40 to 227.40): V


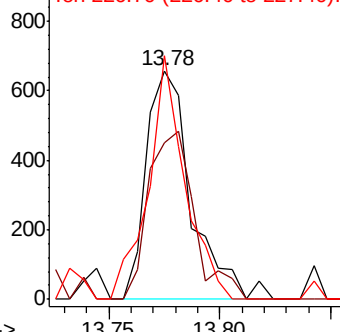



#95
Naphthalene
Concen: 1.622 ug/l
RT: 13.83 min Scan# 2123
Delta R.T. 0.00 min
Lab File: VX015313.D
Acq: 17 Mar 2020 10:44

Tgt Ion:128 Resp: 3225
Ion Ratio Lower Upper
128 100
127 21.6 10.3 15.5#
129 20.9 8.6 13.0#



Abundance Ion 128.00 (127.70 to 128.70): V
Ion 127.00 (126.70 to 127.70): V
Ion 129.00 (128.70 to 129.70): V

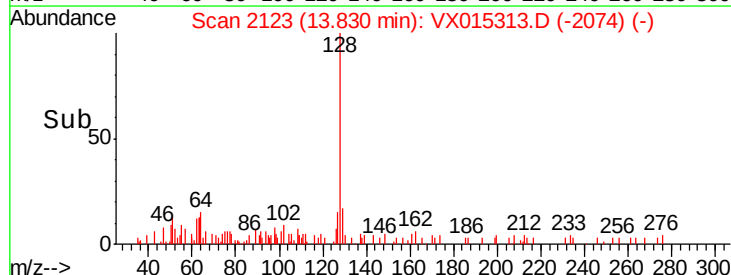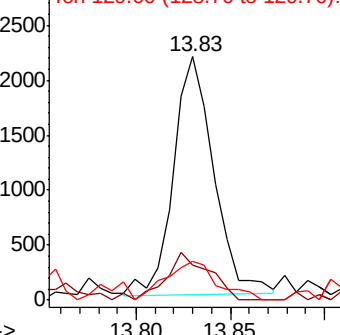

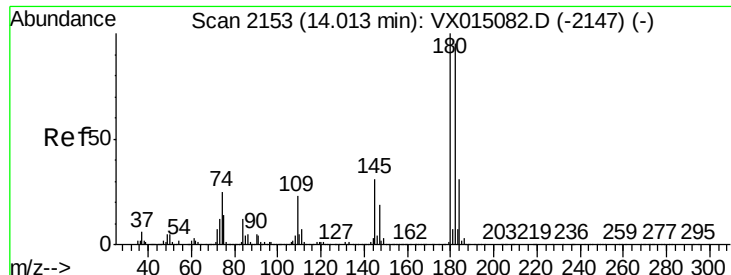

#96

1,2,3-Trichlorobenzene

Concen: 0.396 ug/l

RT: 14.01 min Scan# 2153

Delta R.T. 0.00 min

Lab File: VX015313.D

Acq: 17 Mar 2020 10:44

Instrument :

MSVOA_X

ClientSampleId :

STORAGE-BLANK-SOIL-REF-6


Tot Ion:180 Resp: 1996

Ion Ratio Lower Upper

180 100

182 81.6 47.8 143.4

145 34.4 15.1 45.3



Abundance Ion 179.80 (179.50 to 180.50): V

2000 Ion 181.80 (181.50 to 182.50): V

Ion 144.90 (144.60 to 145.60): V

